

LD BOOK

2020 EDITION



Where **innovation** leads to **success**



LDETEK COMPANY PROFILE


LDetek is a Canadian based company specialized in manufacturing, developing and integrating online gas analyzers, gas chromatograph systems and related accessories. Our mission is to provide reliable and performing systems with the best technology on the market.

With its commitment for continuous improvement, LDetek thinking and its members always aim to push the technology limit further. It brings innovative products and solutions to a market in a severe need of new and better quality material. The wide range of products, applications and patents developed, make LDetek portfolio attractive to many different areas of gas analysis activities. With a constant objective of offering quality products, LDetek always make all effort to get rigorous quality control and all necessary level of approbation and/or certification.

Our products and services are provided by a team of specialists with a strong experience in gas analysis business.

With a well established network of offices and partners in over 30 countries, a complete and pro active worldwide support is provided.

LDETEK, WHERE INNOVATION LEADS TO SUCCESS

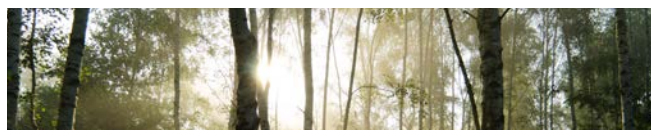

ENVIRONMENT



INDUSTRIAL GAS



PETROCHEMICAL



AGRICULTURE



ELECTRONIC GASES & SEMICONDUCTOR



NATURAL GAS



HYDROCARBONS PROCESSING



FOOD AND BEVERAGE



PHARMACEUTICAL AND MEDECINE



HEALTH AND SAFETY



ENERGY

TABLE OF CONTENTS

1.0 LDETEK PARTNERS

| | | |
|-----|--------------------------|---|
| 1.0 | Offices/Partners Listing | 4 |
|-----|--------------------------|---|

2.0 PRODUCTS

| | | |
|------|--|----|
| 2.1 | MultiDetek series | 7 |
| 2.2 | MultiDetek2 EX | 19 |
| 2.3 | LD8000 online analyser series | 23 |
| 2.4 | LDP1000 purifier series | 34 |
| 2.5 | PlasmaDetek (PED) series | 36 |
| 2.6 | LDGSS stream selector system | 49 |
| 2.7 | LD2000 online THC analyser | 51 |
| 2.8 | LabDetek | 55 |
| 2.9 | LD Accessories | 58 |
| 2.10 | LDGDS gas dilution system | 60 |
| 2.11 | LDrack system integration and LDportable solutions | 62 |

3.0 APPLICATION NOTES

| | | |
|------|---|-----|
| 3.1 | Environment | 65 |
| | LD12-01 - Greenhouse analysis with the PlasmaDetek | 66 |
| | LD15-03 - Measurement of part per billion N2O in air | 69 |
| | LD16-01 - Air analysis using the MultiDetek2 and PlasmaDetek2 | 72 |
| | LD16-13 - Measurement of Greenhouse gases GHG | 74 |
| | LD19-06 - VOCs measurement in the air | 78 |
| 3.2 | Industrial gas | 83 |
| | LD12-02 - Analysis of permanent gases and light hydrocarbons with the PlasmaDetek | 84 |
| | LD12-03 - Analysis of argon in pure oxygen with the PlasmaDetek and ArgoTek | 86 |
| | LD12-04 - Analysis of nitrogen in hydrogen and oxygen bulk with the PlasmaDetek | 88 |
| | LD12-06 - Increasing argon production with the MultiDetek | 91 |
| | LD12-07 - Analysis of Neon-Hydrogen-Argon-Krypton-Nitrogen with the PlasmaDetek & the HSR-Etek column | 93 |
| | LD12-09 - Hydrocarbons measurement for Oxygen production using PlasmaDetek & Multidetek-2 | 96 |
| | LD13-01 - Analysis of UHP Hydrogen production using Plasmadetek-2 & micro GC Multidetek-2 | 99 |
| | LD13-02 - Measurement of nitrogen in a mixture of Argon-Oxygen | 102 |
| | LD14-01 - Light hydrocarbons measurement with the *PlasmaDetek-E system with nitrogen carrier gas and the MultiDetek-2 | 104 |
| | LD15-08 - Measurement of impurities in UHP helium using MultiDetek2 and PlasmaDetek2 | 108 |
| | LD16-02 - Analysis of hydrocarbons, CO2, N2O in Oxygen with the MultiDetek2 compact GC system and the PlasmaDetek-E detection technology | 112 |
| | LD16-06 - LD8000 MultiGas online gas analysis solution for high purity compressed Helium used in cryogenic installations | 115 |
| | LD16-07 - Measurement of impurities in UHP Argon using the MultiDetek 2 and PlasmaDetek 2 | 117 |
| | LD16-08 - Measurement of hydrocarbons in UHP Oxygen using the MultiDetek 2 and PlasmaDetek-E | 119 |
| | LD16-09 - Measurement of trace impurities in UHP Hydrogen | 123 |
| | LD16-10 - Measurement of trace Ar-Kr and N2 in a bulk gas Oxygen | 125 |
| | LD16-11 - Measurement of trace impurities in multiple bulk gases | 127 |
| | LD19-05 - Measurement of impurities in UHP Argon for HIP process | 135 |
| | LD20-04 - MultiDetek2 with PlasmaDetek2 configured as online analyser for fast Crude Argon analysis | 140 |
| 3.3 | Petrochemical | 143 |
| | LD12-08 - Analysis of Sulfurs with the PlasmaDetek | 144 |
| | LD13-03 - Measurement of H2S and COS in Syngas with MultiDetek 2 | 148 |
| | LD16-05 - Refinery gas analyses with MultiDetek2 compact gas chromatograph and PlasmaDetek2 gas detector | 150 |
| | LD17-01 - Trace Hydrocarbons and Permanent gases in Propylene | 154 |
| 3.4 | Agriculture | 157 |
| | LD15-01 - Measurement of hydrocarbons, including the organic hormone (Ethylene) in CO2 production with MultiDetek-2 and PlasmaDetek-E | 158 |
| 3.5 | Electronic gases & semiconductor | 161 |
| | LD15-02 - Measurement of part per billion Ar and N2 in oxygen for semiconductor industry | 162 |
| | LD15-04 - Measurement of silane purity in electronic gases industry | 166 |
| | LD16-03 - Measurement of part per billion H2-NMHC-CH4-N2-CO2-CO for semiconductor gases | 169 |
| | LD18-01 - Measurement of trace impurities in Germane (GeH4) for electronic gas industry using PlasmaDetek2 and MultiDetek2 | 175 |
| | LD18-02 - Measurement of part per billion H2-CO-N2-CH4-CO2 in UHP gases for semiconductor | 179 |
| | LD19-02 - Measurement of trace impurities in high purity Nitrogen trifluoride (NF3) for electronic gas industry | 187 |
| | LD19-03 - Measurement of trace impurities in high purity nitrous oxide (N2O) for electronic gas industry | 191 |
| | LD20-02 - MultiDetek2 gas chromatograph with PlasmaDetek2 detector uses for hydrogen isotopes separation and the analysis of impurities in Deuterium | 197 |
| | LD20-03 - MultiDetek2 gas chromatograph with PlasmaDetek2 detector uses for the analysis of semiconductor specialty gases as UHP Octafluorocyclobutane (C4F8) | 199 |
| 3.6 | Natural gas | 201 |
| | LD15-09 - Measurement of THT in natural gas using MultiDetek2 and PlasmaDetek2 | 202 |
| | LD19-01 - Measurement of THT-TBM odorants in natural gas | 205 |
| | LD19-04 - Measurement of sulfurs & mercaptans combined with THT-TBM in natural gas | 210 |
| 3.7 | Energy | 215 |
| | LD16-04 - Sulfur Hexafluoride (SF6) purity analysis using the MultiDetek 2 and PlasmaDetek 2 | 216 |
| 3.8 | Food and Beverage | 219 |
| | LD16-12 - Trace impurities in Carbon Dioxide for beverage and food packaging industry | 220 |
| | LD17-02 - Gas analysis for wineries | 226 |
| | LD17-04 - Trace impurities in Carbon Dioxide for beverage and food packaging industry | 228 |
| 3.9 | Pharmaceutical and Medical | 233 |
| | LD20-01 - MultiDetek2 uses for medical & pharmaceutical applications | 234 |
| 3.10 | Design Reports | 237 |
| | LD8000 - Design report | 238 |
| | LD12-05 - Design report | 246 |
| | LD2000 - Design report | 250 |
| | Trace moisture analysis - Design report | 255 |
| | LD8000-Multigas - Design report - Configured for cryogenic Helium application | 263 |

4.0 TESTIMONIALS

| | | |
|-----|--|-----|
| 4.1 | LDT-01 - Analysis of permanent gases in different matrix using PlasmaDetek mounted on a Perkin Elmer GC | 272 |
| 4.2 | LDT-02 - Analysis of trace impurities in different gas matrix using PlasmaDetek mounted on Agilent 7890 GC | 273 |
| 4.3 | LDT-03 - Analysis of impurities in Argon using PlasmaDetek2 mounted on a GAS Compact GC | 274 |
| 4.4 | LDT-04 - PlasmaDetek solutions mounted on Perkin Elmer GC | 275 |
| 4.5 | LDT-05 - Analysis of trace impurities in electronic grade hydrogen using PlasmaDetek2 mounted on Agilent 6890 GC | 276 |
| 4.6 | LDT-06 - Analysis of hydrocarbons using PlasmaDetek2 mounted on DANI Master GC | 277 |
| 4.7 | LDT-07 - Trace N2O analysis for greenhouse application using PlasmaDetek2 mounted on Agilent 7890 GC | 279 |
| 4.8 | LDT-08 - Multidetek2 solutions for the energy market | 280 |
| 4.9 | LDT-09 - Application of PlasmaDetek in Determination of Trace Neon in High Purity Helium | 281 |

5.0 CHROMATOGRAMS

| | | |
|-----|------------|-----|
| 5.1 | Impurities | 286 |
| 5.2 | Samples | 302 |

LDETEK PARTNERS

Offices/Partners Listing

Thetford Mines, Canada (*Head Office*)
Beijing, China (*China Office*)

| | |
|-------------------------|------------------------------------|
| Argentina, Buenos Aires | Norway, Oslo |
| Australia, Melbourne | Pakistan, Karachi |
| Australia, Peakhurst | Peru, Lima |
| Austria, Neustadt | Philippines, Laguna, Binan |
| Brazil, Rio De Janeiro | Poland, Wroclaw |
| Brazil, Sao Paulo | Romania, Bucharest |
| Chile, Santiago | Russia, St-Petersburg |
| Colombia, Bogota | Singapore |
| Egypt, Cairo | Slovak Republic, Prievidza |
| Finland, Helsinki | South Africa, Edenvale |
| France, Paris | Spain, Barcelona |
| Germany, Frankfurt | Spain, Madrid |
| Greece, Athens | Sweden, Stockholm |
| Hungary, Budapest | Taiwan, Taipei |
| India, Mumbai | Thailand, Bangkok |
| Indonesia, Jakarta | Turkey, Istanbul |
| Iran, Tehran | UAE, Abu Dhabi |
| Israel, Acre | Ukraine, Kiev |
| Italy, Cesano Maderno | United Kingdom, Oxon, Wantage |
| Japan, Tokyo | Uruguay, Montevideo |
| Korea, Seoul | USA, Colorado, Denver |
| Lithuania, Vilnius | USA, Massachusetts, Peabody |
| Malaysia, Selangor | USA, Oregon, Dayton |
| Mexico, Monterrey | USA, Pennsylvania, King of Prussia |
| Netherlands, Lelystad | USA, Texas, Houston |
| Nigeria, Lagos | Việt nam, Ho chi Minh City |

CONTACT INFORMATION

Head office (Thetford Mines, Canada)

Sales and general request: info@ldetek.com
Technical support: support@ldetek.com
Phone : + 1 418 755 1319
Fax : + 1 418 755 1329

Chinese office

rli@ldetek.com
Phone: 01 87246220
Fax: 010 87806892
Mobile: 13911632686



2.0 PRODUCTS

Gas Chromatograph and detectors




Online Analysers

Cabinet Integration



Dilution System

Gas Purification

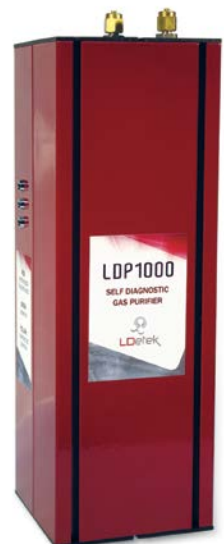

Stream selectors

Engineering Support

MULTIDETEK₂



COMPACT GAS CHROMATOGRAPH FOR INDUSTRIAL AND LAB APPLICATIONS

With its plug and play philosophy and offering more features than ever, LDetek pushes further the possibilities with its chromatograph system. It offers a robust and cost-effective solution for the industrial and laboratory markets.

Based on the LDetek high performance detection technology, this stand-alone Gas Chromatograph is a flexible and customized platform providing the best solution for any type of gas analysis.



FEATURES & DESIGN:

- One chassis configuration (6U Rackmount)
- Multichannels
- Multimethods
- Multidetectors
- Up to 6 isothermal or 3 programmable oven combination
- Up to 5 high purity proportional diaphragm valves (carrier-sample)
- Easy maintenance with its slide out design and front opening door
- ppt, ppb, ppm and % gas analysis
- Built in PC with 8.4" touch screen LCD & user-friendly interface
- Up to 10 high performance diaphragm valves
- Ethernet connectivity for remote control
- Integrated compact purifier with real end of life monitoring
- Serial/Profibus/Modbus communication protocols
- Fast parallel chromatography
- Multi heated zones to avoid cold points
- Purged & real time monitored zones for hazardous gases
- Multi sample injection techniques

BUILT IN PC WITH 8.4" TOUCHSCREEN LCD & USER-FRIENDLY INTERFACE

The Multidetek-2 offers an easy and complete interface working on Windows 7 embedded. With its 8.4" clear LCD touch screen, it allows the operator to navigate easily through the different menus. Moreover, the system includes an Ethernet port for remote control.

PUSH BUTTON

Friendly push button to open the front door.

KEYBOARD OPERATION

Beside the touch screen panel PC, each system is provided with a USB keyboard to operate the user interface.





COMPACT AND RACK MOUNT DESIGN

With a 6U rack mount chassis, this compact GC design can be installed in many different areas going from industrial to laboratory. It can be installed where available space is limited as well as transportable unit.

USB CONNECTOR / EXTERNAL STORAGE

Data can be stored on an external drive and/or move to any other system or computer to be visualized at any time. This USB port is also available for software update or any other windows 7 interfacing.




HIGH PERFORMANCE DIAPHRAGM VALVE

The use of high performance diaphragm valve bring outstanding measurement performance. A longer lifetime and better performance on common GC techniques are achieved. They also allow new analysis methods. 1/16" and/or 1/32" diaphragm valve connections, tubing and columns are used. Using 1/32" can reduce carrier gas consumption reducing operation cost. Consult LDetek application notes for more information.




ISOTHERMAL AND/OR PROGRAMMABLE OVENS FOR ANY TYPE OF COLUMNS


The oven design can accept any type of packed, micro packed and plot columns. It offers a very stable and quick temperature controllable to proceed to high temperature column regeneration in the unit. With its multiple programmable ovens, more applications are feasible with reduced analysis time.

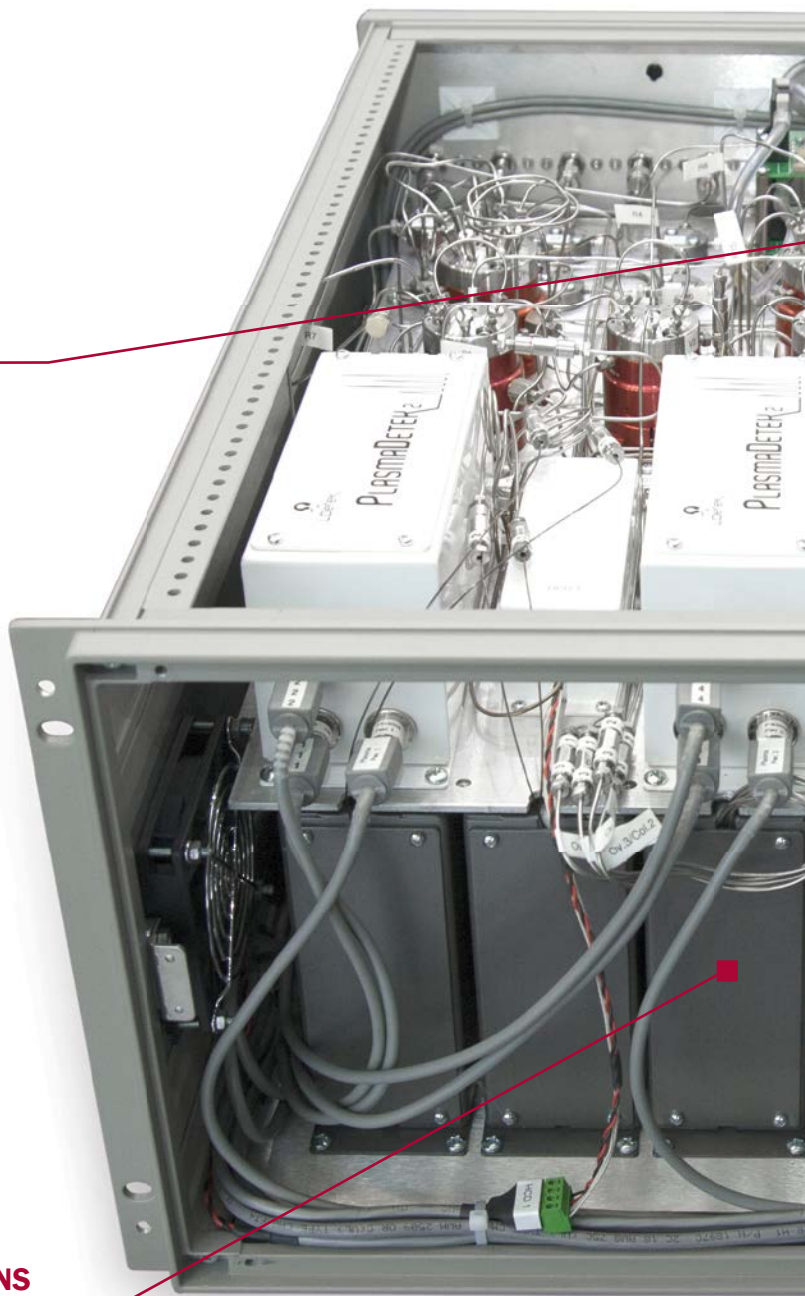

FRONT ACCESS TO THE ISOTHERMAL AND/OR PROGRAMMABLE RAMPING OVENS

The Multidetek-2 has been designed to give a complete access to all the hardware parts without removing the unit from the rack. The complete maintenance of the system can then be done by keeping the system on gas. This design gives the benefits to reduce the recovery time of the GC after proceeding to maintenance of the system. Also, in case of change of configuration the columns can be easily replaced with the front door.

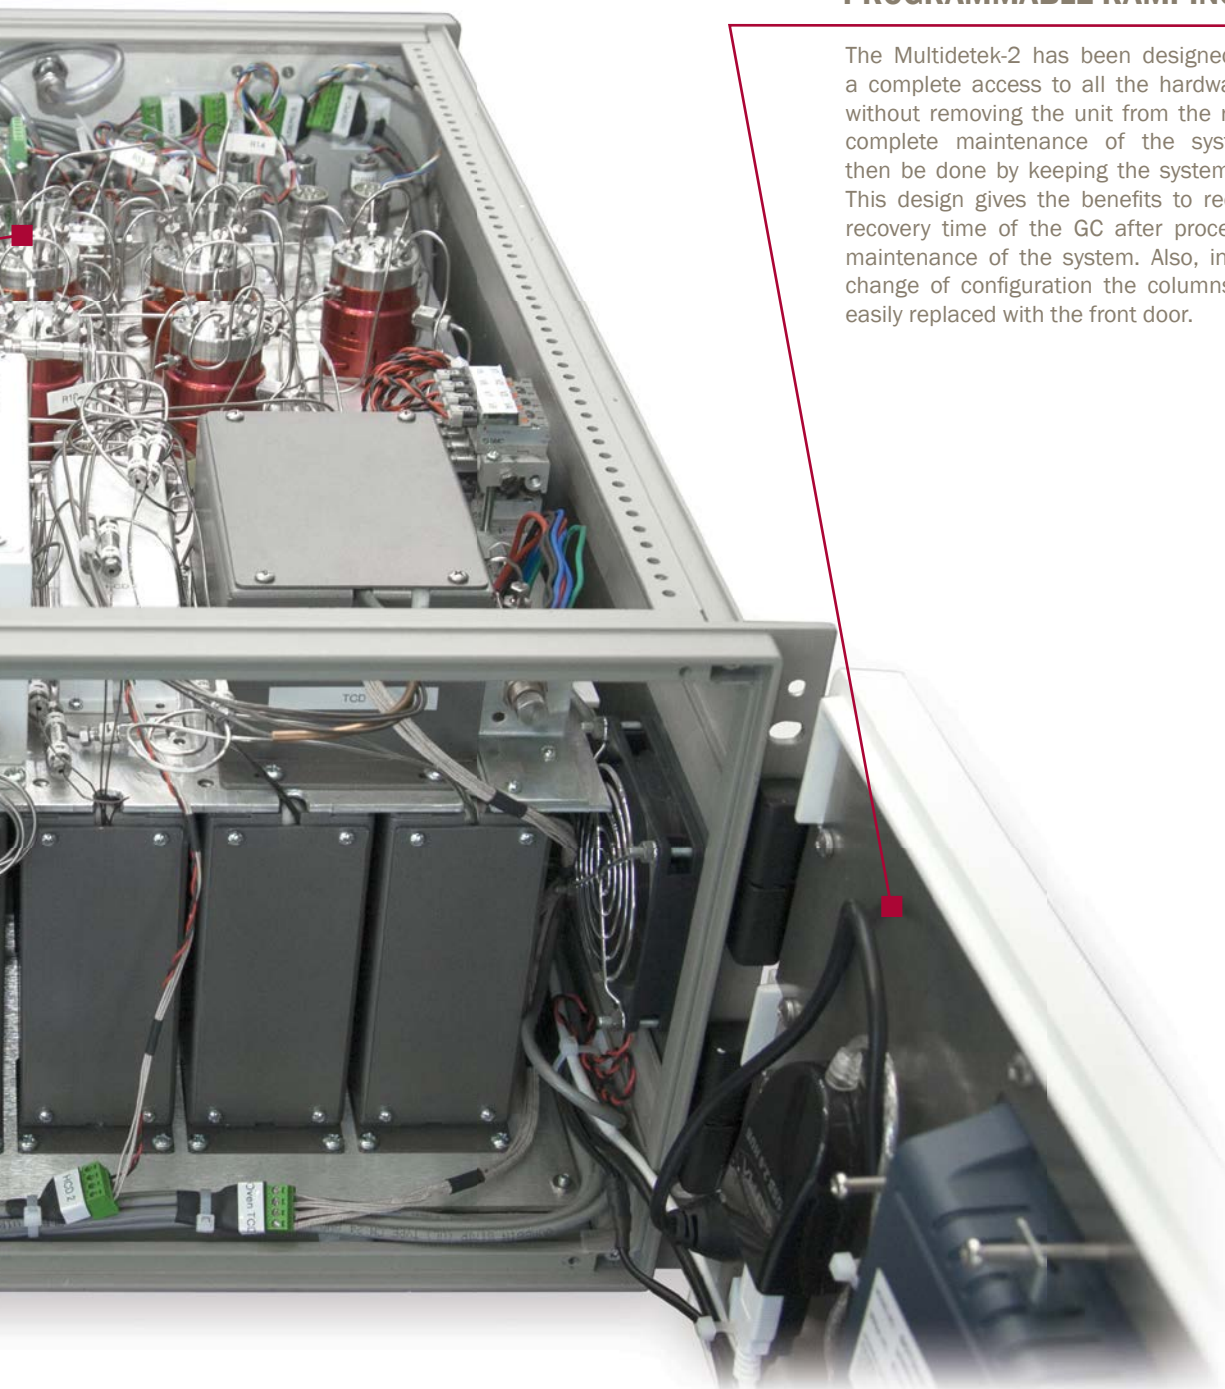

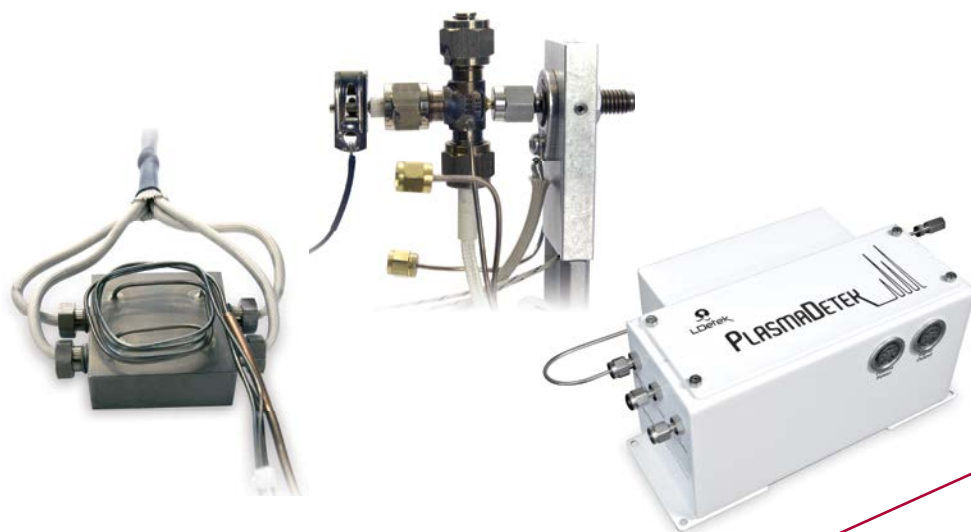



3 DETECTORS COMPATIBLE

Three detectors can be installed in the same chassis with a combination of any PED, TCD and FID detector. It gives more flexibility and the possibility to measure more components with one system.

INPUTS/OUTPUTS INTERFACE

Many inputs/outputs are available to be able to communicate and receive information from the device: Digital outputs for device status, serial communication (RS-232/485, Profibus, Modbus), analog inputs to acquire external device signal, 4-20 mA output for results information, ethernet for remote control, USB port.



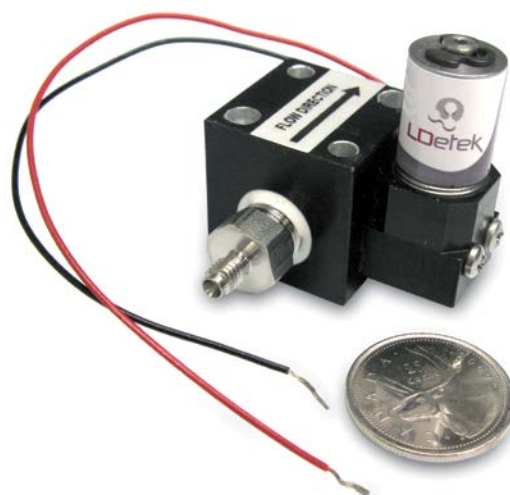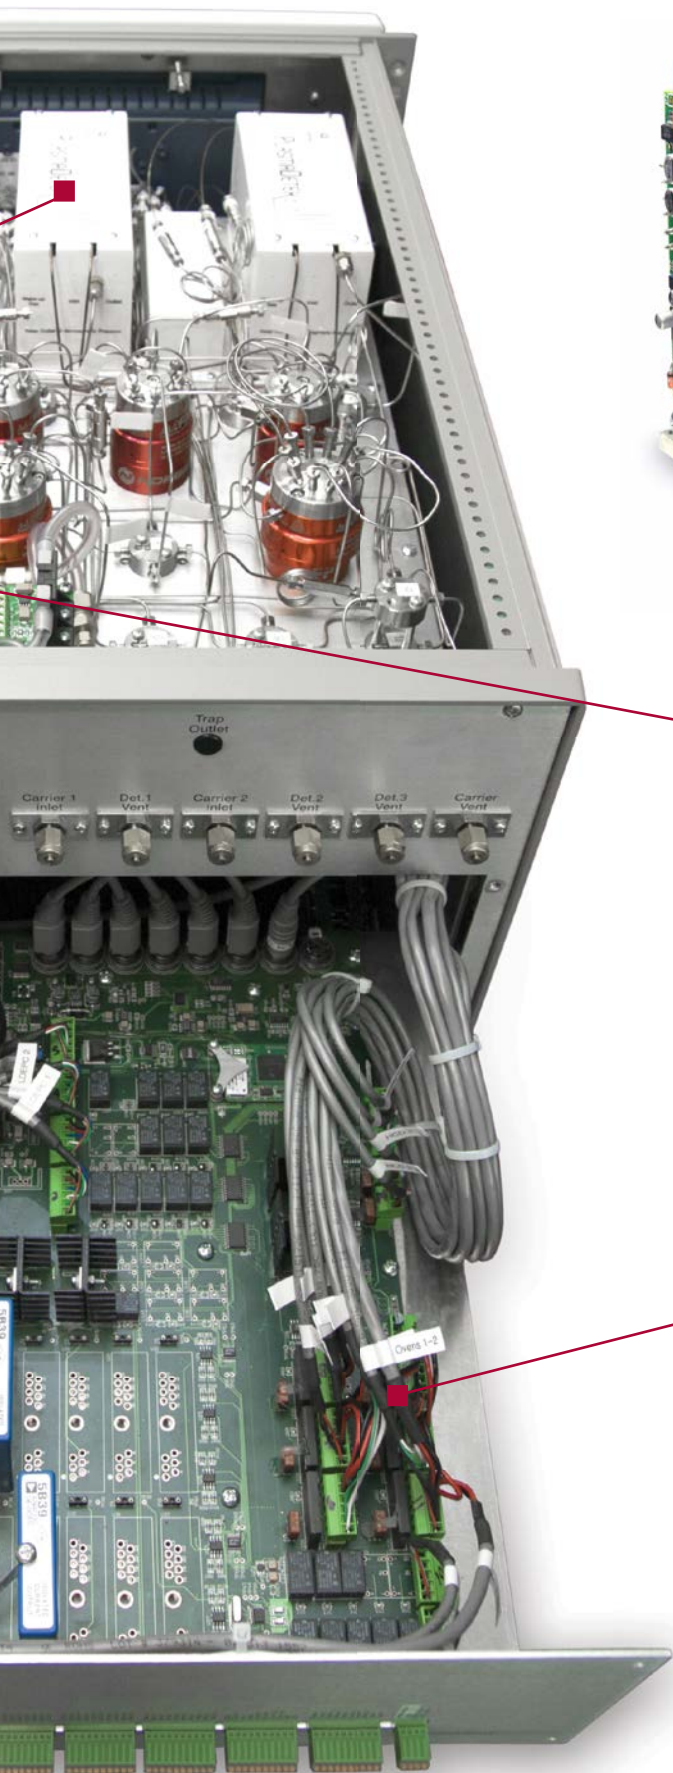


ELECTRONIC FLOW CONTROLLER

With its electronic flow controller, the MultiDetek 2 offers the possibility to have automatic flow adjustment. LDefek has developed its own valve design offering low dead volume and fast response time. A manual version is also available.

EASY MAINTENANCE WITH ITS SLIDE OUT DESIGN

The same approach has been done on the back side of the unit. Other critical components can be reached from the back for maintenance purpose using its pull out rail system. Again, it gives the benefit to perform system maintenance with reduced recovery time without removing the gas lines from the unit.



LDchroma gas chromatography software for process/lab analyses

LDchroma software is used to control the internal components of the MultiDetek2 gas chromatograph and make the bridge with the surrounding industrial environment and the rest of the world offering a full remote control of your instrument.

What it controls internally?

- Temperatures, flows, valves, detectors, A/D inputs, A/D outputs, streams selection, calibration, alarms

What kind of intelligence it offers?

- Maintenance interval/cost and lifetime of components
- A choice across a multiple peak detection algorithms is automatically selected
- Secure, administrator-controlled user access and permissions to ensure data integrity
- Simplified run creation, including sequence, methods and reports

How it communicates with the external world?

LDchroma can talk with automated systems using Modbus, Profibus or Profinet (other protocols available on request) depending on the requirements. It is generally used to send/receive any type of commands and results with the plant.



For the remote control of the LDchroma software, the Ethernet connection also allows the use of any type of remote control software compatible with Windows. It becomes easy to operate your gas analyser at distance and also select your desired method/stream and even calibrate it.




LDreport for data management

LDreport can perform many different types of report format. You can customize the analysis certificate as you desire. LDreport can save in multiple format as pdf, excel and html. You can also print it on your local printer or any printer connected on the network. Adding company logo and other custom information can be put on the report template as well.

LDreport is also used as database where you have access to all chromatograms and results from your instrument. It is very useful to compare results, trends, chromatograms by selecting any period range. LDreport is well designed to simplified backup, searching, and trending of chromatography data.

HOW OUR SOLUTION MAKES **YOUR LIFE EASIER**



ROBUSTNESS & MODULARITY

Nothing better than showing our own gas chromatograph to demonstrate a symbol of robust and modular design offering all the gas analysis possibilities inside one compact instrument. Your application has changed, and your instrument must be re-configured? No problem! Our modularity design makes it easy to readapt the instrument to your actual need. Design by experts, for leaders.

REMOTE ACCESS

Remote connection through network allows our experts to access your instruments for quick support. Our platform infrastructure allows to access the internal database of the instrument to know all the historic events. Years of information, access in a second.

WORLDWIDE HIGH SKILL TECHNICAL RESSOURCES

Wherever you are located, we have high skill experts ready to help you. Our training program within our organization makes our technical resources always up to date and ready.

WARRANTY & TRADE IN PROGRAMS

Extended warranty programs are there to make your life easier. Our high value design product gives you a residual value at its end of life to trade with our latest technology available. Let us work for you!

HOW WE MEASURE **CONFIDENCE**



By having the demonstration of our ability to build robust solutions based on highly skilled involved employees and high quality criteria company philosophy. This is represented by long durability of our instruments being more than 11 years. At the end of this cycle, our company engagement is proud to open discussions to offer the residual value of your highly valuable analytical instrument in exchange for our latest technology device suitable for your application.

ASK US FOR OUR SERVICE
AND WARRANTY PROGRAMS AVAILABLE

FULL WARRANTY 18 MONTHS

EXTENDED WARRANTY PROGRAM UP TO 10 YEARS

MAINTENANCE PROGRAM EVERY 3-5 YEARS



Apply your residual value
with our trade-in program
with latest technology



MULTIDETEK2 CHART V2:

| | Backgrounds → | Air | Ar | He | Ne | Kr | Xe | H ₂ | O ₂ | N ₂ | CH ₄ | CO | CO ₂ | N ₂ O | C ₂ H ₄ | C ₃ H ₆ | NH ₃ |
|-----------------|--|-----|----|----|----|----|----|----------------|----------------|----------------|-----------------|----|-----------------|------------------|-------------------------------|-------------------------------|-----------------|
| Gas Types | Impurities | — | — | — | — | — | — | — | — | — | — | — | — | — | — | — | — |
| ↓ | ↓ | — | — | — | — | — | — | — | — | — | — | — | — | — | — | — | — |
| noble | Ar (argon) | ✓ | — | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| noble | He (helium) | ✓ | ✓ | — | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| noble | Ne (neon) | ✓ | ✓ | ✓ | — | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| noble | Kr (krypton) | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| noble | Xe (xenon) | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| permanent | H ₂ (hydrogen) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| permanent | O ₂ (oxygen) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| permanent | N ₂ (nitrogen) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| permanent | CO (carbon monoxide) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ | ✓ | ✓ | ✓ |
| permanent | CO ₂ (carbon dioxide) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ | ✓ | ✓ |
| permanent | H ₂ O (moisture) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | — | — | — |
| fluorocarbon | CF ₄ (tetrafluoromethane) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| fluorocarbon | C ₂ F ₆ (hexafluoroethane) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| greenhouse | SF ₆ (sulfur hexafluoride) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| greenhouse | N ₂ O (nitrous oxide) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ | ✓ |
| inorganic | NF ₃ (nitrogen trifluoride) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| inorganic/toxic | NH ₃ (ammonia) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | — | — |
| inorganic/toxic | PH ₃ (phosphine) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — |
| inorganic/toxic | AsH ₃ (arsine) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| toxic | CH ₂ O (formaldehyde) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | — | — |
| toxic | C ₂ H ₄ O (acetaldehyde) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | — | — |
| hydrocarbon | CH ₄ (methane) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | NMHC (non methane hydrocarbon) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | — | ✓ |
| hydrocarbon | C ₂ H ₂ (acetylene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₂ H ₄ (ethylene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ |
| hydrocarbon | C ₂ H ₆ (ethane) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ |
| hydrocarbon | C ₃ H ₆ (propylene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ |
| hydrocarbon | C ₃ H ₈ (propane) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ |
| hydrocarbon | C ₃ H ₄ (propadiene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₃ H ₄ (propyne) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₄ H ₆ (1,3 butadiene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₄ H ₈ (butylene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₄ H ₁₀ (isobutane) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₅ H ₈ (pentadiene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₅ H ₁₀ (pentene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₅ H ₁₂ (isopentane) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₆ H ₁₂ (hexene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₆ H ₁₄ (hexane) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₇ H ₁₄ (heptene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₇ H ₁₆ (heptane) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₈ H ₁₆ (octene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| hydrocarbon | C ₈ H ₁₈ (octane) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| btex/aromatic | C ₆ H ₆ (benzene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| btex/aromatic | C ₇ H ₈ (toluene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| btex/aromatic | C ₈ H ₁₀ (xylene) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| sulfur | H ₂ S (hydrogen sulfide) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ |
| sulfur | COS (carbonyl sulfide) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | — | ✓ | ✓ |
| sulfur | SO ₂ (sulfur dioxide) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| sulfur | CS ₂ (carbon disulfide) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| sulfur | CH ₃ S (methyl mercaptan) | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ |
| sulfur | THT (tetrahydrothiophene) | — | — | — | — | — | — | — | — | — | — | — | — | — | — | — | — |
| sulfur | TBM (tert-butylthiol) | — | — | — | — | — | — | — | — | — | — | — | — | — | — | — | — |
| | Backgrounds → | Air | Ar | He | Ne | Kr | Xe | H ₂ | O ₂ | N ₂ | CH ₄ | CO | CO ₂ | N ₂ O | C ₂ H ₄ | C ₃ H ₆ | NH ₃ |

| CF ₄ | C ₂ F ₆ | SF ₆ | NF ₃ | C ₄ F ₈ | C ₃ F ₈ | C ₃ F ₇ | C ₂ F ₅ | SiH ₄ | GeH ₄ | Si ₂ H ₆ | HCl | Cl ₂ | WF ₆ | SiF ₄ | Syngas | Natural gas | ← Back |
|-----------------|-------------------------------|-----------------|-----------------|-------------------------------|-------------------------------|-------------------------------|-------------------------------|------------------|------------------|--------------------------------|-----|-----------------|-----------------|------------------|--------|-------------|---------------------------------|
| -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | Impurities |
| -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ↓ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | Ar |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | -- | He |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | -- | Ne |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | -- | Kr |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | Xe |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | H ₂ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | O ₂ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | N ₂ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | CO |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | CO ₂ |
| ✓ | -- | -- | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | H ₂ O |
| -- | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | -- | CF ₄ |
| ✓ | -- | ✓ | ✓ | -- | ✓ | ✓ | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | C ₂ F ₆ |
| ✓ | ✓ | -- | ✓ | -- | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | -- | SF ₆ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | N ₂ O |
| -- | ✓ | ✓ | -- | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | -- | NF ₃ |
| ✓ | -- | -- | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | -- | NH ₃ |
| ✓ | ✓ | ✓ | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | -- | PH ₃ |
| ✓ | ✓ | ✓ | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | -- | AsH ₃ |
| ✓ | -- | -- | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | -- | CH ₂ O |
| ✓ | -- | -- | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | -- | C ₂ H ₄ O |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | CH ₄ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | NMHC |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | C ₂ H ₂ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | C ₂ H ₄ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | C ₂ H ₆ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | C ₃ H ₆ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | C ₃ H ₈ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | C ₃ H ₄ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | C ₃ H ₄ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | C ₄ H ₆ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | C ₄ H ₈ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₄ H ₁₀ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | C ₅ H ₈ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₅ H ₁₀ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₅ H ₁₂ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₆ H ₁₂ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₆ H ₁₄ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₇ H ₁₄ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₇ H ₁₆ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₈ H ₁₆ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₈ H ₁₈ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₈ H ₆ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₇ H ₈ |
| ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | ✓ | -- | C ₈ H ₁₀ |
| ✓ | ✓ | ✓ | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | ✓ | H ₂ S |
| ✓ | ✓ | ✓ | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | ✓ | COS |
| ✓ | ✓ | ✓ | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | ✓ | SO ₂ |
| ✓ | ✓ | ✓ | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | ✓ | CS ₂ |
| ✓ | ✓ | ✓ | ✓ | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | ✓ | CH ₄ S |
| -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | THT |
| -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | -- | ✓ | TBM |
| CF ₄ | C ₂ F ₆ | SF ₆ | NF ₃ | C ₄ F ₈ | C ₃ F ₈ | C ₃ F ₇ | C ₂ F ₅ | SiH ₄ | GeH ₄ | Si ₂ H ₆ | HCl | Cl ₂ | WF ₆ | SiF ₄ | Syngas | Natural gas | ← Back |


SPECIFICATIONS:

| | |
|--|---|
| DETECTOR TYPE | PED, TCD, FID |
| STANDARD FEATURES | <ul style="list-style-type: none"> • Manual or auto-ranging (user selectable) • Microprocessor controlled • Windows 7 embedded user-friendly interface • Ethernet port for remote control • Isothermal and/or programmable ramping ovens • Electronic flow control regulators for carrier & sample gases • 8.4" LCD large touch screen • Self diagnosis system with auto-resolve alarm • 4-20 mA isolated outputs • Alarm Historic • Digital system status output for remote monitoring (dry relay contact) • 2 alarms contact • High resolution Chromatogram output |
| OPTIONS | <ul style="list-style-type: none"> • Serial communication (RS232/485) / Profibus / Modbus / Ethernet • Compact purifier attached to the chassis for generating high purity carrier gas • Integrated stream selector system • Digital inputs for remote starting • Analog inputs for connecting external instruments • Remote control for stream selector (LDGSS) • Purged zones for hazardous gases • Heated zones to avoid cold points • Monitoring system for hazardous gases • Split/split less injector (can be heated) • Integrated dilution system |
| GAS CONNECTIONS | 1/8" or 1/4" VCR or compression fittings |
| CARRIER PRESSURE REQUIREMENTS | 100 PSIG |
| OPERATING TEMPERATURE | 10 °C to 45 °C |
| SUPPLY | 115 VAC, 50 – 60 Hz or 220 VAC, 50 – 60 Hz |
| POWER CONSUMPTION | Maximum 500W |
| REPEATABILITY | Three times the percentage of deviation (3*CV %) of each component has to be smaller than 5% on ten consecutive cycles |
| LDL | 3 times noise level |
| LOQ | 3 times LDL value |
| LONG TERM STABILITY & DRIFT | Three times the percentage of deviation (3*CV %) of each component has to be smaller than 10% for 8 hours |
| LINEARITY | For 5 points within the measuring range, the linear curve must have its R2 at a value between 0.998 and 1.00 |

CERTIFICATION:

CE In compliance with EMC directive 2004/108/EC, EN 61000-6-2:2005 for immunity & EN 61000-6-4:2007 for emissions.

DIMENSIONS:

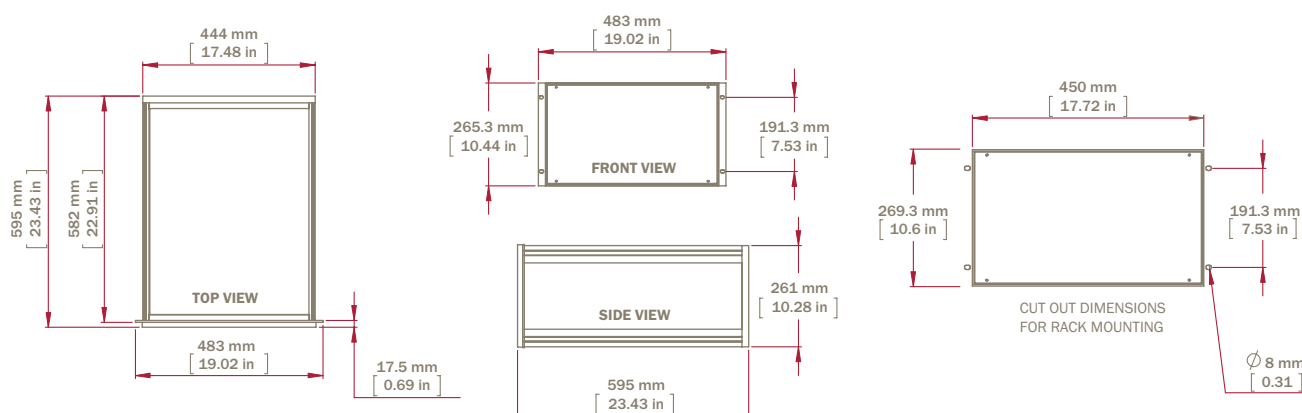

Where innovation leads to success

www.ldetek.com

MultiDetek₂ EX



EXPLOSION PROOF GC SOLUTION DESIGNED FOR HAZARDOUS AREAS



An innovative design based on simplicity. The standard industrial compact GC model MultiDetek2 is now integrated inside a Stainless Steel certified (ATEX-IECEx) purged enclosure to be used in Zone1 and Zone 2 hazardous areas. This “EX” series allows to keep the proven robust industrial platform features of the MultiDetek2 with its LDChroma software interface. It also allows to mount more than one GC or other instruments/accessories in the same MultiDetek2 EX purged enclosure. On top of that, using the standard rackmount platform of the MultiDetek2 mounted on a slide out system makes it easy to swap units inside the enclosure for maintenance or application upgrade. A multi streams/GCs and methods all in one system approaches was the objective with the launch of the MultiDetek2 EX series.

FEATURES

- Explosion proof for use in zone 1 and zone 2
- Capable to integrate multiple instruments and sampling system all in one unit
- Designed to mount up to 2 standard units' model MultiDetek2
- Easy to swap and access units inside the enclosure with its slide out design
- Triclops X purge controller is capable to feed up to 3 enclosures in cascade or parallel for more possibilities.
- Stainless Steel cabinet with secured doors (IP66)
- Wall mount or floor mount available
- Front industrial panel PC
- LAN remote control for GC and stream selector
- LDChroma industrial GC interface with LDReport database software
- Industrial communication protocols (Modbus-Profibus from Ethernet/RS232/RS485)
- Up to 10 analog outputs 4-20mA
- Up to 6 isothermal ovens to fit capillary, micropacked or packed columns with an easy access to replace columns.
- Up to 10 diaphragm/rotary valves to build multiple methods for multiple streams
- Can combine up to 3 detectors in one GC (PED, TCD, FID, Quartz crystal for H₂O, electrochemical sensor or third party sensor)
- Electronic pressure and flow controllers
- Corrosion resistant material available (option)
- Analysis in ppb/ppm/%
- One status alarm contact and two levels alarm contacts are available
- A non-purged version is also available for use in safe zones

INDUSTRIES/APPLICATIONS

- Hydrogen Production
- Hy/CO Plants
- Hydrocarbons Processing
- Petrochemicals (measurement of CO-CO₂)
- Chemical Plants
- Natural Gas/LNG Processing
- Electronic Gases
- Air Separation Units (ASU)
- Refineries (analysis of CO in propylene and ethylene)
- Synthesis Gas (measurement of H₂)
- Other related industries



DESIGN

Area for mounting accessories as extra sensors and/or gas purifier (LDP1000) or others.


Front Panel PC with 8.4" LCD.

MultiDetek2 slide out design for easy access (enough space available for a second slide out for another MultiDetek2).


Tryclops-X purge system proved according to EN 60079 (The same device can feed up to 3 different EX cabinets).

MultiDetek2 GC instrument having capacity to mount multiple ovens(6x)/ detectors(3x)/ valves(10x)/electronic flow controllers(5x) for analysis of multiple streams with multiple methods built in.

An ultra high purity 4 channels stream selector can be integrated in the GC.

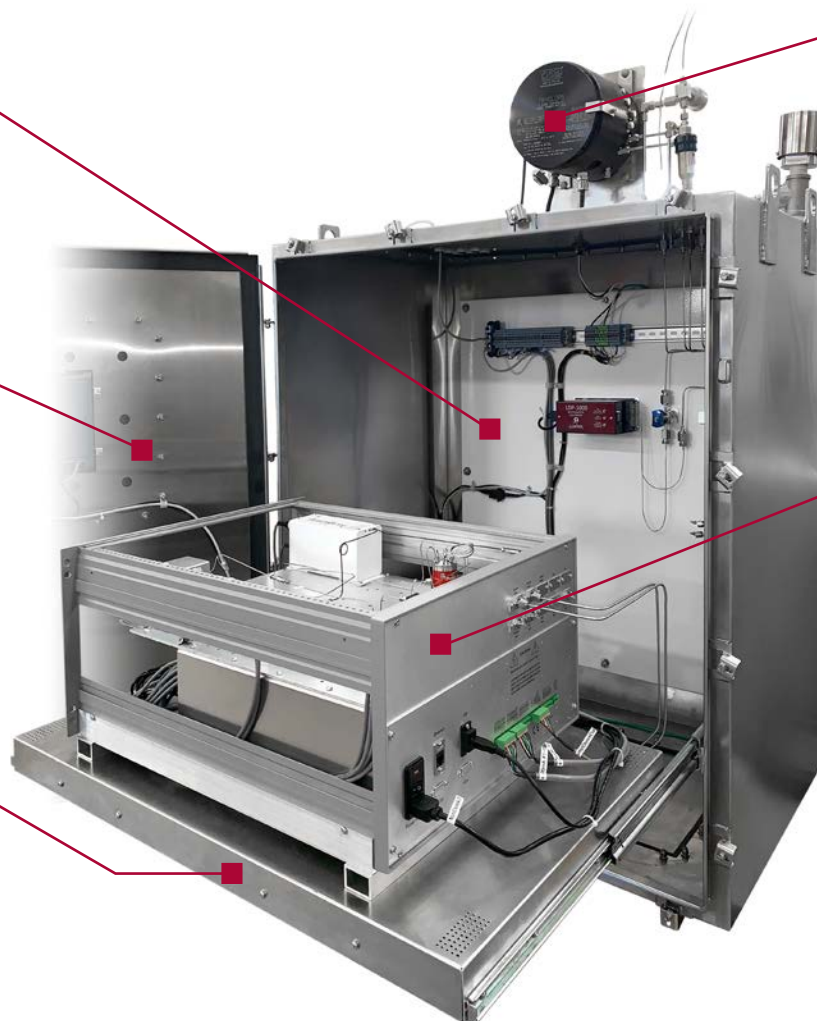

DIMENSIONS

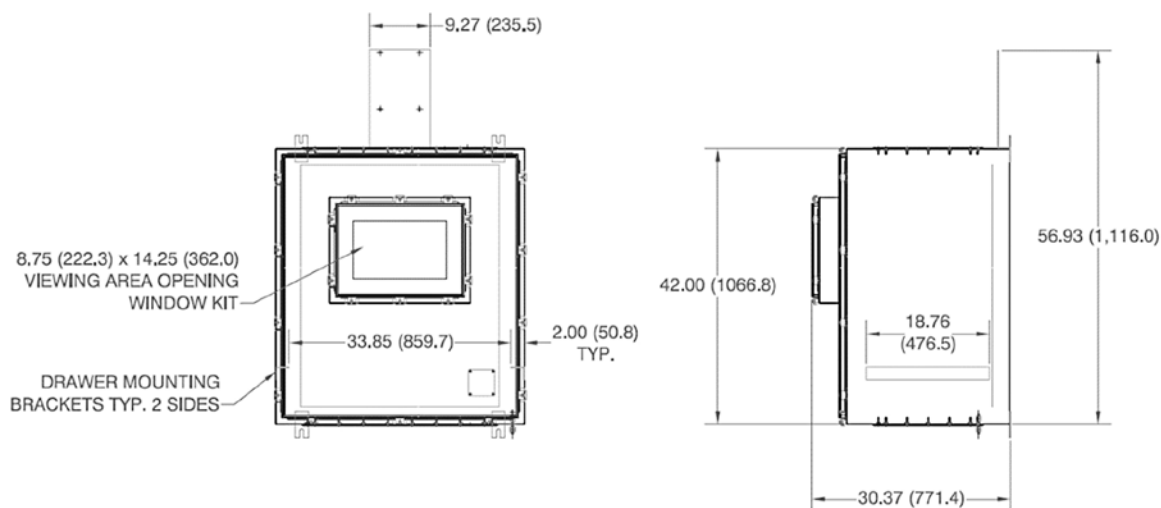

SPECIFICATIONS

| | |
|--|---|
| GENERAL DIMENSIONS | 38" W (965mm) X 30.37"D (771mm) X 56.93" H (1116mm) (other sizes available on request) |
| MATERIAL | Stainless Steel |
| DOOR CLEARANCE | 37" (932 mm) |
| WEIGHT | 227 kg |
| STANDARD FEATURES | <ul style="list-style-type: none"> • 1 Tryclops X-Purge controller, XP version certified for Zone 1 and Zone 2 hazardous areas • 1 air Exhaust • 1 air purge gas inlet kit • 1 8.4" panel PC per MultiDetek2 GC • 1 Adjustable check valve on sample gas • 1 Flashback arrestor on sample gas • 1 pneumatic shut off valve on sample gas |
| OPTIONS | <ul style="list-style-type: none"> • 1 Vortex cabinet cooler with AC muffler • Additional instruments can be added • Up to three purged enclosures can be mounted in cascade using the same Tryclops • Floor mount rack |
| OPERATING ENVIRONMENT | Indoor and outdoor |
| CARRIER GAS PRESSURE | 100 PSI (6.9 bar) |
| SAMPLE GAS PRESSURE | 5-30 PSI (0.35-2 bar) |
| GAS CONNECTIONS | 1/8" or 1/4" VCR or Compression type (Swagelok) |
| PURGE PROTECTIVE GAS SUPPLY QUALITY | Dry air grade : Water and oil-free, - 40° F (- 40° C) dew point, particles 5µ, ISA grade hydrocarbon-free |
| SUPPLY | 115 VAC, 50 – 60 Hz or 220 VAC, 50 – 60 Hz |
| POWER CONSUMPTION | Maximum 660 watts |
| APPLIED STANDARDS | <ul style="list-style-type: none"> • EN60079-0 • EN60079-2 • EN60079-7 • EN60079-11 • EN60079-15 • EN60079-18 |
| CERTIFICATIONS | IECEx : Ex pxb IIB+H2 T4 Gb ATEX : II 2 G Ex pxb IIB+H2 T4 Gb CE (MultiDetek2) |
| OPERATING TEMPERATURE | -20 °C to 47 °C |
| T CLASSIFICATION | T4 |
| IP | 66 |
| ENCLOSURE VOLUME | 727.8 liters |
| MINIMUM PURGE FLOW | 120 L/min |
| MINIMUM PURGE TIME ON START-UP | 78 minutes |
| MAXIMUM OVERPRESSURE | 0.1 PSI (6.7 mBar) |
| MINIMUM OVERPRESSURE | 0.02 PSI (1.24 mBar) |
| MAXIMUM SUPPLY AIR PRESSURE | 100 PSI (6.9 bar) |
| MINIMUM SUPPLY AIR PRESSURE | 15 PSI (1.4 bar) |

LD8000



TRACE NITROGEN IN ARGON, HELIUM AND CRUDE ARGON ANALYZER



The LD8000 is an online analyzer to monitor trace N₂ in Ar/He/Crude Argon. Plasma emission detector is used to selectively measure trace N₂ in Argon or/and Helium bulk gases. The analysis of trace N₂ in Neon, Xenon and Krypton can also be realized.



Plasma Emission
Detector for N₂

FEATURES:

- Trace Nitrogen in Argon/Helium/Crude Argon
- Compact 3U rackmount enclosure
- Large scale measurement
- 4-20 mA outputs as standard
- LAN/Web control
- Range Identification Relay
- Micro-valve for very low dead volume and fast purging time
- Low sample consumption
- Optional zero gas calibration free system

APPLICATIONS:

- Air separation unit
- Helium cryogenic installation
- Cryogenic truck loading station
- Speciality gas laboratories
- Process control
- Argon purification plant
- Steel Industries
- Chemical plants
- Welding gas control
- Helium liquification plants
- Gas management system
- Semiconductor manufacturing
- Quality control for truck fills and gas cylinders
- Inert glove box systems
- Universities and laboratories


SPECIFICATIONS:

| | | |
|--|--|--|
| DETECTOR TYPES | Plasma Emission Detector for N ₂ | |
| RANGE FOR N₂ | 0 – 1 ppm, resolution to 10 ppb 0 – 10 ppm, resolution to .1 ppm | 0 – 100 ppm, resolution to 1 ppm other range possible up to 5000 ppm configurable |
| STANDARD FEATURES | <ul style="list-style-type: none"> Manual or autoranging (user selectable) Microprocessor controlled 5.6" TFT intelligent LCD module with Touch Screen Self diagnosis system with auto-resolve alarm 4-20 mA isolated outputs | <ul style="list-style-type: none"> Alarm Historic Safe calibration procedure to avoid any bad calibration Digital outputs for remote monitoring: (all dry relay contacts) <ul style="list-style-type: none"> - System status (1 output) - Range in use (3 outputs per impurity) - Calibration in use (1 output) |
| OPTIONS | <ul style="list-style-type: none"> Internal sampling system for zero, span and sample | <ul style="list-style-type: none"> Serial port: RS-232 / 422 / 485 / Profibus 2 alarm outputs (user programmable set point) Zero calibration gas free system |
| GAS CONNECTIONS | Sample: 1/8" compression fittings | Vent: 1/8" compression fitting |
| CALIBRATION GAS | Zero: LDP1000 purified gas (Getter) | Span: 8.0 to 9.5 ppm N ₂ (application dependant) |
| SAMPLE FLOW REQUIREMENTS | 75 to 200 sccm | |
| OPERATING TEMPERATURE | 10 °C to 45 °C | |
| SUPPLY | 115 VAC, 50 – 60 Hz or 220 VAC, 50 – 60 Hz | |
| ACCURACY | Better than ± 1% full scale | |
| DRIFT | < ± 1% | |
| RESPONSE TIME | T90 < 10 seconds | |
| OPERATING SAMPLE PRESSURE RANGE | 3-30psig (for lower sample pressure requirement, an additional high purity pump is used) | |
| OUTLET PRESSURE | Atmospheric | |
| ENCLOSURE TYPE | 3U rackmount type | |
| INGRESS PROTECTION | IP20 in accordance with IEC 60529 | |
| ENCLOSURE FINISH | RAL7030 powder coat | |
| CERTIFICATION | In compliance with EMC directive 2004/108/EC, EN 61000-6-2:2005 for immunity & EN 61000-6-4:2007 for emissions | |
| WEIGHT | 29 lbs (13 kg) | |

ORDERING INFORMATION:

| LD8000 | -X | -X | -XXX | -X | -XX | -X | -XXX | -X |
|--------|---------------------|---|--|------------------------|---|--------------------------------|---|-------------------------------------|
| | N2: Nitrogen | A: Argon H: Helium C: Crude Argon D: Dual (Argon + Helium) | Operating Voltage: 120: 120 volts 220: 220 volts | A: Alarm option | Integrated sampling system S1: 1 sample + zero + span S2: 2 samples + zero + span | C: Zero gas free system | Serial communication: RS2: RS-232 RS4: RS-485 PFB: Profibus | P: Purge valve and flowmeter |

DIMENSIONS:

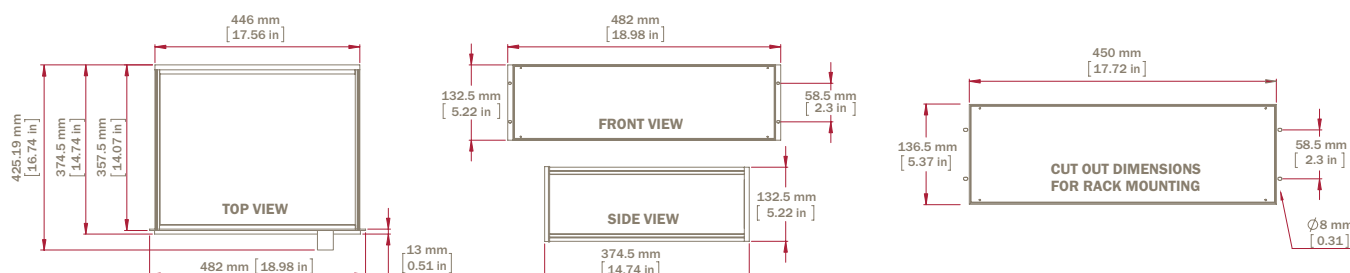


Where innovation leads to success

www.ldetek.com

LD8000 PLUS



ONLINE PPB TRACE NITROGEN IN ARGON/HELIUM ANALYZER

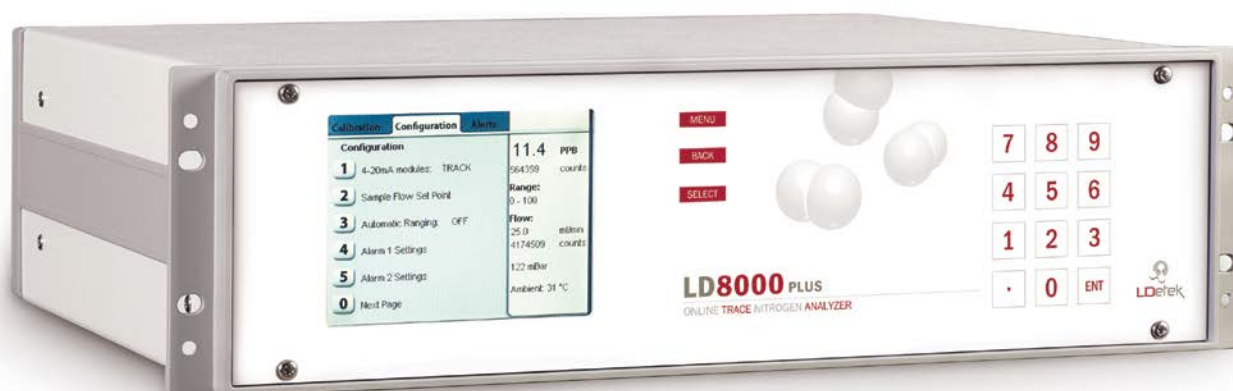

The LD8000-Plus is designed for ultra-pure Argon or Helium gas analysis. With its integrated ppb sub-system, unique performance can be achieved. Low ppb trace nitrogen online is now possible without the need of a gas chromatograph. This compact design makes it very attractive for any industrial or laboratory installation.

FEATURES:

- Unique Plasma Emission Detector design based on a Duty Cycle Controlled System.
- PPB sub-system integrated
- Bootloader integrated for software update via Ethernet
- Large scale measurement
- 4-20 mA output as standard
- Range Identification Relay
- Maintenance free
- Bypass sample flow control to insure high purity
- Low sample consumption
- 3U cabinet

APPLICATIONS:

- Air separation unit
- Speciality gas laboratories
- Process control
- Argon purification plant
- Chemical plants
- Helium liquification plants
- Gas management system
- Semiconductor manufacturing


SPECIFICATIONS:

| | | |
|--|---|--|
| DETECTOR TYPE | Plasma Emission Detector design based on a Duty Cycle Controlled System. Sub ppb system integrated. | |
| RANGE | 0 – 100 : resolution 0.1 ppb 0 – 500 : resolution 1 ppb | 0 – 5000 : resolution to 1 ppb, other range possible |
| REPEATABILITY | < 0.2% of range used | |
| ACCURACY | Better than $\pm 0.5\%$ of range used | |
| STANDARD FEATURES | <ul style="list-style-type: none"> Manual or autoranging (user selectable) Microprocessor controlled 5.6" TFT intelligent LCD module with Touch Screen Self diagnosis system with auto-resolve alarm 4-20 mA isolated output Alarm Historic Safe calibration procedure to avoid any bad calibration Digital outputs for remote monitoring: (all dry relay contacts) <ul style="list-style-type: none"> - System status (1 output) - Range in use (3 output) - Calibration in use (1 output) | |
| OPTIONS | <ul style="list-style-type: none"> Serial port: RS-232 / 422 / 485 / Profibus 2 alarm outputs (user programmable set point) | |
| GAS CONNECTIONS | Sample: 1/8" face seal fittings | Vent: 1/8" compression fitting |
| CALIBRATION GAS | Zero: LDP1000 purified gas (Getter) | Span: 3 to 4 ppm N ₂ /Ar |
| SAMPLE FLOW REQUIREMENTS | 15 to 200 sccm | |
| RECOMMENDED MAXIMUM OPERATING PRESSURE: | 20 PSIG (689 kPAG) | |
| RECOMMENDED MINIMUM OPERATING PRESSURE: | 10 PSIG (28 kPAG) | |
| OPERATING TEMPERATURE | 10°C to 45°C (must be stable) | |
| SUPPLY | 115 VAC, 50 – 60 Hz or 220 VAC, 50 – 60 Hz | |
| POWER CONSUMPTION | Maximum 70 watts | |
| DRIFT | < $\pm 0.5\%$ of range | |
| WEIGHT | 37 lbs (17 kg) | |

ORDERING INFORMATION:

| LD8000-Plus | -XXX | -X | -XXX |
|-------------|--|------------------------|---|
| | Operating Voltage: 120: 120 volts 220: 220 volts | A: Alarm option | Serial communication: RS2: RS-232 RS4: RS-485 PFB: Profibus |

DIMENSIONS:

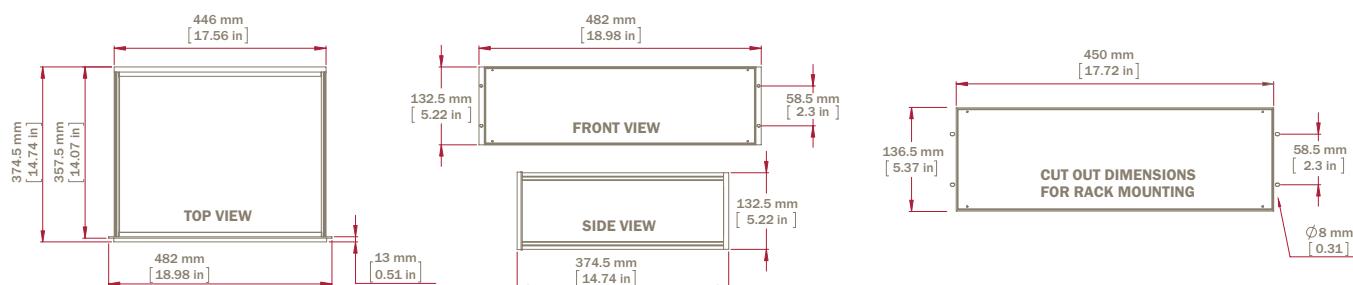

LD8000 MULTIGAS



TRACE NITROGEN, OXYGEN, MOISTURE, HYDROCARBONS ALL IN ONE UNIT



The LD8000MG is an online gas analyzer that can combine multiple sensors and technologies all in one unit to allow multiple impurities detection within a wide range of analysis.



▲ PlasmaDetek2



▲ SenzTx



▲ Easidew



▲ QMA

The unit is a rackmount 3U or 4U enclosure. The configuration depends on the sensors and options selected. Multiple configurations are available through a module platform philosophy.

FEATURES:

- Compact rackmount enclosure (3U or 4U) to cover up to four measurements (N₂, O₂, H₂O, CnHm)
- Bootloader integrated for software update via Ethernet
- Ultra high purity electronic flow controllers for sample flow control
- Large measurement scale
- Touchscreen 5.6" LCD
- 4-20 mA outputs
- Range Identification & alarm status & calibration contacts
- Alarm historic
- LAN/Web control
- Low sample consumption

APPLICATIONS:

- Industrial gas applications
- Inert and bulk gases
- Air separation unit
- Helium cryogenic installation
- Cryogenic truck loading station
- Process control
- Helium liquification plants
- Steel industry
- Chemical plants
- Gas generation
- Additive manufacturing
- Glove box purge and leak detection
- Research centers and laboratories

PROVEN SENSORS TECHNOLOGIES

PLASMADETEK (for more technical information, refer to our Design Report on LD8000 MultiGas series)

The measurement of the trace impurities N₂-O₂-H₂O-CnHm in a helium or argon matrix can be carried out with a PED type detector (PlasmaDetek2) US patent 9,310,308 B2 integrated into an instrument of the LD8000-Multigas type. This technology is based on cold microplasma excited at high voltage / frequency in a helium atmosphere and allowing the selective measurement of each component at a precise optical wavelength. The optical circuit is composed of photodiodes and interference filters combined with an amplification system for converting the measured photons into voltage. All signal processing is then redirected to a microcontroller.

Compared to previous art, the LD8000MG with PED sensor offers an interference free measurement. By the combination of selective bandpass optical filter with a nitrogen doping system and a network of adsorbents & permeation devices, each impurity is accurately measured without being affected by other impurities presence in the sample gas.

Several variants and options on this device are possible depending on the needs of the customer.

Low maintenance and cost of ownership

Using a non depleting PED sensor, the unit can be used for long term operation (over 10 years) without having to change it. This is also due to the network of protection adsorbent and the detector shut off system during upset conditions. The traps used in the unit are also protected by an isolation valve shut off in case of upset conditions. This is to ensure the durability of the traps and detectors inside the unit. All these factors combined together make our solution robust and minimize the maintenance on the unit.

Fast response time

The unit design allows to keep a minimal sample flow consumption and ensure a quick response time (T₉₀ at 10sec)by the use of 1/16"OD coated stainless steel lines. The flow controllers are mounted in bypass mode to minimize the gas volume and dead legs upfront of the PEDs.

SENZTX

With a choice of either zirconia or electrochemical sensor technology the SenzTx offers reliability, accuracy and flexibility. Both technologies have a broad measurement capability allowing the user to measure from selected ranges from 1ppm to 96% oxygen.

Zirconia sensor

The Ntron zirconia oxygen sensor is a nondepleting zirconia solid electrolyte sensor. A small capillary on the sensor controls the diffusion of oxygen into the sensor. When heated to over 400°C oxygen is electronically reduced causing current flow through the zirconia electrolyte. Zirconiumoxide allows the movement of oxygen ions through the substrate from a high to a low concentration. The measurement of oxygen is determined by the current flowing through the electrodes. The zirconia sensor has an unlimited shelf life without the loss of calibration and has an expected life in excess of 5 years. The zirconia sensor is not position sensitive and has low cross sensitivity to other gases and does not dry out.

Low maintenance and cost of ownership

Due to the highly stable nature of the sensor, a calibration interval of once per year is required, allowing for significant cost savings. The construction of our zirconia oxygen sensor means that only 100 mL/min of sample gas is required, providing application flexibility and further potential cost savings.

Fast response time

Zirconia oxygen sensors respond very quickly to oxygen concentrations in both directions with a T₉₀ of less than 10 seconds within a set range.

Electrochemical sensor

The key elements of the electrochemical sensors are a membrane, cathode, anode, electrolyte and measurement circuit. The sensing membrane (covering the cathode) is made of PTFE and is mounted over a metal perforated electrode. The space between the membrane and the electrode is filled either with an aqueous alkaline or an acid electrolyte. In normal operation, all portions of the anode and cathode are immersed in the electrolyte. As oxygen diffuses through the membrane into the electrolyte it causes a reaction between the cathode and anode generating an EMF. This current is proportional to the amount of oxygen present in the sample gas. In the absence of oxygen there is no output from the electrochemical sensor, meaning only one calibration is required.

EASIDEW

The Easidew transmitter has a wide measurement range from -110 to +20°Cdp (-166 to +68°Fdp) and one stocked product can be used across all class 1 to class 6 industrial dryer applications. The Easidew family of industrial transmitters incorporates the latest Michell advanced ceramic technology providing stable, reliable and repeatable moisture measurements for all dew point applications.

Ease of Installation

Flexible product design ensures the unit can be quickly and economically installed. • Mini DIN 43650 form C or M12 5 pin electrical connectors • 5/8" UNF, 3/4" UNF, G1/2" BSP process connections • 316 stainless steel transmitter sample blocks.

Measurement Performance

The transmitter uses Michell's market leading ceramic measurement technology coupled with the latest generation, sophisticated microcontroller electronics to provide accurate and stable measurement across the transmitter's product life.

QMA (for more technical information, refer to our Design Report for trace moisture analysis integrated inside the MultiDetek2 GC)

The Advanced Quartz Crystal Microbalance sensor from Michell Instruments is now integrated inside the LD8000MG to provide reliable, fast and accurate measurement of trace moisture content in a variety of applications where keeping moisture to a minimum is of critical importance. The analyzer provides consistently accurate measurements of trace moisture. This consistency is achieved using a self-calibration system, which adjusts the sensor with reference to an internal moisture generator.

Having such module inside the LD8000 multigas series allows to combine multiple impurities analysis with trace moisture inside the same instrument.

Quartz crystal microbalance sensor

A quartz crystal is sensitised with a thin film of hygroscopic material. Water molecules are adsorbed into the hygroscopic layer deposited on the surface. The change in mass modifies, in a very precise and repeatable manner, the oscillation frequency. The moisture concentration is measured as a change in the oscillation.

Quartz crystal sensor principle

The change in the oscillation is evaluated by switching the gas inside the sensor and by measuring the response delta. For sampling response, the sensor is balanced between a dry gas source and the sample source. The difference is then calculated. The same principle is applied for the span gas calibration. However, this time the comparison is between a dry gas and a source of wet gas. A cycling time of 30 seconds on each gas is used to compare the response delta.

Quartz crystal module principle

The dry gas comes from a reference gas source. The sensor is supplied by a known Helium or Argon or Nitrogen grade 5.0 carrier source going through a heated gas purifier model LDP1000 series. This combination generates a gas purity of 8N. By using this technique, the dry gas source contains less than 10ppb H₂O what is ideal as zero gas reference.

The wet gas comes from a certified water filled permeation tube heated at a controlled temperature of 45 Celsius. It generates a stable amount of moisture used for span calibration. The moisture generator is made of coated stainless steel to reduce the surface absorption of water molecules and then keep the moisture rate very stable and accurate. The flow inside the module is controlled and maintained by a network of calibrated orifices. All flow passageways upfront the sensor are less than 0.030"ID, all coated with an inert coating to accelerate the response/purge time and improve the performances of the system.

SPECIFICATIONS:

| SENSOR MODEL | PLASMADETEK | PLASMADETEK | PLASMADETEK | PLASMADETEK | SENZTX | SENZTX | EASIDEW | QMA |
|---------------------------------|---|-----------------------------|-----------------------------|-----------------------------|-----------------------------|-----------------------------|-----------------------------|-----------------------------|
| MEASUREMENT TECHNOLOGY | PED | PED | PED | PED | Zirconia (ZR) | Electrochemical (EC) | Ceramic sensor | Quartz crystal |
| SENSOR MANUFACTURER | LDetek | LDetek | LDetek | LDetek | NTRON | NTRON | Michell Instruments | Michell Instruments |
| IMPURITY DETECTED | N2 | O2 | H2O | CnHm | O2 | O2 | H2O | H2O |
| SAMPLE GAS | Ar-He | Ar-He | Ar-He | Ar-He | multiple gases | multiple gases | multiple gases | multiple gases |
| RANGES* (DEFAULT) | 0-1ppm (resolution 10ppb) | 0-3ppm (resolution 10ppb) | 0-3ppm (resolution 10ppb) | 0-3ppm (resolution 10ppb) | 0-10ppm (resolution 0.5ppm) | 0-10ppm (resolution 0.1ppm) | 0-10ppm (resolution 0.5ppm) | 0-10ppm (resolution 100ppb) |
| | 0-10ppm (resolution 100ppb) | 0-30ppm (resolution 100ppb) | 0-30ppm (resolution 100ppb) | 0-30ppm (resolution 100ppb) | 0-100ppm (resolution 1ppm) | 0-100ppm (resolution 1ppm) | 0-100ppm (resolution 1ppm) | 0-100ppm (resolution 1ppm) |
| | 0-100ppm (resolution 1ppm) | 0-50ppm (resolution 1ppm) | 0-100ppm (resolution 1ppm) | up to 30ppm available | 0-1000ppm (resolution 1ppm) | 0-1000ppm (resolution 1ppm) | 0-1000ppm (resolution 1ppm) | 0-1000ppm (resolution 1ppm) |
| | up to 5000ppm available | up to 50ppm available | up to 100ppm available | | up to 96% available | up to 25% available | up to 3000ppm available | up to 2000ppm available |
| LIMIT OF DETECTION (LDL) | 10ppb | 50ppb | 50ppb | 50ppb | 0.5ppm | 0.1ppm | 0.5ppm | 20ppb |
| ACCURACY | <+/- 1% of scale | <+/- 1% of scale | <+/- 1% of scale | <+/- 1% of scale | <+/- 1% of scale | <+/- 1% of scale | <+/- 1% of scale | <+/- 1% of scale |
| RESPONSE TIME (T90) | <10 sec | <10 sec | <10 sec | <10 sec | <10 sec | <10 sec | <5 min | <5 min |
| SENSOR LIFE EXPECTATION | 10 years | 10 years | 10 years | 10 years | 3-5 years | 1 year | 3-5 years | 3-5 years |
| OPERATING TEMPERATURE RANGE | 5-45 Celsius | | | | | | | |
| SAMPLE GAS TEMPERATURE | 0-100 Celsius | | | | | | | |
| SAMPLE FLOW REQUIREMENT | 25-200ml /min | 25-200ml /min | 25-200ml /min | 25-200ml /min | 100-200ml /min | 100-200ml /min | 1-5 L /min | 300-500ml /min |
| OPERATING SAMPLE PRESSURE RANGE | 3-30psig (for lower sample pressure requirement, an additional high purity pump is used) | | | | | | | |
| OUTLET PRESSURE | Atmospheric | | | | | | | |
| INLET FITTINGS | 1/8" or 1/4" Swagelok compression or VCR | | | | | | | |
| OUTLET FITTINGS | 1/8" or 1/4" Swagelok compression or VCR | | | | | | | |
| DOPING GAS REQUIREMENT | N/A | Nitrogen grade 5.0** | Nitrogen grade 5.0** | Nitrogen grade 5.0** | N/A | N/A | N/A | Nitrogen grade 5.0*** |
| STANDARD FEATURES | Manual or autoranging, MCU embedded system, touchscreen 5.6" LCD, 4-20mA outputs, alarm historic, digital outputs for status, 3 ranges, calibration in progress | | | | | | | |
| OPTIONS | Internal sampling system for zero/span/sample, serial communication RS232-RS485-Modbus-Profibus, 2 level alarms, zero gas free calibration system | | | | | | | |
| SUPPLY | 110VAC 50-60Hz / 220VAC 50-60Hz | | | | | | | |
| POWER CONSUMPTION | 100-250 watts depending of the combination of sensors and options mounted in the unit | | | | | | | |
| ENCLOSURE TYPE | 3U or 4U rackmount type depending of the combination of sensors and options mounted in the unit | | | | | | | |
| INGRESS PROTECTION | IP20 in accordance with IEC 60529 | | | | | | | |
| ENCLOSURE FINISH | RAL7030 powder coat | | | | | | | |
| WEIGHT | 25-40 lbs (11-18kg) depending of the combination of sensors and options mounted in the unit | | | | | | | |
| CERTIFICATION | In compliance with EMC directive 2004/108/EC, EN 61000-6-2:2005 for immunity & EN 61000-6-4:2007 for emissions | | | | | | | |

* Ranges can be factory set to other values. ** Refer to LD8000MG design report for more details *** Zero & Span gas dry gas source

Where innovation leads to success


www.ldetek.com

ORDERING INFORMATION:


| LD8000MG | -X-X-X-X | -XXX | -X | -XXX | -X | -XXX |
|----------|--|--|------------------------|---|--------------------------------|--|
| | PEDN2: N2 by PED PED02: O2 by PED PEDH20: H2O by PED PEDCnHm: HC's by PED EC02: O2 by Electrochemical ZR02: O2 by Zirconia DPH20: H2O by ceramic sensor QMAH20: H2O by quartz crystal | Operating Voltage: 120: 120 volts 220: 220 volts | A: Alarm option | Integrated sampling system S1: 1 sample + zero + span S2: 2 samples + zero + span | C: Zero gas free system | Serial communication RS2: RS-232 RS4: RS-485 PFB: Profibus |

DIMENSIONS:

3U RACKMOUNT ENCLOSURE:

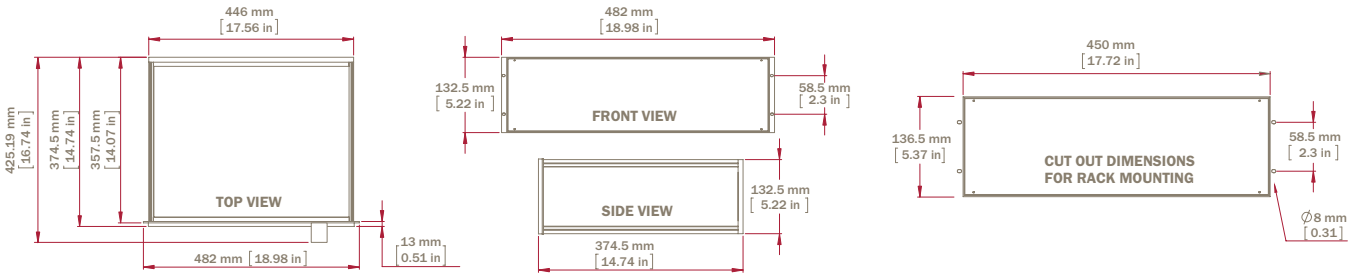

4U RACKMOUNT ENCLOSURE:

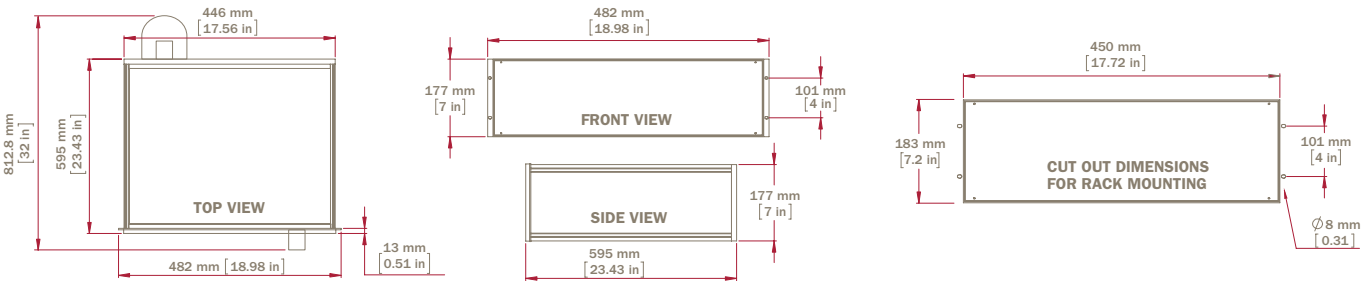

LD8000-TCD



BINARY GAS ANALYZER



The LD8000-TCD is a Thermal Conductivity-based Gas Analyzers used to measure and monitor binary gas streams. It can also monitor one component in a more complex gas mixture when the background gases have the same ratio to each other, or have similar thermal conductivity values.

FEATURES:

- Unique Thermal Conductivity Detector (TCD)
- Bootloader integrated for software update via Ethernet
- Large scale measurement
- 4-20 mA output as standard
- Range Identification Relay
- Maintenance free
- LAN/Web control
- Micro-valve for very low dead volume and fast purging time
- 3U cabinet

APPLICATIONS:

- Gas Manufacturing Facilities: monitoring Pressure Swing Adsorption (PSA) Systems
- Gas management system
- Gas Blending Equipment
- Air Liquification Plants: monitoring purity of Ar, O₂, H₂, N₂, He, CO₂, or Ne
- Welding gas control
- Steel Mills: CO₂ in off-gas from gas generators
- Petroleum Refineries: H₂ purity in C₁ - C₆ hydrocarbons
- Speciality gas laboratories
- Heat Treating: H₂ in N₂ and other annealing gases
- Process control
- Power Generation Plants: H₂ cooling gas in turbine generator housings; CO₂ in turbine generator housing; checking H₂ purity
- Ammonia Plants
- Chemical plants
- Refrigeration Facilities

SPECIFICATIONS:


| | | |
|---------------------------------|---|--------------------------------|
| DETECTOR TYPE | Thermal Conductivity Detector (TCD) | |
| RANGE | Ppm to % (application dependant) | |
| ACCURACY | Better than $\pm 1\%$ full scale | |
| STANDARD FEATURES | <ul style="list-style-type: none"> Manual or autoranging (user selectable) Microprocessor controlled 5.6" TFT intelligent LCD module with Touch Screen Self diagnosis system with auto-resolve alarm LAN/Web control 4-20 mA isolated output Alarm Historic Digital outputs for remote monitoring: (all dry relay contacts) <ul style="list-style-type: none"> - System status (1 output) - Range in use (3 output) - Calibration in use (1 output) | |
| OPTIONS | <ul style="list-style-type: none"> Internal sampling system for zero, span and sample Serial port: RS-232 / 422 / 485 / Modbus 2 alarm outputs (user programmable set point) | |
| GAS CONNECTIONS | Sample: 1/8" compression fittings | Vent: 1/8" compression fitting |
| SAMPLE FLOW REQUIREMENTS | 0 to 300 sccm | |
| OPERATING PRESSURE | 3 to 30 PSIG | |
| OPERATING TEMPERATURE | 10 °C to 45 °C | |
| SUPPLY | 115 VAC, 50 – 60 Hz or 220 VAC, 50 – 60 Hz | |
| POWER CONSUMPTION | Maximum 40 watts | |
| DRIFT | Dependent of calibration | |
| WEIGHT | 30 lbs (14 kg) | |

ORDERING INFORMATION:

| LD8000-TCD | -XXX | -X | -XX | -XXX |
|------------|--|------------------------|--|---|
| | Operating Voltage: 120: 120 volts 220: 220 volts | A: Alarm option | Integrated sampling system: S1: 1 Stream + zero + span S2: 2 Streams + zero + span | Serial communication: RS2: RS-232 RS4: RS-485 MOD: Modbus |

Binary gases must be specified. Please contact factory.

DIMENSIONS:

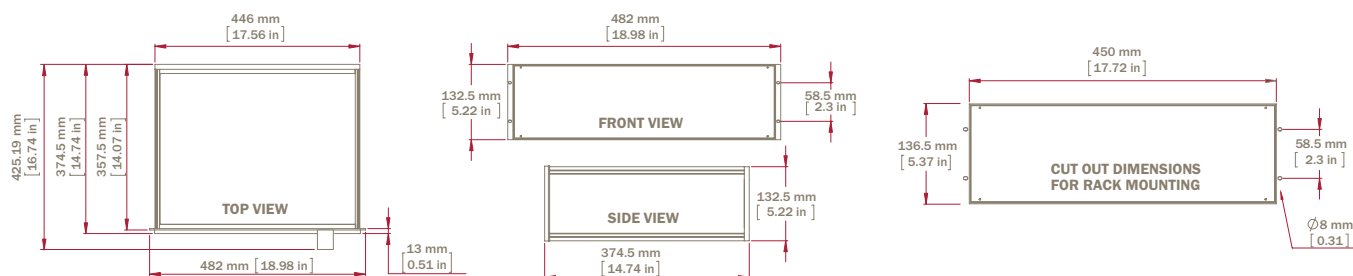

LDP1000 SERIES



GAS PURIFIER COMPATIBLE WITH ANY TRACE GAS ANALYSIS SYSTEM

The LDP1000 series is a sub ppb purifier used for generating high purity calibration gas for online analyzers as well as generating high purity carrier gas for gas chromatograph.

Designed with two steps of purification, this purifier design ensures no undesired impurity is released during process.

WHY CHOOSING LDP1000 SERIES ?

- **2 beds of purification**
Allows perfect purification
- **RS-232 port**
Monitor the temperature of the 2 beds of purification
- **LEDs indication**
Self-diagnostic and status of the purifier
- **Cost effective solution for long-term use**
Interchangeable getter
- **Available in different format**
Compact version makes it ideal when space is limited
- **Real end of life monitoring**
Combined with PED technology and MultiDetek series, LDP1000 series gas purity can be monitored in real time to offer real auto diagnostic.



SPECIFICATIONS:

| | |
|--------------------------------|--|
| GETTER TYPE | Alloy of Zr/V/Fe 2 beds (350 and 200 Celsius) |
| GASES PURIFIED | Ar/He/Ne/Xe/Kr - Nitrogen and hydrogen version available |
| IMPURITIES REMOVED | H ₂ O, O ₂ , CO, CO ₂ , N ₂ , THC, H ₂ , CH ₄ (heated) H ₂ O, O ₂ , CO, CO ₂ , H ₂ (room temperature) |
| IMPURITY LEVEL | <10 ppb and <1 ppb available |
| FLOW | Compact & LDP1000 versions flow rate are 0.2LPM nominal to 1LPM maximal Large LDP1000 version flow rate is 2LPM nominal to 10LPM maximal |
| GAS CONNECTIONS | 1/8" – 1/4" compression or VCR® |
| RECOMMENDED OPERATING PRESSURE | 100 PSIG (689 kPAG) |
| SUPPLY | 120 VAC, 50 – 60 Hz or 220 VAC, 50 – 60 Hz |
| POWER CONSUMPTION | Start-up : maximum 200 Watts (allows quick start-up) Normal operation : maximum 50 Watts (designed for low consumption) |
| WEIGHT | 8 lbs (3.63 kg) Large LDP1000 • 5 lbs (2.26 kg) LDP1000 • 2 lbs (0.90 kg) Compact-LDP1000 |


CERTIFICATION:

CE In compliance with EMC directive 2004/108/EC, EN 61000-6-2:2005 for immunity & EN 61000-6-4:2007 for emissions.


ORDERING INFORMATION:

| LDP1000, LARGE LDP1000, COMPACT LDP1000, GETTER LDP1000 OR MINI LDP1000 | -XXX | -X | -X | -X | -X |
|---|--|--|--|--|--|
| | Operating Voltage: 120 volts (-120) 220 volts (-220) | Gas type: N: Noble gases N2: Nitrogen version H2: Hydrogen | Connection size: 1/8" 1/4" | Connection Type: Compression (-C) VCR (-V) | Supporting plate: P-1/8C: Stainless steel supporting plate/ 1/8" compression with high purity bypass valve & 2 in/out isolation valves P-1/8V: Stainless steel supporting plate/ 1/8" VCR with high purity bypass valve & 2 in/out isolation valves P-1/4C: Stainless steel supporting plate/ 1/4" compression with high purity bypass valve & 2 in/out isolation valves P-1/4V: Stainless steel supporting plate/ 1/4" VCR with high purity bypass valve & 2 in/out isolation valves None: no plate |

DIMENSIONS LDP1000:

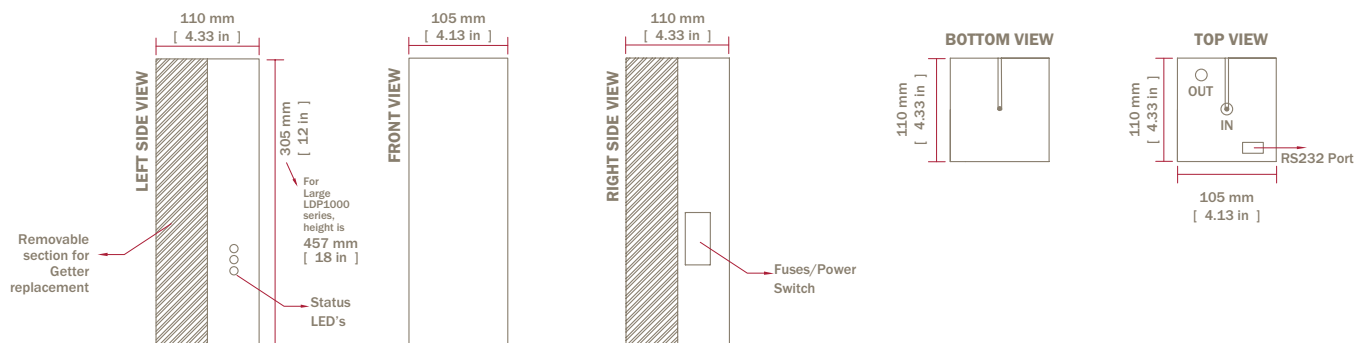

DIMENSIONS COMPACT-LDP1000:

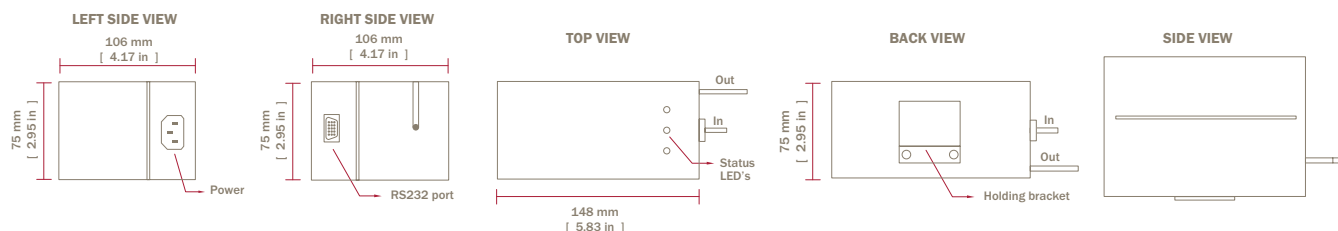

PLASMA EMISSION DETECTOR SYSTEM FOR GAS CHROMATOGRAPH

This plasma emission detector gives the opportunity to any system integrator or GC manufacturer to integrate a plug and play philosophy detector system. With its unique design, the PlasmaDetek allows to do new techniques and existing analysis configuration based on simplicity. PPB to % analysis can be done with capillary or packed columns. With the choice of argon or helium as carrier gas, combined with the selectivity configuration, the chromatography becomes easier.



FEATURES:

- Argon or helium carrier gas
- 4 in 1 detector
- Selective and non-selective configuration
- Wide range of applications
- Easy to interface with any GC and analyzer design
- PPB to % detection
- Very stable signal
- Maintenance free
- Fast installation and tune up
- Intelligent version based on DSP platform
- Low noise detector

APPLICATIONS:

- Laboratory and industrial gas chromatograph
- High purity gases
- Permanent gases
- Noble and rare gases
- Petrochemical and Hydrocarbon Processing
- Air analysis
- Environmental
- Energy industries
- Greenhouse application
- Etc...

Other gas analysis possible, please contact factory.

SPECIFICATIONS:

| | |
|--|---|
| CARRIER GAS | Argon and Helium |
| POWER | 80 to 240 VAC, 50-60 Hz |
| GAS CONNECTIONS | 1/16" (can be customized) |
| OPERATION OUTLET PRESSURE | Atmospheric or Vacuum |
| OPERATING TEMPERATURE | 10 °C to 50 °C (in stable environment) |
| FILTER | 10u SS particle filter on the gas inlet |
| DETECTOR SIGNAL OUTPUT CONNECTION | BNC Coaxial type (can be customized) |
| POWER CONSUMPTION | Max 10 Watts |
| OUTPUT VOLTAGE | 0-5 Volts (can be customized) |



PRINCIPLE OF PLASMA EMISSION DETECTOR (PED):

The PED is a quartz cell with a unique design submitted to a high intensity and frequency electromagnetic field.

The principle based on spectroscopic emission cell is not a new technique, but the characteristics of the Plasma-Detek system that make it stable and efficient are the frequency, the intensity as well as the mechanical and electro- des design.

A luminous phenomenon, called electroluminescence, is created and is used as emission technique to quantify analytes.

When the carrier gas is ionized, spectral lines are emitted and detected by an optical system including filter and photo-diode. The emission varies for each substance that is brought along with the carrier gas.

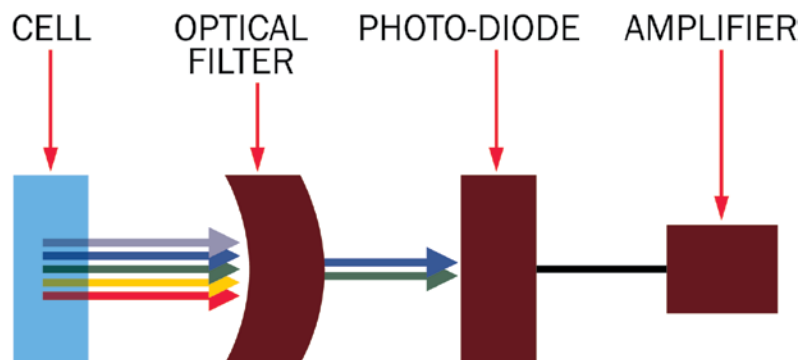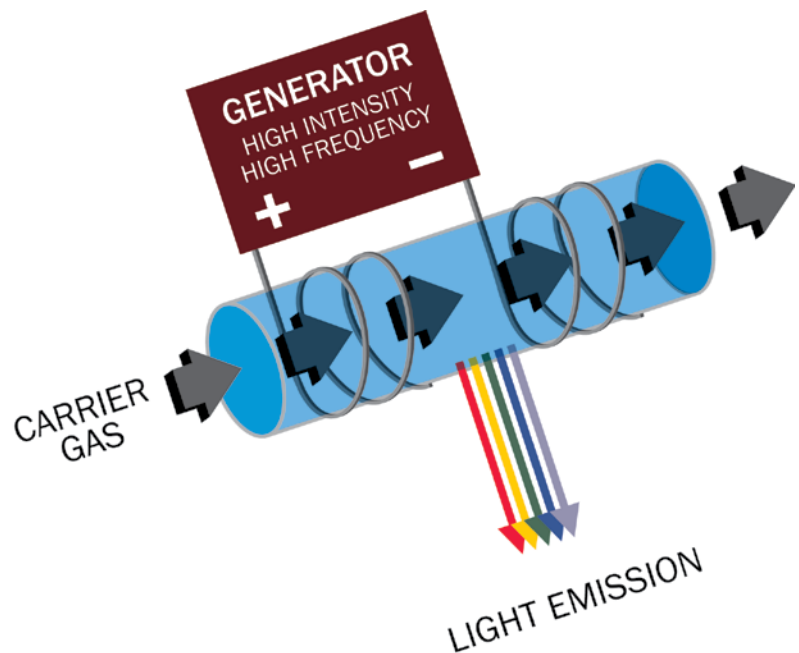

SELECTIVITY:

The selective configuration gives the possibility to be more sensitive on some impurities to make the chromatography easier and get better results. No need to add a supporting gas or other devices. The specific optical filter system is chosen for the application desired.

By having such selectivity, you can reduce analysis time and make fast chromatography. In some cases, consumables such as traps can be avoided. It becomes a cost effective solution, maintenance free system and can give better limit of detection by reducing residual background effect.

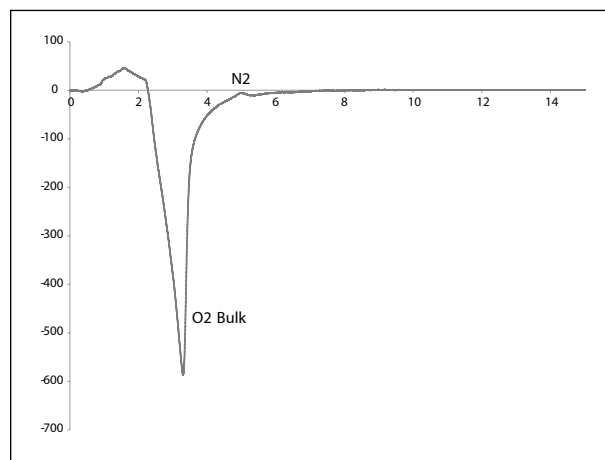


Figure 1: 1 ppm N2 in pure O2 with non-selective detector system


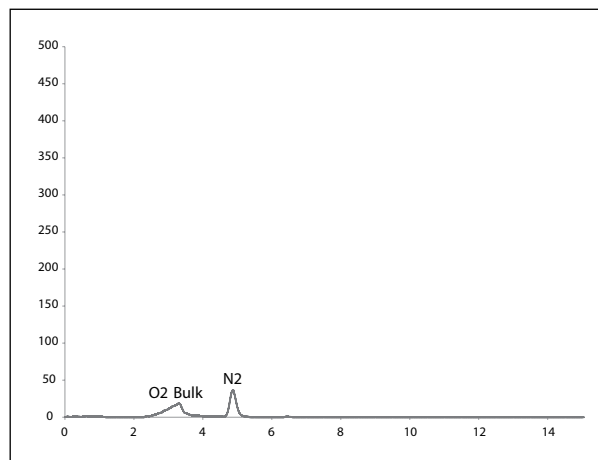


Figure 2: 1 ppm N2 in pure O2 with PlasmaDetek N2 selective configuration

ALL IN ONE DETECTOR:

The PlasmaDetek can replace many detectors and get all measurements with only one module. No need of doping gas, fuel or other support devices. Measuring permanent gases and light hydrocarbons have never been so easy. Many other gases can be detected, please contact LDetek for more information.

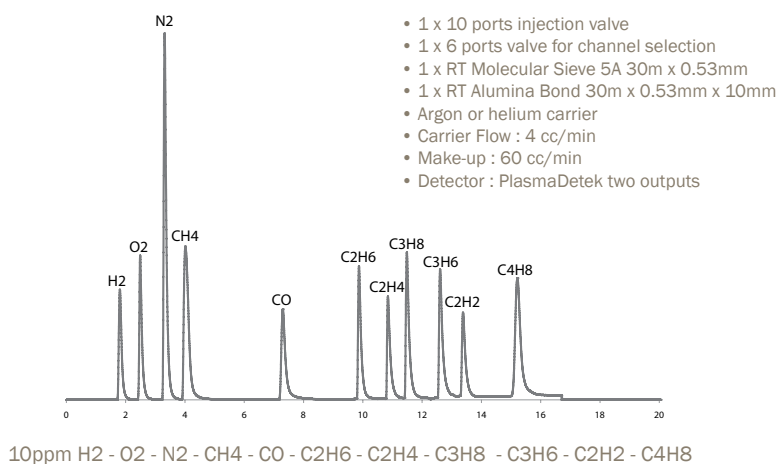

ARGON AND HELIUM CARRIER GAS:

Having the choice of argon or helium as carrier gas brings the advantage of making easier chromatography configuration. Argon can be cost effective compared to helium in some cases.

Good sensitivity is also obtained with both carriers giving the possibility to work from ppb to % application.

PLASMADETEK₂



INTELLIGENT PLASMA EMISSION DETECTOR SYSTEM FOR GAS CHROMATOGRAPH




This microprocessor based plasma emission detector system gives all the tools to the GC integrator, manufacturer and user to integrate a plug and play detection system. With its customizable configuration capability, a detector has never been so intelligent.

IN A GLANCE:

- Argon or helium carrier gas
- No dead volume design
- All in one detector by replacing existing technologies commonly used
- Selective and non-selective configuration
- Analog or digital interface
- Wide range of applications
- Easy to interface with any GC and analyzer design
- PPB to % detection
- Very stable signal
- Maintenance free
- Fast installation and tune up
- Configuration software
- Possibility of customizable protocol to control the device
- Detect organic and inorganic compounds, permanent gases and noble gases (including Ne)

DOPING AGENT INJECTOR TEMPERATURE CONTROLLED

By controlling the temperature of the doping agent injection device, better stability of the measurement is achieved. The temperature is controlled by the PlasmaDetek controller and can be adjusted for the specific application. The use of different doping agents is application dependant is part of the selectivity mode.

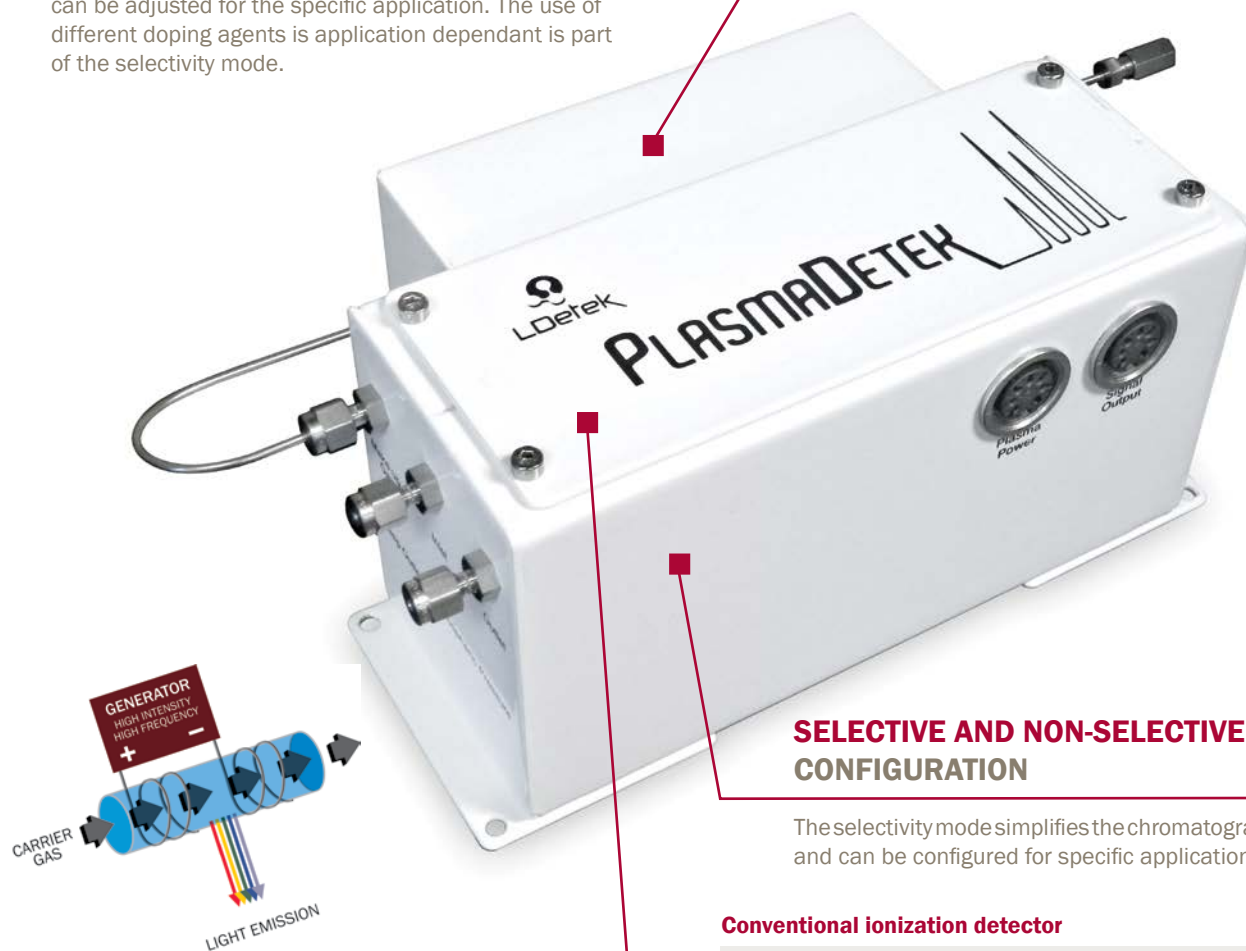


SELECTIVE AND NON-SELECTIVE CONFIGURATION

The selectivity mode simplifies the chromatography and can be configured for specific application.


PED DESIGN WITH NO DEAD VOLUME

The PlasmaDetek design avoids the creation of phantom peaks that occurs in conventional ionization detector. Its unique design made of a monolithic quartz makes the detector dead volume free. It is not affected by pressure or flow swings.

Conventional ionization detector

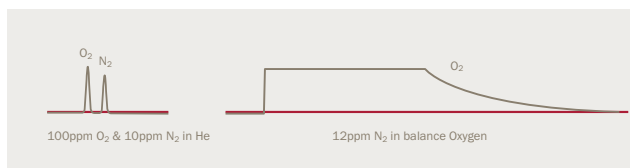

Plasmadetek

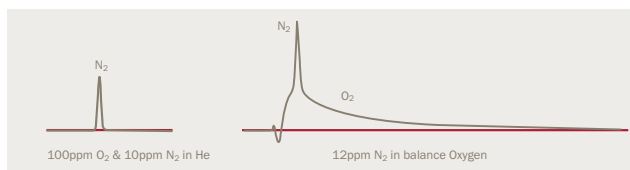


MICROPROCESSOR BASED CONTROLLER

With an integrated DSP, the signal can be processed to improve measurement as well as providing desired signal for any GC. Configurable with LDetek plasma configurator provided with each PlasmaDetek. Cost saving by having no electrometer needed to acquire the signal. Multiple stage of amplification integrated to achieve low to high concentration.

2 ANALOG OUTPUTS AS STANDARD

Both analog output can be used in parallel to interface with the desired signal acquisition system. Coaxial cables are provided with detector.

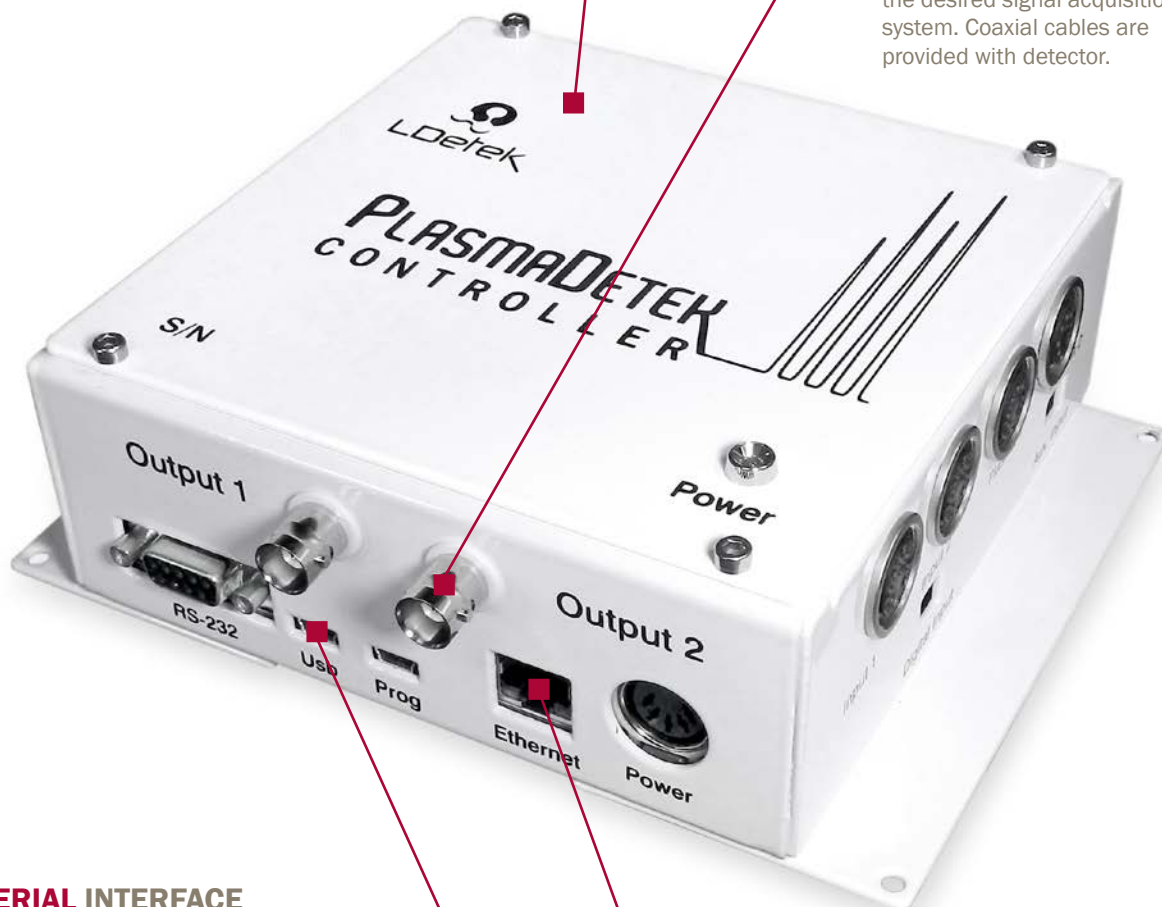


SERIAL INTERFACE

USB and RS-232 connection are available to provide digital signal and avoid analog interface. Custom digital communication can also be implemented to communicate and configure the PlasmaDetek from your own system.

ETHERNET PORT


Connect the PlasmaDetek to your network to communicate with the device.

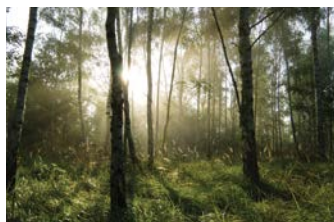

SPECIFICATIONS:

| | |
|--|---|
| CARRIER GAS | Argon and Helium |
| POWER | 80 to 240 VAC, 50-60 Hz |
| GAS CONNECTIONS | 1/16" (can be customized) |
| OPERATION OUTLET PRESSURE | Atmospheric or Vacuum |
| OPERATING TEMPERATURE | 10 °C to 50 °C (in stable environment) |
| FILTER | 10u SS particle filter on the gas inlet |
| DETECTOR SIGNAL OUTPUT CONNECTION | BNC Coaxial type (can be customized) |
| POWER CONSUMPTION | Max 10 Watts |

PLASMADETEK CONFIGURATOR:

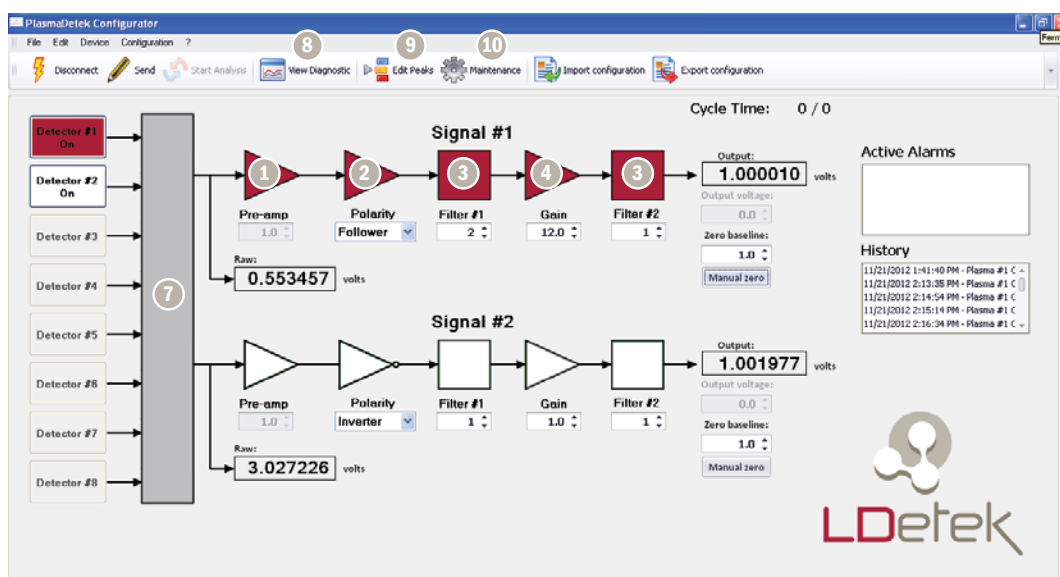

- Adjust the amplification directly on the source light of the plasma to change the measurement scale of the detector. PPB to % application can be achieved with the same detector.
- SIGNAL POLARITY:** negative peaks can now be inverted to get positive peaks.
- FILTERING:** Digital filtering can be applied to improve signal provided to the GC.
- GAIN:** adjust the gain of the signal for the specific measurement.
- OUTPUT VOLTAGE:** set the output voltage scale that fits to the GC signal acquisition system.
- ZERO BASELINE:** set and perform zero baseline directly in the detector.
- Connect up to 8 detector to the same plasma controller.
- DIAGNOSTIC TOOL:** Graphic tool to trend the raw or the output voltage.
- PEAK TABLE:** edit a peak event table to change all possible parameters at specific time analysis can be started manually or by digitally and the detector will follow your specific configuration.
- Maintenance menu: all tools to troubleshoot the detector is provided.

PLASMADETEK₃



HEATED CAPABLE MICRO PLASMA EMISSION DETECTOR WITH INTERCHANGEABLE OPTICS



Flexible plasma emission detector for gas chromatograph. The ideal gas detector for ppb/ppm trace impurities in different gas matrix. The modular philosophy of this detector makes it suitable for lab operations as well as industrial applications.

FEATURES:

- Stand alone detector for any GC
- Heating up to 200 Celsius
- Up to 4 removable/changeable optical filters for a more flexible detector
- Changeable plasma cell
- Possibility to connect a spectrometer fiber optic direct on the cell for specific lab or research project
- Compatible with the PlasmaDetek 2 controller which makes it compatible with any previous installation
- Compatible with Clarity from DataApex
- Ideal for ppb/ppm trace impurities
- Replace ECD-FID-TCD-DID all in one detector
- Compatible with Helium, Argon, Nitrogen as carrier gas
- Selective, sensitive and generic configurable
- Quick switchable carrier gas type

Four changeable optical filters that offers flexibility. It can be changed anytime within seconds to adapt the analysis needs. It becomes possible to switch the application easily to find selectivity and sensitivity desired. The light collection system has been optimized to avoid light collection response loss by high temperature operation.



Heated capable housing up to 200 Celsius extending the application possibilities.

With its interchangeable quartz plasma cell module design, it becomes possible to do the maintenance on the detector. The application can be modified easily as well. The detector module design makes it easy to replace or change any component without damaging or creating leaks. The design offers an integrated leak detector to auto diagnostic the carrier gas and make up leak rate.



MICROPROCESSOR BASED CONTROLLER


With an integrated DSP, the signal can be processed to improve measurement as well as providing desired signal for any GC. The parameters can easily be changed with the use of the LDetek configurator software interface that comes with each PlasmaDetek detector. Cost saving by having no electrometer needed to acquire the signal. Multiple stage of amplification integrated to achieve low to high concentration.

2 ANALOG OUTPUTS AS STANDARD

Both analog output can be used in parallel to interface with the desired signal acquisition system. Coaxial cables are provided with detector.

MULTIPLE I/Os

Multiple I/Os are available on the controller module to extend the application capabilities. It becomes possible to use the controller to acquire signal from other devices or detectors. It is also possible to control different devices as valves actuation, ovens or other components.

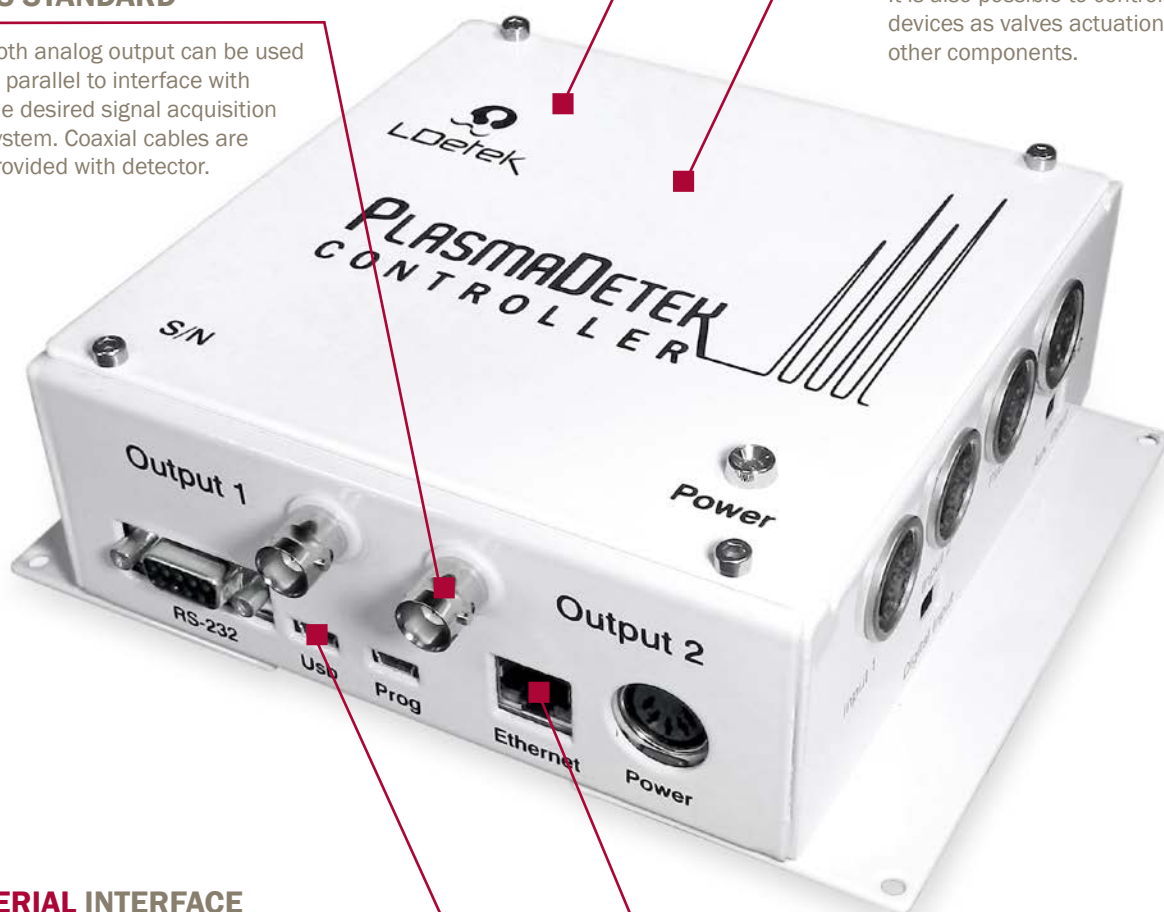


SERIAL INTERFACE

USB and RS-232 connection are available to provide digital signal and avoid analog interface. Custom digital communication can also be implemented to communicate and configure the PlasmaDetek from your own system.

ETHERNET PORT


Connect the PlasmaDetek to your network to communicate with the device.

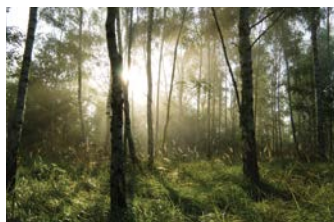

SPECIFICATIONS:

| | |
|-----------------------------------|---|
| CARRIER GAS | Argon, Helium, Nitrogen |
| POWER | 80 to 240 VAC, 50-60 Hz |
| GAS CONNECTIONS | 1/16" (can be customized) |
| OPERATION OUTLET PRESSURE | Atmospheric or Vacuum |
| OPERATING TEMPERATURE | 10°C to 200°C |
| FILTER | 10u SS particle filter on the gas inlet |
| DETECTOR SIGNAL OUTPUT CONNECTION | BNC Coaxial type (can be customized) |

PLASMADETEK CONFIGURATOR:

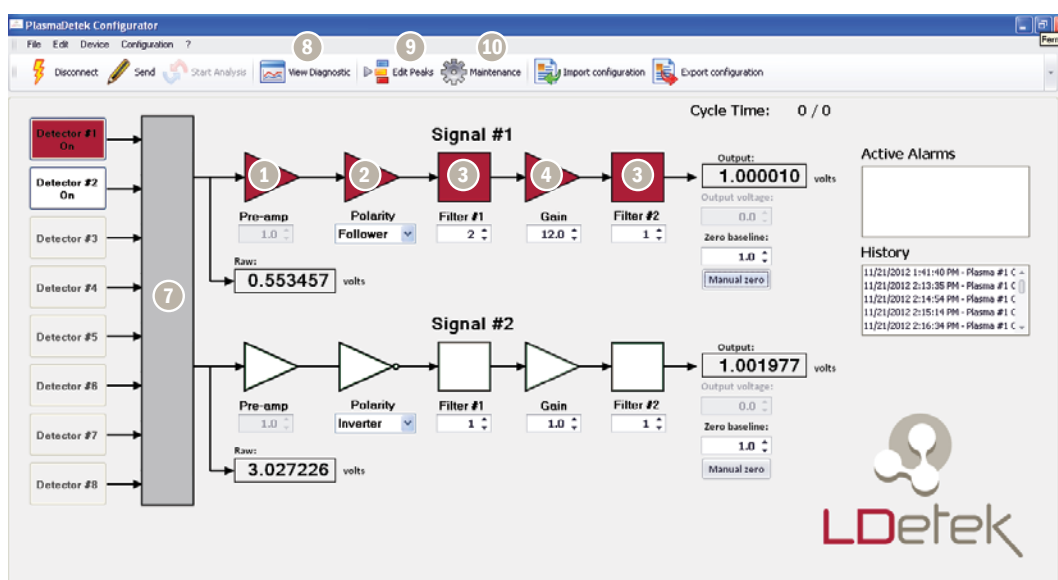

- 1 Adjust the amplification directly on the source light of the plasma to change the measurement scale of the detector. PPB to % application can be achieved with the same detector.
- 2 **SIGNAL POLARITY:** negative peaks can now be inverted to get positive peaks.
- 3 **FILTERING:** Digital filtering can be applied to improve signal provided to the GC.
- 4 **GAIN:** adjust the gain of the signal for the specific measurement.
- 5 **OUTPUT VOLTAGE:** set the output voltage scale that fits to the GC signal acquisition system.
- 6 **ZERO BASELINE:** set and perform zero baseline directly in the detector.
- 7 Connect up to 8 detector to the same plasma controller.
- 8 **DIAGNOSTIC TOOL:** Graphic tool to trend the raw or the output voltage.
- 9 **PEAK TABLE:** edit a peak event table to change all possible parameters at specific time analysis can be started manually or by digitally and the detector will follow your specific configuration.
- 10 Maintenance menu: all tools to troubleshoot the detector is provided.

NEW ERA



OF LIGHT HYDROCARBON MEASUREMENT

Looking for a **SAFE, SENSITIVE, LOW OPERATION COST** and **MAINTENANCE FREE** system?

The patent pending **PlasmaDetek-E** is the solution



SAFE

No fuel (H_2) and no related safety accessories



SENSITIVE

< 1 ppb lowest detection possible



LOW OPERATING COST


Only N_2 carrier gas supply



MAINTENANCE FREE

No periodic detector cleaning

TYPICAL INSTALLATION FOR LIGHT HYDROCARBON MEASUREMENT

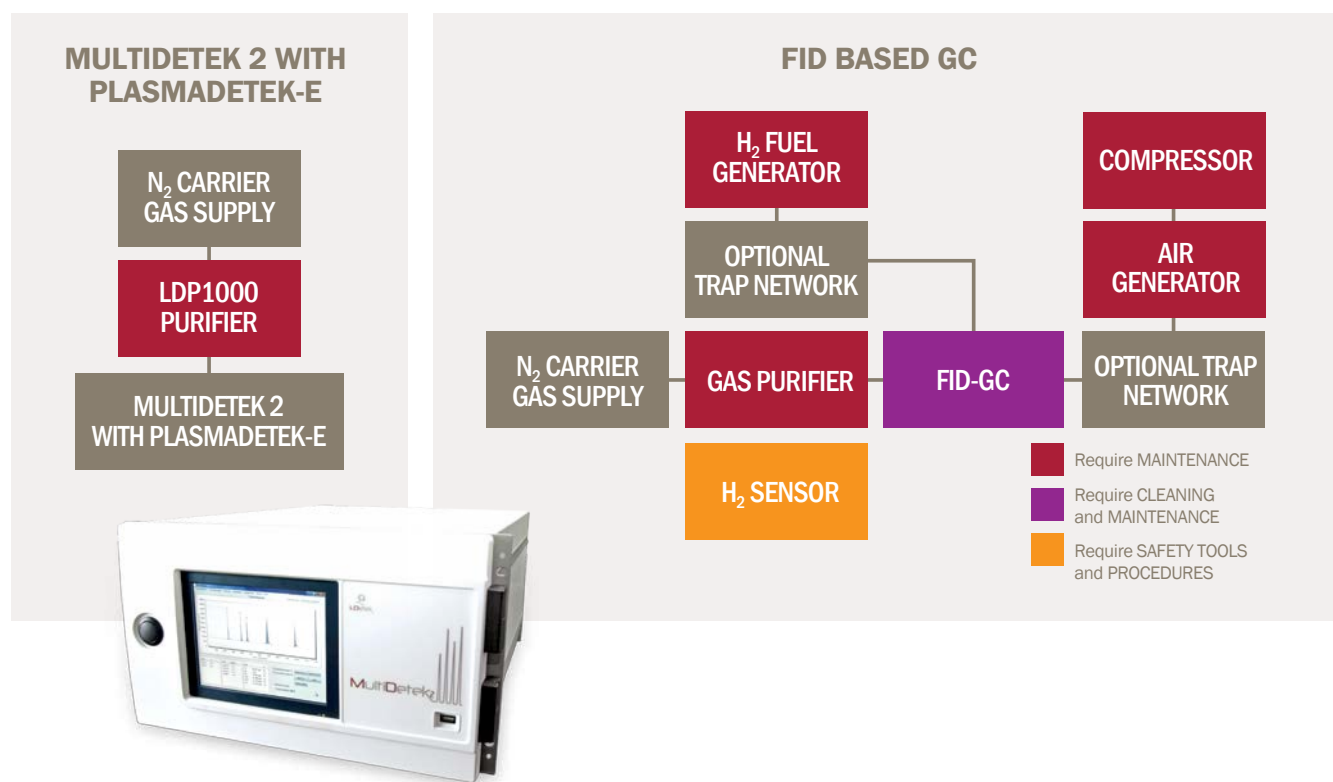

INSTALLATION COST* COMPARISON


| Parts | MultiDetek 2 with PlasmaDetek-E | FID-GC |
|-----------------------------------|---------------------------------|-----------------|
| H ₂ generator | N/A | \$7200 |
| Zero air generator | N/A | \$2125 |
| Air compressor | N/A | \$1200 |
| H ₂ safety accessories | N/A | \$1500 |
| 2 year maintenance cost | \$2000 | \$5000 |
| Total cost* | \$2000 | \$17 025 |

* costs are approximate and may vary for each system

N/A: not applicable

Please consult Application Note LD14-01 on LDetek web site for more technical details.

HIGH PURITY GAS STREAM SELECTOR

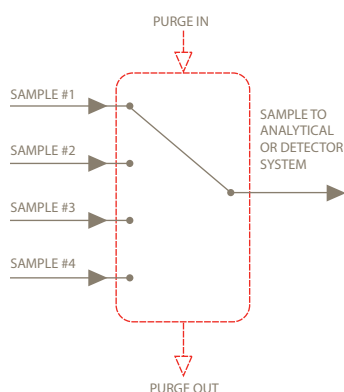

The LDGSS now brings to the gas industry the most reliable and easy way to provide clean gas to any process GC and on line process analyzers. It's compact design, based on high purity connections with an unique diaphragm valve with no dead volume, is the ideal solution for any streams selection needs. This concept allows a quick response time, the possibility to work in vacuum mode and avoid drifting problems.

FEATURES:

- Compact design reducing project costs.
- Leak proof, tested and certified
- Air diffusion resistant
- Unique diaphragm valve with no dead volume for stream selection
- No stream cross contamination
- Quick purging time
- Optional purge gas flow to avoid contamination
- Easy to operate
- Oxygen cleaned and compatible
- Can be easily integrated to any type of process G.C. or on line process analyzers

APPLICATIONS:

- Air Separation industry
- Semiconductor manufacturing
- Laboratory GC's installation
- System's Integrators
- Glove box


SPECIFICATIONS:

| | |
|--|---|
| NUMBER OF INLETS | 2 to 9 streams configurable |
| STANDARD FEATURES | Front mounted stream bypass valves Dry contacts that remotely give status of selected channel Local or Remote control via 12VDC or 24VDC supply Front Mounted rotary switch selector 10u particle filter installed on every inlet Stainless Steel diaphragm valve or peek 3 ways solenoid valve (must be specified when ordering) |
| OPTIONS | BPR : Sample outlet back pressure regulator to maintain a constant sample outlet pressure. VPB : Valves purge box for toxic and/or hazardous gases. PG : Purging gas port for diaphragm valve version for high purity application or toxic/hazardous gases. PR : Stream inlet pressure regulator for reducing stream pressure C : Coated flow path for corrosive and absorbent gases MBP : Metal bellow pump for low pressure application O2 : Oxygen clean certified |
| SAMPLE BYPASS ADJUSTABLE VALVE FLOW RANGE | 0 to 500 ml/min |
| GAS INLET & OUTLET CONNECTIONS | 1/16"- 1/8" or 1/4" Stainless Steel Compression Type Swagelok compatible. 1/8" or 1/4" Stainless Steel High Purity VCR type. |
| PURGED GAS VENT CONNECTIONS | 1/8" Stainless Steel Compression Type Swagelok compatible |
| SUPPLY | 85VAC to 240VAC 50/60Hz |
| POWER CONSUMPTION | 10 watts |
| MAXIMUM OPERATING PRESSURE | 30 PSIG (206Kpa) with peek solenoid valve version 300 PSIG (2068Kpa) with stainless steel diaphragm valve version |
| MINIMUM OPERATING PRESSURE | 3 PSIG (20Kpa) (lowest pressure can be achieved for glove box application by adding the optional metal bellow pump) |
| NOMINAL WORKING PRESSURE | 20 PSIG (138Kpa) |
| REMOTE CONTROL VOLTAGE INPUT | 12 VDC or 24VDC at 200mA maximum |

ORDERING INFORMATION:

| LD8000 | -XXX | -X | -X/X | -XXX | -XXX |
|--------|--|--|--|--|---|
| | Operating Voltage 120 Volts (-120) 220 Volts (-220) | Number of Inlets 2 to 9 : 2 to 9 streams | Gas Inlets Connections Size 1/16 : 1/16 inches 1/8 : 1/8 inches 1/4 : 1/4 inches | Gas Inlets Type VCR : face seal type SWG : compression type | Options BPR C VPB MBP PG O2 PR |

DIMENSIONS:

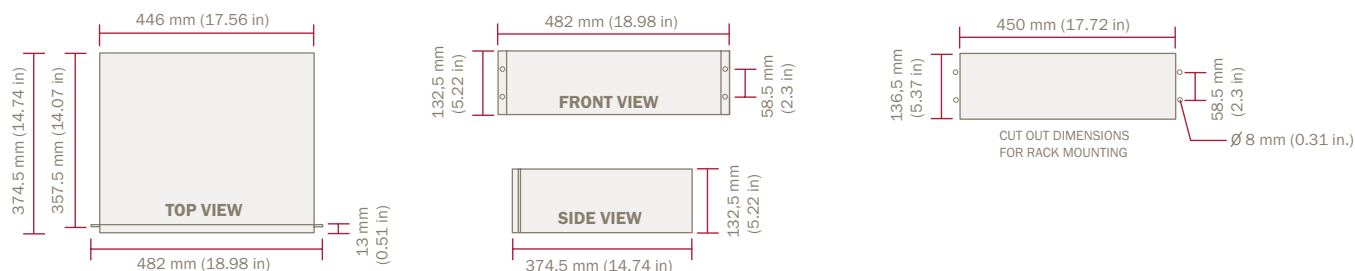

LD2000



ONLINE TRACE TOTAL HYDROCARBON ANALYZER



The LD2000 is an easy to use instrument that offers the ideal solution for the total hydrocarbon measurements. Its compact and robust design perfectly fits on any industrial installation. The LDetek FID and electronic platform bring the performances required by the market.

FEATURES:

- LDetek FID design offering low maintenance
- Bootloader integrated for software update via Ethernet
- Large scale measurement
- 4-20 mA output as standard
- Range Identification Relay
- Unique LDetek Electronic flow controller design
- 3U cabinet

APPLICATIONS:

- Air separation unit
- Cryogenic truck loading station
- Speciality gas laboratories
- Process control
- Steel Industries
- Chemical plants
- Welding gas control
- Gas management system
- Quality control for truck fills and gas cylinders
- Safety
- Product validation
- Scrubber & oxidizer efficiency
- Carbon bed breakthrough detection
- Well logging
- Industrial hygiene & safety monitoring
- Fence line (perimeter) monitoring around industrial sites
- CEMS (continuous emission monitoring systems)


SPECIFICATIONS:

| | |
|---|--|
| DETECTOR TYPE | Flame Ionisation Detector |
| RANGE | 0-10 ppm 0-100 ppm 0-1000 ppm other range possible |
| REPEATABILITY | < 1% full scale |
| ACCURACY | Better than $\pm 1\%$ full scale |
| STANDARD FEATURES | <ul style="list-style-type: none"> • Manual or autoranging (user selectable) • Microprocessor controlled • 5.6" TFT intelligent LCD module with Touch Screen • Self diagnosis system with auto-resolve alarm • 4-20 mA isolated output • Alarm Historic • Digital outputs for remote monitoring: (all dry relay contacts) <ul style="list-style-type: none"> - System status (1 output) - Range in use (3 output) - Calibration in use (1 output) |
| OPTIONS | <ul style="list-style-type: none"> • Serial port: RS-232 / 422 / 485 / Profibus • 2 alarm outputs (user programmable set point) |
| GAS CONNECTIONS | Sample: 1/8" compression fittings Vent: 1/8" compression fitting |
| CALIBRATION GAS | Zero: LDP1000 purified gas (Getter) Span: 80%-90% of full scale of methane |
| SAMPLE FLOW REQUIREMENTS | 50 to 200 sccm |
| AIR FLOW REQUIREMENTS | 200 to 600 sccm |
| FUEL FLOW REQUIREMENTS | 40 to 150 sccm |
| RECOMMENDED MAXIMUM OPERATING PRESSURE | 40 PSIG |
| RECOMMENDED MINIMUM OPERATING PRESSURE | 10 PSIG |
| OPERATING TEMPERATURE | 10 °C to 45 °C |
| SUPPLY | 115 VAC 50 - 60 Hz or 220 VAC 50 - 60 Hz |
| POWER CONSUMPTION | Maximum 50 watts |
| DRIFT | < $\pm 1\%$ over 24 hours |
| WEIGHT | 27 lbs (12 kg) |

ORDERING INFORMATION:

| LD2000 | -X | -XXX | -X | -XXX |
|--------|---|--|------------------------|--|
| | Ar: Argon H: Helium O: Oxygen N: Nitrogen A: Air | Operating Voltage: 120: 120 volts 220: 220 volts | A: Alarm option | Serial communication RS2: RS-232 RS4: RS-485 PFB: Profibus |

DIMENSIONS:

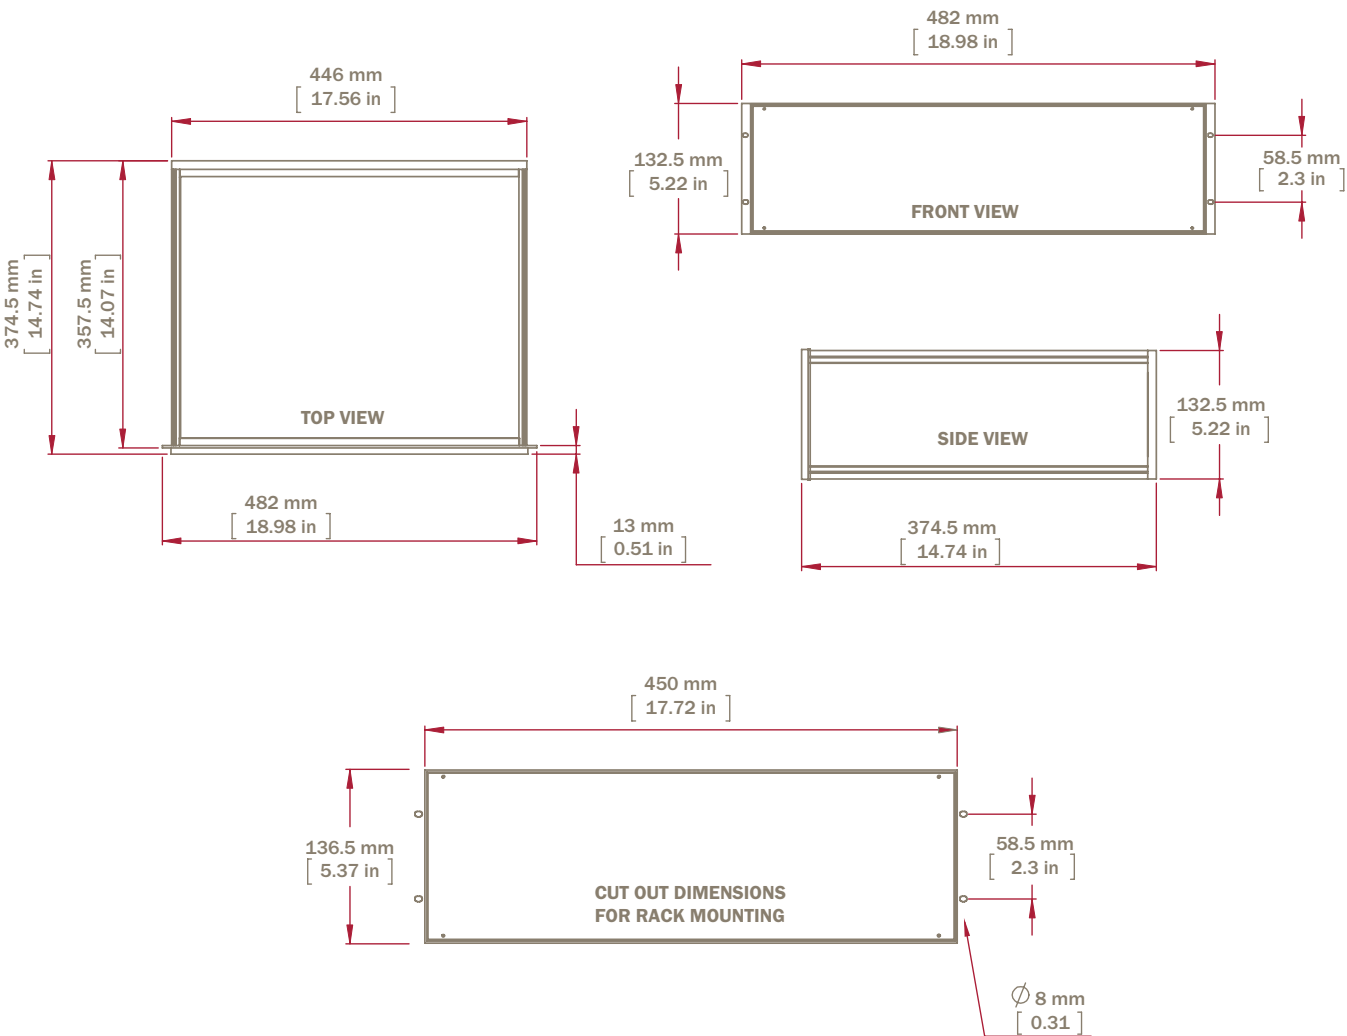

LABORATORY CHASSIS WITH MULTIPLE HEATED ZONES

The LabDetek module offers extra heated zones to extend the gas analysis possibilities. It can be used as a standalone unit having its own software interface or be used in combination with the MultiDetek2 compact gas chromatograph system. In both cases, a sophisticated and user friendly interface allows the parameters setting. This module can be used as well as an extension of an existing third party gas chromatograph to extend the applications possibilities. The flexibility and versatility of this modular platform make it suitable to work in cooperation with any GC system.






AMBIANT ZONE


A free area is available to mount the flow controllers and the compact gas purifier for the gas flow control and to generate high purity carrier gas.



PROGRAMMABLE HEATING ZONE

This zone offers a large heated space for fast temperature ramping going up to 350 Celsius. It can fit up to 5 x 6 inches + 5 x 3.5 inches coil diameter columns for a total of 10 columns. A well designed column support allows an easy mounting of the columns and end fittings individually. This is perfect for maintenance and column replacement. This zone can also be used to fit any combination of columns and valves that have to be heated.

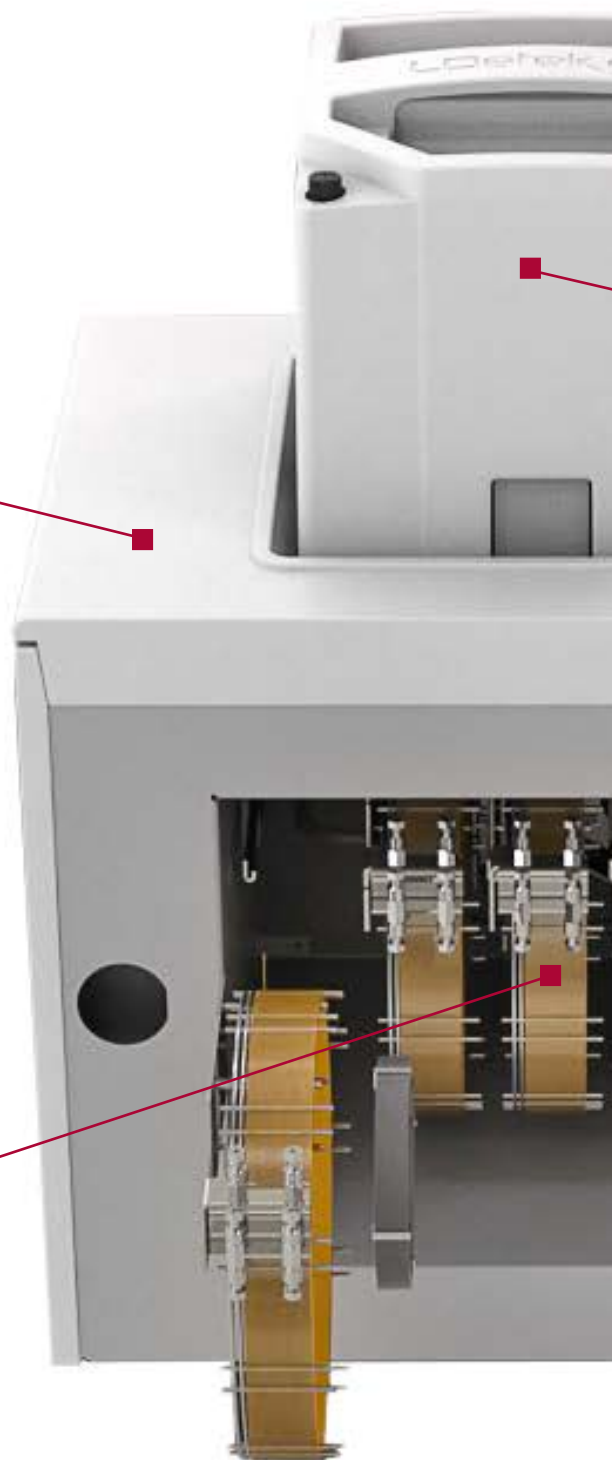

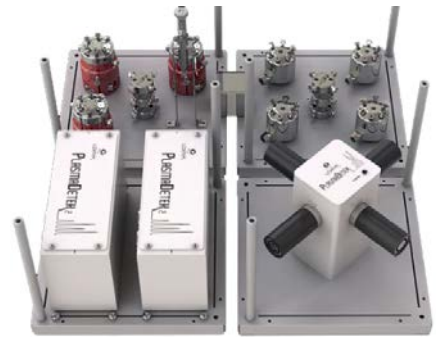

ISOTHERMAL HEATING ZONE

Based on a universal heated mounting plate system, this extra area can accept detectors, valves and columns in an isothermal environment that can achieve an operating temperature up to 200 Celsius. An injection port is also accessible on top of this zone to inject using a syringe or a headspace auto sampler system.



The LabDetek controller is used with the platform. This device offers multiple I/Os that can be used for different tasks like signal acquisitions, valves actuation, ovens and flows control. The controller communicates with the LabDetek interface module using Clarity from DataApex. The controller also offers serial and LAN communication protocols.

LD ACCESSORIES



WHY USING TRAPS?



They are necessary to remove interference components in carrier and sample gas used for GC's and on-line instruments. For the GC's, a combination of moisture, hydrocarbons and Oxygen traps is used to prevent column degradation what is well known to increase detector noise and create ghost peaks. The use of such traps is also necessary on Make-up gas that must also be interference free.

A selection of single component removal traps or multi-components removal traps is also necessary to remove interference components presents in sample lines with on-line instruments.

Our selection of traps is normally used when the LDP1000 (Gas purifier) cannot be used.

MOISTURE REMOVAL LDH20-T

Our Moisture Trap LDH20-T is used to remove moisture at the outlet of it. It can be installed on any carrier gas line, make-up gas line and sample line to remove moisture interference. Different sizes and connection types are available depending of the flow rate and the outlet purity specifications needed.

HYDROCARBON REMOVAL LDHC-T

The hydrocarbons trap series are commonly used when trace HC's is present in sample, carrier or make-up gas lines. Presence of hydrocarbons in gas lines creates a deterioration of some type of detector like common PED. Different sizes and connection types are available depending of the flow rate and the outlet purity specifications needed.

OXYGEN REMOVAL LD02-T

The Oxygen traps series are also offer with numerous configuration types that can cover any needs.

MULTI-COMPONENTS REMOVAL LDH20/HC/O2-T

Our LDetek special trap that combines removal of H₂O/HC's and O₂ in one unit is also a great alternative when the removal of all interference components is necessary. It avoids having complex tubing configuration with multiple fittings that increase leakage possibilities in the installation. Our Multi-Components trap can be configured the way you need it.

LDEPC ELECTRONIC FLOW CONTROLLER



LDetek is now offering its LDEPC as a stand alone flow controller unit for any gas type. Its high purity design combined with multiple communication mean is the ideal tool for gas flow control. This tool can be controlled with analog voltage, SPI, serial or usb port.

MINI-LDP1000



The Mini-LDP1000 gas purifier is the best solution for generating high purity Argon/Helium/Nitrogen/Hydrogen and other noble gases for any gas chromatograph when space available is restricted. Its compact design is ideal for portable gas analyzer. It is also the best solution to avoid problems coming from any source of contaminations that results to columns degradation and detector instability.

COLUMNS

LDetek can also offer a large selection of Packed type columns that can cover your needs for any GC application. Our columns can be coiled within your specifications and can be activated/regenerated in house. LDetek also have the capabilities to configure your custom request. We can also offers numerous types of columns ending:

- Stainless Steel or Brass Double ferrules type
- Stainless Steel single ferrules type
- Stainless Steel Face Seal fittings type
- Silver brazed type
- Argotek column
- HSR-Etek column

LDGDS



GAS DILUTION SYSTEM



The LDGDS is a user's friendly gas dilution system that offers all the flexibility to generate manually or automatically the desired gas mixtures. The Windows user's interface gives the ability to control and monitor the mixtures, flows, pressures and the concentrations. The system can store multiple gas cylinders mixture and it becomes easy to select the right cylinder to generate different blends. It reduces the cost of having specific standard for each blend needed. The dilution system is designed with a manual or automatic pressure controller installed on the zero gas line, on the span gas line and to regulate the outlet blended gas line pressure. This way, it improves the stability and the regularity of the flow controls. Each flow table uses a 10 points calibration curve to characterize the linearity of each flow controller.

To ensure ultra high purity zero gas reference to generate ppb blends, an optional integrated heated gas purifier can be mounted on the zero gas flow path.


FEATURES:

- Automatic calculation of dilution concentrations
- Manual or automatic pressure controller
- Broad range of dilution ratios (up to 1000 to 1)
- Windows user's interface through serial communication
- Multiple gas standard libraries available
- Alarms management
- 3U cabinet
- Integrated heated gas purifier to generate ultra high purity zero gas reference (optional)

APPLICATIONS:

- Multi-point calibration of gas analyzers
- Gas mixture
- Calibration standard of ppb/ppt concentrations for the electronic gas grade instrument.
(The integrated heated gas purifier is required)

SOFTWARE INTERFACE:

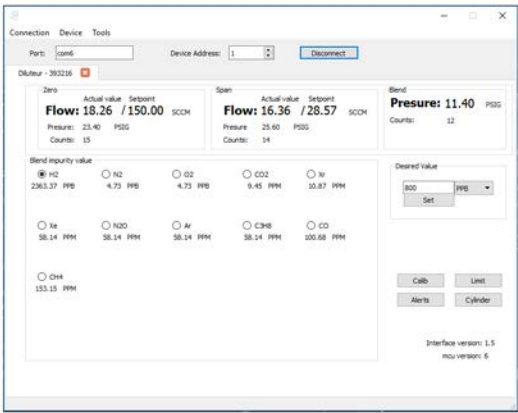


SPECIFICATIONS:

| | | |
|------------------------|---|---|
| PRESSURE CONTROLLERS | Manual pressure regulator or Electronic pressure regulator | |
| DILUTION RATIOS | 0 – 10 0 – 100 | 0 – 1000 other ratios possible on request |
| REPEATABILITY | < 1% | |
| ACCURACY | Better than $\pm 1\%$ | |
| OPTIONS | Integrated heated gas purifier for Zero gas reference | |
| GAS CONNECTIONS | Inlets/Outlets: 1/8" compression fittings (Swagelok type) 1/4" compression fittings (Swagelok type) | 1/8" VCR fittings (Swagelok type) 1/4" VCR fittings (Swagelok type) Vents: 1/8" compression fitting (Swagelok type) |
| MAX OPERATING PRESSURE | 100 PSIG (6.89 Bar) | |
| MIN OPERATING PRESSURE | 10 PSIG (0.7 Bar) | |
| OPERATING TEMPERATURE | 10 °C to 50 °C | |
| SUPPLY | 115 VAC, 50 – 60 Hz or 220 VAC, 50 – 60 Hz | |
| POWER CONSUMPTION | Maximum 10 watts Maximum 60 watts with optional integrated heated gas purifier | |
| DRIFT | < $\pm 1\%$ over 24 hours | |
| WEIGHT | 16 lbs (13 kg) | |


ORDERING INFORMATION:

| LDGDS | -X | -X | -X | -XXXX | -XXX | -X |
|-------|---|---|---|--|--|---|
| | Zero Gas type: A: Argon H: Helium N2: Nitrogen (other possible on request) | Span Gas type: A: Argon H: Helium N2: Nitrogen (other possible on request) | Ratio: 10: 10 to 1 100: 100 to 1 1000: 1000 to 1 (other possible on request) | Inlet/Outlets Fittings 2SWG: 1/8" Swagelok 4SWG: 1/4" Swagelok 2VCR: 1/8" VCR 4VCR: 1/4" VCR | Operating Voltage: 120: 120 volts 220: 220 volts | C: Integrated heated gas purifier for zero reference |

DIMENSIONS:

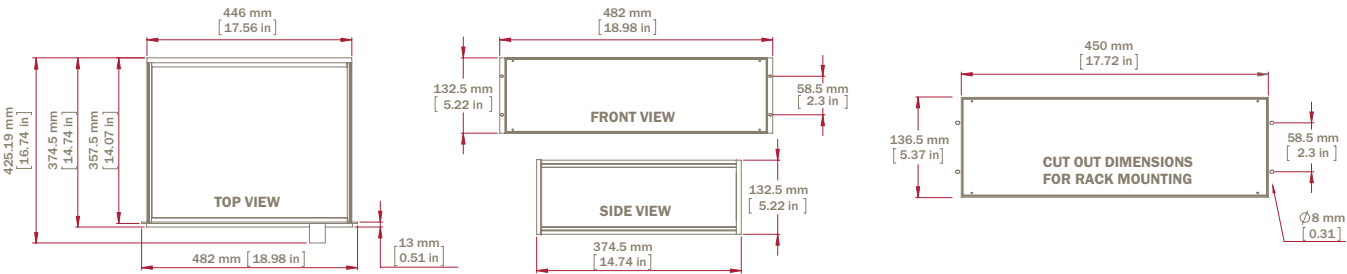

SYSTEM INTEGRATION INTO 19" CABINETS SEMICONDUCTOR & INDUSTRIAL GASES APPLICATIONS

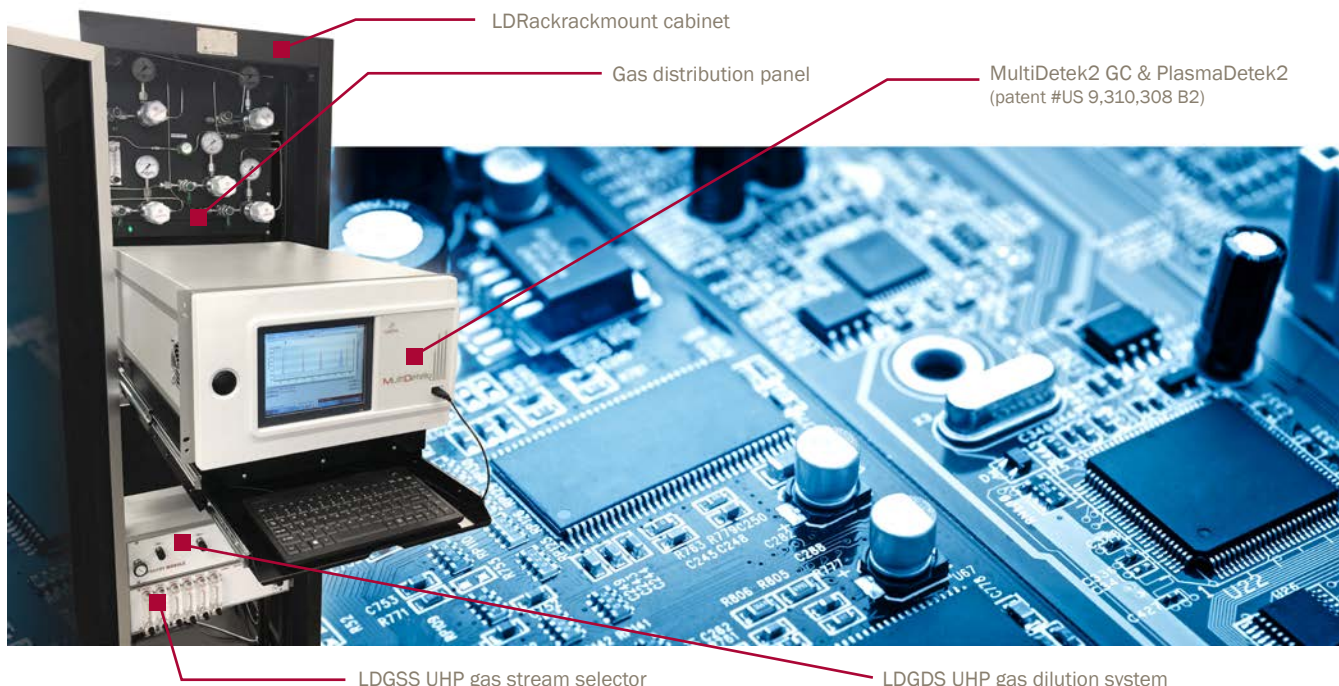

NEMA CABINETS

- ▶ Unique slide out design to offer easy access for maintenance without removing unit from gas sources.
- ▶ Welded equipment and VCR fittings/valves/regulators to ensure proper installation for the semi-conductors industry.
- ▶ Installation of third party analysers when required.
- ▶ Portable cabinets solution available

LDportable



LDetek also offers a portable solution for gas analysis. Its robust transportable rackmount enclosure with carrying handles and wheels is the perfect solution when moving the analyser to different locations is required.



The system allows quick starting mode by having the LDP1000 series integrated gas purifier for carrier and reference gas integrity in place. High purity isolation valves are also mounted to isolate the system against air contamination during transportation. All gas connections are mounted on the back plate for an easy and quick access.



A stream selection system and gas regulators can be mounted on the front panel for proper sample regulation before entering into the analyser.

Gas chromatograph or online gas analyser can be integrated in our solution easily. Our analyser design with its front door gives a full access to inside the instrument easily. An integrated touchscreen interface and PC allows direct access to data. A remote access is also available in all our instruments.

Anti vibration protection system is in place in each corner to minimize the vibrations and reduce the risk to damage the system during transportation.



3.0 APPLICATION NOTE

3.1 ENVIRONMENT



APPLICATION NOTE

LD12-01



Greenhouse analysis with the PlasmaDetek

The popularity to measure greenhouse gases (CH₄, CO₂ and N₂O) has increased considerably in the last years with the global warming concerns. Chromatography is the well known technique to measure them and different detectors are used to achieve this task. This application note will explain how we can effectively do it with a simple gas chromatograph configuration involving the PlasmaDetek detector.

PLASMADETEK CONFIGURATION:

The PlasmaDetek has the advantage that it can be configured to be more sensitive on some compounds than the others. This selectivity configuration helps the chromatography to be more effective and easier to setup.

For this application, the detector system is configured to be selective on all three impurities with two dedicated outputs signal:

- Output 1 : N₂O
- Output 2 : CH₄ and CO₂



▲ PlasmaDetek detector

CHROMATOGRAPHY CONFIGURATION:

Typical configuration to make such measurement requires methanizer, FID and ECD detectors, H₂ Fuel, make up gas and air supply.

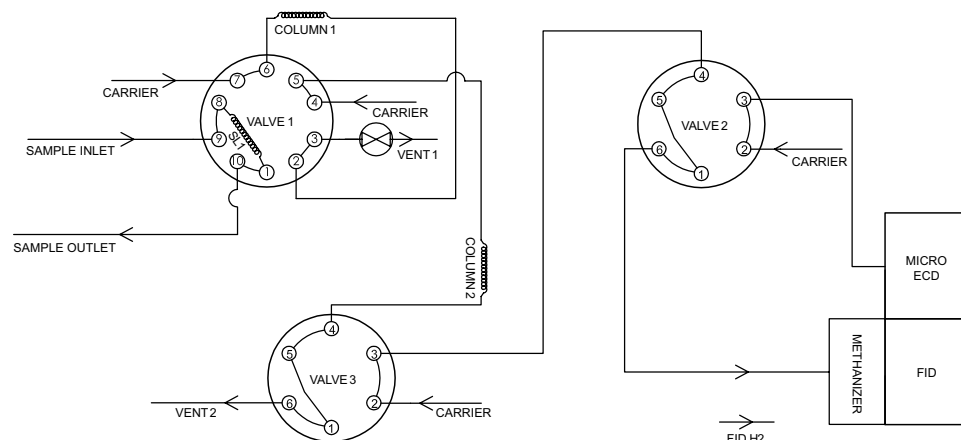


Figure 1: Typical configuration for greenhouse measurement

With the PlasmaDetek, only one detector can be used to measure CH₄, CO₂ and N₂O in air. All three components elute in the same detector. That reduces cost and complexity of the system.

Another advantage is the use of argon or helium as carrier gas. Both carriers are suitable and give the performance desired.

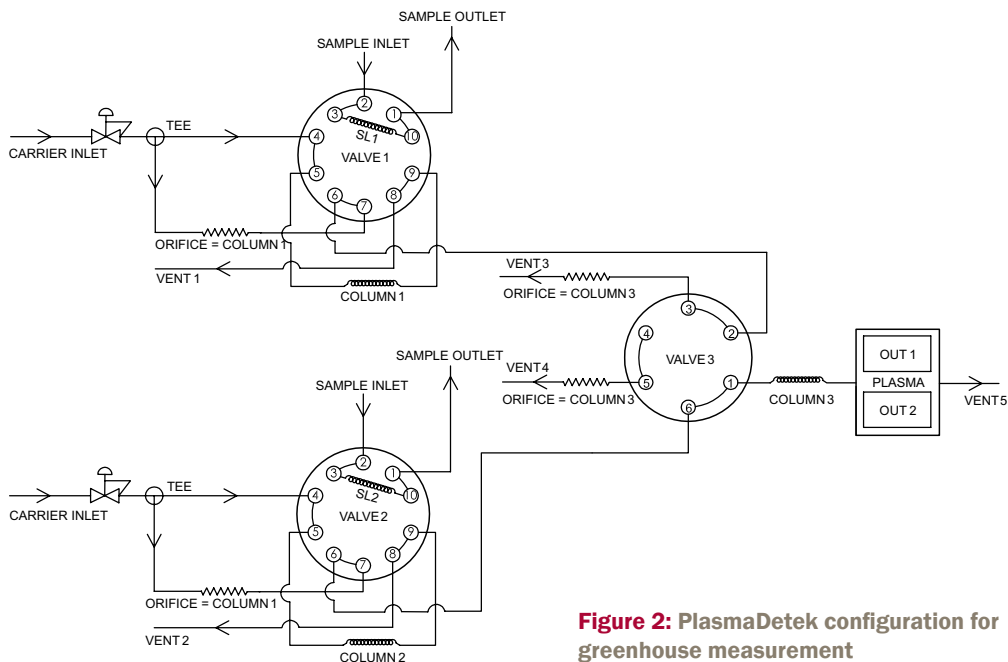


Figure 2: PlasmaDetek configuration for greenhouse measurement

Valve 1 is used for CH₄ and CO₂ measurement. The backflush to vent configuration vents out water from the sample with a HayeSep D 100/120 10'(column 1). Valve 3 is used to vent out air before going to the other HayeSep D 100/120 10'(column 3). This second column separates CH₄ and CO₂ from the remaining air.

Valve 2 is also configured in a backflush to vent with a HayeSep D 100/120 10'(column 2). A different sampling loop size is used to be able to measure N₂O. Valve 3 is used to vent out air and CO₂. N₂O is then brought to the detector by itself and can be measured in very low concentration.

RESULTS AND PERFORMANCE:

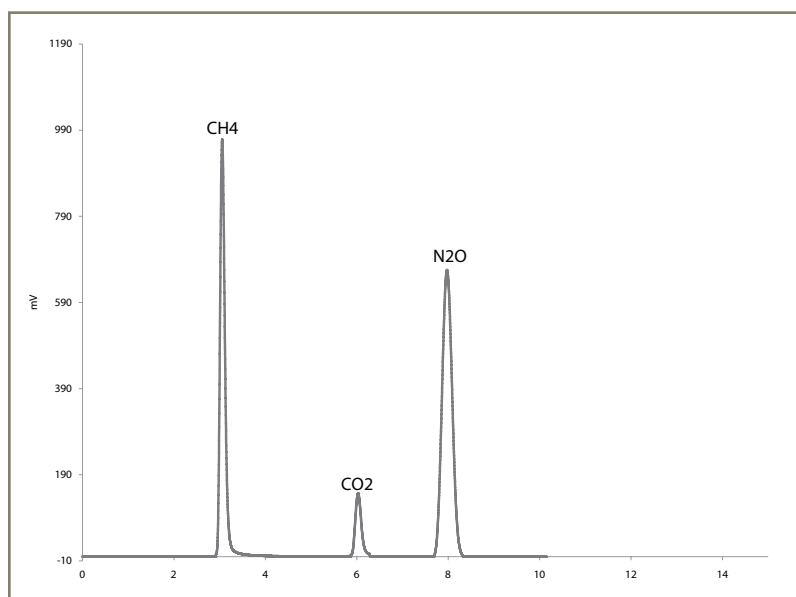


Figure 3: 8 ppm CH₄, 50 ppm CO₂ and 10 ppm N₂O in helium

Figure 3 shows the chromatogram obtained with the LDetek configuration described above, with a 8 ppm CH₄, 50 ppm CO₂ and 10 ppm N₂O standard. This result was used to calculate the LOQ and LOD of each compounds shown in figure 4.

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | S/N | LOD (ppb) S/N = 3 | LOQ (ppb) S/N = 5 |
|------------------|---------------|-------------|---------|-------|----------------------|----------------------|
| CH ₄ | 8 ppm | 965 mV | 0.04 mV | 24125 | 1 | 1.65 |
| CO ₂ | 50 ppm | 143 mV | 0.04 mV | 3575 | 42 | 70 |
| N ₂ O | 10 ppm | 671 mV | 0.04 mV | 16775 | 1.8 | 3 |

Figure 4: LOQ and LOD calculation

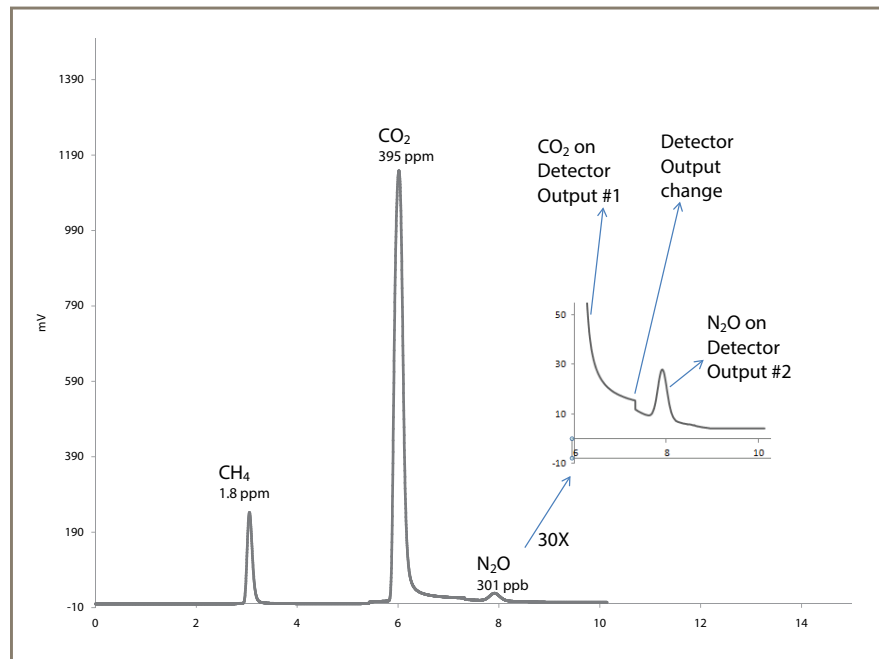


Figure 5: CH₄, CO₂ and N₂O in ambient air

All three components are measured without interference in air providing accurate and very sensitive detection. The LOD of N₂O ensures that its measurement in air is detected easily.

Those results and performances depend on the chromatographic system and conditions of operation.

CONCLUSION:

This technique is simple and cost effective compared to the most common configurations that can be found on the market. No make-up gas, fuel, air, FID and ECD radioactive detector are required to make this measurement. Only one PlasmaDetek detector with two outputs using argon or helium as carrier gas can be used to achieve level of sensitivity needed. The ease of installation and startup of the PlasmaDetek makes it perfectly suitable for this environmental application.

APPLICATION NOTE

LD15-03



Measurement of part per billion N₂O in air




With the global warming concerns, it is more and more critical to measure the nitrous oxide (N₂O) concentration in the ambient air. This application note will demonstrate how efficient the use of the PlasmaDetek-E is for the measurement of extremely low concentration of N₂O in ambient air without interference.

LDETEK SOLUTION:

It is well known that the measurement of N₂O can be achieved with different kinds of detectors using specific chromatography techniques. The ECD, HID and conventional PED are the mostly used type of detectors for this greenhouse application. The radioactive source coming from the ECD makes this detector less attractive due to the latest worldwide regulations about radioactivity, even for low source of radioactivity. The HID and conventional PED are relatively good detectors for such analysis, but create more chromatography challenges caused by lack of selectivity and sensitivity. With the LDetek PlasmaDetek-E, the enhanced sensitivity and selectivity make it the ideal tool for measuring extremely low concentration N₂O in ambient air with reduced interference mostly coming from the high concentration carbon dioxide and moisture.

The improved operation's mode and the optical design of the PlasmaDetek-E combined with right chromatography configuration in the MultiDetek-2 compact GC remove the interference usually coming from the carbon dioxide and moisture.

The MultiDetek-2 system is configured with one injection diaphragm valve V1, which is used for injecting the sampling volume into the chromatography system. A first packed Shincarbon column is combined with a heartcut diaphragm valve V2 and a second packed Shincarbon column to catch the desired N₂O peak and flush to vent the undesired interference gases. The N₂O peak is then going to the PlasmaDetek-E where proper analysis is performed.

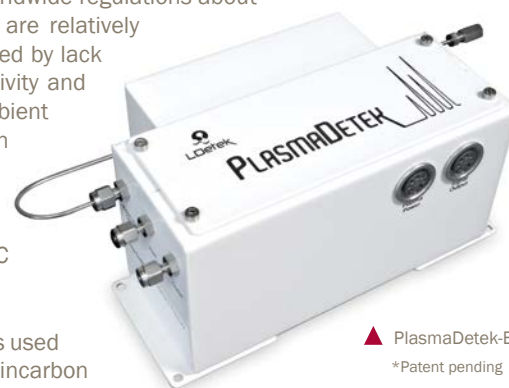


▲ PlasmaDetek-E
*Patent pending

This combination makes it ideal to measure extremely low concentration N₂O in air without having the N₂O peak integrated in the high concentration CO₂ tailing. This technique has been tested up to 5000ppm CO₂ for measuring as low as 1ppb N₂O as demonstrated in the chromatograms.


The MultiDetek-2 can be configured with different sampling mode to get the sample gas ready for analysis. The drawing of this application note shows the use of a micro pump that is mounted just before the sampling loop. The pump is fully controlled from the software interface and can be switched On/Off adequately for a specific period of time to allow proper sample gas quantity going to the sampling loop mounted on the diaphragm valve V1. This way, the loop is filled just before running an analysis. This technique allows to minimize the sample gas volume required for analysis since in many cases, the sample gas comes from bags, balloons, canisters or others. It is then critical to minimize the sample gas volume for every analysis.

An optional sample line purge system can also be added to the sampling mode of the MultiDetek-2. This system uses the carrier gas to purge the sample line prior to pump the sample gas from its source. This way, the sample flow path and sampling loop are totally purged with N₂O free gas since the carrier gas used as purge gas comes from the heated LDetek, model LDP1000 getter that removes N₂O down to 0.01ppb level.

The MultiDetek-2 can also have an injector system with septum for syringe injection mode. The system is directly mounted on the injection diaphragm valve V1.

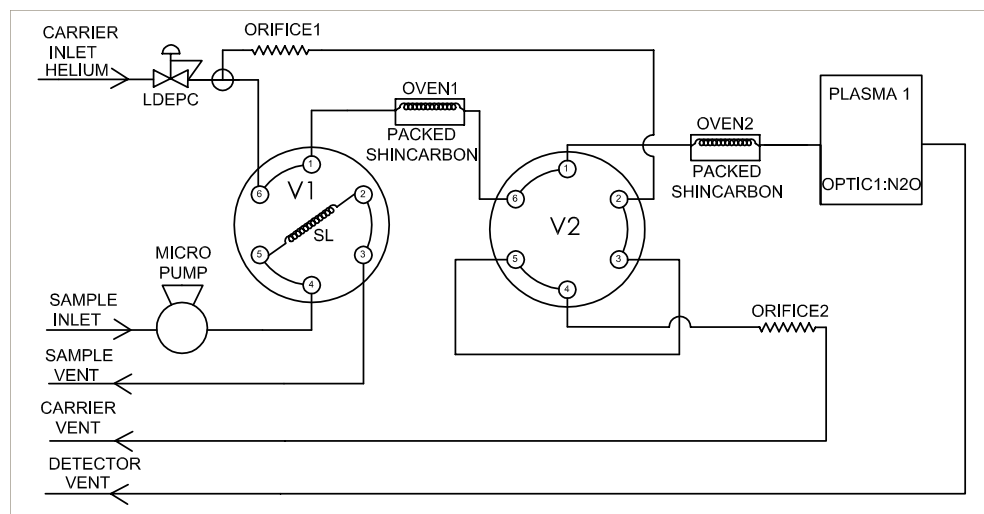


MultiDetek-2 configuration diagram 1: V1 position OFF: Filling sampling loop
V2 position OFF: Catches N₂ peak from the first packed Shincarbon in oven #1 to the second packed Shincarbon in oven #2

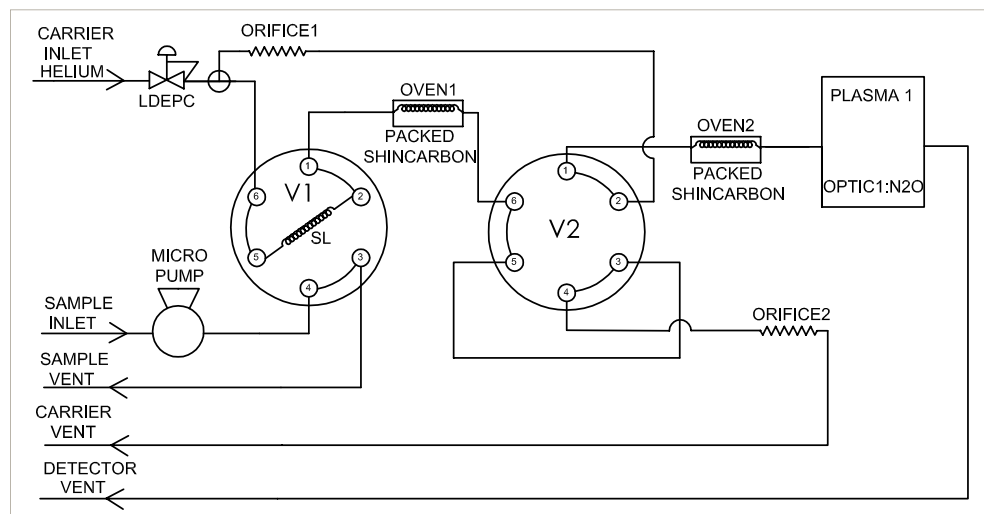


MultiDetek-2 configuration diagram 2: V1 position ON: Injecting sampling loop
V2 position ON: Flushes to vent the interference gases (air, carbon dioxide, moisture and others) coming out from the first packed Shincarbon in oven #1

RESULTS:


Low ppb Chromatogram examples

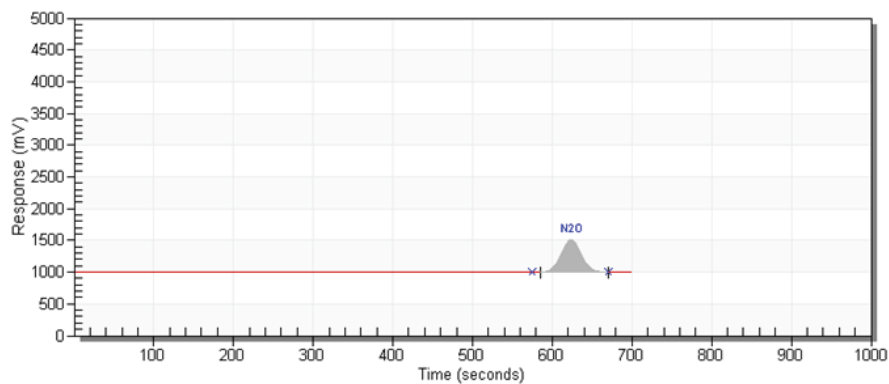

Chromatogram 1:
140ppb N₂O in air

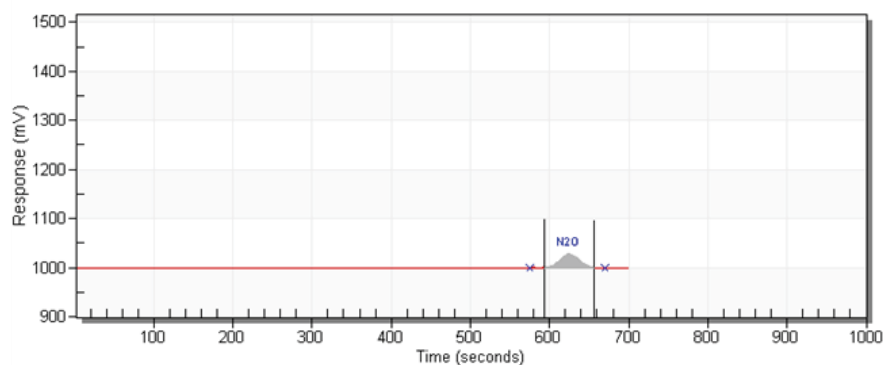

Chromatogram 2:
7ppb N₂O in air

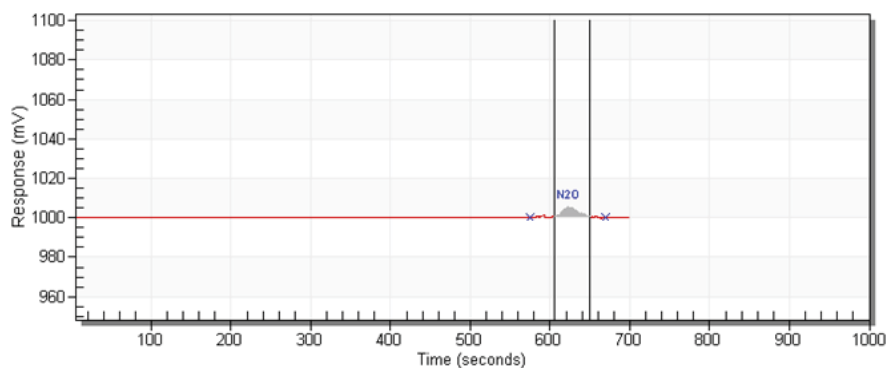

Chromatogram 3:
1ppb N₂O in air

LDL calculation:

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|------------------|---------------|-------------|--------|----------------|
| N ₂ O | 1ppb | 6 mV | 0.2 mV | 0.1 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

CONCLUSION:

With its user-friendly interface and the simple configuration of this compact GC, the MultiDetek-2 is a perfect fit for this greenhouse application. The enhanced sensitivity and selectivity of the PlasmaDetek-E allow extreme low limits of detection. This new measurement technique combined with the integrated purged low volume sampling gas system brings this technology over the existing conventional measurement methods and systems.

APPLICATION NOTE

LD16-01



Air analysis using the MultiDetek2 and PlasmaDetek2



▲ MultiDetek2

▲ PlasmaDetek2

LDETEK SOLUTION:

The air analysis for environmental applications is more and more required in different regions of the world. In this application note, the trace analysis of acids, sulfurs and nitrous oxide has been combined in one single compact instrument using one detection technology based on plasma emission (PlasmaDetek2). The MultiDetek2 compact GC has been configured with parallel channels to achieve the measurement at low ppb level for the different impurities. The sample collection can be performed with micro pump for ambient pressure application or bags, with a proportional micro valve for positive pressure application to control flow rate or with our auto injector headspace for vials. The MultiDetek2 was built using heated zones to avoid cold points between the columns and the plasma detector. The detector, valves, fittings and tubing are made of coated stainless steel to avoid surface adsorption. This ensures good sensitivity and repeatability measuring impurities.

RESULTS:


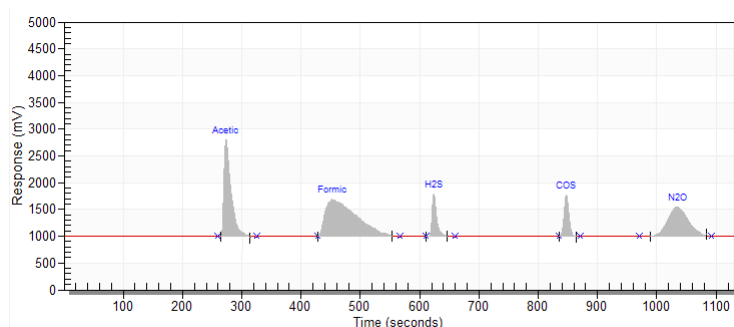


Figure 1 :
Chromatogram of trace
impurities in balance air

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-------------|---------------|-------------|--------|----------------|
| Acetic acid | 0.27 ppm | 2850 mV | 36 mV | 0.010 ppm |
| Formic acid | 0.20 ppm | 1785 mV | 46 mV | 0.015 ppm |
| H2S | 3.00 ppm | 1860 mV | 1.6 mV | 0.008 ppm |
| COS | 3.00 ppm | 1870 mV | 1.9 mV | 0.009 ppm |
| N2O | 2.30 ppm | 1595 mV | 0.4 mV | 0.001 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

Figure 2 : LDL based on 3 times noise ratio

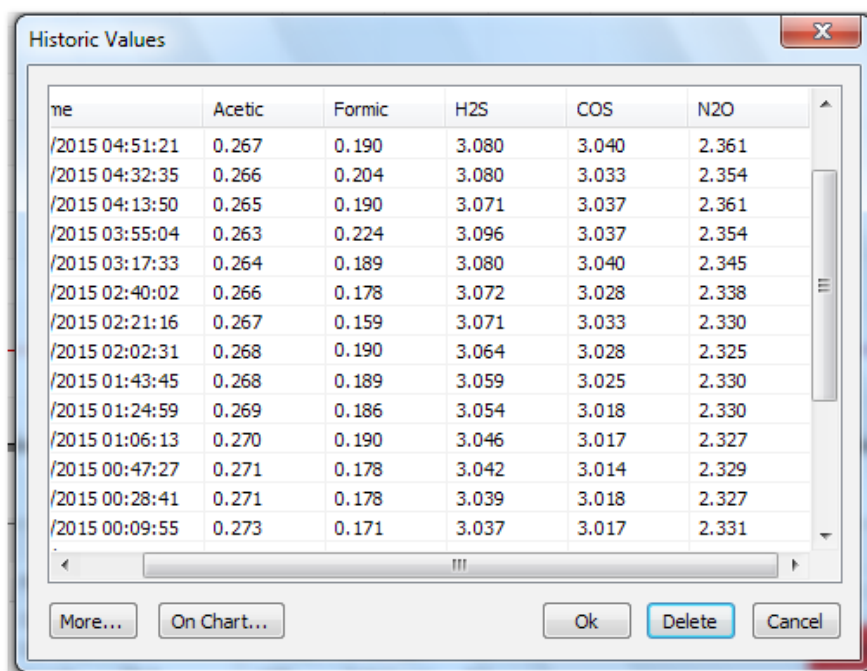

| Time | Acetic | Formic | H2S | COS | N2O |
|----------------|--------|--------|-------|-------|-------|
| /2015 04:51:21 | 0.267 | 0.190 | 3.080 | 3.040 | 2.361 |
| /2015 04:32:35 | 0.266 | 0.204 | 3.080 | 3.033 | 2.354 |
| /2015 04:13:50 | 0.265 | 0.190 | 3.071 | 3.037 | 2.361 |
| /2015 03:55:04 | 0.263 | 0.224 | 3.096 | 3.037 | 2.354 |
| /2015 03:17:33 | 0.264 | 0.189 | 3.080 | 3.040 | 2.345 |
| /2015 02:40:02 | 0.266 | 0.178 | 3.072 | 3.028 | 2.338 |
| /2015 02:21:16 | 0.267 | 0.159 | 3.071 | 3.033 | 2.330 |
| /2015 02:02:31 | 0.268 | 0.190 | 3.064 | 3.028 | 2.325 |
| /2015 01:43:45 | 0.268 | 0.189 | 3.059 | 3.025 | 2.330 |
| /2015 01:24:59 | 0.269 | 0.186 | 3.054 | 3.018 | 2.330 |
| /2015 01:06:13 | 0.270 | 0.190 | 3.046 | 3.017 | 2.327 |
| /2015 00:47:27 | 0.271 | 0.178 | 3.042 | 3.014 | 2.329 |
| /2015 00:28:41 | 0.271 | 0.178 | 3.039 | 3.018 | 2.327 |
| /2015 00:09:55 | 0.273 | 0.171 | 3.037 | 3.017 | 2.331 |

Figure 3 :
Repeatability results

CONCLUSION:

Using a solution combining the PlasmaDetek 2 and the MultiDetek 2 is the best way to achieve sensitivity, robustness and speed in an industrial or laboratory compact system for air analysis.

APPLICATION NOTE

LD16-13



Measurement of Greenhouse gases GHG



Energy (fossil fuel) and agriculture required for human activities on Earth produce Greenhouse gases (GHG) such as Carbon Dioxide (CO₂), Methane (CH₄), Nitrous Oxide (N₂O) and Fluorinated gases mainly Sulfur Hexafluoride (SF₆). These gases tend to absorb infrared radiation emitted by the Earth surface resulting to reduce the atmospheric heat loss into space and keeping Earth warmer.

The source of every GHG type is associated to different sectors resulting of human activities:

CO₂ → *Fossil fuel, industrial processes, forestry, land use for agriculture*

CH₄ → *Agriculture, waste management, energy use, biomass burning*

N₂O → *Agriculture (such as fertilizer use) and biomass burning*

F-gases (SF₆) → *Industrial processes and refrigeration*

For this reason, the Kyoto Protocol was established in 1997 by the industrialized countries with an objective to measure, control and decrease the GHG in order to reduce the continuous global warming.

Figures 1, 2 and 3 show some data that demonstrate the impact of human activities to increase the Greenhouse gases level worldwide.

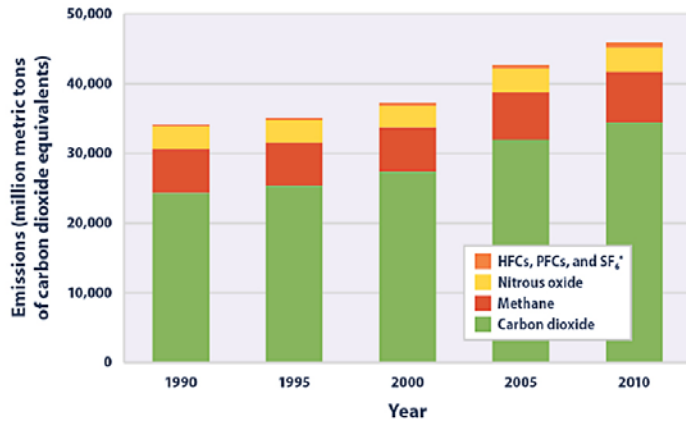


Figure 1:
Global Greenhouse gas emissions by gas type,
1990-2010

(Data sources WRI 2014, FAO 2014) ¹

This figure shows worldwide emissions of carbon dioxide, methane, nitrous oxide and several fluorinated gases from 1990 to 2010. For consistency, emissions are expressed in million metric tons of carbon dioxide equivalents. These totals include emissions and sinks due to land-use change and forestry.

*HFCs are hydro fluorocarbons, PFCs are per fluorocarbons and SF₆ is hexafluoride

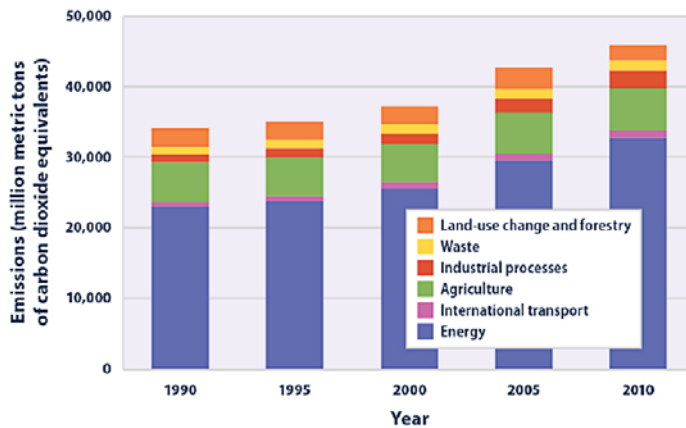


Figure 2:
Global Greenhouse gas emissions by sector,
1990-2010

(Data sources WRI 2014, FAO 2014) ¹

This figure shows worldwide gas emissions by sector from 1990 to 2010.

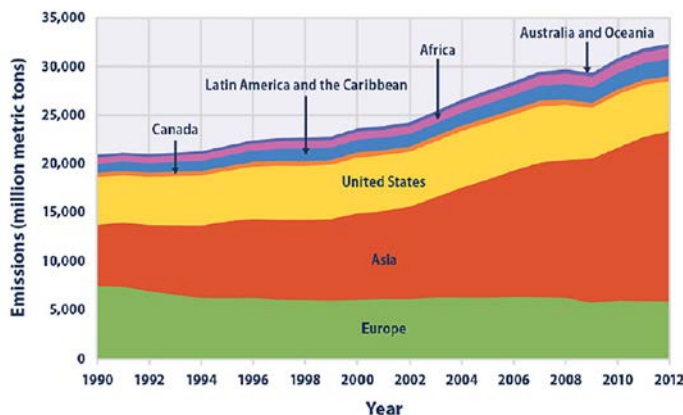


Figure 3:
Global Greenhouse gas emissions by regions,
1990-2012

(Data sources WRI 2015) ¹

This figure shows carbon dioxide emissions from 1990 to 2012 for different regions of the world.

¹ Data and analysis come from the World Resources Institute's Climate Analysis Indicators Tool (CAIT), which compiles data from peer reviewed and internationally recognized greenhouse gas inventories developed by EPA and other government agencies worldwide.

The well known technique to measure and quantify the GHG is Gas Chromatography. It can determine the rate of emission or absorption. These rates are mainly measured using samples of soil, rice, maize or wheat from different areas. The measurement of ambient air is also used. The worldwide GHG can then be better measured and controlled to facilitate the proper actions to be taken to reduce the global warming.

ALTERNATIVE SOLUTION USING GAS CHROMATOGRAPH

The use of multiple detectors in a gas chromatography system is generally necessary to cover the greenhouse application.

A FID detector and a methanizer system for detection of trace impurities of Methane (CH₄) and Carbon Dioxide (CO₂). Such detector requires Fuel (H₂), Air and the carrier gas source to make it works.

An ECD detector to measure traces Nitrous Oxide (N₂O) and Sulfur Hexafluoride (SF₆). This type of detector is a source of radioactivity and results in complication for storage, handling and transport.

A TCD is also required for measuring high concentration Carbon Dioxide (CO₂) when necessary.

It is then a solution combining multiple types of detection technology which makes the system more complex to operate and increases the operating cost.

OUR SOLUTION

Using the PlasmaDetek2 (PED) plasma detector and the MultiDetek2 compact gas chromatograph, the analysis of the most critical trace impurities in air can be achieved in one unit with a single detection technology (PED).

By default, the configuration has 2 channels to cover the analysis of Methane, Carbon Dioxide, Nitrous Oxide and Sulfur Hexafluoride. If additional options for the analysis of other impurities like fluorinated gases (F-gases) are required, then an additional channel still using a Plasma Emission Detector can be added in the same instrument.

Channel#1: This channel measures 0-1000ppm Methane (CH₄) and 0-5000ppm Carbon Dioxide (CO₂) using the PlasmaDetek2 (PED). Other measuring ranges can be configured. The system is protected against moisture using a pre column in back flush to vent configuration.

Channel#2: 0-10ppm Sulfur Hexafluoride (SF₆) and Nitrous Oxide (N₂O) still uses the PlasmaDetek2 (PED). Other ranges are also possible. A pre column to protect the system against moisture is also used in this channel.

Channel#3 (optional): Analysis of other fluorinated gases (F-gases) that would still be using the PlasmaDetek2 (PED) as detector.

The sample preparation is managed by the HTA Headspace auto sampler system mounted on the MultiDetek2 GC. The auto sampler tray configuration can be for 14 or 42 vials having size range of 10ml or 20ml depending of the application requirements. The oven can accept 1 or 6 vials for heating and shaking in preparation of analysis. The auto sampler offers syringe auto cleaning and a purge routine in between each sample collection. The syringe volume can be 2.5ml or 5ml depending of the application.

The Headspace can be controlled from its keypad, touch screen interface or from the software environment installed on an external PC or in the integrated PC of the MultiDetek2.

The data management is done with the MultiDetek2 interface. The unit can be control locally from the MultiDetek2 touch screen interface or remotely using LAN connectivity.

RESULTS

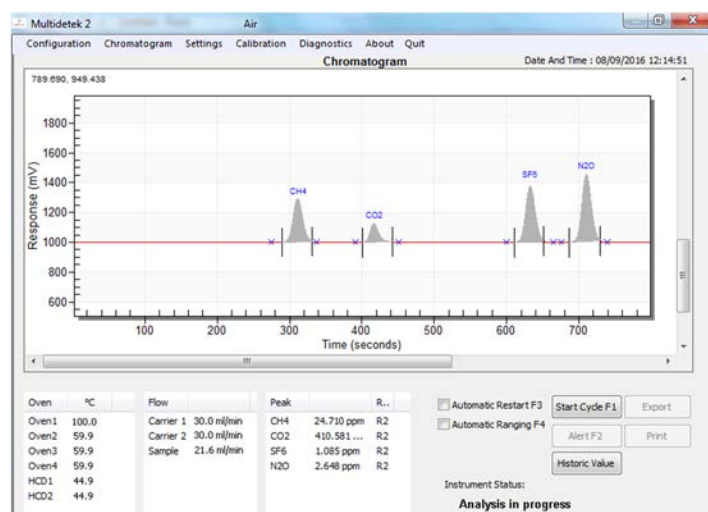


Figure 1: chromatogram of trace impurities in balance air coming from a certified gas bottle.

For this application, a measuring range of 0-1000ppm was required for the CH4 with a LDL of 200ppb.

A measuring range of 0-5000ppm was required for the CO2 with a LDL of 500ppb.

A measuring range of 10ppm was required for the SF6 and N2O with a LDL of 20ppb.

The figure 2 shows a table where the LDL calculation was obtained with a noise/response ratio. It shows the system can achieve better specifications than what was required for the application. Lower detection limits can be obtained with the same system just by changing the injected sampling loop volume. An extended range with lower detection limit capabilities can be obtained with our optional multiple sampling loop injection system.

It becomes possible to measure ppt/ppb/high ppm with the same detector in the same instrument.

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------|---------------|-------------|---------|----------------|
| CH4 | 24.710 ppm | 331 mV | 0.4 mV | 89.6 ppb |
| CO2 | 410.581 ppm | 177 mV | 0.06 mV | 417.5 ppb |
| SF6 | 1.085 ppm | 389 mV | 1.6 mV | 13.4 ppb |
| N2O | 2.648 ppm | 479 mV | 0.9 mV | 14.9 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic condition

Figure 2

CONCLUSION

The combination of the PlasmaDetek2 (PED) detector with the MultiDetek2 compact gas chromatograph and the HTA Headspace auto sampler becomes an interesting reliable and robust solution for the laboratory requirements where Greenhouse (GHG) gases must be measured.

APPLICATION NOTE

LD19-06



VOCs measurement in the air



MultiDetek2 ▲

The analysis of indoor/outdoor air quality is becoming an important part of our day-to-day priorities due to the increasing contaminant level caused by the industrial processes. The main contaminants to be controlled in the air are the VOCs (volatile organic compounds).

VOCs are human-made contaminants used and produced in the processing of product manufacturing as paints, adhesives, petroleum products, pharmaceuticals, and refrigerants. This includes emissions from automotive and industrial activity among other sources.

This classification includes different compound groups with various structural characteristics and chemical properties:

- ▶ **Halogenated hydrocarbons**
- ▶ **Aromatics**
- ▶ **Ketones**
- ▶ **Nitriles**
- ▶ **Acrylates**
- ▶ **Acetates**
- ▶ **Ethers**
- ▶ **Sulfides**

Many of these compounds contaminate our environment today. Acceptable exposure limits and regulations for the release of VOCs to the environment are provided by the EPA and other regulatory bodies.

The most common technique used to detect, identify and quantitate VOC is gas chromatography coupled with an FID (flame ionization detector).

LDETEK SOLUTION

The MultiDetek2 compact GC, configured with one FID can offer multiple methods for the analysis of VOCs in the air. This document will show the most common configuration for the air quality monitoring.

The first channel having an injection valve and an arrangement of columns is used for the analysis of trace CH₄, NMHC and THC. The second channel, having similar configuration of valve/column can be added for the analysis of BTEX when it is required. Both channels merge in the FID for the analysis of the components. The diaphragm valves, the columns and the detector are mounted in their respective isothermal heated area to maintain the temperature and the reading stable.

By default, the system comes with a choice of 2 pre-configured/calibrated methods:


Method 1 → Trace CH₄-NMHC-THC in the air

Method 2 → Trace CH₄-NMHC-THC-benzene-toluene-xylenes in the air

RESULTS

This chromatogram represents the method 2 analysis. It has been performed using a certified gas bottle containing 105mg/NM³ CH₄, 93.7mg/NM³ benzene, 95.3mg/NM³ toluene and 96mg/NM³ xylenes in a balance of air. The response time for complete analysis of VOC + BTEX is below 4 minutes. The NMHC are calculated and offered when required. The results for the method 1 are the same, except that the measured impurities are CH₄-NMHC-THC only. The analysis time is then reduced to 1 minute for the method 1.

| PEAK | UNIT | CALIBRATION VALUE | _AREA COUNTS |
|-----------------|--------------------|-------------------|--------------|
| CH ₄ | mg/Nm ³ | 105.00 | 15784 |
| THC | mg/Nm ³ | 105.00 | 1837 |
| Benzene | mg/Nm ³ | 93.70 | 13519 |
| Toluene | mg/Nm ³ | 95.30 | 17703 |
| Xylenes | mg/Nm ³ | 96.00 | 78188 |

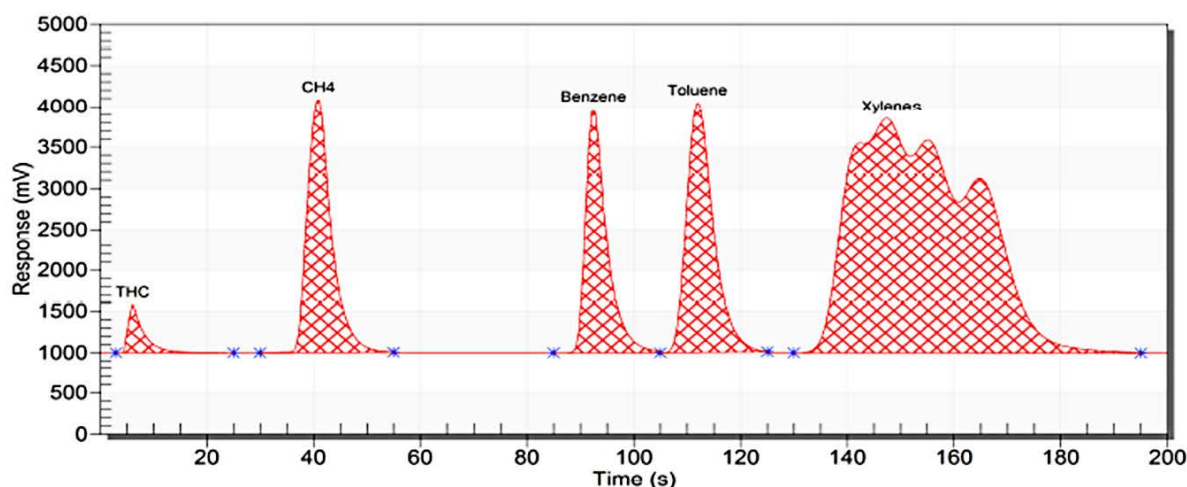

LIMIT OF DETECTION


Running at low concentration, the ldl value is identified as being 3 times the noise level. Refer to the chromatograms and chart below.

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE AVERAGE | LDL (3X NOISE) |
|-----------|---------------|-------------|---------------|----------------|
| THC | 1.0mg/NM3 | 12mV | 0.2mV | 0.050mg/NM3 |
| CH4 | 0.225mg/NM3 | 5.5mV | 0.4mV | 0.049mg/NM3 |
| Benzene | 0.332mg/NM3 | 7.5mV | 0.3mV | 0.040mg/NM3 |
| Toluene | 0.338mg/NM3 | 6.9mV | 0.25mV | 0.037mg/NM3 |
| Xylenes | 0.176mg/NM3 | 15mV | 1.5mV | 0.053mg/NM3 |


Note: other LDL could be obtained with different injection volume and chromatographic condition

LOW CONCENTRATION CHROMATOGRAM



THC: 1.5mg/NM3

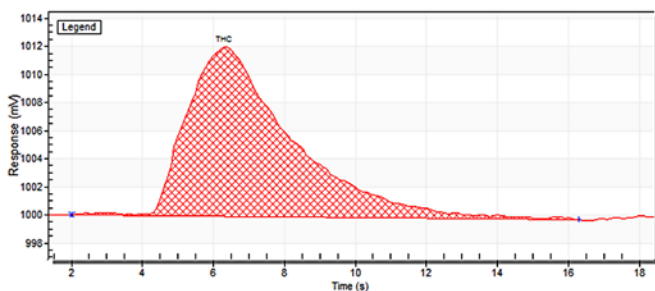



NOISE BASELINE IDENTIFICATION




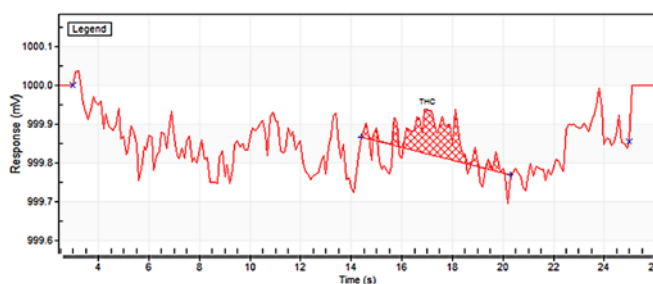


CH4: 0.225mg/NM3

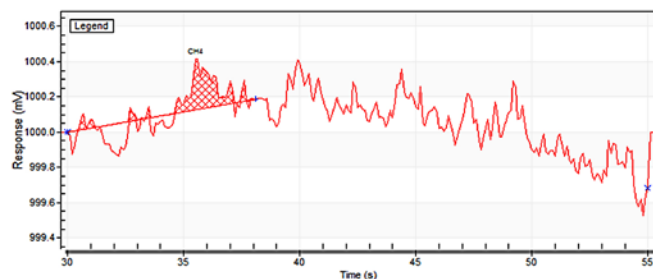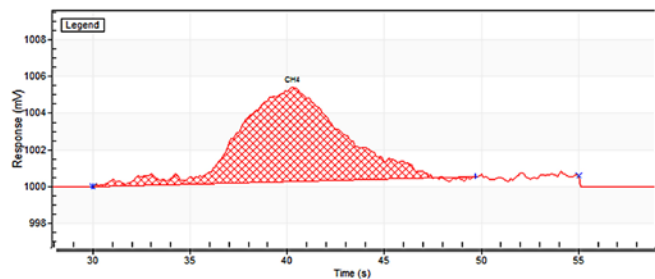

Benzene: 0.332mg/NM3

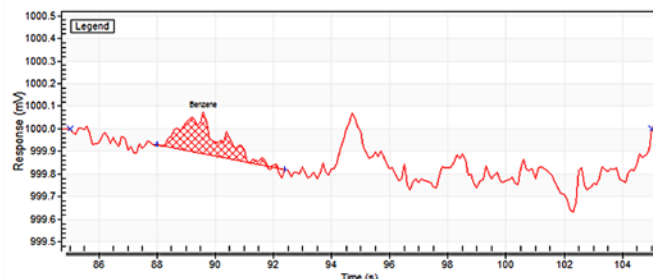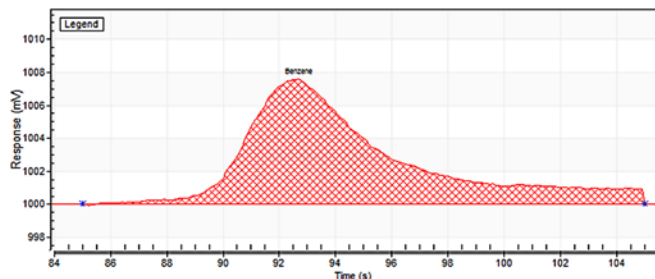

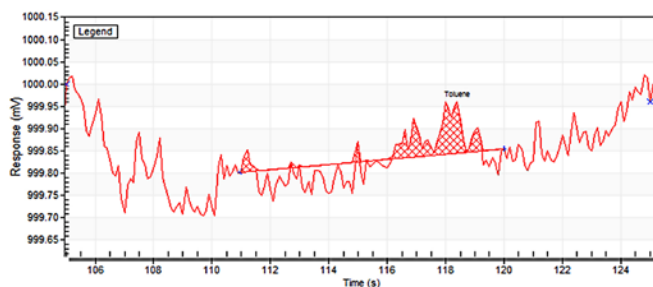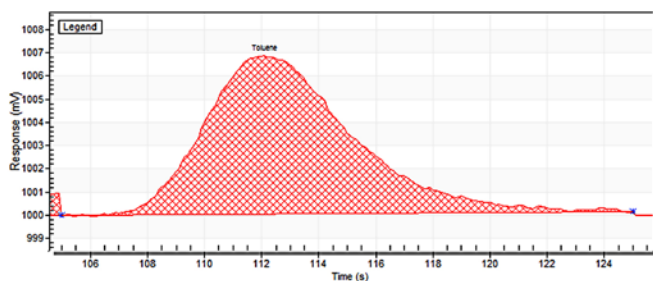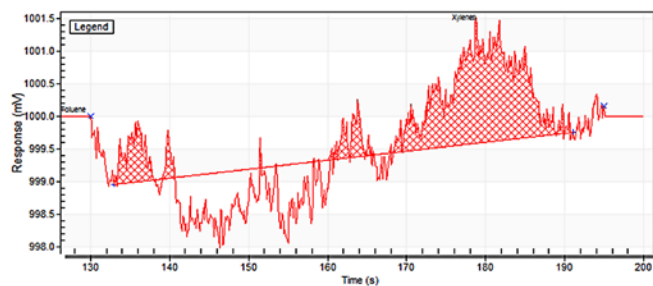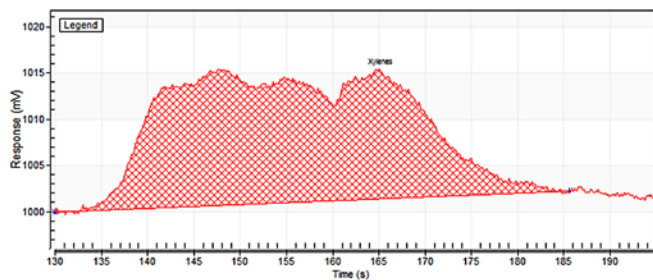Toluene: 0.338mg/NM3**Xylenes: 0.576mg/NM3****REPEATABILITY**

A value of $CV\% \times 3 < 5\%$ for a series of consecutive analysis at a fix concentration in a balance gas of air has to be performed. Refer to the charts below.

| COMPONENTS | Repeatability (CV% x 3) |
|------------|-------------------------|
| NMHC | 0.59% |
| THC | 0.58% |
| CH4 | 0.46% |
| Benzene | 0.52% |
| Toluene | 0.48% |
| Xylenes | 0.23% |

ANALYSES

| Start | NMHC | THC | CH4 | Benzene | Toluene | Xylenes |
|------------------|----------------|----------------|--------------|--------------|--------------|---------------|
| 2019-09-13 08:07 | 259.962 mg/Nm3 | 263.538 mg/Nm3 | 3.575 mg/Nm3 | 3.164 mg/Nm3 | 3.222 mg/Nm3 | 15.617 mg/Nm3 |
| 2019-09-13 08:03 | 258.758 mg/Nm3 | 262.330 mg/Nm3 | 3.572 mg/Nm3 | 3.166 mg/Nm3 | 3.221 mg/Nm3 | 15.607 mg/Nm3 |
| 2019-09-13 08:00 | 258.895 mg/Nm3 | 262.466 mg/Nm3 | 3.570 mg/Nm3 | 3.169 mg/Nm3 | 3.218 mg/Nm3 | 15.601 mg/Nm3 |
| 2019-09-13 07:56 | 258.861 mg/Nm3 | 262.427 mg/Nm3 | 3.566 mg/Nm3 | 3.174 mg/Nm3 | 3.216 mg/Nm3 | 15.584 mg/Nm3 |
| 2019-09-13 07:53 | 259.375 mg/Nm3 | 262.943 mg/Nm3 | 3.568 mg/Nm3 | 3.174 mg/Nm3 | 3.216 mg/Nm3 | 15.583 mg/Nm3 |
| 2019-09-13 07:50 | 259.759 mg/Nm3 | 263.328 mg/Nm3 | 3.569 mg/Nm3 | 3.177 mg/Nm3 | 3.211 mg/Nm3 | 15.594 mg/Nm3 |
| 2019-09-13 07:46 | 259.381 mg/Nm3 | 262.952 mg/Nm3 | 3.571 mg/Nm3 | 3.182 mg/Nm3 | 3.206 mg/Nm3 | 15.580 mg/Nm3 |
| 2019-09-13 07:43 | 259.111 mg/Nm3 | 262.681 mg/Nm3 | 3.570 mg/Nm3 | 3.190 mg/Nm3 | 3.207 mg/Nm3 | 15.571 mg/Nm3 |
| 2019-09-13 07:39 | 259.326 mg/Nm3 | 262.899 mg/Nm3 | 3.573 mg/Nm3 | 3.190 mg/Nm3 | 3.209 mg/Nm3 | 15.561 mg/Nm3 |
| 2019-09-13 07:36 | 258.653 mg/Nm3 | 262.222 mg/Nm3 | 3.568 mg/Nm3 | 3.189 mg/Nm3 | 3.207 mg/Nm3 | 15.559 mg/Nm3 |

Model : MultiDetek2
 Serial Number : MD2-67719
 Method : VOC + BTEX

CONCLUSION

Using our MultiDetek2 GC combined with our FID, the air quality monitoring can be performed quickly using the well-known international standards for the detection of VOCs. The unit design is compact, robust and offering all the standard industrial communication protocols.



3.0 APPLICATION NOTE

3.2 INDUSTRIAL GAS



3.0 APPLICATION NOTES

APPLICATION NOTE

LD12-02



Analysis of permanent gases and light hydrocarbons with the PlasmaDetek

The PlasmaDetek is ideal to measure permanent gases and light hydrocarbons in different matrices. Only one detector system is needed to accomplish this task. Such measurement is required in many different applications field: industrial, petrochemical, energy, environmental, etc. The sensitivity, the stability, the ease of start-up and installation make this system very attractive for any users.

PLASMADETEK CONFIGURATION:

The PlasmaDetek is configured with two outputs signal to be able to detect all components. Both argon or helium carrier gas can be used.

- Output 1 : H₂, C₁ to C₄
- Output 2 : O₂, N₂, CO, CO₂


No need of fuel, air, doping gas, methanizer or other devices with the system. This is a stand-alone detector system that requires only carrier gas to make the measurement of each compound.



Figure 1:
▲ PlasmaDetek detector

CHROMATOGRAPHY CONFIGURATION:

To make the measurement of all components described above, figure 2 describes an easy configuration. Only one 10 ports injection valve and one selection valve are used. One RT Molecular Sieve 5A 30m x 0.53mm(column 2) separates H₂, O₂, N₂, CH₄, CO before being measured by the detector. The other column, a RT Alumina Bond 30m x 0.53mm x 10mm(column 1), does the same for the CO₂ and C₁ to C₄.

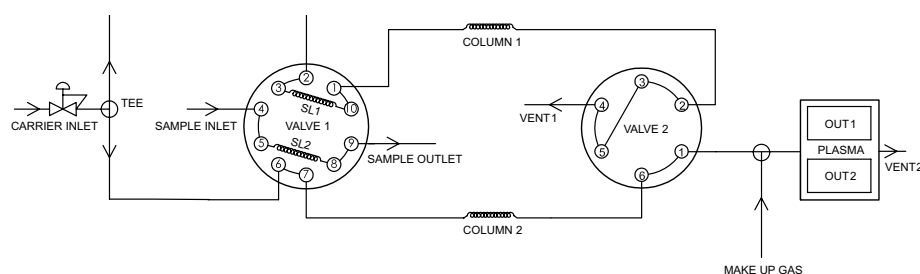

- 1 x 10 ports injection valve
- 1 x 6 ports valve for channel selection
- 1 x RT Alumina Bond 30m x 0.53mm x 10mm (column 1)
- 1 x RT Molecular Sieve 5A 30m x 0.53mm (column 2)
- Argon or helium carrier
- Carrier Flow : 4 cc/min
- Make-up : 60 cc/min
- Detector : PlasmaDetek two outputs

Figure 2: Plumbing configuration for H₂,O₂,N₂,CO, C₁ to C₄ in Helium or Argon

RESULTS AND PERFORMANCE:

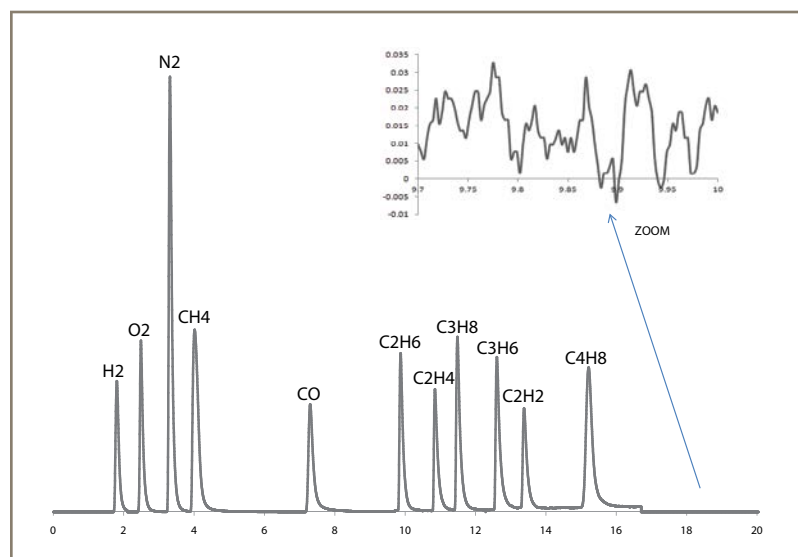


Figure 3 shows the chromatogram obtained from this configuration. The chromatograph uses output 1 to measure H₂ and the HC's and output 2 for the others.

Figure 3: 10ppm H₂ - O₂ - N₂ - CH₄ - CO - C₂H₆ - C₂H₄ - C₃H₈ - C₃H₆ - C₂H₂ - C₄H₈

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | S/N | LOD (ppb) S/N = 3 | LOQ (ppb) S/N = 5 |
|-------------------------------|---------------|-------------|----------|-------|----------------------|----------------------|
| H ₂ | 10 ppm | 342 mV | 0.039 mV | 8769 | 3.4 | 5.7 |
| O ₂ | 10 ppm | 450 mV | 0.039 mV | 11538 | 2.6 | 4.3 |
| N ₂ | 10 ppm | 1142 mV | 0.039 mV | 29282 | 1.0 | 1.7 |
| CH ₄ | 10 ppm | 576 mV | 0.039 mV | 14769 | 2.5 | 4.1 |
| CO | 10 ppm | 282 mV | 0.039 mV | 7230 | 4.1 | 6.9 |
| C ₂ H ₆ | 10 ppm | 402 mV | 0.039 mV | 10307 | 2.9 | 4.9 |
| C ₂ H ₄ | 10 ppm | 330 mV | 0.039 mV | 8461 | 3.6 | 5.9 |
| C ₃ H ₈ | 10 ppm | 442 mV | 0.039 mV | 11333 | 2.6 | 4.4 |
| C ₃ H ₆ | 10 ppm | 426 mV | 0.039 mV | 10923 | 2.7 | 4.6 |
| C ₂ H ₂ | 10 ppm | 274 mV | 0.039 mV | 7025 | 4.3 | 7.1 |
| C ₄ H ₈ | 10 ppm | 366 mV | 0.039 mV | 9384 | 6.4 | 5.4 |

Figure 4: LOQ and LOD calculation

Figure 4 shows the performance of the PlasmaDetek for such components obtained with the configuration described above. Those results and performances depend on the chromatographic system and conditions of operation.

CONCLUSION:

With the PlasmaDetek, we can measure permanent gases and C₁-C₄ with only one detector. This is a very cost effective solution in terms of gas supply, plumbing configuration and time consuming. The performance is indisputable. Application in ppb is now easy to make with such configuration.

Selectivity on some impurities can also be configured in the PlasmaDetek to make Chromatography easier when working on different background or focus on some impurities. Heavier hydrocarbons can also be measured. Please contact LDetek for more information.

APPLICATION NOTE

LD12-03



Analysis of argon in pure oxygen with the PlasmaDetek and ArgoTek

The complexity of measuring argon as impurity in chromatography comes from the fact that typical columns on the market do not separate argon and oxygen. Both elute at the same time making the analysis difficult in low concentration. There are typical techniques for this measurement:

- Using an oxygen trap which involves regeneration procedure with H₂ supply, maintenance, consumable and complex chromatography system.
- Cryogenic configuration where columns need to be used in cold environment which involves complex manipulation.
- Using an online oxygen analyzer in parallel and subtract the oxygen from the measurement of Ar+O₂. But this requires a second analyzer and it is difficult to get an accurate measurement in low concentration.

But the combination of the PlasmaDetek and the ArgoTek column is the ideal solution to measure argon in ppt to %.

PLASMADETEK CONFIGURATION:

The PlasmaDetek is configured with one output signal to be selective to argon. The detector system becomes more sensitive to argon than oxygen by at least a factor of 10.


This is a stand-alone detector system that requires only helium carrier gas to make the measurement. No need of doping gas or other devices to make it selective to argon against oxygen.



▲ PlasmaDetek detector

CHROMATOGRAPHY CONFIGURATION:

This measurement is done by using a simple backflush to vent configuration. The ArgoTek (column 1) is used to separate the argon from oxygen. The argon comes out first of the column and it is sent to the detector. When the argon is out of the ArgoTek, we simply flush outside the oxygen.

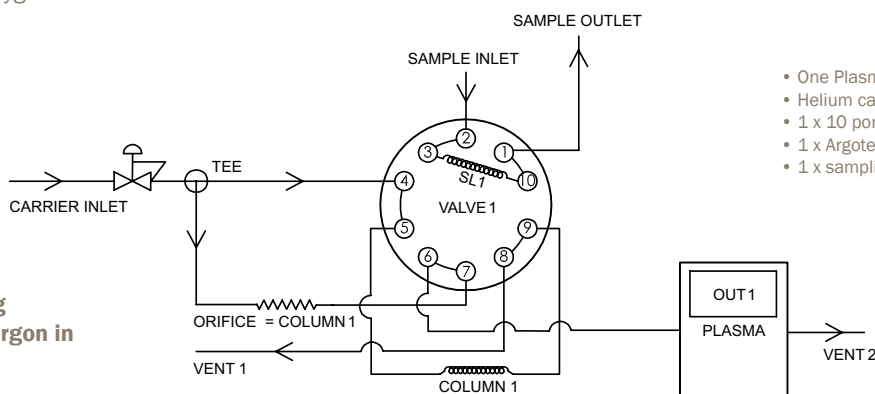

- One PlasmaDetek selective to Argon
- Helium carrier gas: 30cc/min
- 1 x 10 ports diaphragm valve
- 1 x ArgoTek column
- 1 x sampling loop: 20 µl

Figure 1: Plumbing configuration for argon in pure oxygen

RESULTS AND PERFORMANCE:

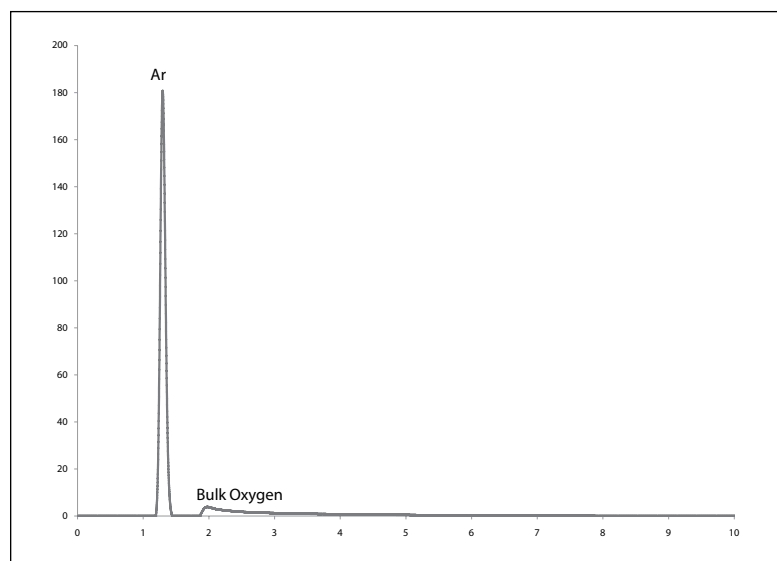


Figure 2 shows the chromatogram obtained from this configuration. The low concentration of argon impurity is easily separated from the oxygen bulk. But more importantly, the selectivity of argon with the detector, gives a better separation of the two compounds, which allows a faster recovery time.

Figure 2: 1 ppm Argon in pure Oxygen

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | S/N | LOD (ppb) S/N = 3 | LOQ (ppb) S/N = 5 |
|-----------|---------------|-------------|----------|------|----------------------|----------------------|
| Ar | 1 ppm | 180 mV | 0.039 mV | 4615 | 0,65 | 1 |

Figure 3: LOQ and LOD calculation

Figure 3 shows the performance of the system obtained with the configuration described above. This PlasmaDetek and ArgoTek combination gives ppt limit of detection with no oxygen interference. Higher concentration, up to %, can be also measured by simply changing the sample volume.

CONCLUSION:

Using the Argotek and PlasmaDetek combination, it becomes very easy to measure this compound compared to other available technologies. This is a cost effective, maintenance free configuration and quick analysis technique avoiding consumables and regeneration procedures that will reduce complexity of the chromatography system.

APPLICATION NOTE

LD12-04



Analysis of nitrogen in hydrogen and oxygen bulk with the PlasmaDetek

Measuring nitrogen as impurity in low concentration is not an easy task. It is mostly the case in hydrogen and oxygen background. Even if the chromatography system is quite efficient, the remaining bulk gas could influence the reading of nitrogen.

The PlasmaDetek, configured to be selective on nitrogen, brings very good result for this measurement. This document will demonstrate how this technology can help to make better analysis on nitrogen with any gas chromatograph system.

PLASMADETEK CONFIGURATION:

The PlasmaDetek has the advantage that it can be configured to be more sensitive on some compounds than the others. This selectivity configuration helps the chromatography to be more effective and easier to setup.

By using proper optical system, the detector becomes selective on nitrogen. No need of doping gas or other devices to make it selective. There is no other such detector on the market that will give this nitrogen selectivity.



▲ PlasmaDetek detector

CHROMATOGRAPHY CONFIGURATION:

A simple backflush configuration is used to make the measurement of N_2 in H_2 or O_2 . Column 1 will initiate a separation of H_2 or O_2 from N_2 and bulk gas will be vented out as much as possible. Before N_2 goes out, the flow is directed to column 2. Both carrier gases can be used: argon or helium.

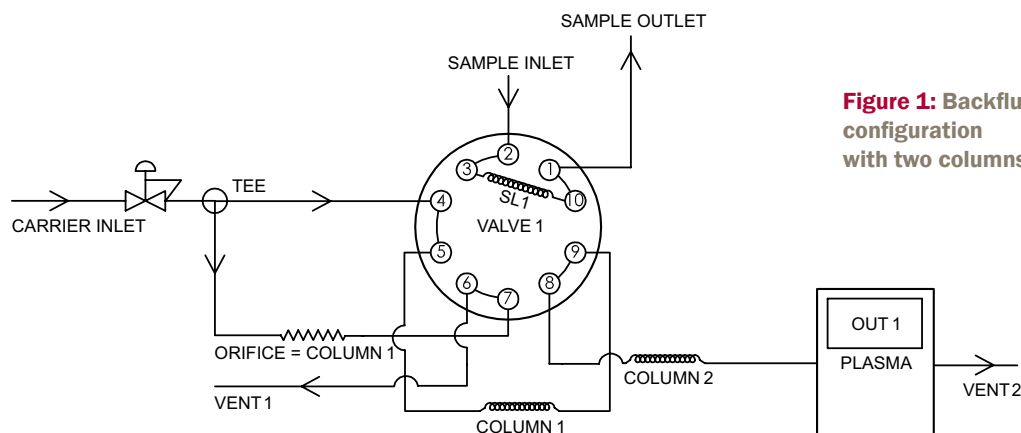


Figure 1: Backflush configuration with two columns

RESULTS AND PERFORMANCE:

Using a 5 ppm standard nitrogen in bulk hydrogen as sample, two chromatograms were generated with the chromatography configuration described above with a helium carrier. **Figure 2** is using a non-selective detector and **figure 3** the PlasmaDetek N₂ selective configuration. As it is clearly shown, the selectivity from the PlasmaDetek is improving the chromatogram. Almost no hydrogen is seen by the detector.

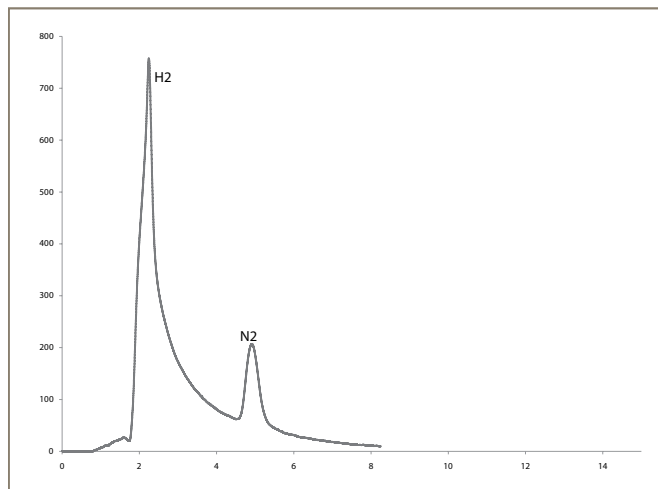


Figure 2: 5 ppm N₂ in H₂ with non-selective detector system

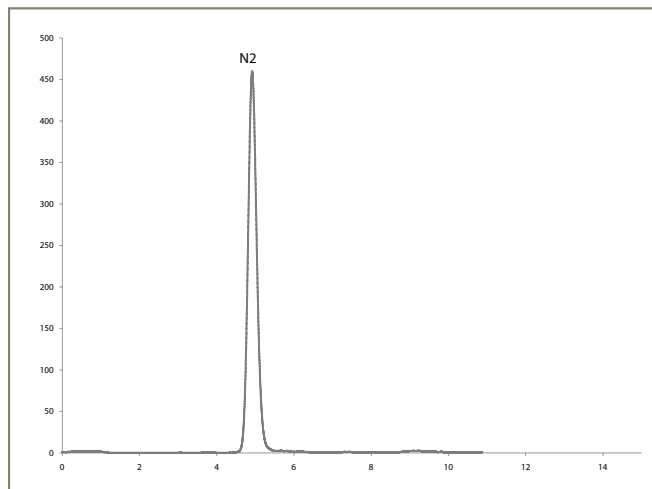


Figure 3: 5 ppm N₂ in H₂ with PlasmaDetek N₂ selective system

Same procedure was done with a standard of 420 ppb nitrogen in oxygen in similar backflush configuration with helium carrier. **Figure 4** and **figure 5** show the comparison with a non-selective detector and the PlasmaDetek N₂ selective configuration. It is also obvious in this case that selectivity helps to have better results and less drifting problem for the peak from remaining bulk.

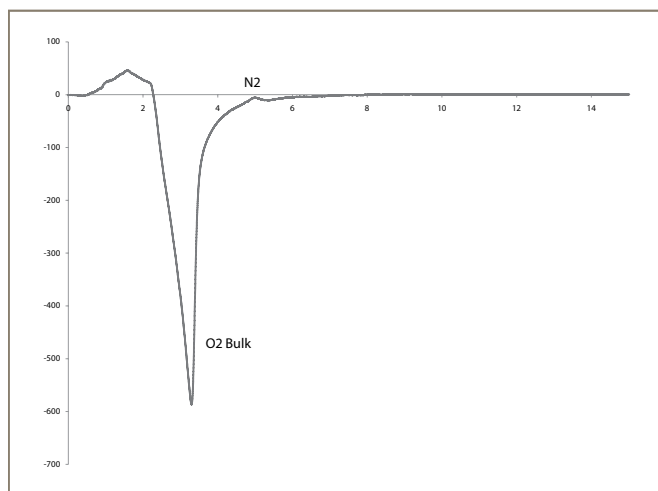


Figure 4: 420 ppb N₂ in O₂ with non-selective detector system


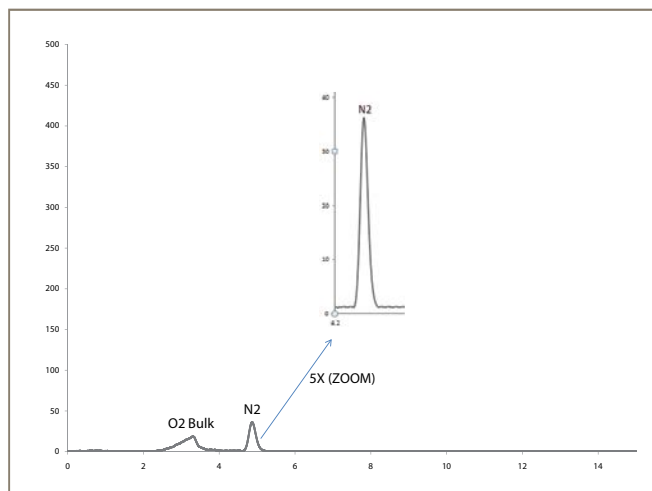


Figure 5: 420 ppb N₂ in O₂ with PlasmaDetek N₂ selective system

Having 79% of nitrogen in air, It is important to ensure that the chromatographic system is leak free. Low concentration nitrogen requires good hardware components to avoid any inboard and outboard leakages. It is even more the case, when measuring in pure H₂ or O₂.



Figure 6: High performance diaphragm valve

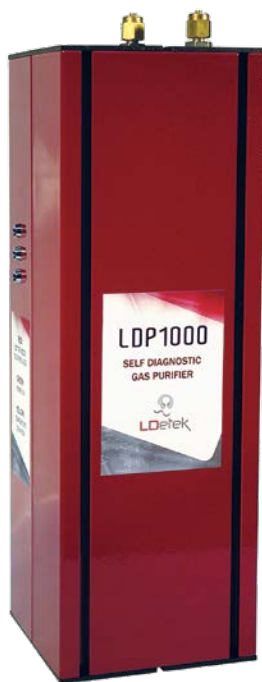

Good quality carrier gas is also mandatory to get analysis in low concentration. With its unique specific design, the LDP1000 noble gas purifier is a cost effective device for any gas chromatograph. It eliminates any contamination problems coming from the gas source.

Figure 7: LDP1000 noble gas purifier

In **figure 8**, we have evaluated the performance of both analysis. With the fact that the PlasmaDetek has a very low noise and a good response on the nitrogen, low concentration can be measured. LOD and LOQ can vary depending on sample volume or condition of operation. < 1 ppb LOD can also be obtained by optimizing the system.

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | S/N | LOD (ppb) S/N = 3 | LOQ (ppb) S/N = 5 |
|----------------------------------|---------------|-------------|----------|-------|----------------------|----------------------|
| N ₂ in H ₂ | 5 ppm | 455 mV | 0.038 mV | 11973 | 1,25 | 2,1 |
| N ₂ in O ₂ | 0.42 ppm | 38 mV | 0.038 mV | 1000 | 1,26 | 2,1 |

Figure 8: LOQ and LOD calculation

CONCLUSION:

This is the ideal configuration to measure nitrogen in different matrices. By having such selectivity, you can reduce analysis time and make fast chromatography. In some cases, consumables such as traps can be avoided. It becomes a cost effective solution, maintenance free system and can give better limit of detection by reducing residual background effect.

The PlasmaDetek can also be configured with multiple selective outputs to allow measurements of different compounds. Please contact LDetek for more information.

APPLICATION NOTE

LD12-06



Increasing argon production with the MultiDetek

Air is composed of nitrogen (78.09%), oxygen (20.94%) and argon (0.934%). To produce pure argon, distillation process separates the air constituent by the use of distillation columns. Such installation on an air separation plant is used for many years.

This separation process is based on vapor pressure of each component. Argon is taken from a low pressure column and introduced in a second column called crude argon. Since argon vapor pressure is close to oxygen, and also between nitrogen and oxygen, its extraction is between those two other components in the low pressure column before being introduced in the second column.

However, the level of nitrogen can be problematic when introducing the extracted gas to the crude argon column. Introducing high volume of nitrogen in the crude argon column will make it stop working. Dumping phenomenon can also arise from the crude argon column.

The extraction of argon in the low pressure column is critical, the goal is to get as much as possible argon and reduce the nitrogen level. Figure 1 shows the vapor pressure of each compound in such column. The maximum level of argon has too much nitrogen. A compromise between argon and nitrogen level must be done.

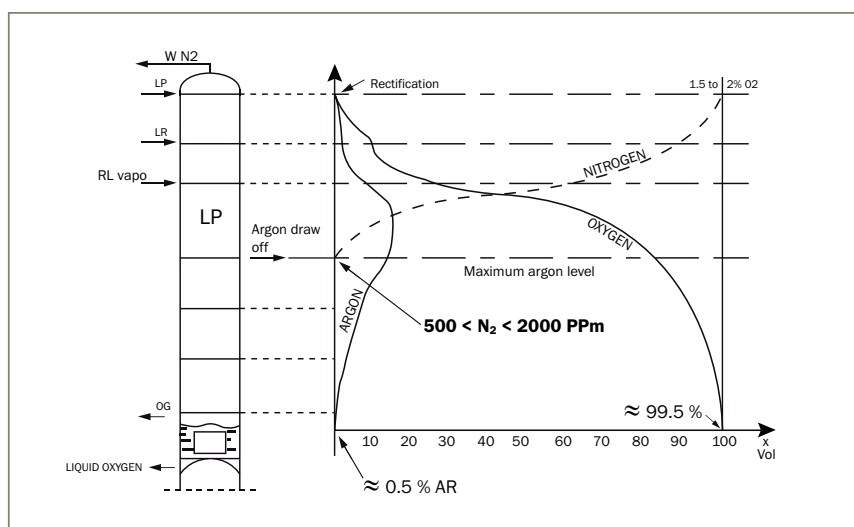


Figure 1

Most of the plants will then take argon at a point where it is safe to keep nitrogen level low. Nitrogen is lower, but argon as well. Oxygen is then relatively high in the crude argon column.

Typical analytical tools are the oxygen and argon measurement. Nitrogen can be approximated and you keep the introduction of nitrogen at minimal level.

Such analysis method gives a safe system, but not optimal argon production can be achieved.

WHAT CAN BE DONE ?

By using proper analytical tool to measure nitrogen level in the low pressure column, the plant can reach the maximum level of argon extraction with the acceptable nitrogen in the crude argon column. The LDetek's MultiDetek is the ideal tool to measure nitrogen in oxygen/argon mixture. By measuring continuously nitrogen in such mixture, optimal argon production can be achieved.

In some cases, increase of 5% argon can be achieved just by measuring nitrogen level accurately.

The MultiDetek can be interfaced with any acquisition system on ASU. Analog signal or digital signal can be provided. Ethernet connection is also available.

Such analyzer is easy to operate with its user friendly interface and can operate 24/24 to ensure extraction is well tuned up.

Such MultiDetek is using the PlasmaDetek technology with nitrogen selectivity. This avoids any oxygen trap consumable.



▲ MultiDetek



PlasmaDetek detector ▲

CONCLUSION:

The pay back of such analytical tool is fast. It will operate for many years and gives optimal efficiency of any argon production plant. The combination of MultiDetek platform with the PlasmaDetek technology is a reliable, efficient and accurate system that any plant is looking for.

APPLICATION NOTE

LD12-07



Analysis of Neon-Hydrogen-Argon-Krypton-Nitrogen with the PlasmaDetek & the HSR-Etek column

The analysis of Neon, Hydrogen, Argon, Krypton and Nitrogen by chromatography has always been problematic. The bad separation and the poor sensitivity for the analysis of these impurities are the reasons that make it complicated to realize. Even with the use of capillary columns, cryogenic system and/or hydrogen trapping system, the analysis of low ppb of these impurities cannot be performed in one run. Furthermore, the detectors available in the industry have some sensitivity limitation. It is then very difficult to measure low ppb for the mentioned impurities especially for Neon with the existing technologies.

LDetek has then developed a method for the analysis of Neon, Hydrogen, Argon, Krypton and Nitrogen. Using the PlasmaDetek system and the HSR-Etek column, the low ppb analysis without any interference can be successfully realized using a simple injection.

PLASMADETEK SYSTEM:

The PlasmaDetek can be configured in a non selective or in a selective mode depending of the lowest detection limit requested and the interference gases. Using its selective mode, the response ratio between the analyte of interest and the interference gases will be increased. The detector can then be very sensitive to the Neon, Hydrogen, Argon, Krypton and Nitrogen without being affected by background gases or interference gases.



Figure 1: PlasmaDetek detector

This is a stand-alone detector system that requires only helium or argon carrier gas to make the measurement. No need of doping gas or other devices. By using argon as carrier gas, the analysis of neon and argon cannot be realized.

CHROMATOGRAPHY CONFIGURATION:

This measurement is done by using a simple injection (see figure 2). The sample is injected through the HSR-Etek column and then goes directly to the PlasmaDetek inlet port. The carrier flow rate must be regulated at 30sccm and maintained stable. The column temperature must operate at 45Celsius until minute 4. The column temperature is then ramped up to 90Celsius at 10Celsius/minute. Using the temperature ramping mode, the analysis of Krypton and Nitrogen can be included in less than 16 minutes.

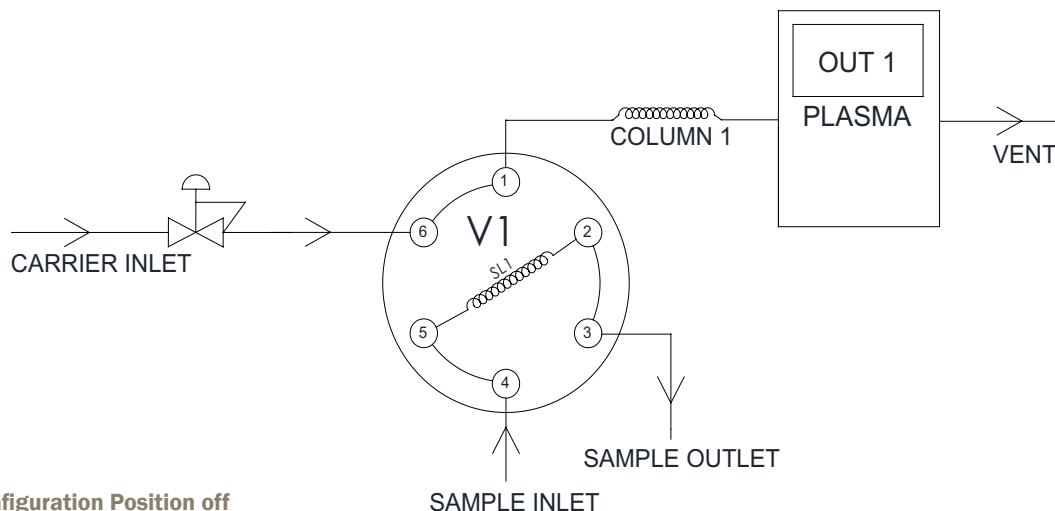


Figure 2: Configuration Position off

RESULTS AND PERFORMANCE:

Figure 3 shows the chromatogram obtained from this configuration.

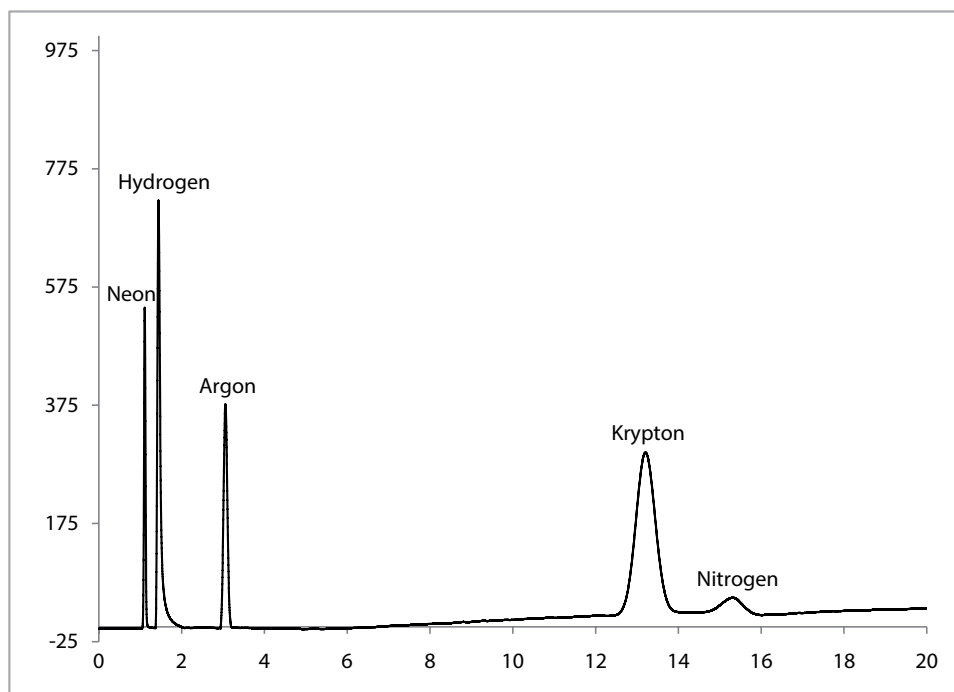


Figure 3: Mixture 4ppm Neon, 5ppm Hydrogen, 1ppm Argon, 4ppm Krypton, 0.5ppm Nitrogen in balance Helium

Figure 4 shows the performance of the system obtained with the configuration described above. The PlasmaDetek and HSR-Etek combination gives the possibility to achieve low ppb limit of detection with good resolution for Neon/Hydrogen, Argon/Oxygen and Krypton/Nitrogen using a simple injection. Higher concentration, up to %, can be also measured with the same system.

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | S/N | LOD (ppb) S/N = 3 | LOQ (ppb) S/N = 5 |
|-----------|---------------|-------------|----------|-------|----------------------|----------------------|
| Neon | 4 ppm | 562 mV | 0.049 mV | 11469 | 1.04 | 1.74 |
| Hydrogen | 5 ppm | 756 mV | 0.049 mV | 15428 | 0.97 | 1.62 |
| Argon | 1 ppm | 381 mV | 0.049 mV | 7775 | 0.39 | 0.64 |
| Krypton | 4 ppm | 341 mV | 0.049 mV | 6959 | 1.72 | 2.87 |
| Nitrogen | 0.5 ppm | 38 mV | 0.022 mV | 1727 | 0.86 | 1.45 |

Figure 4: LOQ and LOD calculation

PLASMADETEK SELECTIVITY:

Using its selectivity, the PlasmaDetek gives the advantage of being very sensitive to desired impurities only. See below an example of analysis of 2ppm Krypton and 4ppm Nitrogen in a balance of Oxygen using HSR-Etek column.

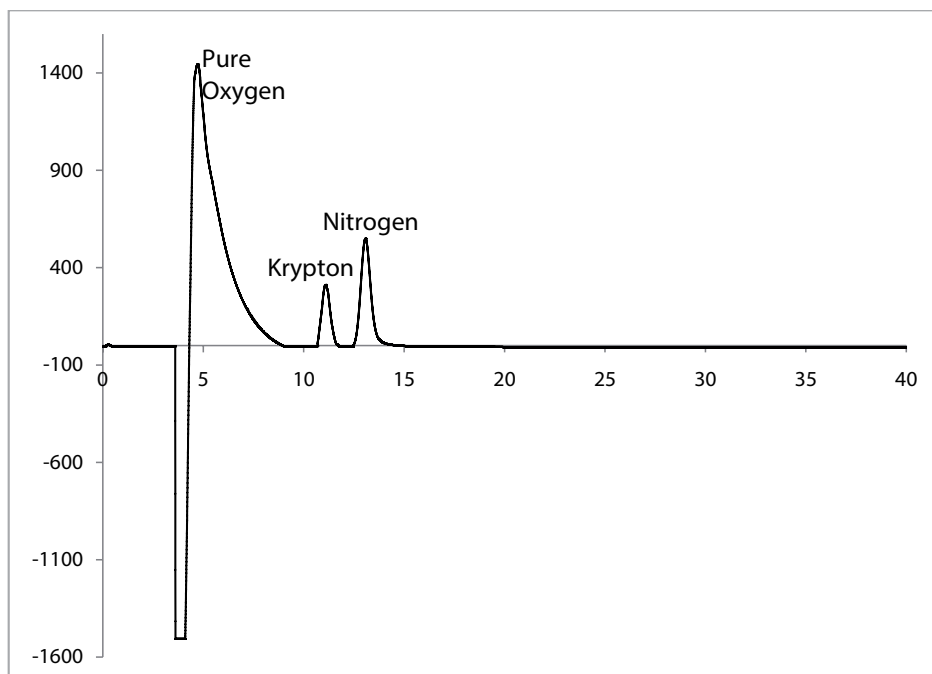


Figure 5: Mixture 2ppm Krypton, 4ppm Nitrogen in balance Oxygen

CONCLUSION:

Using the combination of the PlasmaDetek and the HSR-Etek column, the analysis of Neon, Hydrogen, Argon, Krypton and Nitrogen becomes an easy task. A simple injection through the HSR-Etek column and to the PlasmaDetek allow to measure ppb, ppm or percentage level of the mentioned compounds. This is a cost effective, maintenance free system and quick analysis technique avoiding consumables and regeneration procedures that will reduce complexity of the chromatography system.

APPLICATION NOTE

LD12-09



Hydrocarbons measurement for Oxygen production using PlasmaDetek & Multidetek-2



Oxygen is one of the basic chemical elements. In its most common form, oxygen is a colorless gas found in air. It is one of the life-sustaining elements on Earth and is needed by all animals. Oxygen is also used in many industrial, commercial, medical, and scientific applications. It is used in blast furnaces to make steel, and is an important component in the production of many synthetic chemicals, including ammonia, alcohols, and various plastics. Oxygen and acetylene are combusted together to provide the very high temperatures needed for welding and metal cutting.

The most common commercial method for producing oxygen is the separation of air using either a cryogenic distillation process or a vacuum swing adsorption process. Nitrogen and argon are also produced by separating them from air. The figure 1 represents a common cryogenic distillation process for producing oxygen.

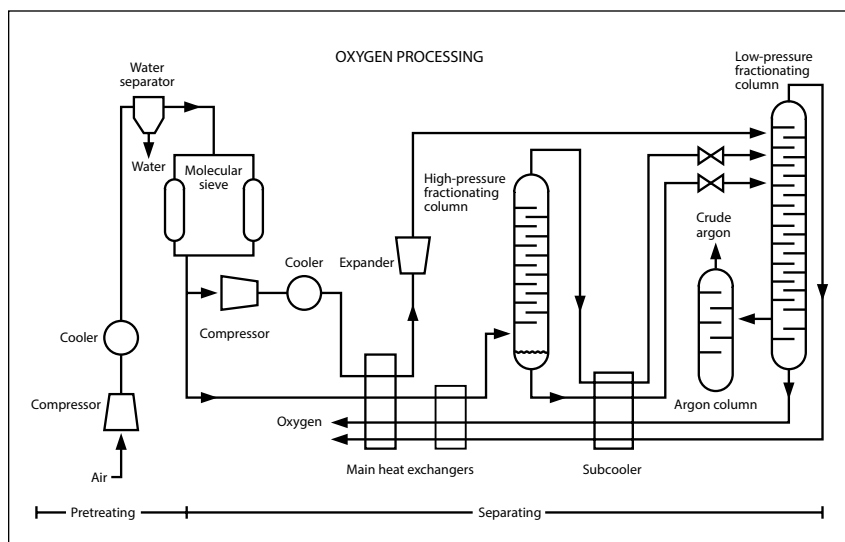


Figure 1: Diagram of a cryogenic distillation process

Because this process utilizes an extremely cold cryogenic section to separate the air, all impurities that might solidify—such as water vapor, carbon dioxide, and certain heavy hydrocarbons—must first be removed to prevent them from freezing and plugging the cryogenic piping what could result to an hazardous situation. The removal of hydrocarbons is also very important to avoid any problem in the subsequent air distillation that could lead to explosion.

Then, the operation of cryogenic distillation air separation units must be monitored by automatic analytical instruments. As a result, their output is consistent in quality and ensures safety of the site. Periodic sampling and analysis of the final product ensures that the standards of purity are being met. A good analytical instrument is then necessary to monitor the various sampling points of the air separation unit.

LDETEK SOLUTION:

With its integrated plasma technology, The LDetek's Multidetek-2 becomes the ideal tool to measure the purity of the oxygen. Its capability to monitor the hydrocarbons level from ppb level up to high ppm level using its plasma detector gives the ideal alternative to the standard use of a FID detector. With the use of the plasma for monitoring the hydrocarbons, there is no more need of using Fuel/Air mixture additionally to the carrier gas. The Multidetek-2 and its plasma only require argon carrier gas. It is then a big advantage since there is no handling and storage of hydrogen anymore on site. Moreover, the use of argon as carrier gas is also a great benefit because the argon is low cost and is already produced and available on any air separation plant.

The use of the Multidetek-2 for monitoring hydrocarbons level in oxygen production is also the ideal tool for a safety point of view. It is critical to have a reliable unit able to monitor 24/7 basis the level of hc's in oxygen on ASU. Being very sensitive to hydrocarbons, including C₂H₂ which is the most critical component, the Multidetek-2 becomes the best tool to use.

The Multidetek-2 unit can have multiple configurations to allow the measurement of different sampling points of the air separation unit. The monitoring of quality control at the end of oxygen production process can then be easily realized with a configuration allowing low ppb detection. This will ensure an accurate reading necessary for producing high quality grade oxygen. Using the same unit, a higher scale configured for high ppm measurement necessary to monitor the different sampling points of the crude material is also integrated in the unit.

An analysis example of hydrocarbons measurement in pure oxygen appears on the figure 2.

The Multidetek-2 can be interfaced with any acquisition system on ASU. Analog signal or digital signal can be provided. Ethernet connection is also available for remote control. Such analyzer is easy to operate with its user friendly interface and can operate 24/24 to ensure good oxygen production. For this application, such Multidetek-2 is using the PlasmaDetek technology with its hydrocarbons selective detector. This avoids any consumable.

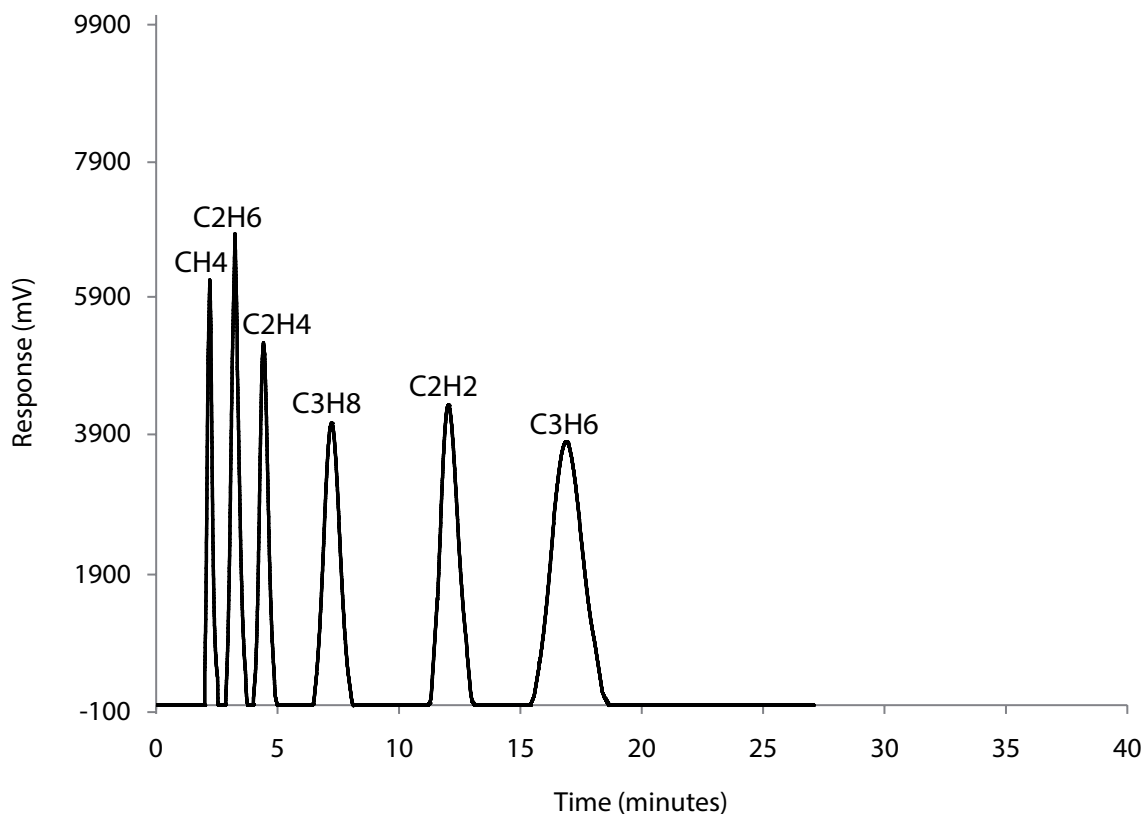


Figure 2: Chromatogram of hydrocarbons in pure oxygen using PlasmaDetek and Multidetek-2

MORE POSSIBILITIES:

A good return on investment can be also realized by configuring the same instrument for more components:

The analysis of CO₂ and any other permanent gases or sulfurs impurities can be added to the same instrument. Even more, the Multidetek-2 also offers the possibility to have multiple background gas configurations. The analysis of argon and nitrogen purity can then be added to the same unit.

One more time, with the simple use of argon as carrier gas and its integrated plasma, the Multidetek-2 can handle multiple measurements in multiple background gases.

CONCLUSION:

The pay back of such analytical tool is fast. It requires only argon as carrier gas which is available at low cost on any air separation plant. There is no more need of handling and storing hydrogen what is usually more expensive due to the need of safety sensors and procedures on site. The PlasmaDetek use in the Multidetek-2 is maintenance free and is a clean detector. It requires no cleaning procedure. The Multidetek-2 will operate for many years and gives optimal efficiency of any oxygen production plant.

The combination of Multidetek-2 platform with the PlasmaDetek technology is a reliable, efficient and accurate system that any plant is looking for.

APPLICATION NOTE

LD13-01



Analysis of UHP Hydrogen production using Plasmadetek-2 & compact GC Multidetek-2



◀ PlasmaDetek2



▲ MultiDetek2

The high purity hydrogen production demand is rising quickly and the need of measuring low ppb trace in a quick analysis run is then required. Most of the GC technologies available on the market use the same methods for years which required quite complex systems. Those systems require the use of different detectors to cover the application and a complex chromatograph configuration what make the price of such system increasing. The complexity of the chromatograph operations, the long analysis time and the limitations to achieve low ppb measurement are often faced.

LDETEK SOLUTION:

With its integrated plasma technology, The MultiDetek-2 from LDetek becomes the ideal tool to measure the hydrogen purity. Its capability to monitor the permanent gases and hydrocarbons from ppb level up to high ppm level using only one plasma detector gives the ideal solution. In comparison to the existing method, the PlasmaDetek-2 gives the advantage of being selective to the desired impurities and then block the interference coming from the matrix gas. In the case of UHP hydrogen production, measuring low ppb traces of O₂ and N₂ is complex since their elution time is very close to the hydrogen matrix.

Then, to allow the analysis of O₂ and N₂, relatively long molecular sieve columns are required in combination with multiple valves for flushing out the hydrogen gas. In some cases, a hydrogen trapping module may be necessary. It then increases the cost of the system and extends the analysis time. Peaks shape can be also affected with the use of longer columns.

With the PlasmaDetek-2, a simple system having one valve and one Molecular Sieve column is required. The detector is configured with two sensors to measure O₂ and N₂ respectively in selective mode. Refer to Figure 1 for the configuration drawing. Going this way, the analysis time can be reduced, the sensitivity increased and it gives an easy to use system with no consumable or maintenance required.

An analysis example of impurities O₂ & N₂ in a hydrogen sample, using a standard ionization detector in combination with the same configuration that appears on Figure 1, has been used to generate the chromatogram that appears on Figure 2. We can clearly see the interference of the hydrogen over the traces O₂ and N₂. The hydrogen matrix interference overlapping the traces O₂-N₂ will be amplified when going lower at low ppb level and it will become not possible to measure the impurities without using another techniques requiring more long columns, additional valves and H₂ trap.

At the opposite, on Figure 3 appears a chromatogram of traces O₂ and N₂ with the use of the PlasmaDetek-2 using its selective mode. It is clearly demonstrated that the selectivity gives an important benefit that makes such type of analysis possible with a simplified chromatography method demonstrated on Figure 1.

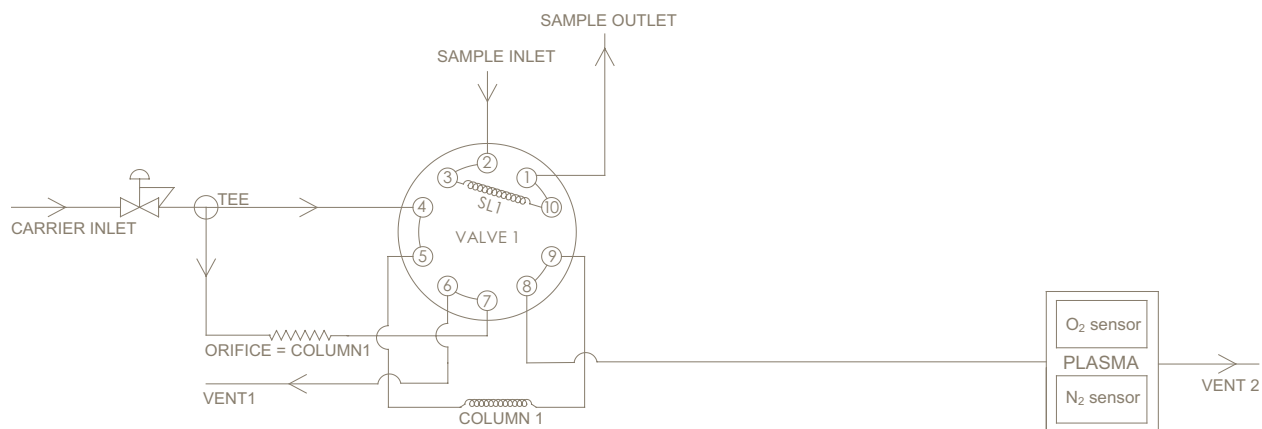


Figure 1: Configuration used for measuring traces O₂ - N₂ in matrix hydrogen. (One additional non selective sensor can be added to the same plasma for measuring traces CH₄ - CO with the same channel.)

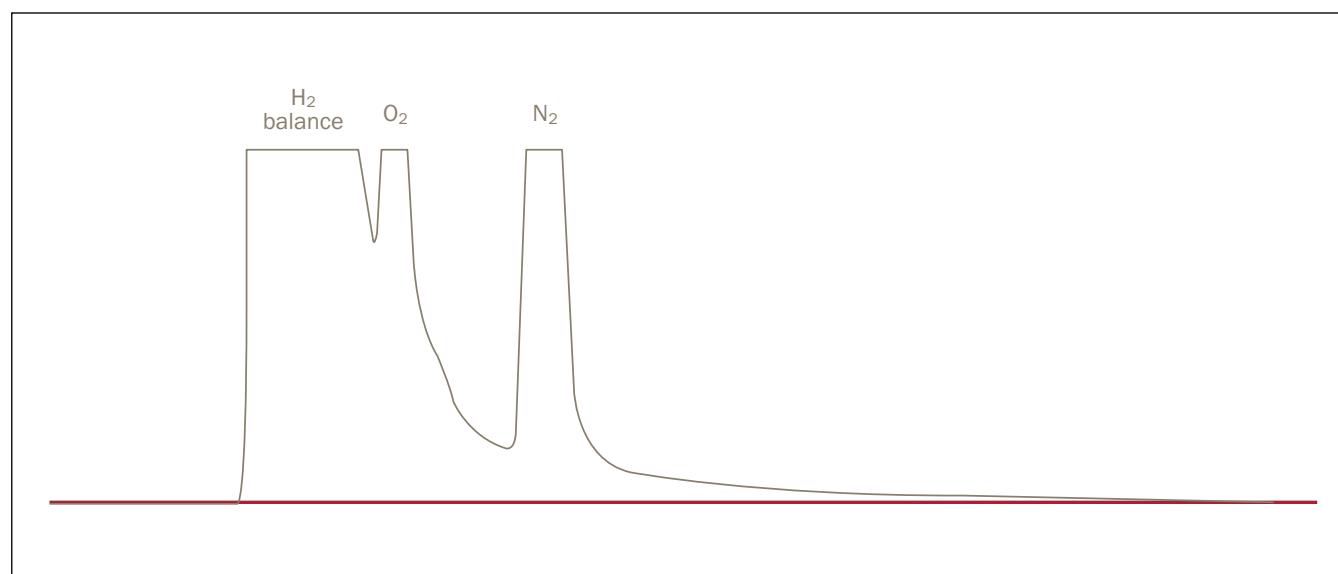


Figure 2: Chromatogram of traces O₂ - N₂ in a hydrogen matrix using a conventional non selective ionization detector.

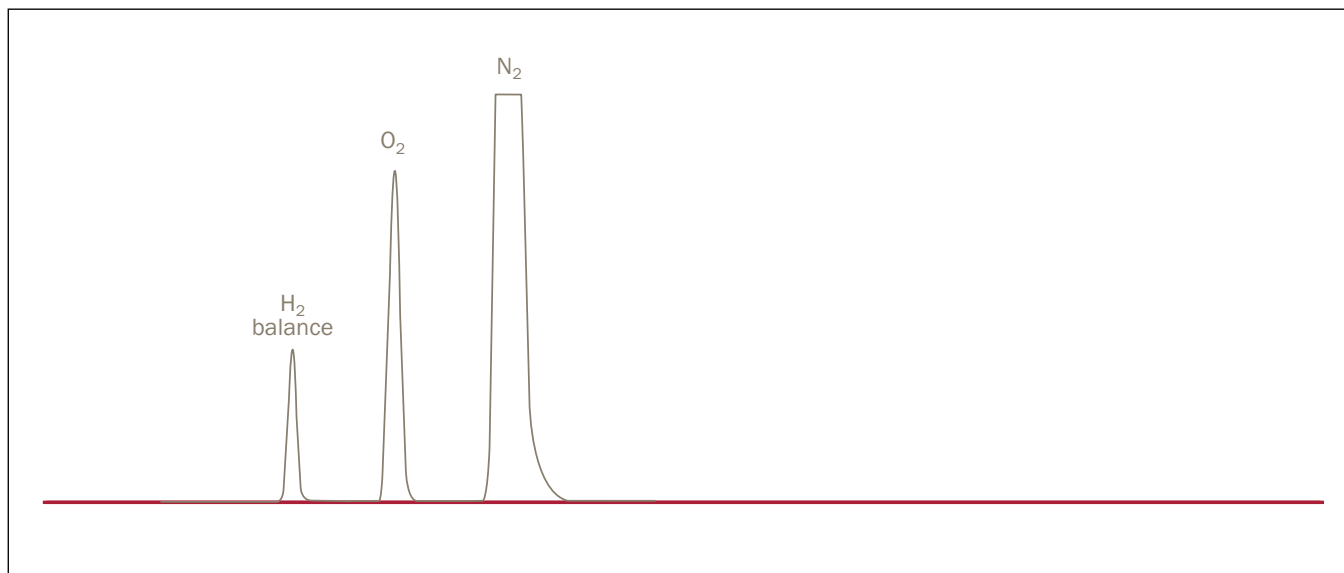


Figure 3: Chromatogram of traces O_2 - N_2 in a hydrogen matrix using PlasmaDetek-2 in a selective mode.

ARGON AS CARRIER GAS:

Since the PlasmaDetek-2 can be used with argon as carrier gas, you get some more advantages over conventional ionization detector.

Operation cost of the system is reduced compared to system that requires helium. With the helium shortage worldwide and its price increasing constantly, the use of argon becomes the best alternative to keep same sensitivity level.

Furthermore, in the case when argon as impurity is not required, the use of argon as carrier gas simplifies the chromatography. With conventional ionization detector using helium, the Ar will interfere with O_2 measurement. If Ar measurement is needed, the PlasmaDetek-2 can also be used and configured accordingly to get Ar and O_2 separately (see application note LD12-3).

COMPLETE SOLUTION:

Using the PlasmaDetek-2 as detector and the MultiDetek-2 as compact GC platform, the same instrument can be used to measure additional components in hydrogen matrix.

The analysis of traces Ar-Ne- CH_4 -CO- CO_2 and hydrocarbons can be added to the same instrument just by configuring additional channels to the compact GC MultiDetek-2. Some other sensors can be added to the same plasma for the added impurities. No needs of additional detectors like FID or consumables are required.

CONCLUSION:

The pay back of such analytical tool is fast. It requires only argon as carrier gas which is available at low cost on any air separation plant. The PlasmaDetek-2 used in the MultiDetek-2 is maintenance free and is a clean detector. It requires no cleaning procedure. The compact GC MultiDetek-2 will operate for many years and gives optimal efficiency of any hydrogen production plant.

The combination of MultiDetek-2 compact GC with the PlasmaDetek-2 technology is a reliable, efficient and accurate system that any plant is looking for.

APPLICATION NOTE

LD13-02



Measurement of nitrogen in a mixture of Argon/Oxygen (crude argon) online with the LD8000-Crude



▲ LD8000

The measurement online of nitrogen in UHP argon is widely used and the LD8000 is now a reference in such measurement. However when measuring crude argon with a few % of oxygen, the conventional online instruments are not suitable anymore. Such crude liquid argon (also called CLAR) needs to be analyzed in many cases to be sure the level of nitrogen is within the specification either as a final product for steelmaking or welding applications or before being purified to produce UHP argon. Good analytical tool is then required to have a good process control. The use of Gas Chromatograph (GC) has been widely used to measure this nitrogen level. Even if GC is giving good and accurate results, the analysis time is quite long. In many cases the response time is too long to take proper action if the nitrogen goes too high in concentration. A few minutes are required to get the analysis results and this delay can bring a lot of problems to the plant if it increases suddenly.

The need of having an online instrument with a few second response time has been desired for a long time. The LD8000-Crude can now achieve this task and give a better process control for any plant or application that needs to measure N₂ in the Crude Argon having up to 5% oxygen.

DESIGN:

The LD8000-Crude is still using the unique PlasmaDetek technology, but incorporated in a special design, it makes possible to have this plasma emission detector (PED) working with up to 5% oxygen. Common PED cannot create a stable plasma with oxygen. The interference and instability of the plasma is a big challenge. But LDetek has developed a method and a design to have such argon micro-plasma being able to measure from ppb to % of nitrogen with up to 5% oxygen.

A specific algorithm has been developed and implemented in the microcontroller unit giving a linear and accurate measurement of nitrogen.

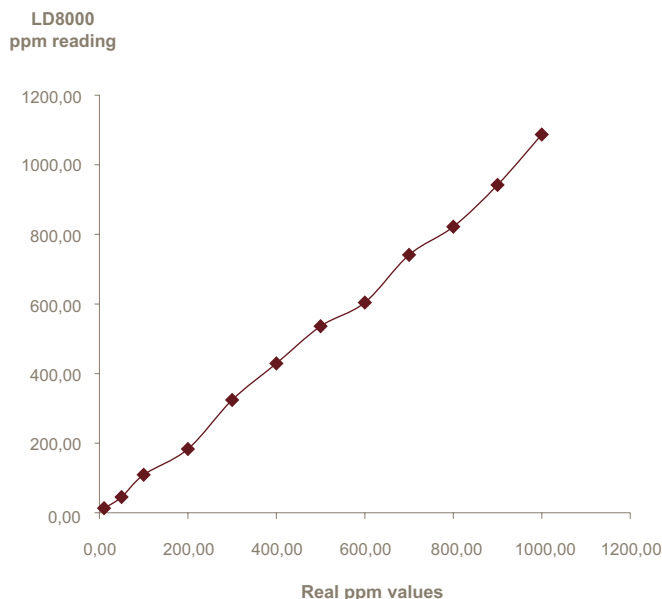


Figure 1 : LD8000 Crude linearity 0-1000 ppm

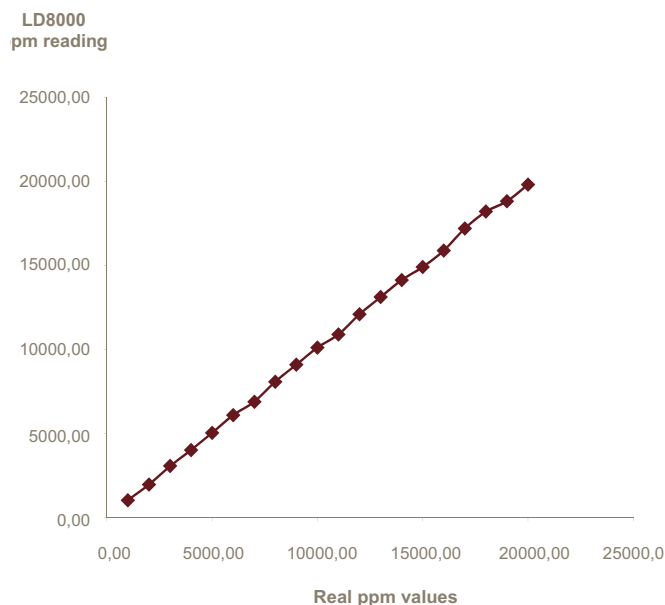


Figure 2 : LD8000 Crude linearity 0-20000 ppm

With the 3U cabinet, this instrument can fit in any rackmount cabinet or plant installation. No need of carrier gas and external consumable parts like purifier or oxygen scrubber. Only sample is needed to provide this quick measurement.

The micro controller unit inside combined with the LCD display provide a user friendly interface easy to operate. But it also gives all features that such instrument needs on a plant (dry contact relay for range ID, status contact for error monitoring, 4-20 mA output for value reading, auto-resolve alarms system, etc).

RESPONSE TIME:

The response time for such application is critical. The use of a gas chromatograph has been widely used and it gives good results, however the analysis time can be as high as 5-6 minutes. It is very important, in most of such applications, to have a quick response time to act quickly on the process when the level of nitrogen goes too high.

Using the LD8000-Crude, you get a response time of a few seconds ($T_{90} < 20$ sec) with a measurement of a few ppm. With the 4-20mA output signal, the process plant can track the level of nitrogen continuously. If serial communication is required, this instrument can send and be controlled by such communication port.

HIGHER OXYGEN CONTENT:

For measurement of N₂ in Crude Argon containing more than 5% Oxygen level, the LD8000-Crude instrument can be configured to achieve such task. The unique plasma detection system (PED) for Crude Argon measurement stays the same. An additional module for sample gas treatment is added to the instrument, which makes the detection of N₂ in Crude Argon having more than 5% Oxygen possible.

For more information and details, do not hesitate to contact LDetek.

APPLICATION NOTE

LD14-01



Light hydrocarbons measurement with the *PlasmaDetek-E system with nitrogen carrier gas and the MultiDetek-2.



◀ PlasmaDetek-E



MultiDetek-2 ▲

Hydrocarbons are ones of the most important impurities measured in the industry. Whether it is for safety, quality control, special gases or any other needs, those compounds are everywhere.

The techniques used to measure those compounds have been the same for quite some years. The FID (Flame Ionization Detector) is surely the most widely used in the industry. The selectivity for hydrocarbon (HC) gives the simplicity desired for all gas chromatograph (GC) users. However the need of air, but mostly hydrogen as fuel is the drawback of this technology. Many plants and laboratories would like to get rid of the hydrogen as potential explosive gas. All the safety feature (valves, extra lines, procedures, etc) are required and brings extra cost and manpower.

Other technologies to measure the light hydrocarbon have arisen over the years. The Discharge Ionization Detector (DID) brought a solution without the need of air and fuel. Working on helium carrier gas, the safety problem was resolved. However the selectivity is not present and the need of helium is required. With the worldwide shortage of helium and its increasing price constantly, it becomes a more costly solution not attractive enough for gas chromatograph developer.

Another solution was brought to the market: the Plasma Emission Detector (PED). With its advantage to work in helium and argon carrier gas, this solution becomes more attractive because of argon pricing. It is also produced and available anywhere in the world. Furthermore, the PED has some selectivity against some other gases, not completely, but enough to make the GC user life easier. However, there is no selectivity for HC against many compounds, including air and oxygen. Measuring HC in a stream of Oxygen or Air is very important in Air Separation Unit (ASU). There is also a lack of sensitivity in some case by using argon as carrier. Measuring C₂H₂ for a ASU plant is critical and it needs to be measured in low concentration.

LDETEK SOLUTION:

With the patent pending PED system (PlasmaDetek-E) provided by LDetek, it is now possible to improve and overcome the drawbacks of other available technologies.

NITROGEN CARRIER GAS:

First of all, such system can work with argon and helium, but with nitrogen carrier as well. Nitrogen is a low cost and inert gas that makes it very attractive to use in a GC. Air contamination and leak are not much problematic as it is with other PED systems. Typical PED detector can be sensitive, but it needs to be in a very pure environment. A little leak or contamination can compromise the whole measurement. The recovery time from column changes and GC start-up is then extremely fast with the PlasmaDetek-E using nitrogen as carrier gas.

A simple injection configuration has been used to inject different matrices to evaluate the response and selectivity over CnHm components. Figure 1 shows such configuration with the PlasmaDetek-E system.

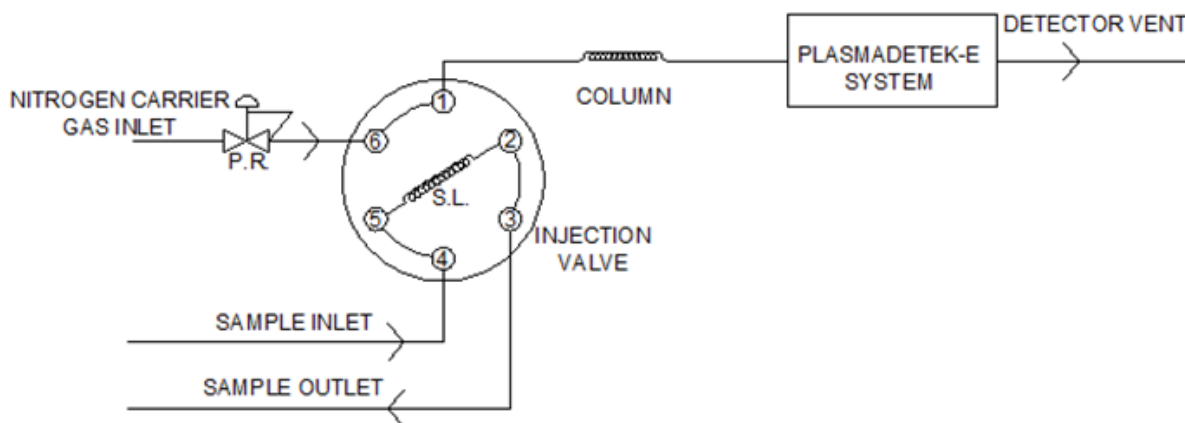


Figure 1

SENSITIVITY:

To evaluate the response and sensitivity, injection of CnHm impurities in Argon balance has been used. Figure 2 shows the chromatogram with indication of each compounds detected by the PlasmaDetek-E.

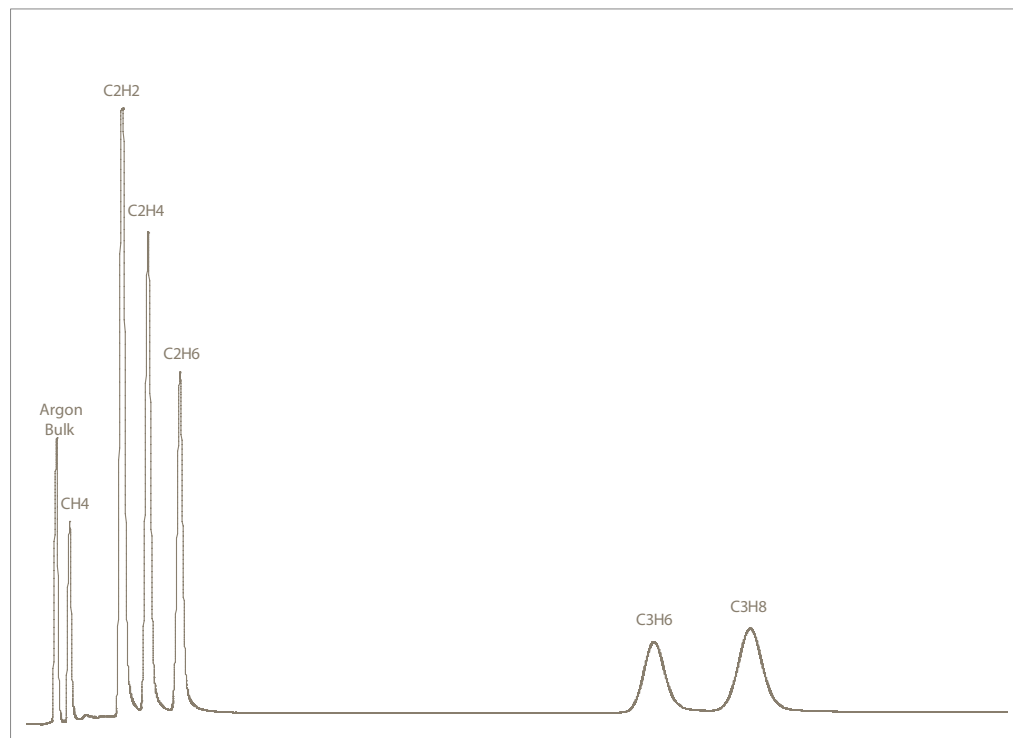


Figure 2

By evaluating the noise level and peak height, LDL for each compounds can be evaluated by considering the limit as 3 times the noise level. Figure 3 is showing the results of this analysis.

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-------------------------------|---------------|-------------|--------|----------------|
| CH ₄ | 9.56 ppm | 1300 mV | 1.5 mV | 11 ppb |
| C ₂ H ₂ | 10.50 ppm | 4800 mV | 1.5 mV | 3 ppb |
| C ₂ H ₄ | 9.96 ppm | 3100 mV | 1.5 mV | 4 ppb |
| C ₂ H ₆ | 10.80 ppm | 2300 mV | 1.5 mV | 7 ppb |
| C ₃ H ₆ | 10.40 ppm | 460 mV | 1.5 mV | 33 ppb |
| C ₃ H ₈ | 9.20 ppm | 560 mV | 1.5 mV | 24 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

Figure 3

By using different injection volume and/or chromatographic configuration, even lower LDL could be obtained. However, by comparing with same the chromatographic condition than a traditional argon PED, LDL is improved by a factor of about 10 times with the PlasmaDetek-E. It is even more the case for C₂H₂, where it is about 100 times more sensitive.

SELECTIVITY:

By using the same configuration as figure 1, air has been injected to evaluate the interference that can occur with the first hydrocarbon content out of the column, which is CH₄. Figure 4 shows an injection with the PlasmaDetek-E using argon as carrier gas optimized for the best response to Hydrocarbon in air. It is obvious that the CH₄ is influenced by the residual air. In such cases, extra valves or hardware would be required to achieve possible measurement.

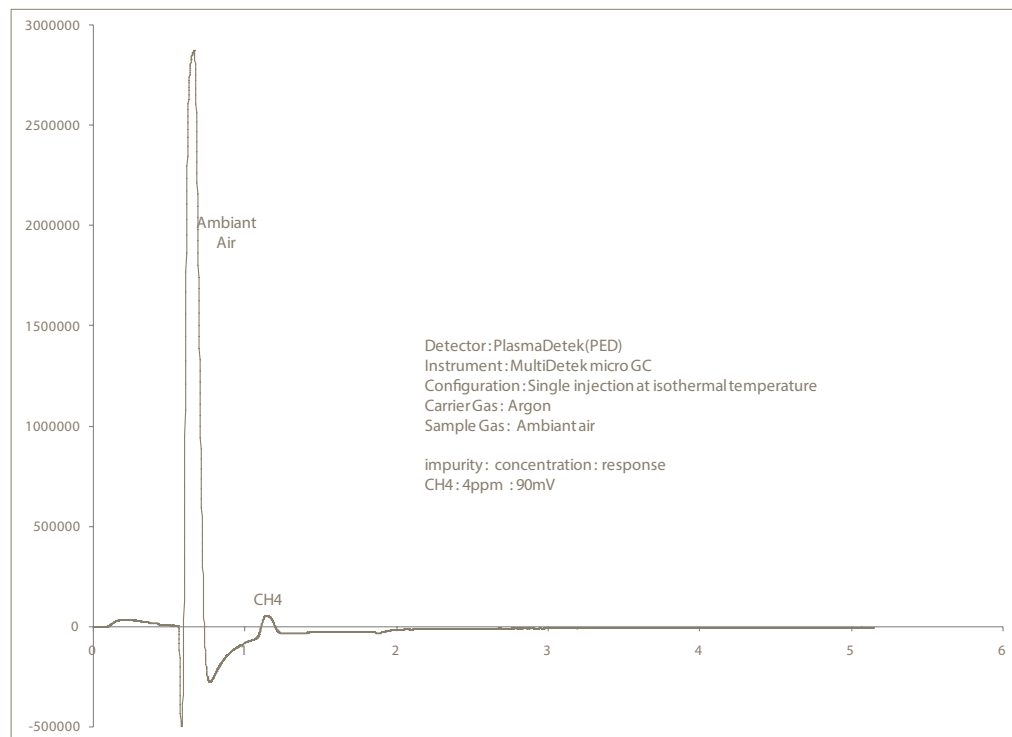


Figure 4

Figure 5 is using the same system with nitrogen carrier gas. Air response has been reduced considerably compared to argon carrier gas. Only with a simple injection configuration will make the CH₄ detectable.

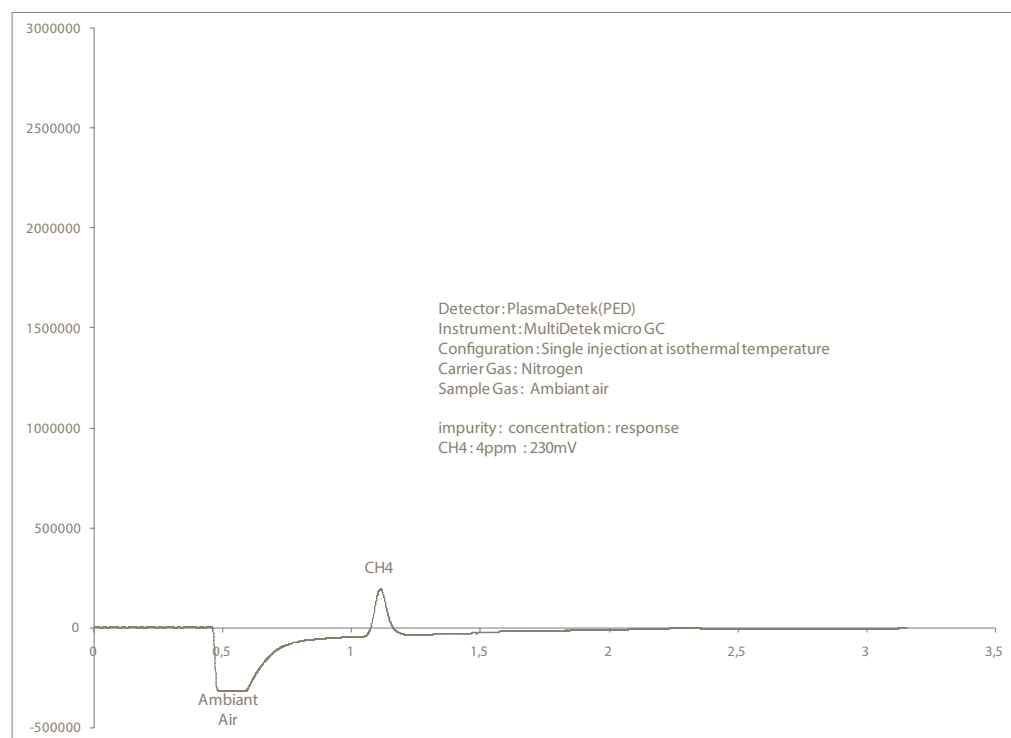


Figure 5

CONCLUSION:

With the PlasmaDetek-E system, lights hydrocarbon measurement is now safe and easy. No fuel, no air and no safety features needed, only nitrogen carrier gas.

It is also the lowest operation cost solution, but the sensitivity is not compromised where low ppb can be achieved.

APPLICATION NOTE

LD15-08



Measurement of impurities in UHP helium using MultiDetek2 and PlasmaDetek2



▲ MultiDetek2

▲ PlasmaDetek2

Helium is a widely used gas in different needs such as cryogenics, pressurizing and purging, welding, controlled atmospheres, leak detection and breathing mixtures. Having a good analytical tool is mandatory to ensure the required purity of helium.

The most popular technique for UHP helium analysis is to detect impurities by gas chromatography. But some detection technologies within the GC do not provide the desired detection limit or can simply not measure some critical impurities like neon.

LDETEK SOLUTION:

The MultiDetek2 combined with the PlasmaDetek2 detector provides an ideal solution to measure the different impurities in UHP helium. With the PlasmaDetek2, based on plasma emission detection, impurities in low ppb can be detected, even neon. The discharge ionisation detector (DID) can simply not detect neon or require a different operation mode to achieve ppm measurement. Which is not enough for many helium producers where they need lower detection limit in ppb. The operation is also more complex since the ionisation voltage needs to be changed when neon has to be detected.

LDetek solution gives an easy system to use with very good sensitivity. Figure 1 shows such configuration.

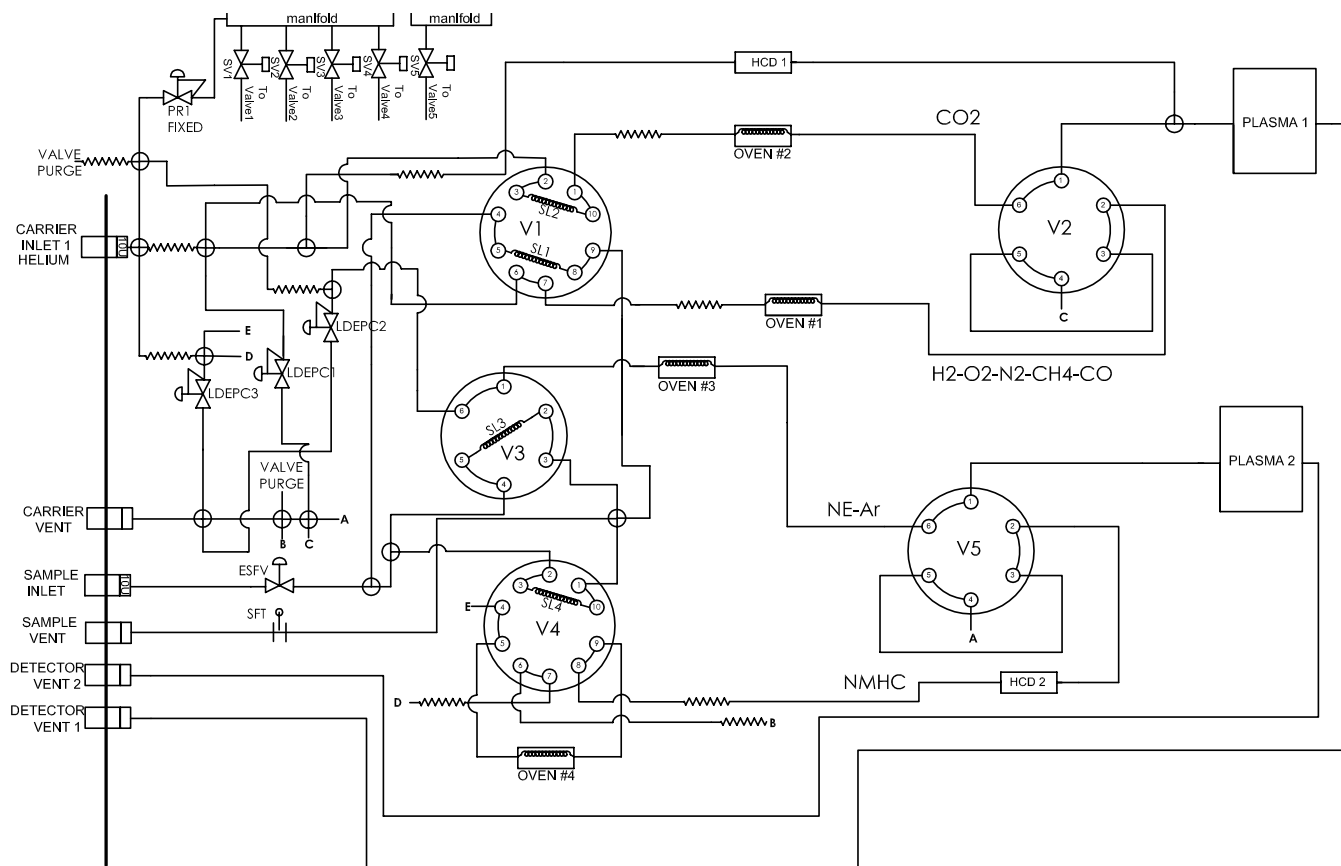


Figure 1

Two plasma cells are used to reduce the number of selection valves. Simultaneous injection in both plasmas is possible to accelerate analysis time. The parallel analysis feature within the MultiDetek2 software can be enabled to give the opportunity to acquire two chromatograms at the same time.

Neon and argon are measured within the same channel using the argotek column from LDetek. Such column gives a true argon peak by separating O2 and argon completely. Be sure to check application note LD12-3 on our website for more details. It also makes possible the measurement of neon against H2.

When using the PlasmaDetek2 technology, different optical filters are used to ensure true measurement of the components when interference can occur. For example, O2 is measured accurately against argon by using a specific optical filter giving a signal specifically to O2 and not argon.

Figure 2 shows a chromatogram of such system with a standard gas.

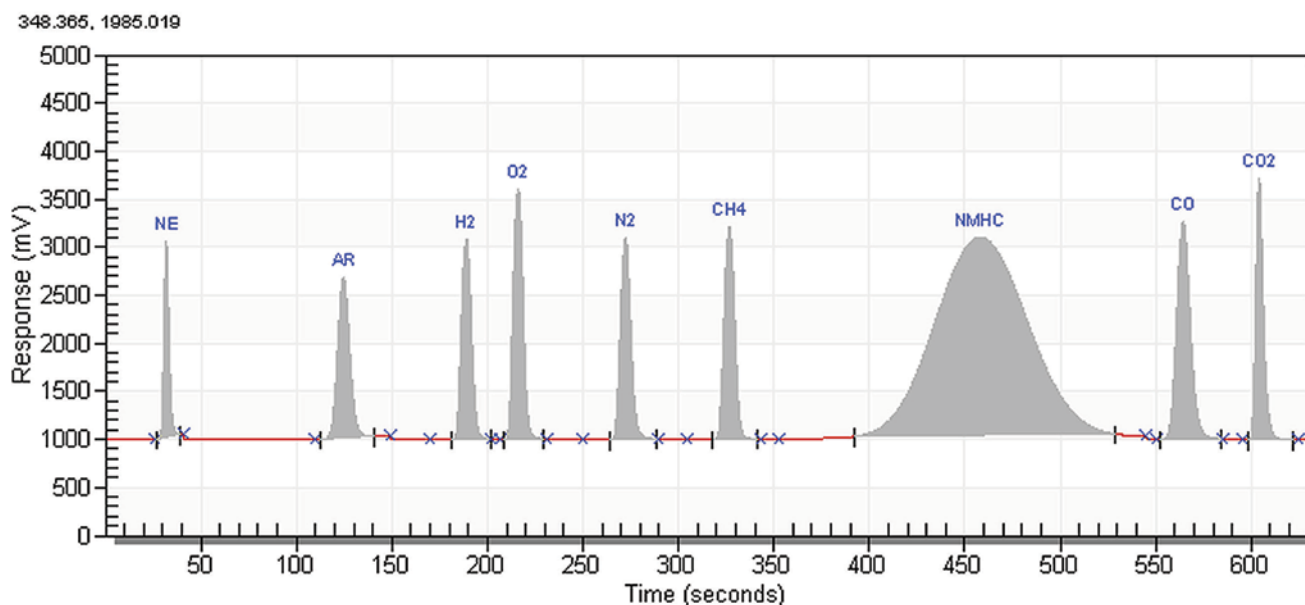


Figure 2

Based on noise to ratio, LDL is calculated as follows:

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------------|---------------|-------------|-------|----------------|
| Ne | 4.8 ppm | 3010 mV | 2 mV | 0.009 ppm |
| Ar | 4.1 ppm | 2720 mV | 2 mV | 0.009 ppm |
| H ₂ | 5.5 ppm | 3120 mV | 2 mV | 0.011 ppm |
| O ₂ | 6.2 ppm | 3552 mV | 2 mV | 0.010 ppm |
| N ₂ | 5.4 ppm | 3099 mV | 2 mV | 0.010 ppm |
| CH ₄ | 5.5 ppm | 3254 mV | 2 mV | 0.010 ppm |
| NMHC | 4.6 ppm | 3101 mV | 3 mV | 0.007 ppm |
| CO | 5.4 ppm | 3331 mV | 2 mV | 0.013 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

COMPLETE SOLUTION:

Our Helium purity analysis offers a complete cabinet solution including the MultiDetek2 compact GC system, the LDGSS ultra high purity remote stream selector system, the LDP1000 carrier gas purifier and the moisture analysis instrument all integrated in one cabinet. The stream selector can be manually controlled using the front switch or can be remotely controlled with the MultiDetek2. A pre programmed sequence can also be done with LDGSS. The moisture analysis is re-directed to the MultiDetek2 analog input. This way, all data can be managed by MultiDetek2 using one channel communication protocol. The system is pre-configured and certified by experts at LDetek facility before shipping.



CONCLUSION:

Using both the PlasmaDetek2 and the MultiDetek2, only one system can measure all permanent gases with the sensitivity required. No need of additional oxygen analyzer or other setup for neon measurement. Furthermore, with the LDetek technology this maintenance free system avoids any trap or scrubber for the argon impurity.

APPLICATION NOTE

LD16-02



Analysis of hydrocarbons, CO₂, N₂O in Oxygen with the MultiDetek2 compact GC system using Nitrogen as carrier gas and the PlasmaDetek-E detection technology



▲ MultiDetek2

▲ PlasmaDetek2

LDETEK SOLUTION:

The hydrocarbon analysis for the production of high purity Oxygen on air separation plants is essential for safety of the operations and quality of the product. For a very long time, the flame ionisation detector has been used for detection of trace hydrocarbons in different gas mixtures. This detector has now many different designs all based on carbon ions collection. The FIDs require a mixture of Air and Hydrogen to generate the flame used for ionisation. It is also necessary to have extra safety based on Hydrogen gas handling. All these points result in increase of operating and start-up costs as demonstrated in Figure 1.

LDetek has developed a detection system based on plasma emission detector (PlasmaDetek E) for the analysis of trace hydrocarbons in different gas mixtures. This PED technology offers enhanced sensitivity and selectivity to hydrocarbons using Nitrogen as single discharge/carrier gas. Other emission and ionisation detection technologies are known in the market for the analysis of hydrocarbons using Argon or Helium as discharge/carrier gas. However, these systems don't offer the selectivity and sensitivity to allow running a single injection through a column without having interferences from residual Oxygen. Other techniques offering NMHC detection are also available and are sufficient in certain cases. Nevertheless, the NMHC detection doesn't give the ability to focus on the measurement of critical impurities like low concentration acetylene in Oxygen production. Using the MultiDetek E with Nitrogen carrier gas, the system can be customized for the range and LDL that are specifically required for each impurity. This way, it is possible to configure the system according to each air separation plant specification. As shown in figures 2 and 3, low detection is possible using Nitrogen as carrier gas with PED technology. No need of complex valve and column chromatography configuration for flushing out the background gases.

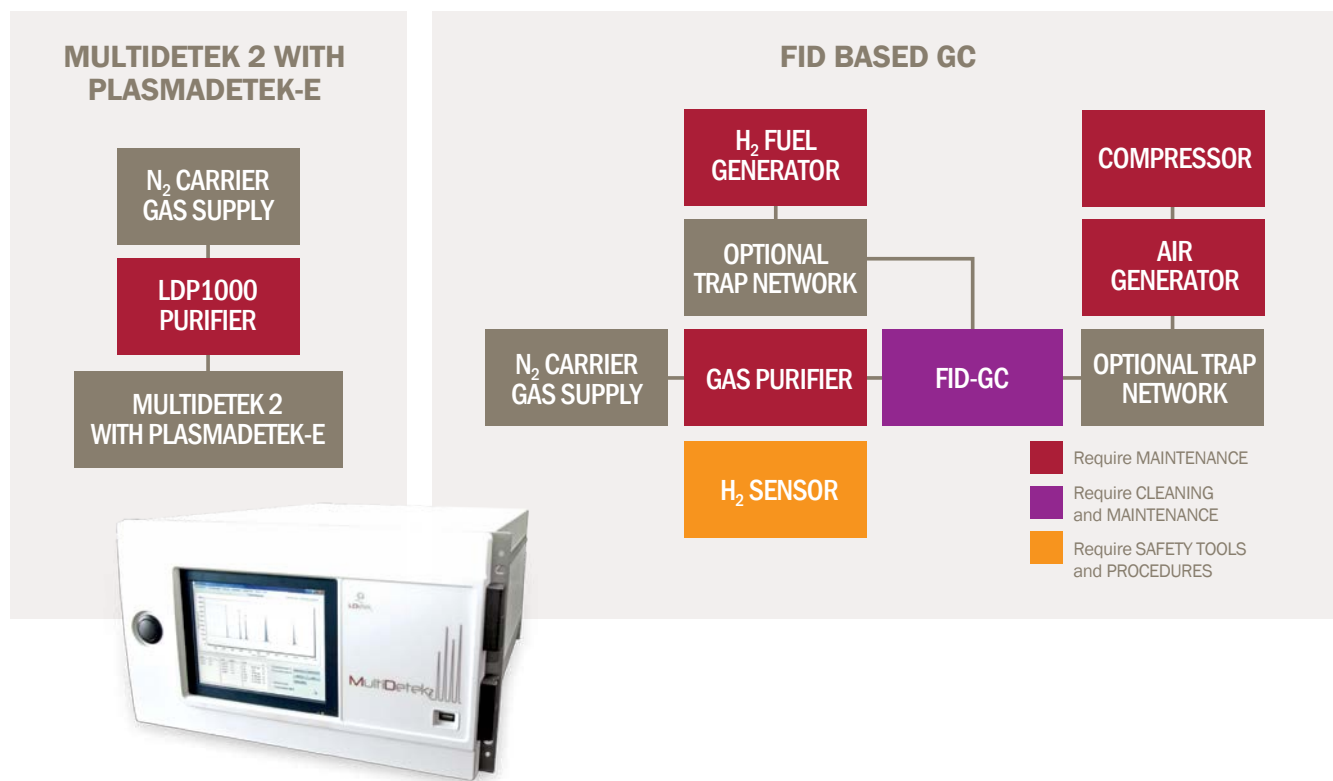


Figure 1 : Comparison between FID based GC and MultiDetek2 compact GC with PlasmaDetek-E

RESULTS:

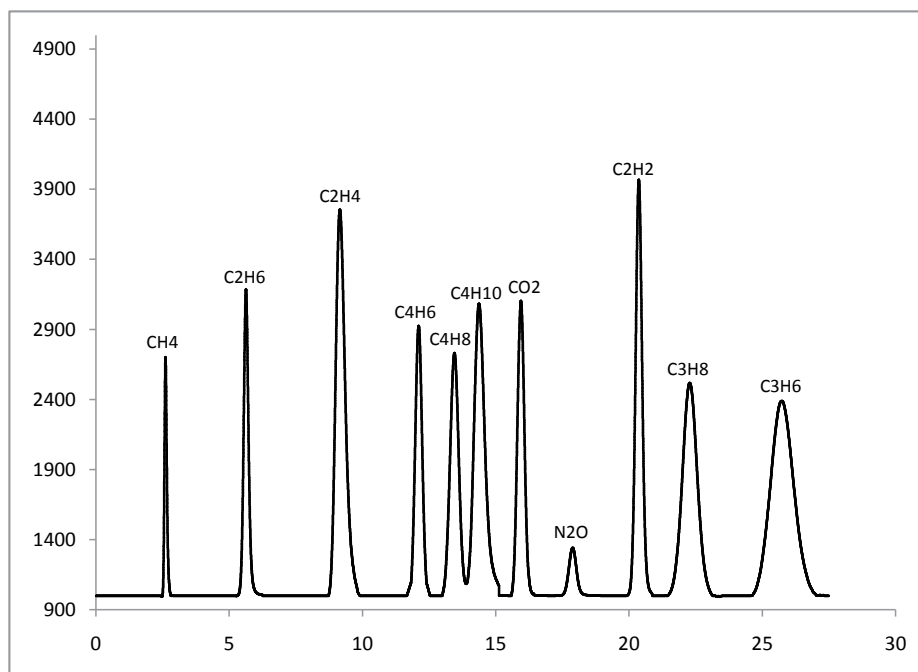


Figure 2 : Chromatogram of trace impurities in balance Oxygen

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------|---------------|-------------|---------|----------------|
| CH4 | 18.1 ppm | 2760 mV | 2.1 mV | 0.041 ppm |
| C2H6 | 8.6 ppm | 3308 mV | 4.0 mV | 0.031 ppm |
| C2H4 | 8.2 ppm | 3888 mV | 4.3 mV | 0.027 ppm |
| C4H6 | 2.1 ppm | 2969 mV | 11.0 mV | 0.023 ppm |
| C4H8 | 1.8 ppm | 2798 mV | 11.8 mV | 0.023 ppm |
| C4H10 | 2.1 ppm | 3190 mV | 11.5 mV | 0.023 ppm |
| CO2 | 4.1 ppm | 3199 mV | 11.0 mV | 0.042 ppm |
| N2O | 0.8 ppm | 1401 mV | 3.0 mV | 0.005 ppm |
| C2H2 | 1.1 ppm | 4098 mV | 10.5 mV | 0.007 ppm |
| C3H8 | 8.9 ppm | 2559 mV | 4.1 mV | 0.043 ppm |
| C3H6 | 8.7 ppm | 2501 mV | 3.9 mV | 0.041 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

CONCLUSION:

With Nitrogen gas used as carrier, the MultiDetek2 with Plasmadetek-E becomes the ideal gas measuring instrument for trace detection of hydrocarbons on the air separation plants for high purity Oxygen monitoring. Keeping the start-up and operating costs low and offering enhanced hydrocarbon detection, LDetek is proud to offer its robust and easy to operate system.

APPLICATION NOTE

LD16-06



LD8000 MultiGas online gas analysis solution for high purity compressed Helium used in cryogenic installations.



▲ LD8000 MultiGas

▲ PlasmaDetek2

Cryogenics is the branch of physics that deals with the production and effects of very low temperatures. Helium was a natural choice of coolant as its properties allow components to be kept cool over long distances. Super fluid helium has remarkable properties, including very high thermal conductivity; it is an efficient heat conductor. These qualities make helium an excellent refrigerant for cooling and stabilising the LHC's large-scale superconducting systems. The Large Hadron Collider (LHC) at institutions like the CERN in Switzerland is the largest cryogenic system in the world and one of the coldest places on Earth. It is one of the examples where the use of cryogenic Helium is essential for good working of the system.

The difference from conventional industries is that repairing a cryogenic system and reaching the process nominal conditions is a time-consuming action due to the thermodynamic constraints. For this reason, fault diagnostic functions, capable to detect and identify faults before their degeneration into failures, become more and more important. In cryogenic installations, the most critical class of equipment consists of rotating machinery, such as pump, turbines and compressors. Beside the problems related to failures of compressors, turbines, etc... The limitation of plant runtime and failures are also due to impurity loads to the cold box. Mostly smaller sources of water and air contamination are found just before the beginning of appearance of the Breox oil in the vacuum screw compressors that leads to a high load of the cold box with water, formaldehyde and other organic components. This fault situation must absolutely be detected at the beginning to minimize the impact of failure.

This is why it is required to have an impurity monitoring instrument for the cold box feed gas that measures the ratios of air, water, hydrocarbons and oil in the gas running from the recycle compressor to the cold box. This way, the maintenance and actions can be taken at the right moment. The analytical instrument must monitor trace N₂-O₂-water and hydrocarbons in high purity Helium.

LDetek SOLUTION:

LDetek offers its online LD8000 MultiGas based on plasma emission technology (PlasmaDetek2) to trace the O₂-N₂-CnHM and water impurities in cryogenic Helium. Using a single detection technique based on plasma emission, the trace impurities can be measured with an online mode. The required range for this type of application is usually 0-100ppm for O₂ and N₂, 0-25ppm for moisture and 0-10ppm for CnHM. Other ranges can be configured on request. The system monitors in continue the Helium purity without the use of Chromatography columns. The response analysis time for each gas can be done within 30 seconds. Better response time can be achieved depending on the purge flow rate that is adjustable on the LD8000. Since the Helium cost is an important factor, LDetek has designed its unit to ensure low sample flow consumption and this with consideration to ensure keeping a quick response time.

On top of that, the design is based on independent micro plasmas to ensure the protection of the system from oil contamination on long-term operation. A first plasma is isolated for measuring O₂ and N₂ together, having their own selective mode. A second plasma is used for measuring independently the H₂O concentration alone having its own flow path specifically designed for moisture analysis. And a third plasma combining a plasma converter system is used for measuring the trace CnHM. This third plasma system is designed to ensure that the optic used for measuring the CnHM isn't submitted to carbon deposit contamination.

FEATURES:

The instrument comes with a touchscreen interface and a keypad that facilitate the navigation through the different menus. It has one 4-20mA analog output per impurity. Each impurity has 2 ranges of operation and an individual ID range contact. It also has 2 configurable alarm contacts and one status contact. The unit has an automatic proportional valve for controlling the sample flow rate and a manual valve for adjusting the sample bypass flow rate.

Based on dual plasma operation, a safe mode has been implemented if the oil level goes over a certain concentration. It protects the alternative plasmas to be contaminated with carbons to guarantee a long-term operation in presence of dirty Helium gas containing high level of oil.

CONCLUSION:

The LD8000 MultiGas uses a parallel plasma system configuration that is individually selective to each measured gas to avoid the interferences from other impurities. Using this technique, the LD8000 becomes the right online instrument to be used for Helium purity for monitoring multiple impurities in a single unit on cryogenic installation.

APPLICATION NOTE

LD16-07



Measurement of impurities in UHP Argon using the MultiDetek 2 and PlasmaDetek 2



▲ MultiDetek2

▲ PlasmaDetek2

Argon is a widely used gas in different needs such as steel industries, air separation, welding, purging, chemical plants, semiconductor and others. Having a good analytical tool is mandatory to ensure the required purity of argon.

The most popular technique for UHP argon analysis is to detect trace impurities by gas chromatography. Some of the most common technologies will use a combination of multiple detectors to achieve the analysis requirements. Most commonly used are FID (flame ionization detector) combined with PDD (pulse discharge detector). This technique requires the need of helium as carrier gas what is an expensive gas to be used as carrier gas for the analysis of H₂-N₂-CO-CO₂. The analyses of hydrocarbons will be performed using the FID what requires extra cost due to air and fuel. On top of that, the oxygen analysis must be performed using a separated trace oxygen analyzer due to the co elution of argon and oxygen in the gas chromatography system with helium ionization detection technique.

LDETEK SOLUTION:

The MultiDetek 2 combined with the PlasmaDetek 2 detector provides an ideal solution to measure the different impurities in UHP argon. With the PlasmaDetek 2, based on plasma emission detection, impurities in low ppb can be easily detected.

The system is simply configured with 3 channels and one plasma detector. Each channel has its own chromatography column mounted in a compact isothermal oven. A simple injection with sampling loop technique mounted on a diaphragm valve is used to introduce the sample gas to the detector.

Channel 1 to trace H₂-O₂-N₂-CH₄-CO
 Channel 2 to trace CO₂
 Channel 3 to trace NMHC (NMHC can be measured as required hydrocarbon equivalent depending on the need)

A diaphragm valve network is used for synchronizing the impurities to the plasma detector.

Figure 1 shows a chromatogram of such system with a standard gas containing trace impurities in a balance of Argon. Figure 2 shows the LDL that such Argon purity system can achieve based on noise level to signal ratio calculation.

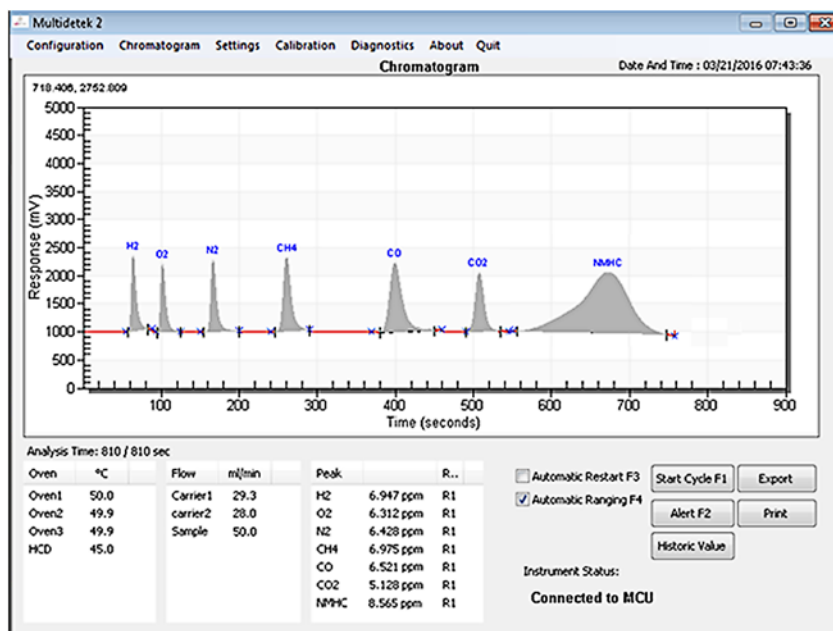


Figure 1

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------------|---------------|-------------|--------|----------------|
| H ₂ | 6.947 ppm | 1391 mV | 2.5 mV | 0.037 ppm |
| O ₂ | 6.312 ppm | 1311 mV | 2.1 mV | 0.030 ppm |
| N ₂ | 6.428 ppm | 1377 mV | 1.0 mV | 0.014 ppm |
| CH ₄ | 6.975 ppm | 1390 mV | 2.0 mV | 0.030 ppm |
| CO | 6.521 ppm | 1270 mV | 2.6 mV | 0.040 ppm |
| CO ₂ | 5.128 ppm | 1168 mV | 2.3 mV | 0.030 ppm |
| NMHC | 8.565 ppm | 1201 mV | 1.6 mV | 0.034 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic condition

Figure 2

CONCLUSION:

Using the MultiDetek 2 compact GC, it becomes the most convenient solution for argon purity analysis. It is a maintenance free system that offers the required performances. The use of argon as carrier gas entails a low cost of operation. On top of that, the MultiDetek2 offers all the features required by the industrial market for such type of application.

APPLICATION NOTE

LD16-08



Measurement of hydrocarbons in UHP Oxygen using the MultiDetek 2 and PlasmaDetek-E



▲ MultiDetek2

▲ PlasmaDetek2

This application note shows different methods that have been developed by LDetek for measuring the hydrocarbons in a stream of Oxygen (other matrixes can be analysed as well since the PlasmaDetek-E is strictly selective to hydrocarbons). This application note is the continuity of the application note LD16-02. It is then suggested to first read the LD16-02 to be advised about the technology that was used.

LDETEK SOLUTION:

The chromatograms shown in figure 1 and in figure 3 have been performed using a single column with a Plasmadetek-E. The system uses nitrogen as a unique carrier gas. The simplicity of this configuration makes this solution very efficient and simple for operation. No maintenance is required for such micro plasma based system.

Method for chromatogram in figure 1:

The MultiDetek2 configuration uses a 10 port diaphragm valve mounted in an injection/backflush mode. The sample gas is then introduced in the packed porous polymer type column for eluting the Air/O2 followed by CH4 in one direction to the detector before to reverse the flow in the column to get the NMHC redirected to the detector. The selective mode of the PlasmaDetek-E makes the detector being strictly selective to hydrocarbons and makes oxygen/air being invisible to the detector. The detector response and LDLs are demonstrated in figure 2. Please note that different performances can be achieved depending on the maximum and minimum ranges required.

Method for chromatogram in figure 3:

Using the same valve configuration combined with a different column type and system conditions, the analysis of separated C2's becomes possible. For some applications, where it is critical to measure C2s individually, especially acetylene at low concentrations, this method is preferred. The addition of C3+ measurement can be done in the same system to cover the whole hydrocarbon analysis solution. It offers better accuracy, sensitivity and simplicity than conventional FID or Argon plasma method. Figures 4-5 and 6 show an example of performances using this method in real life conditions.

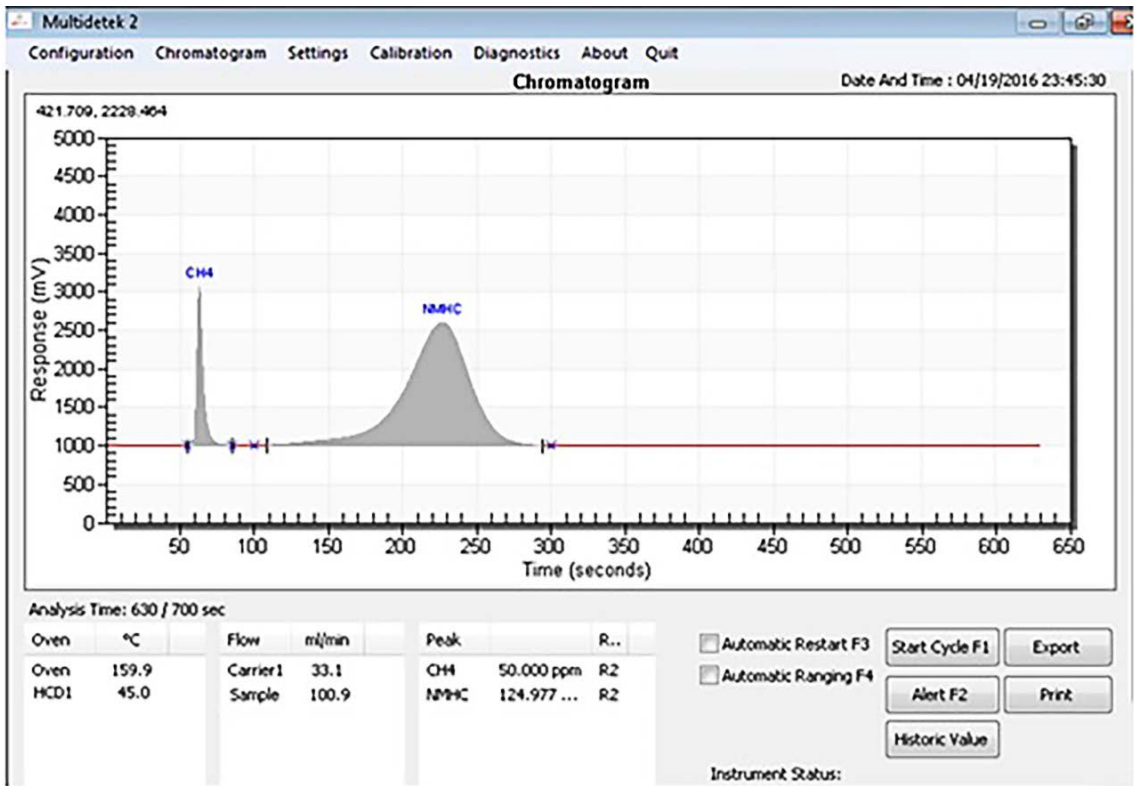


Figure 1: Chromatogram of CH4 & NMHC in oxygen matrix

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------------|---------------|-------------|--------|----------------|
| CH ₄ | 50.000 ppm | 2211 mV | 0.8 mV | 0.054 ppm |
| NMHC | 124.977 ppm | 1622 mV | 0.4 mV | 0.092 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic condition

Figure 2

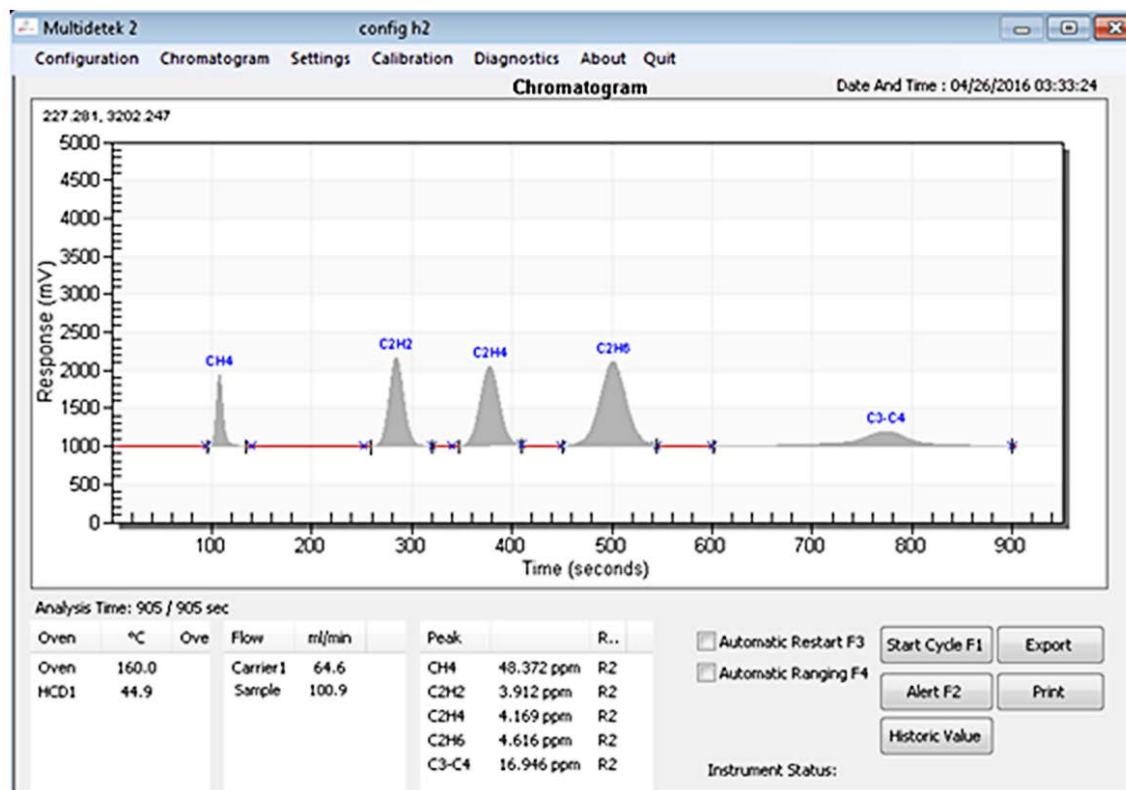


Figure 3: Chromatogram of trace CH₄, C₂H₂, C₂H₄, C₂H₆ & C₃⁺ in oxygen matrix

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-------------------------------|---------------|-------------|--------|----------------|
| CH ₄ | 48.372 ppm | 951 mV | 0.3 mV | 0.046 ppm |
| C ₂ H ₂ | 3.912 ppm | 1241 mV | 3.3 mV | 0.031 ppm |
| C ₂ H ₄ | 4.169 ppm | 1111 mV | 3.3 mV | 0.037 ppm |
| C ₂ H ₆ | 4.616 ppm | 1146 mV | 3.3 mV | 0.040 ppm |
| C ₃ ⁺ | 16.946 ppm | 220 mV | 0.9 mV | 0.207 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic condition

Figure 4

| ne | CH4 | C2H2 | C2H4 | C2H6 | C3+ |
|----------------|-------|-------|-------|-------|--------|
| /2016 04:23:29 | 7.278 | 7.368 | 7.252 | 6.947 | 23.382 |
| /2016 04:08:18 | 7.283 | 7.365 | 7.250 | 6.947 | 23.383 |
| /2016 03:53:07 | 7.281 | 7.364 | 7.253 | 6.955 | 23.397 |
| /2016 03:37:56 | 7.282 | 7.361 | 7.246 | 6.942 | 23.387 |
| /2016 03:22:45 | 7.289 | 7.362 | 7.253 | 6.954 | 23.409 |
| /2016 03:07:34 | 7.290 | 7.368 | 7.254 | 6.965 | 23.422 |
| /2016 02:52:23 | 7.280 | 7.369 | 7.259 | 6.968 | 23.428 |
| /2016 02:37:12 | 7.265 | 7.369 | 7.260 | 6.960 | 23.419 |
| /2016 02:22:01 | 7.278 | 7.377 | 7.266 | 6.965 | 23.419 |
| /2016 02:06:50 | 7.293 | 7.379 | 7.264 | 6.960 | 23.406 |
| /2016 01:51:39 | 7.275 | 7.382 | 7.269 | 6.951 | 23.417 |
| /2016 01:36:28 | 7.276 | 7.385 | 7.266 | 6.965 | 23.420 |
| /2016 01:21:17 | 7.290 | 7.390 | 7.268 | 6.980 | 23.424 |
| /2016 01:06:06 | 7.288 | 7.390 | 7.273 | 6.983 | 23.453 |

Figure 5: Example of stability results over 10 consecutive cycles

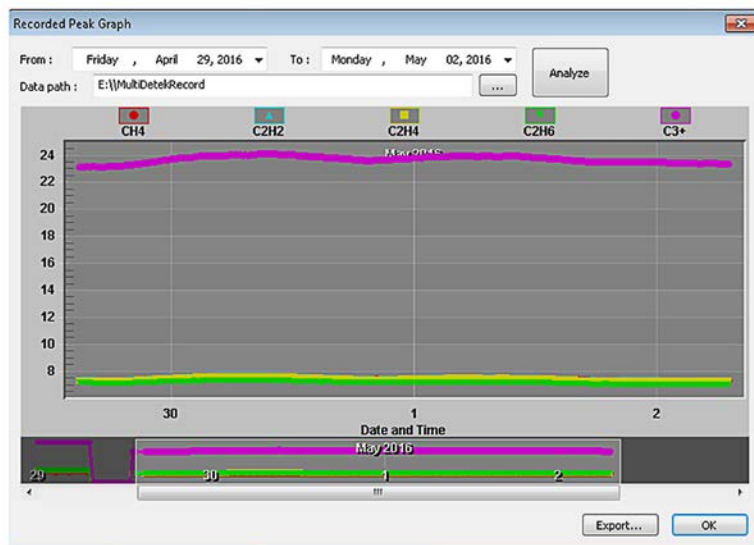


Figure 6: Example of stability results over a 3 day period

APPLICATION NOTE

LD16-09



Measurement of trace impurities in UHP hydrogen



▲ MultiDetek2

▲ PlasmaDetek2

The production of UHP hydrogen requires analysis of trace impurities to control and certify the gas purity. Multiple instruments are usually dedicated to this task. Combining everything in the same instrument, the MultiDetek2 compact gas chromatograph is very efficient for this type of requirement. The detection down to part per billion can be achieved, what makes the instrument capable of certifying different hydrogen grades.


LDETEK SOLUTION:

Most of the gas chromatographs will use some combinations of hydrogen traps or membranes for measuring some impurities like Ar-O₂ and N₂ at low part per billion to eliminate the interference from hydrogen. The selectivity of the PlasmaDetek2 detector has the ability to measure those difficult impurities down to ppb level without the use of any hydrogen traps or membranes. It reduces the operation cost and simplifies the running operations of the system.

The configuration has 5 channels all converging in 3 different plasma detectors as follows:

- ▶ **Channel#1:** Measuring CH₄-CO₂ with HayeSep columns merging in plasma#1
- ▶ **Channel#2:** Measuring O₂-N₂ with Molecular Sieve columns merging in plasma #1
- ▶ **Channel#3:** Measuring NMHC with HayeSep column merging in plasma #2
- ▶ **Channel#4:** Measuring CO with Molecular Sieve column merging in plasma #2
- ▶ **Channel#5:** Measuring Ar with ArgoTek* column merging in plasma #3

*ArgoTek column is manufactured by LDETEK to offer the trace argon separation from matrix Oxygen or Hydrogen. The column is packed type operating at 45 Celsius / 20 sccm helium carrier flow rate. With these conditions, the column offers the desired separation for measuring part per billion argon in either oxygen or hydrogen.

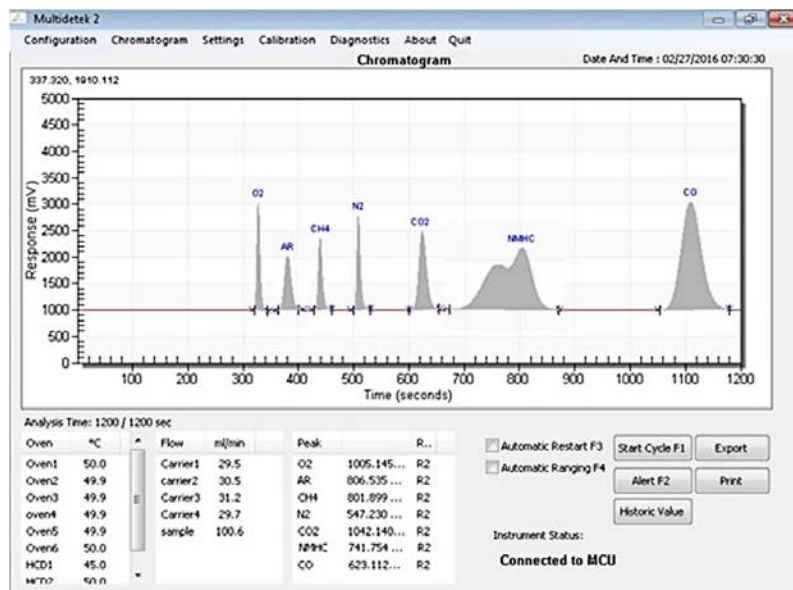

The three plasma detectors are respectively configured with the appropriate optical filters for blocking the hydrogen matrix and focussing on the dedicated impurities. This plasma configuration allows the analysis of multiple impurities in one single compact gas chromatograph unit.

Figures 1 and 2 show an example of results that such configuration can achieve for measuring low ppb/ppm concentrations of UHP hydrogen.

Figure 1: chromatogram of trace impurities in UHP hydrogen

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------------|---------------|-------------|--------|----------------|
| O ₂ | 1005.1 ppb | 2090 mV | 2.1 mV | 3.02 ppb |
| Ar | 806.5 ppb | 1017 mV | 0.8 mV | 1.90 ppb |
| CH ₄ | 801.8 ppb | 1415 mV | 1.6 mV | 2.71 ppb |
| N ₂ | 547.2 ppb | 1821 mV | 1.4 mV | 1.26 ppb |
| CO ₂ | 1042.1 ppb | 1500 mV | 2.2 mV | 4.58 ppb |
| NMHC | 741.7 ppb | 1299 mV | 2.2 mV | 3.76 ppb |
| CO | 623.1 ppb | 2055 mV | 5.1 mV | 4.63 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic condition

Figure 2

CONCLUSION:

The analysis of UHP hydrogen can be performed using this LDetek solution that combines a selective plasma detector configuration, a complete industrial compact gas chromatograph system, a unique separation column type with an impressive expertise in this field of application. Having all this makes LDetek solution perfect for this type of industrial application.

APPLICATION NOTE

LD16-10



Measurement of trace Ar-Kr and N2 in a bulk gas Oxygen



▲ MultiDetek2

▲ PlasmaDetek2

Detecting and measuring trace Ar-Kr and N2 in a bulk gas Oxygen without the need of a cryogenic system, or a trapping adsorbent or an extra long column as generally used to measure trace ppb/ppm Argon as impurity from bulk Oxygen and for separating Krypton and Nitrogen.


LDETEK SOLUTION:

Using the compact MultiDetek2 gas chromatograph, with a dual channel mode merging in one PlasmaDetek2 (PED) detector, the analysis of trace Ar-Kr and N2 can be realized easily in a robust and maintenance free system.

- **Channel#1:** Used for measuring trace Argon in bulk Oxygen with the Argotek* column. The sample gas is injected using a standard 6 ports diaphragm valve directly in the packed type column that operates at isothermal temperature and with a fix carrier flow rate.
- **Channel#2:** Used for measuring trace Krypton and Nitrogen in bulk Oxygen with the HSR-Etek* column. The sample gas is injected using a standard 6 ports diaphragm valve directly in the packed type column that operates at isothermal temperature and with a fix carrier flow rate.

*ArgoTek column is manufactured by LDetek to offer the trace argon separation from matrix Oxygen. The column is packed type operating at 45Celsius/20sccm helium carrier flow rate. With these conditions, the column offers the desired separation for measuring part per billion argon in oxygen. (more details appear in application note LD12-3)

*HSR-Etek column is manufactured by LDetek to offer the trace Krypton and Nitrogen separation from matrix Oxygen. The column is packed type operating at 45Celsius/20sccm helium carrier flow rate. With these conditions, the column offers the desired separation for Kr/N2. (more details appear in application note LD12-7)

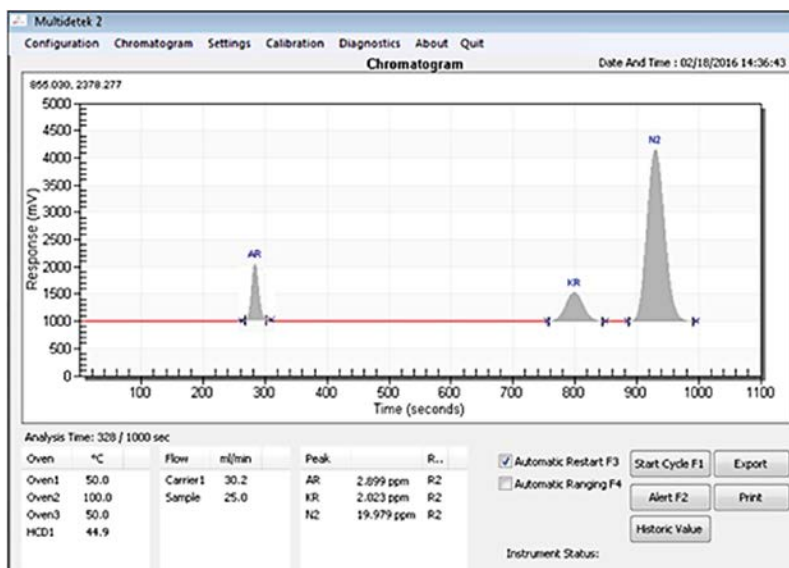

Figures 1 and 2 show an example of results that such configuration can achieve for measuring low ppb/ppm concentrations in bulk oxygen.

Figure 1: chromatogram of trace impurities in Oxygen

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------|---------------|-------------|--------|----------------|
| Ar | 2.899 ppm | 1091 mV | 0.7 mV | 5.6 ppb |
| Kr | 2.023 ppm | 503 mV | 0.8 mV | 9.6 ppb |
| N2 | 19.979 ppm | 3211 mV | 0.7 mV | 13.0 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic condition

Figure 2

CONCLUSION:

The analysis of specific trace impurities in bulk Oxygen can be performed using this LDetek solution that combines a selective plasma detector with the right chromatography solution. It gives a robust and maintenance free system. Other impurities can be added to this system simply by adding extra channels.

APPLICATION NOTE

LD16-11



Measurement of trace impurities in multiple bulk gases



▲ MultiDetek2

▲ PlasmaDetek2

Having an analytical system that is able to measure multiple impurities in different bulk gases is sometimes required. It is usually a big challenge to combine all the hardware in the same instrument.

LDETEK SOLUTION:

The MultiDetek2 (compact gas chromatograph)

This compact gas chromatograph can handle up to 3 detectors with 6 parallel chromatographic channels through a network combining up to 10 diaphragm valves and 12 chromatographic columns. It opens the doors to many applications requiring multiple bulk gases analysis using the same compact analytical instrument.

One configuration (method) is pre programmed for each bulk gas analysis requirement. This way, the user can simply load the desired configuration and the analyser is ready to start the analysis. As well, the impurities can be independently configured with specific ranges and minimum detection limits.

No external PC is required since the robust industrial PC is mounted in the instrument and gives access to a data storage capacity. The instrument can be controlled remotely through the Ethernet connectivity. All industrial communication protocols are accessible. Automatic or manual report printing can be handled.

The LDGSS (stream selector)

Multiple bulk gases analysis usually requires a stream selector system being able to be controlled locally or remotely. A manual switch is available on the front to select manually the desired stream. Otherwise, the stream can be selected via the MultiDetek2 interface. The interface gives the possibility to edit the names of the streams, to program multiple sequences and to set specific purging time between each stream. The streams can also be selected and identified by a standard DCS system through a dry contacts network.

This ultra high purity system offers a quick response time due to its dead volume free design. An adjustable sample purge valve and flow meter is independent to each stream to adjust the gas line purging before the stream selector. A purge gas being the same of the carrier gas of the MultiDetek2 is used to keep the ambient air away of the analytical flow path to ensure ultra high purity analysis gas for all the streams. Specifically when trace impurity of a bulk gas is also the pure gas of its neighbor stream that was just analysed in the previous analysis. The design of a back purged stream selector system is very important and this is what is included in this solution.

For this application note, since the analysis of hydrogen and oxygen is required, 2 LDGSS systems have been used to avoid mixing of both gases together. The purge gases are independent to each stream selector to avoid any chance of mixing oxygen and hydrogen. The LDGSS used for Oxygen can be certified for O2 Clean.

The COMPACT-LDP1000 (gas purifier)


The gas purifier generates ultra high purity carrier gas certified for a total of 10ppb total impurities. This compact high capacity gas purifier keeps the system clean and intact even if carrier gas cylinders purity can vary from batch to batch introducing a variation of baselines which has impact on the accuracy of the analytical device. Or in another instance, if by mistake, an air contamination gets in the carrier flow path during the process of changing the carrier gas cylinder.

The gas purifier can also communicate in real-time with the MultiDetek2 to inform about his status. In the event of a default, it generates an alarm in the MultiDetek2 to automatically advise about the fault.

The LDRACK (certified cabinet)

The complete solution comes assembled and certified in a cabinet. Such system is fully tested to certify the analytical response time when switching between streams. This is more than necessary when low ppb analysis of nitrogen and oxygen are targeted. It doesn't only guarantee that the sample gas lines offers no dead volume and leaks, but also guarantees that the carrier gas lines are properly mounted. It is the best practice to get the best analytical performances especially when traces of impurity at ppb level are also present in ambient air must be detected.

THE COMPLETE SOLUTION

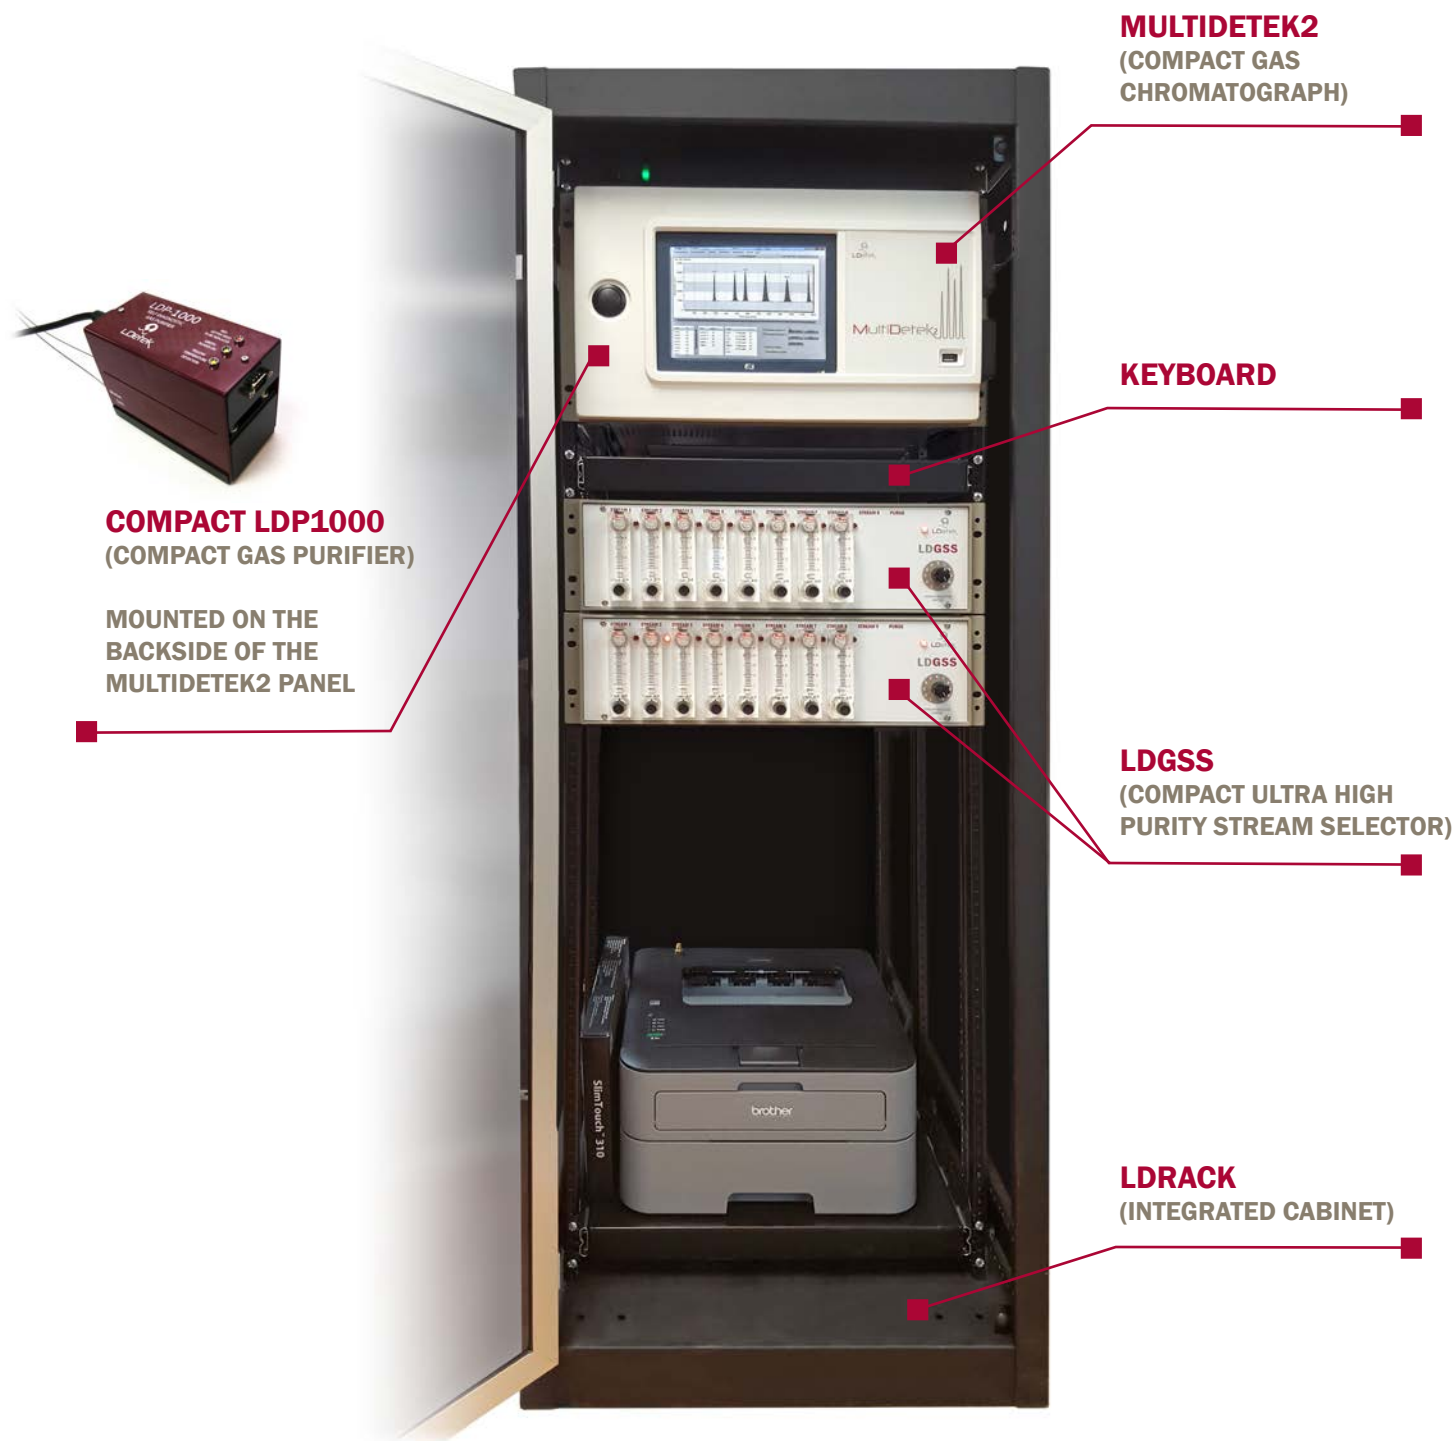

RESULTS:

Figures 1 to 12 show some examples of results that such configuration can achieve for measuring low ppb/ppm concentrations of multiple trace impurities in multiple bulk gases.

In this example, trace impurities H2-Ar-O2-N2-CH4-CO-CO2 in bulk gases Argon, Carbon dioxide, Hydrogen, Helium, Nitrogen and Oxygen were measured.

An optimized method for high range(HR) covering up to 1000ppm and another method for low range(LR) to ensure good peak detection and stability down to 10ppb are used. This dual methods technique gives the possibility to extend the dynamic range as desired. Conventional analysis techniques will tend to have some limitations on the low ppb detection when a high ppm analysis is required. The linearity and accuracy of our system is improved by having an optimized method for a specific analysis range.

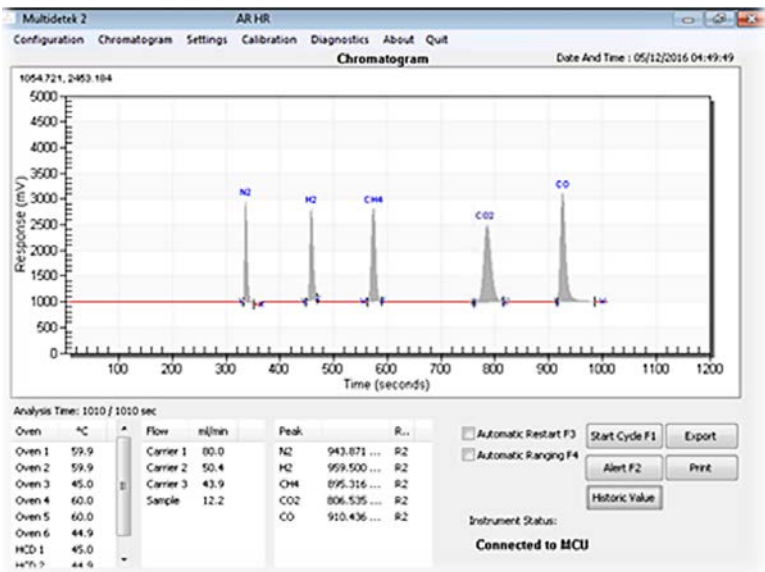


Figure 1: chromatogram of trace impurities in Argon (High range ppm)

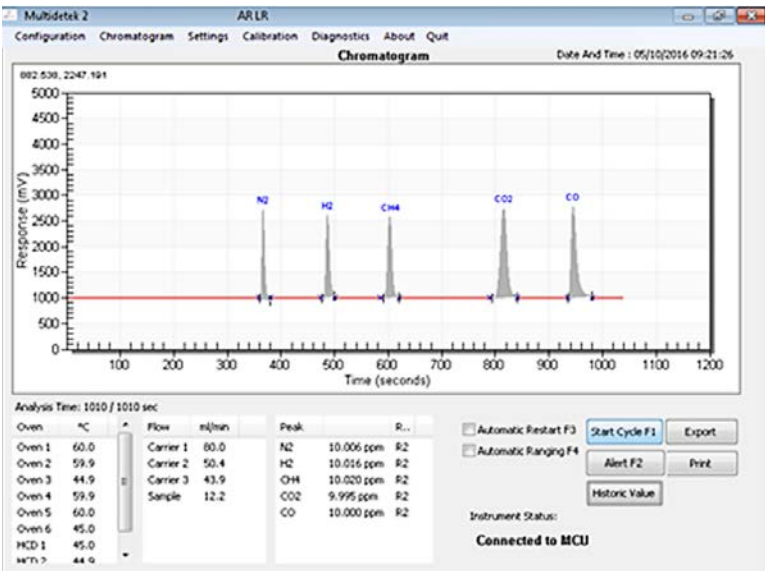


Figure 2: chromatogram of trace impurities in Argon (Low range ppb/ppm)

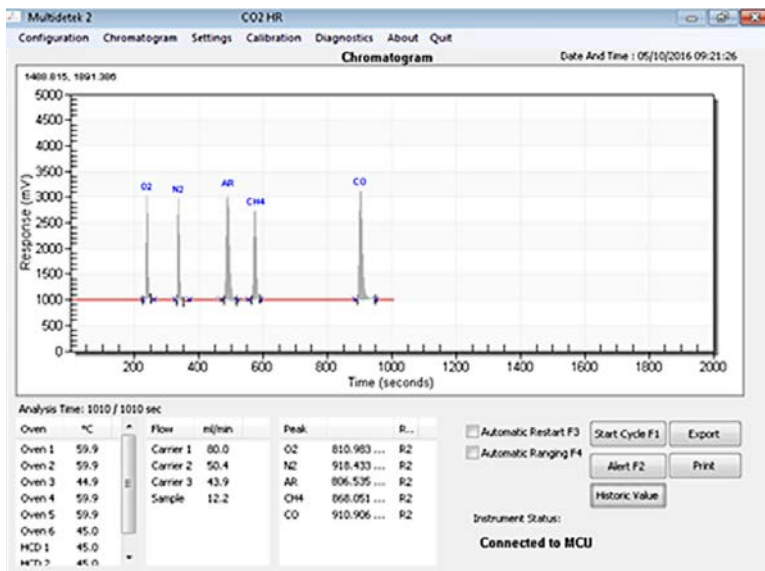


Figure 3:
chromatogram of trace impurities in Carbon Dioxide
(High range ppm)

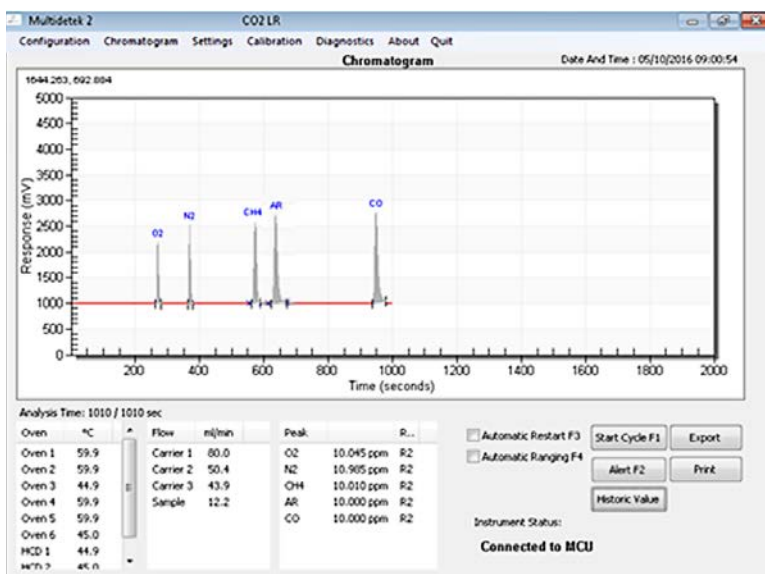


Figure 4:
chromatogram of trace impurities in Carbon Dioxide
(Low range ppb/ppm)

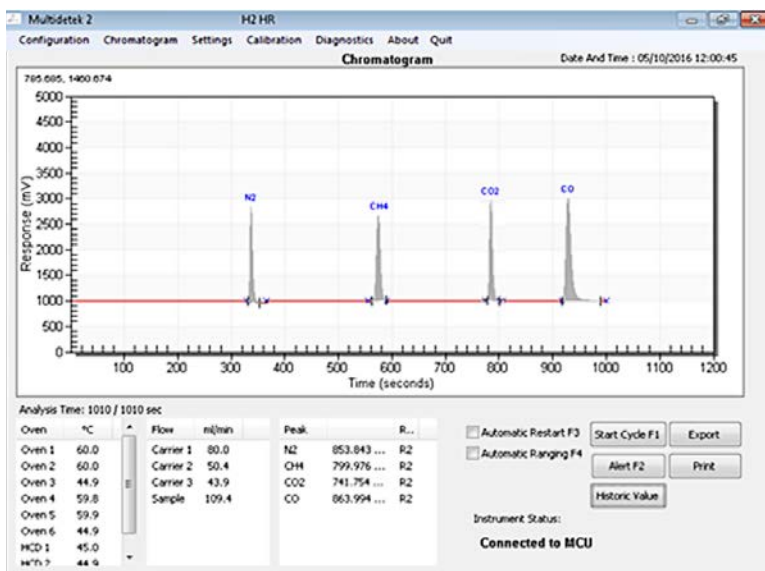


Figure 5:
chromatogram of trace impurities in Hydrogen
(High range ppm)

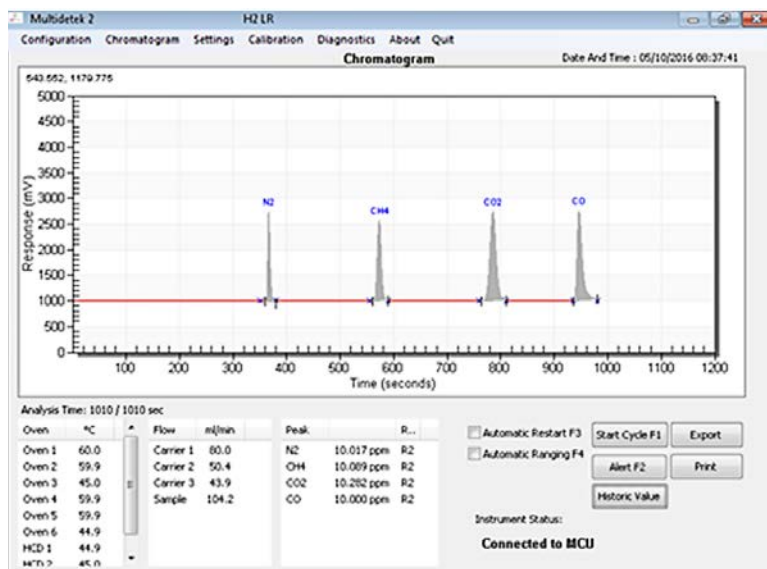


Figure 6:
chromatogram of trace impurities in Hydrogen
(Low range ppb/ppm)

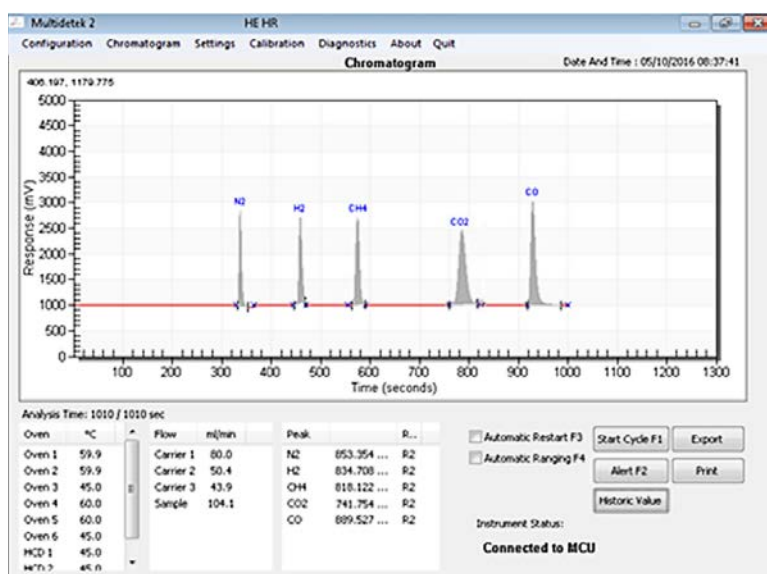


Figure 7:
chromatogram of trace impurities in Helium
(High range ppm)

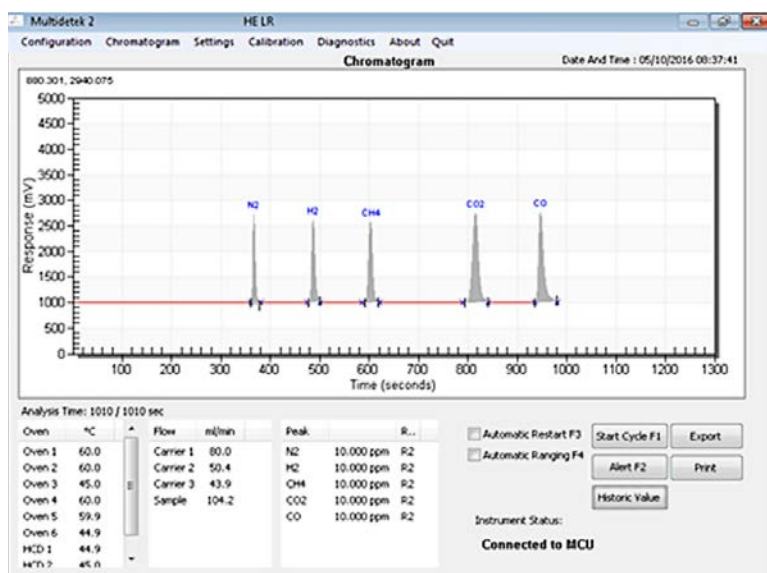


Figure 8:
chromatogram of trace impurities in Helium
(Low range ppb/ppm)

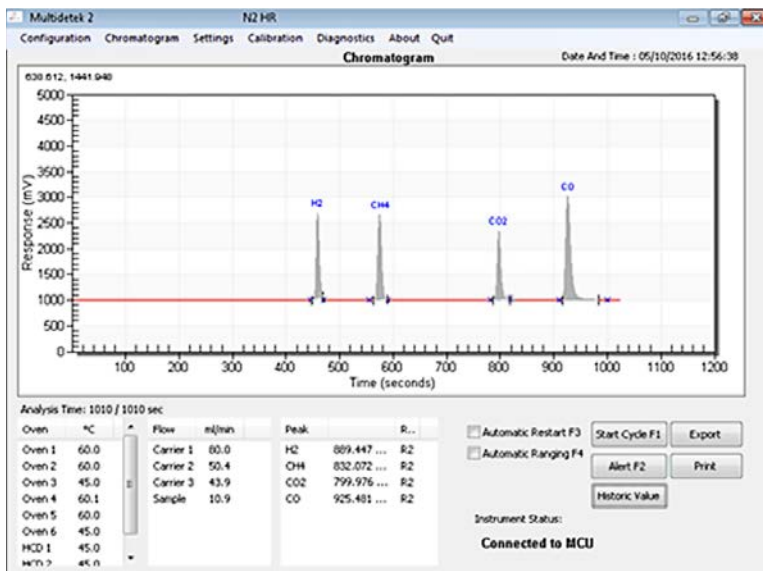


Figure 9:
chromatogram of trace impurities in Nitrogen
(High range ppm)

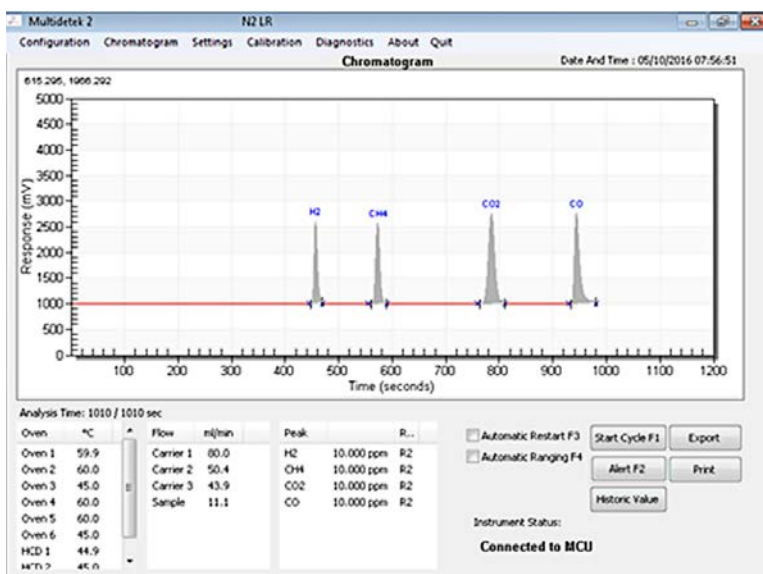


Figure 10:
chromatogram of trace impurities in Nitrogen
(Low range ppb/ppm)

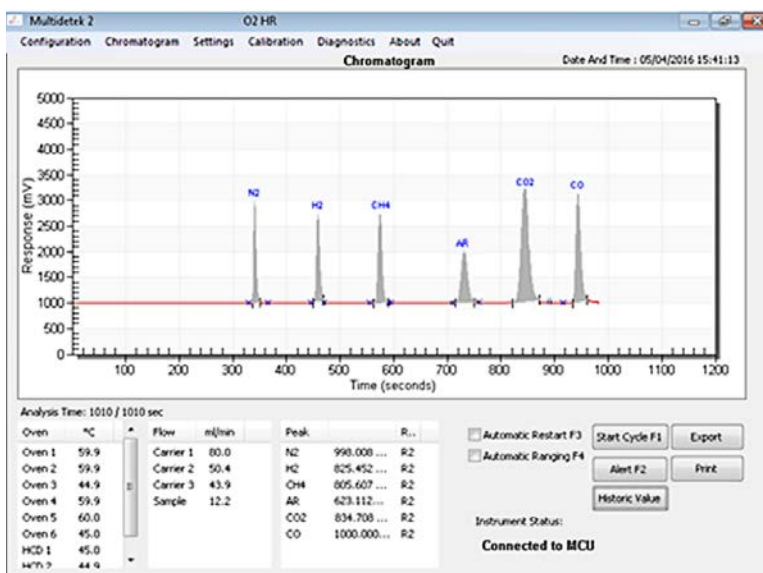


Figure 11:
chromatogram of trace impurities in Oxygen
(High range ppm)

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-------------|---------------|-------------|--------|----------------|
| H2 (fig.8) | 10.000 ppm | 1621 mV | 0.7 mV | 12.9 ppb |
| Ar (fig.4) | 10.000 ppm | 1780 mV | 0.4 mV | 6.7 ppb |
| O2 (fig.4) | 10.045 ppm | 1320 mV | 0.6 mV | 13.7 ppb |
| N2 (fig.2) | 10.006 ppm | 1821 mV | 0.5 mV | 8.2 ppb |
| CH4 (fig.6) | 10.089 ppm | 1612 mV | 0.6 mV | 11.3 ppb |
| CO (fig.10) | 10.000 ppm | 1806 mV | 0.9 mV | 14.9 ppb |
| CO2 (fig.6) | 10.282 ppm | 1823 mV | 0.8 mV | 13.5 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic condition

Figure 12

CONCLUSION:

Our complete integrated gas analysis solution guarantees the best performances and robustness for any applications combining multiple impurities in multiple streams and/or bulk gas types. It is compact and compatible with standards of the industry.

APPLICATION NOTE

LD19-05



Measurement of impurities in UHP Argon for HIP process using the MultiDetek2 and PlasmaDetek2



▲ MultiDetek2

▲ PlasmaDetek2
patent US 9,310,308 B2

Argon is a widely used gas in different needs such as steel industries, air separation, welding, purging, chemical plants, semiconductor and others. Having a good analytical tool is mandatory to ensure the required purity of argon.

This application note is the continuity of the LD16-07. In this application note, we will particularly covers the HIP (hot isostatic pressing) process in the steel industry with the use of the MultiDetek2 gas analyser GC for trace impurities in Argon.

What is the HIP?

HIP combines very high temperatures, very high pressures, and inert gas to eliminate porosity in castings and consolidate powder into dense materials. Temperatures are up to 2,000 deg C, pressures are up to 30,000 psi and UHP inert gas generally argon are the conditions required.

What is the utility of using HIP?

The hot isostatic pressing is used extensively to prolong the working life of components and protect them from environmental factors such as corrosion and abrasion. It provides thermal processing which improve material properties such as strength, durability and corrosion resistance, enabling manufacturers' components to work more efficiently with significantly extended operational lifetimes. It is used to alter the microstructure of materials, such as metals and alloys, to impart properties which benefit the working life of a component, for example: increased surface hardness, temperature resistance, ductility and strength. Hot isostatic pressing uses very high pressures in addition to high temperature to achieve engineering outcomes that are impossible by other methods. HIP is used to eliminate porosity in castings and consolidate encapsulated powders to dense materials. Dissimilar materials can be bonded together to manufacture unique, cost effective components.

What are the markets that require products to be manufactured from this HIP process?


HIP installations will process many tons of titanium, aluminium, steel and super-alloy castings, removing porosity and improving the performance of parts such as turbine blades and oilfield components. In almost all cases metals in any state require heat treatment to improve their properties, if components are to achieve desired levels of longevity and corrosion performance in use. Without heat treatment car engine components, for example, might last for hundreds of miles rather than the tens of thousands we expect. The use of the specialist surface technologies offers further improve in-use characteristics, particularly in severe environments such as in aircraft engines and in sub-sea oil & gas applications.

Why gas analysis is required for HIP?

An inert gas is required to prevent chemical reactions during the HIP process at elevated temperatures, making argon the ideal candidate. Monitoring of the HIP argon gas and its impurities is required to control the quality and repeatability of the HIP process.

The general quality control requires the analysis of the trace impurities in a range of 0-100ppm for H₂-O₂-N₂-CH₄-CO-CO₂-NMHC-H₂O in UHP argon.

HIP typical installation:

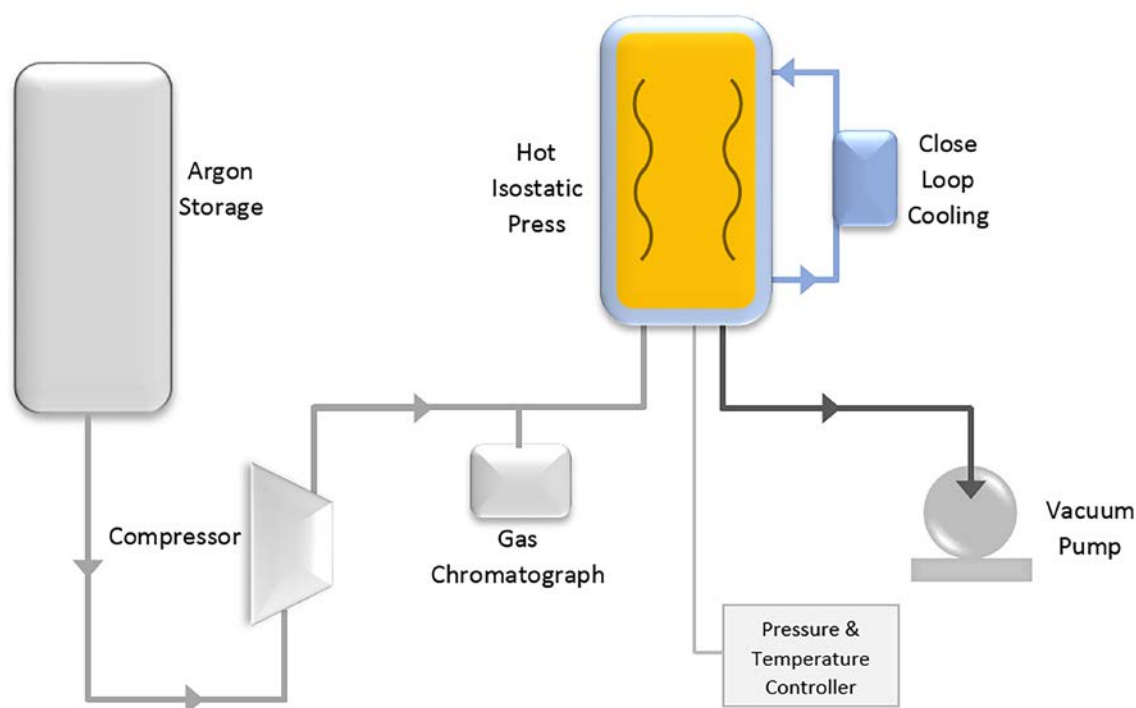


LDETEK SOLUTION:

The MultiDetek 2 combined with the PlasmaDetek 2 detector provides an ideal solution to measure the different impurities in UHP Argon.

The system is simply configured with 2 blocks, each one merging in one PED. Each block has its own chromatography column mounted in a compact isothermal oven. A simple injection with sampling loop technique mounted on a diaphragm valve is used to introduce the sample gas to the detector.


Block 1 is used to measure trace H₂-O₂-N₂-CH₄-CO and CO₂

For block 1 configuration, a selection diaphragm valve is used for synchronizing the impurities coming out of the columns to the plasma detector. The PED is configured with selective optics for each measured impurity improving the sensitivity.

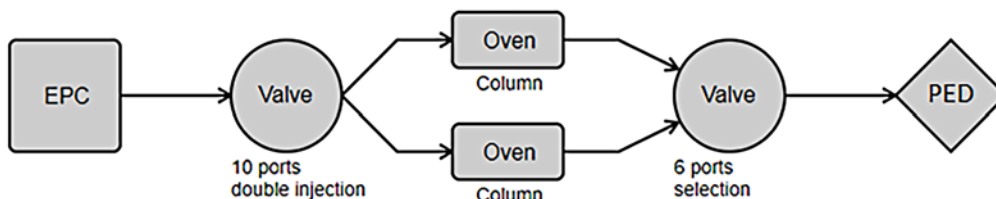

Block 2 is used to measure trace NMHC


The block 2 arrangement allows to inject light impurities to vent and by reverting the valve position, the C₂s-C₃s-C₄s hydrocarbons are grouped together as one peak to form NMHC to the PED. The PED has the right optic, selective to hydrocarbons.

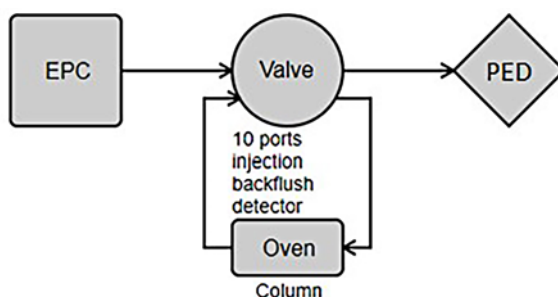

For the analysis of trace H₂O, 2 solutions are offered depending of the requirements.

1. A Michell DewPoint sensor can be added to the MultiDetek2, connected in parallel. The 4-20mA output of the sensor is wired back to the MD2 analog input. Then, all results can be report on the GC interface. Going this way a LDL of 0.5ppm can be achieved for H₂O impurity.
2. If an Idl lower than 0.5ppm is required, then a third block is mounted inside the MultiDetek2 containing a quartz crystal micro balance moisture sensor. Using this way, a span and zero calibration system is integrated inside the GC unit for calibrating the H₂O sensor.

Block 3 is represented for measuring trace H₂O

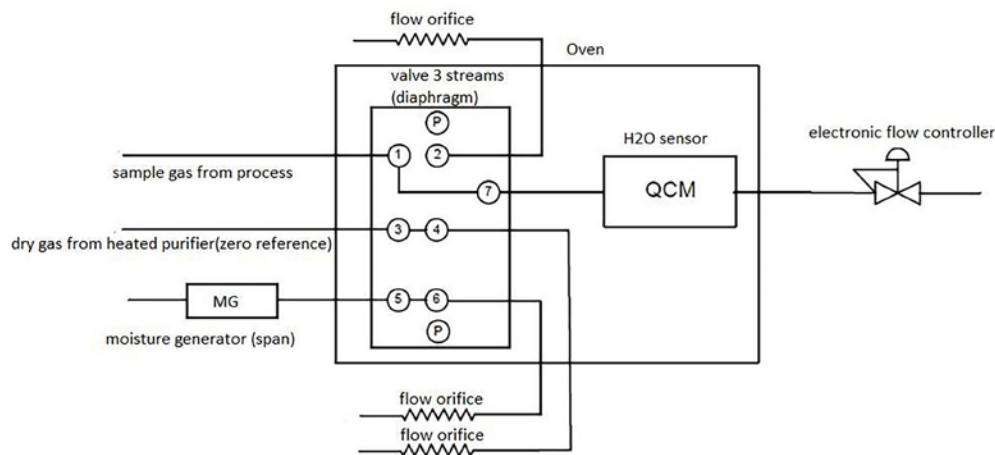

LDRACK INTEGRATED COMPLETE SOLUTION

MULTIDETEK2

GC gas analyser for measuring trace H₂-O₂-N₂-CH₄-CO-CO₂-H₂O in UHP argon.

LDGSS

ultra high purity gas stream selector system for switching between the different streams and the span calibration gas (Up to 10 streams in one device is available).


LDP1000

heated gas purifier to generate UHP grade 99.999999% from grade 99.999% for carrier gas of the GC.



RESULTS:

A chromatogram of such system with a standard gas containing trace impurities in a balance of Argon. An analysis time of less than 10 minutes is required for H₂-O₂-N₂-CH₄-CO-CO₂ and by adding the NMHC impurity, the analysis time goes to 12 minutes.

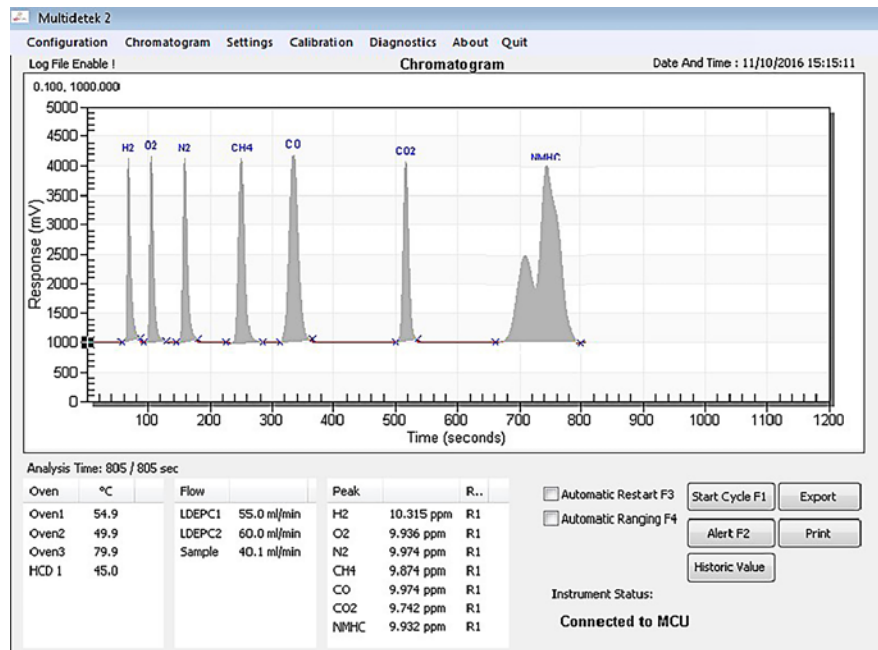

The following chart gives the limit of detection for such GC configuration

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------|---------------|-------------|--------|----------------|
| H2 | 10.315 ppm | 3202 mV | 2.4 mV | 0.023 ppm |
| O2 | 9.936 ppm | 3221 mV | 2.1 mV | 0.019 ppm |
| N2 | 9.974 ppm | 3205 mV | 1.0 mV | 0.010 ppm |
| CH4 | 9.874 ppm | 3201 mV | 2.0 mV | 0.019 ppm |
| CO | 9.974 ppm | 3251 mV | 2.6 mV | 0.024 ppm |
| CO2 | 9.742 ppm | 3191 mV | 2.3 mV | 0.021 ppm |
| NMHC | 9.932 ppm | 3051 mV | 2.1 mV | 0.021 ppm |

Figure 2 Note: other LDL could be obtained with different injection volume and chromatographic condition

CONCLUSION:

With the MultiDetek2 compact GC combined with PlasmaDetek2 detector, the analysis of trace impurities in UHP argon can be realized in one rackmount instrument with one type of detector. The use of argon as carrier gas entails a low cost of operation. On top of that, the MultiDetek2 offers all the features and industrial protocols/controls required by the industrial market for such type of application.

Our fully integrated solution LDrack combining the analytical instrument MultiDetek2 with our stream selector system LDGSS with the integrated analysis for trace H₂O makes a reliable turnkey solution for the HIP furnace manufacturers, 3D printer manufacturers and some controlled atmosphere manufacturers.

APPLICATION NOTE

LD20-04



MultiDetek2 with PlasmaDetek2 configured as online analyser for fast Crude Argon analysis



▲ MultiDetek2

▲ PlasmaDetek2

LDETEK SOLUTION:

In continuity to our application note LD12-06 that explains the benefit of measuring the trace N₂ in Crude Argon to improve the Argon production in ASU, this document will show the benefit of using our online trace N₂ in Crude Argon analyser for such type of application.


In some cases, when the oxygen concentration stays below a maximum level of 5%, it is strongly suggested to refer to our LD8000MG instrument that can measure trace nitrogen in such low percent oxygen level. Our application note LD13-03 well describes what our LD8000MG series with PED technology can offer.

When the Crude Argon analysis requires an oxygen level being over 5% up to 80-100%, then the use of our MultiDetek2 analyser with the PlasmaDetek2 detector mounted as an online gas analyser instrument is strongly suggested. Conventional gas analyser for such type of application will use a basic gas chromatograph which requires a certain analysis time and GC columns. In most cases, the analysis time isn't quick enough to be able to control and improve the Argon production level. Our MD2 analyser combined with the PED in a selective and sensitive mode can performs the nitrogen analysis in a crude argon sample gas without the need of having a GC column.

The MD2 uses a diaphragm injection valve with a micro sampling loop to inject through a straight copper catalyst-based bed. The combination of the highly selective/sensitive PED with the absorption bed makes the N₂ analysis possible within 50 seconds. With this quick analysis time, the Argon production can be improved to reduce the cost of production.

RESULTS

Chromatogram of trace ppm impurity N₂ in Crude Argon sample gas (sample contains 90% Oxygen, balance Argon)

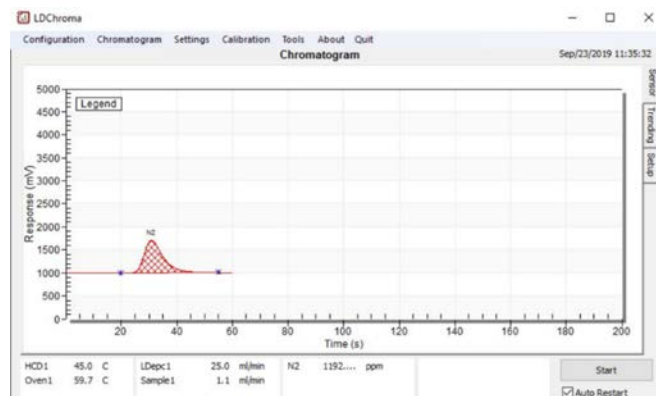

LDL is identified based on three times the noise level

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|----------------|---------------|-------------|--------|----------------|
| N ₂ | 1192 ppm | 765 mV | 1.3 mV | 6,07 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic condition

Repeatability is demonstrated here by running 12 consecutive cycles at a concentration of 1200ppm N₂ in a sample gas containing 90% Oxygen balance Argon.

| Start | N2 |
|------------------|--------------|
| 2019-09-21 04:04 | 1203.670 ppm |
| 2019-09-21 04:03 | 1202.633 ppm |
| 2019-09-21 04:02 | 1201.522 ppm |
| 2019-09-21 04:01 | 1201.335 ppm |
| 2019-09-21 03:59 | 1202.315 ppm |
| 2019-09-21 03:58 | 1203.796 ppm |
| 2019-09-21 03:57 | 1203.044 ppm |
| 2019-09-21 03:56 | 1203.868 ppm |
| 2019-09-21 03:55 | 1203.715 ppm |
| 2019-09-21 03:54 | 1203.070 ppm |
| 2019-09-21 03:53 | 1201.403 ppm |
| 2019-09-21 03:52 | 1201.770 ppm |

CONCLUSION:

The MultiDetek2 gas analyser combined with the PlasmaDetek2 detector offers the requirements for such type of application. The analysis time is quick enough to reduce the production cost of Argon in ASU. Compared to a conventional GC method, the MultiDetek2 online method here allows a straight and fast crude argon analysis. The method proposed in this document is rackmount, robust and industrial as required by this market. The system also offers a full remote control. The industrial communication protocols are all built in and must simply be selected specifically for your requirements.



3.0 APPLICATION NOTE

3.3 PETROCHEMICAL



APPLICATION NOTE

LD12-08



Analysis of Sulfurs with the PlasmaDetek

The analysis of sulfurs can now be performed using the PlasmaDetek technology. With its sulfurs selective mode, the analysis of low ppb sulfurs can be easily quantified.

PLASMADETEK CONFIGURATION:

The PlasmaDetek is configured with one output signal to be selective to sulfurs.




Figure 1: PlasmaDetek detector

This is a stand-alone detector system that requires only **argon or helium** as carrier gas to make the measurement. No need of doping gas or other devices to make it selective to sulfurs.

CHROMATOGRAPHY CONFIGURATION:

The detector can be used with different configurations to run the sulfurs analysis. As example, the H₂S and COS analysis in balance nitrogen has been tested using a 2 meter RT-XLSulfur column from Restek with a backflush to detector configuration using a 10 ports diaphragm valve. The carrier flow rate has been adjusted to 5sccm using helium (**Argon can also be used as carrier gas to reduce operational cost**).

The diaphragm valve is first set to "position on" to allow the sample injection through the chromatographic column. Most of the nitrogen and/or air are then vented out of the system. The valve position is hold to "position on" until the major parts of the nitrogen and/or air have been vented out. The valve is then set to "position off" just before the hydrogen sulfide elution time to avoid venting it out. The sulfurs impurities then flow back through the 2 meter RT-XLSulfur and goes one by one to the PlasmaDetek for analysis.

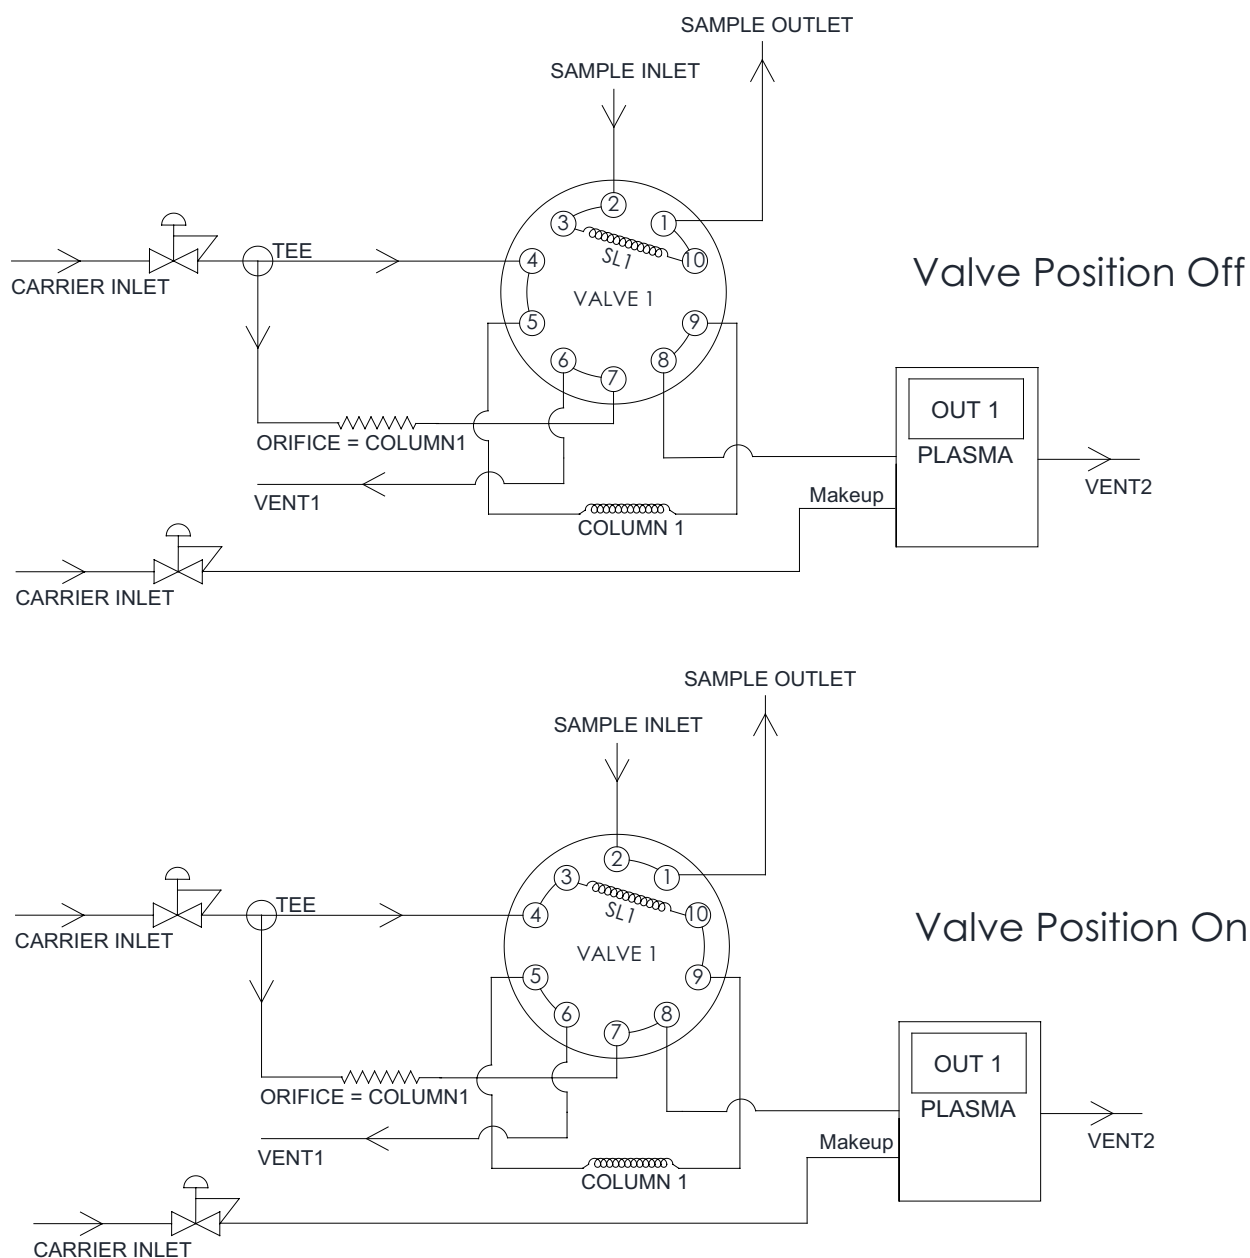

- One PlasmaDetek selective to sulfurs
- Helium carrier gas: 5 cc/min
- 1 x 10 ports diaphragm valve
- 1 x 2 meters RT-XLSulfur micro packed column
- 1 x sampling loop: 250 μ l

Figure 2: Plumbing configuration for analysis of H₂S & CO₂ in balance Nitrogen

RESULTS AND PERFORMANCE:

Figure 3 shows a chromatogram run with this configuration with a sample containing ppm H₂S and COS in a nitrogen balance. The chromatogram demonstrates the high sensitivity and selectivity to sulfurs in comparison with pure nitrogen.

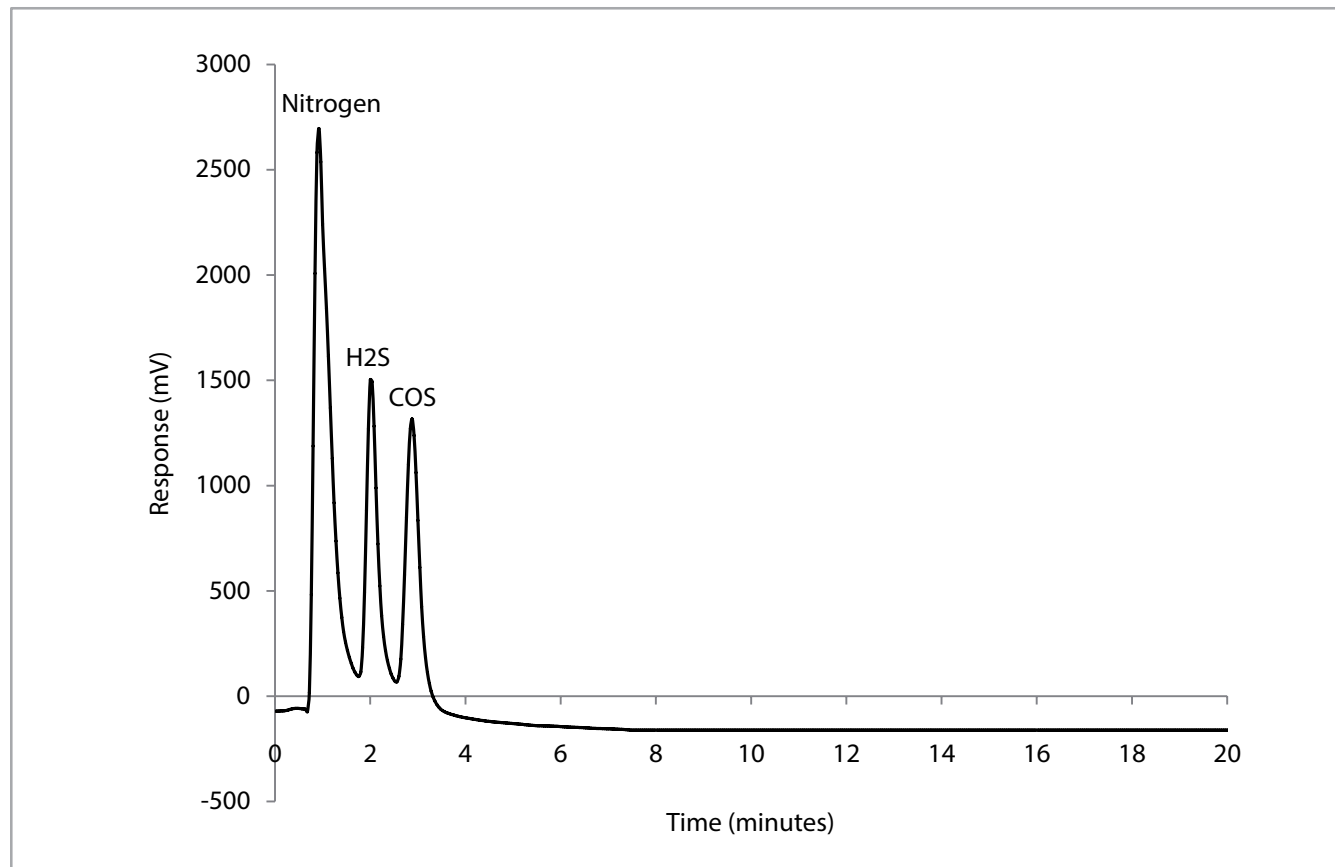


Figure 3: Mixture 10ppm H₂S, 9ppm COS in balance Nitrogen

Figure 4 shows the performance of the PlasmaDetek system obtained with the configuration described above. The results demonstrate the high level of sensitivity to sulfurs.

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | S/N | LOD (ppb) S/N = 3 | LOQ (ppb) S/N = 5 |
|------------------|---------------|-------------|----------|-------|----------------------|----------------------|
| Hydrogen sulfide | 10 ppm | 1410 mV | 0.054 mV | 26111 | 1.10 | 1.9 |
| Carbonyl sulfide | 9 ppm | 1302 mV | 0.054 mV | 24111 | 1.11 | 1.8 |

Figure 4: LOQ and LOD calculation

APPLICATIONS:

The PlasmaDetek can be easily installed in any laboratory, industrial or portable gas chromatography system. For the sulfurs analysis, the use of a portable unit is often required since the GC system needs to be moved at different locations. The ability of the PlasmaDetek to offer a quick purging and stabilization makes it ideal for portable unit like demonstrated on figure 5.



Figure 5: PlasmaDetek installed in a portable unit

CONCLUSION:

Using the PlasmaDetek, the analysis of sulfurs can be performed with success. The possibility to use argon or helium as carrier gas gives more flexibility and allows reducing operational cost. Its ability to be very sensitive to sulfurs simplifies the chromatographic configuration. This is a cost effective and maintenance free system that offers many benefits.

APPLICATION NOTE

LD13-03



Measurement of H₂S and COS in Syngas with MultiDetek 2



▲ MultiDetek 2

Syngas (Synthesis gas) a fuel gas mixture, primarily composed of hydrogen, carbon monoxide and carbon dioxide, is mainly used as intermediate in creating synthetic natural gas (SNG) or ammonia or methanol.

To be able to use a clean and environmental friendly fuel and feedstock, the sulfurs compounds must be removed. Right analysis tool is needed to ensure that the concentration of sulfurs is kept at the minimum desired level.

LDETEK SOLUTION:

The MultiDetek 2 (MD2) along with the PlasmaDetek technology bring an ideal and cost effective solution to monitor hydrogen sulfide (H₂S) and carbonyl sulfide (COS) in syngas.


Other common technologies used on the market, like SCD (Sulfur Chemiluminescence Detector) or FPD (Flame Photometric Detector), need hydrogen and air. By using the PlasmaDetek and argon as carrier gas, the MD2 gives a low cost of operation and safer solution. All safety installation for the supply of hydrogen is avoided.





▲ PlasmaDetek

A simple frontflush configuration is used to get rid of the synthesis gas background with the first column. The sulfurs compounds are then well separated by the second column and sent to the PlasmaDetek (PED) especially configured for sulfurs gases. With the use of micro packed type columns, the system can operate with very low carrier flow consumption. The use of argon as carrier gas brings the system even more interesting cause of the low operational cost due to low cost of Argon gas.



Such MultiDetek operates with column carrier flow of 5sccm. A make up gas of 20sccm is required to the detector to allow good stability and sensitivity. No additional gases or consumables parts are required what minimize the operation and installation cost.

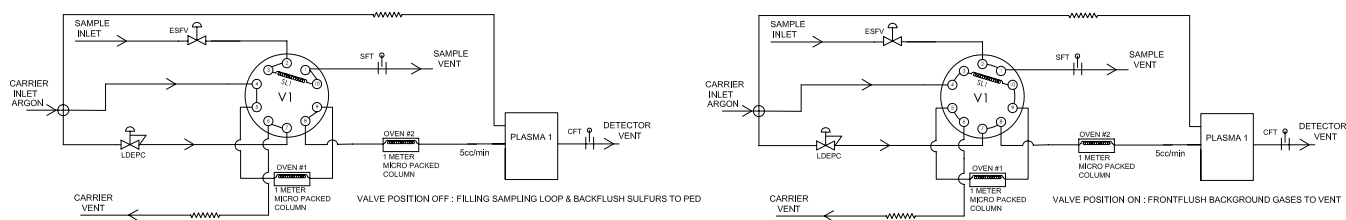

With the combination of the PlasmaDetek and argon carrier gas, detection as low as a few ppb is possible.

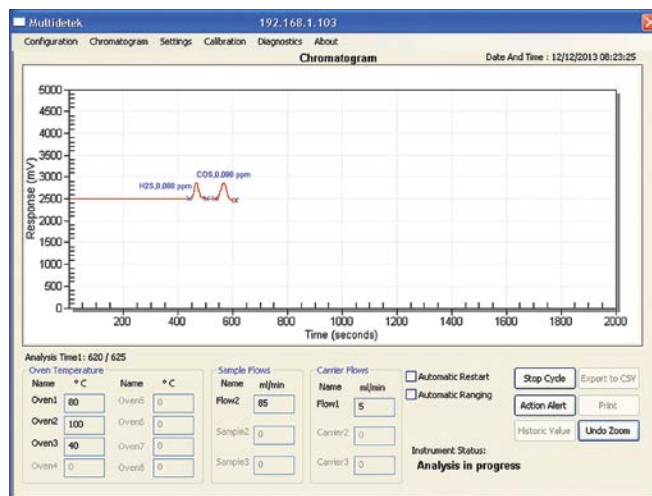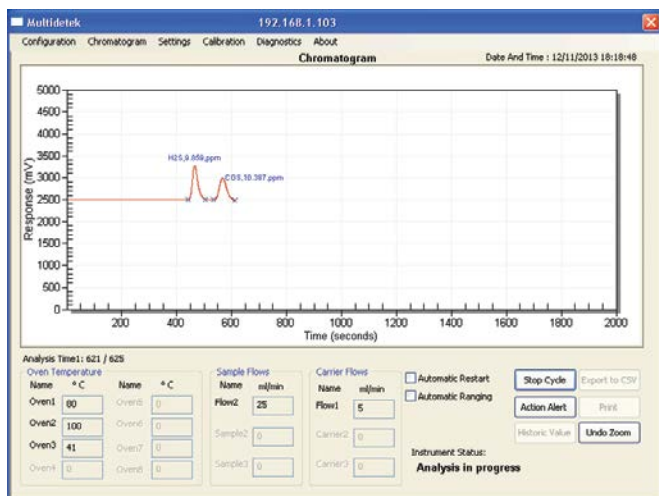

Analysis results showing stability on 19 consecutive cycles for H2S & COS at concentration of 400ppb. Then switch on span gas at 10ppm for H2S & COS, then switch on zero gas for H2S & COS.

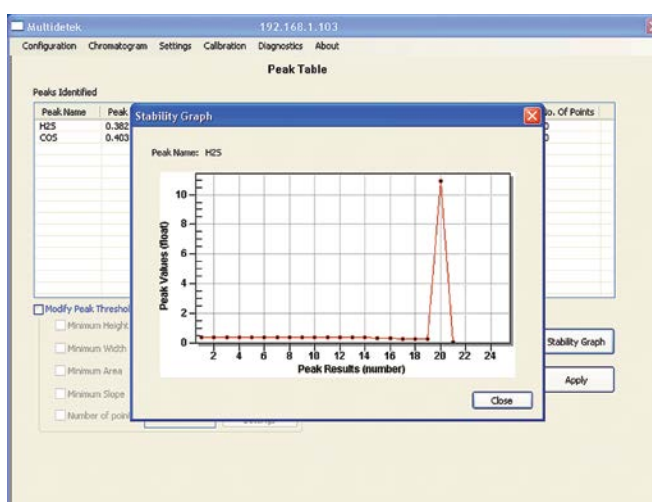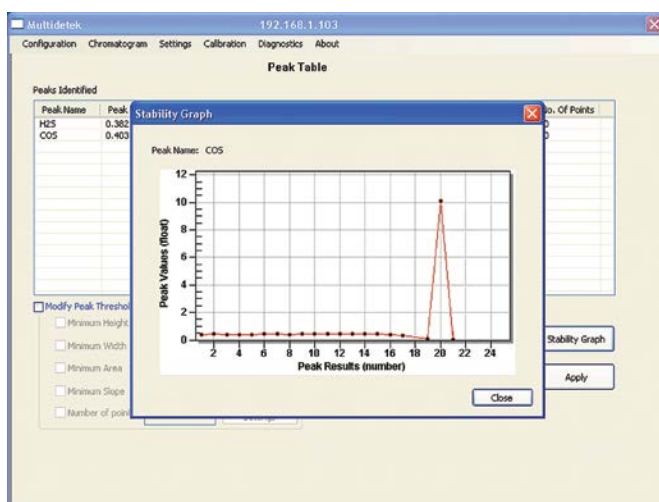

With the user friendly interface and the configuration of the MD2, it is easy to use the instrument as a process control device or simply a laboratory gas chromatograph to make sporadic analysis.

APPLICATION NOTE

LD16-05



Refinery gas analyses with MultiDetek2 compact gas chromatograph and PlasmaDetek2 gas detector



The analysis of trace permanent gases has many different fields of application in the petrochemical industry. One of the most important is for controlling the manufacturing process and the product quality. For example, some contaminants as carbon monoxide and carbon dioxide tend to deteriorate the catalysts in the propylene and ethylene polymer grade production.

An instrument for monitoring trace impurities is then required. Many different GC techniques are available on the market. Most of the techniques use a combination of TCD, FID and methanizer for the trace analysis of H₂-O₂-N₂-CH₄-CO-CO₂ in propylene and ethylene. More precisely, an FID and a methanizer are used to trace CH₄-CO and CO₂. A TCD with Hydrogen or Helium carrier gas is used to trace O₂-N₂ detection. Finally, a second TCD with Argon or Nitrogen carrier gas must be added to trace H₂ detection. These solutions require complex GC solutions with multiple detectors and multiple gas sources for carrier, fuel and air. On top of that, an FPD must be added in some cases when the trace analysis of H₂S is required.

LDETEK SOLUTION:

The MultiDetek2 compact GC solution combined with the PlasmaDetek2 (PED) can perform the analysis of low concentration H₂-O₂-N₂-CH₄-CO-CO₂ in different petrochemical gases as propylene, ethylene, propane, butylenes, butane and some others.

This solution offers the advantage of having a single detection technology based on plasma emission detector to achieve detection limits from ppb to ppm as required for this type of application. A single carrier gas source is necessary. It can be Helium or Argon depending on the availability of gases on site.


The method is configured with 2 channels merging in one PlasmaDetek2(PED). The first channel has a 10 port injection/backflush diaphragm valve with a Q Bond pre- column that allows the elution of H₂-O₂-N₂-CH₄-CO as one peak and then vent out the heavier gases. The second column is a molecular sieve used for the separation of the previously mentioned impurities that will go one by one to the PED through a diaphragm selection valve. The second channel will use the same hardware configuration as the first channel except that no molecular sieve column will be added. Then, after the elution of CO₂ through the pre- column, the heavier impurities as propylene, ethylene and others will be vented out of the system. Again, the CO₂ will be redirected to the PlasmaDete2 through the selection valve.

For some other RGA applications, it is also required to measure some light hydrocarbons and sulfurs. For these cases, the MultiDetek2 is so flexible that the configuration can be modified to achieve such measurement capability in the same compact chassis.

For example, the trace H₂S analysis can be added in the same channel as the one already used to trace CO₂ with the Q Bond column. No need to add extra detector as FPD or PFPD as generally used since the same PlasmaDetek2 can detect low concentration sulfurs. In the case that H₂S is added, then coated gas lines must be used to reduce surface adsorption. The detector doesn't have to be modified since it is made of Quartz, which is perfectly inert to trace sulfur.

For the light hydrocarbon analysis using the same MultiDetek2, a diaphragm valve network channel combined with Alumina type column and a second PlasmaDetek2 configured for hydrocarbons can be added. It is also possible to add an FID detector in the same unit if required.

THE MULTIDETEK2 CAN BE USED IN MANY DIFFERENT APPLICATION FIELDS RELATED TO THE REFINERY GAS ANALYSES.

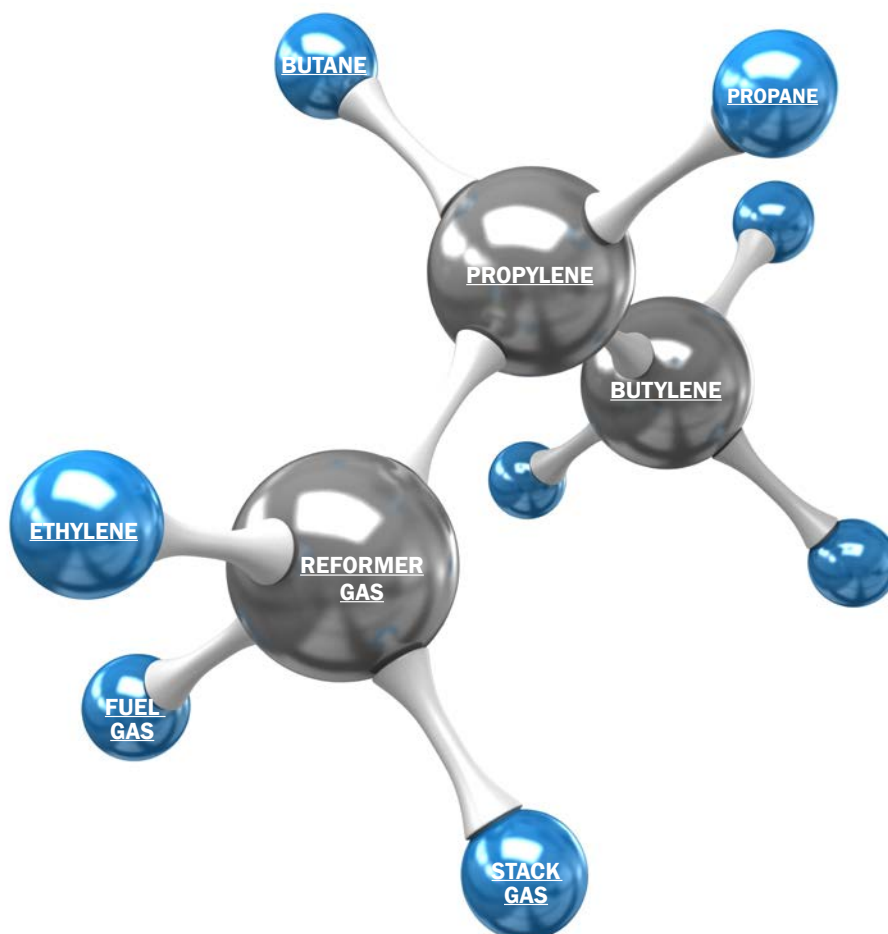

RESULTS:

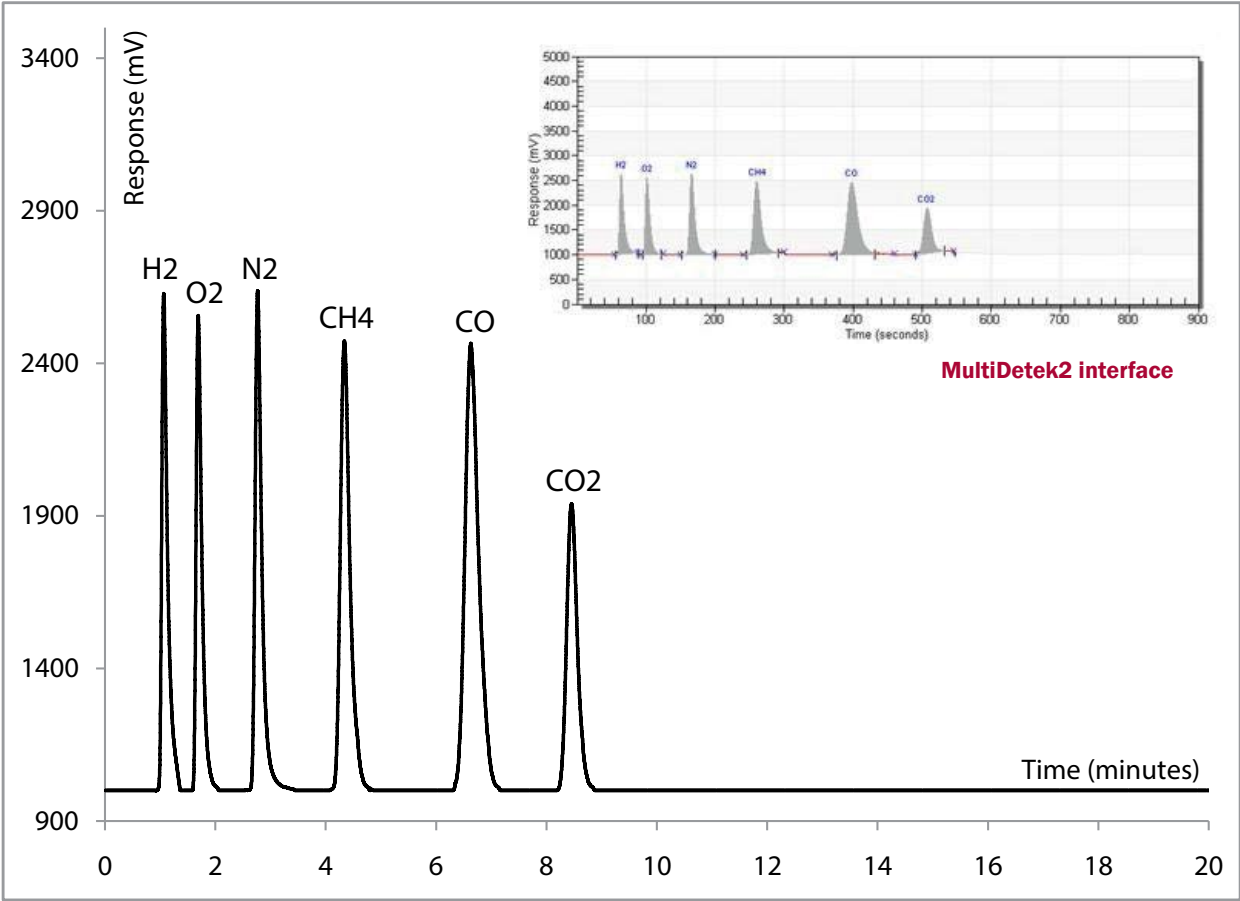


Figure 1: Chromatogram of trace impurities in balance Propylene

Historic Values

| | H2 | O2 | N2 | CH4 | CO | CO2 |
|------|-------|-------|--------|-------|-------|-------|
| 0:31 | 8.103 | 9.177 | 10.531 | 9.687 | 9.675 | 5.186 |
| 7:05 | 8.090 | 9.163 | 10.532 | 9.680 | 9.578 | 5.193 |
| 3:39 | 8.140 | 9.185 | 10.545 | 9.674 | 9.544 | 5.198 |
| 0:14 | 8.113 | 9.184 | 10.537 | 9.657 | 9.578 | 5.171 |
| 4:03 | 8.044 | 8.981 | 10.532 | 9.657 | 9.475 | 5.188 |
| 0:37 | 8.155 | 9.197 | 10.564 | 9.695 | 9.578 | 5.198 |
| 7:11 | 8.155 | 9.209 | 10.586 | 9.694 | 9.695 | 5.113 |
| 3:46 | 8.253 | 9.129 | 10.596 | 9.668 | 9.578 | 5.138 |
| 0:19 | 8.232 | 9.163 | 10.655 | 9.638 | 9.535 | 5.198 |
| 5:53 | 8.233 | 9.226 | 10.612 | 9.602 | 9.544 | 5.226 |
| 3:28 | 8.017 | 9.163 | 10.564 | 9.628 | 9.475 | 5.193 |
| 0:02 | 8.265 | 9.271 | 10.545 | 9.602 | 9.475 | 5.233 |
| 5:35 | 8.218 | 9.267 | 10.579 | 9.644 | 9.578 | 5.198 |
| 3:10 | 8.155 | 9.129 | 10.564 | 9.657 | 9.696 | 5.236 |

More... On Chart... Ok Delete Cancel

Figure 2: Results showing stability from a mixture cylinder containing trace impurities in balance gas Propylene

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------------|---------------|-------------|--------|----------------|
| H ₂ | 8.155 ppm | 2701 mV | 2.2 mV | 0.020 ppm |
| O ₂ | 9.129 ppm | 2655 mV | 1.5 mV | 0.015 ppm |
| N ₂ | 10.564 ppm | 2740 mV | 1.1 mV | 0.012 ppm |
| CH ₄ | 9.657 ppm | 2501 mV | 2 mV | 0.023 ppm |
| CO | 9.696 ppm | 2482 mV | 2.5 mV | 0.029 ppm |
| CO ₂ | 5.236 ppm | 2010 mV | 2.1 mV | 0.016 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

Figure 3: LDL based on 3 times noise ratio

CONCLUSION:

With this simple method, the MultiDetek2 compact and robust GC brings an innovative solution for this type of application. The platform also offers the standard industrial communication protocols, the remote connectivity and a built- in or external PC with software interface. The refinery gas analysis market can now have a compact, robust and flexible GC analyzer using a single detector type (PlasmaDetek2) and a single carrier type to cover the whole range of applications.

APPLICATION NOTE

LD17-01



Trace Hydrocarbons and Permanent gases in Propylene



The high purity Propylene is used for the production of Polypropylene in Petrochemical industry. The analysis of trace impurities is critical to ensure a good quality of the final product. The analysis of hydrocarbons and permanent gases are required at a level below 10ppm to ensure the good operation of the production process.

LDETEK SOLUTION:

Using the PlasmaDetek2(PED) plasma detector and the MultiDetek2 compact gas chromatograph, the analysis of the most critical trace impurities in Propylene can be achieved in one unit with a single detection technology (PED).

The main advantage of our solution is to use the same PlasmaDetek2 (PED) detector to measure trace impurities hydrocarbons and permanent gases in the same system. Usually, the alternative solutions have to combine more than one detector to be able to cover this application. Typically, FID and PDHID have to be combined, resulting of multi gas feeding for the different detectors. Our solution requires only one PED detector with only carrier gas to feed the system.

Our configuration has 4 channels having each an independent oven/column. The four channels all merge in the same PlasmaDetek2 detector. The detector is optimized with a combination of selective optic circuits especially for each impurity. This allows a good sensitivity and selectivity over the propylene background gas.

- ▶ **Channel#1:** Trace O₂, N₂, CH₄, CO
- ▶ **Channel#2:** Trace CO₂, C₂H₂, C₂H₄, C₂H₆, C₃H₈
- ▶ **Channel#3:** Trace i-C₄H₁₀, n-C₄H₁₀
- ▶ **Channel#4:** Trace t-2-C₄H₈, i-C₄H₈, i-C₅H₁₂, C-2-C₄H₈, n-C₅H₁₂, 1.3-C₄H₆

RESULTS

The chromatogram below shows an example of a typical calibration containing trace impurities in a balance gas of pure propylene. The concentrations of each impurities along with the response and detection limit are listed in the LDL chart below.



| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------------------------------|---------------|-------------|--------|----------------|
| CO ₂ | 8.024 ppm | 2820 mV | 2.2 mV | 18.8 ppb |
| C ₂ H ₂ | 9.408 ppm | 2556 mV | 2.2 mV | 24.2 ppb |
| C ₂ H ₄ | 10.574 ppm | 2899 mV | 2.2 mV | 24.0 ppb |
| C ₂ H ₆ | 12.845 ppm | 3009 mV | 2.2 mV | 28.2 ppb |
| C ₃ H ₈ | 4.386 ppm | 3086 mV | 2.9 mV | 12.3 ppb |
| O ₂ | 10.305 ppm | 1770 mV | 0.9 mV | 15.7 ppb |
| N ₂ | 9.507 ppm | 2758 mV | 1.1 mV | 11.4 ppb |
| CH ₄ | 9.892 ppm | 3176 mV | 2.2 mV | 20.5 ppb |
| CO | 9.122 ppm | 3096 mV | 2.8 mV | 24.7 ppb |
| T-2-C ₄ H ₈ | 2.165 ppm | 578 mV | 2.2 mV | 24.7 ppb |
| I-C ₄ H ₈ | 2.311 ppm | 764 mV | 2.2 mV | 19.9 ppb |
| I-C ₅ H ₁₂ | 8.887 ppm | 2865 mV | 2.2 mV | 20.5 ppb |
| C-2-C ₄ H ₈ | 9.102 ppm | 3643 mV | 2.2 mV | 16.5 ppb |
| N-C ₅ H ₁₂ | 7.994 ppm | 2424 mV | 2.2 mV | 21.8 ppb |
| I-C ₄ H ₁₀ | 9.111 ppm | 3110 mV | 2.2 mV | 19.3 ppb |
| N-C ₄ H ₁₀ | 9.291 ppm | 3121 mV | 2.2 mV | 19.6 ppb |
| 1,3C ₄ H ₆ | 4.100 ppm | 1256 mV | 2.2 mV | 21.5 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

CONCLUSION:

Our solution combining a PlasmaDetek2 (PED) with a compact GC MultiDetek2 is simple and robust for this type of application required by the market. Our solution also includes the standard industrial communication protocols to control the unit.



3.0 APPLICATION NOTE

3.4 AGRICULTURE



3.0 APPLICATION NOTES

APPLICATION NOTE

LD15-01



Measurement of hydrocarbons, including the organic hormone (Ethylene) in CO₂ production with MultiDetek-2 and PlasmaDetek-E.




MultiDetek-2

A Greenhouse CO₂ environment is commonly used for the production of organics like fruits, plants and flowers. In this case, the production and control of the CO₂ gas purity are critical to ensure the proper growth of the organics.


LDETEK SOLUTION:

The recovery of the flue gas waste is one major source of low cost CO₂ production and it is also part of an environmental well-known solution. The sample gas is extracted from the flue gas or the pure CO₂ source by the gas provider via a sampling unit. After cooling it back to an acceptable temperature, the sample is filtered and dried by sampling filters and a dew point dryer. After this step, a sample pump is simply carrying the sample with a limited flow at a fixed pressure to the MultiDetek-2 and other flue gas sensors. The analyzers are located on the outside of the catalyst building. The sample gas is pumped from the MultiDetek-2 integrated pump that is used to fill the sampling loops for analysing.

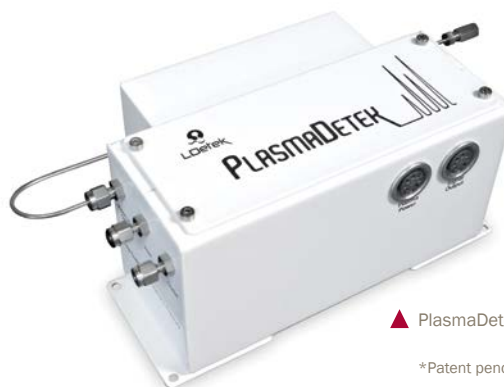


PlasmaDetek-E

*Patent pending

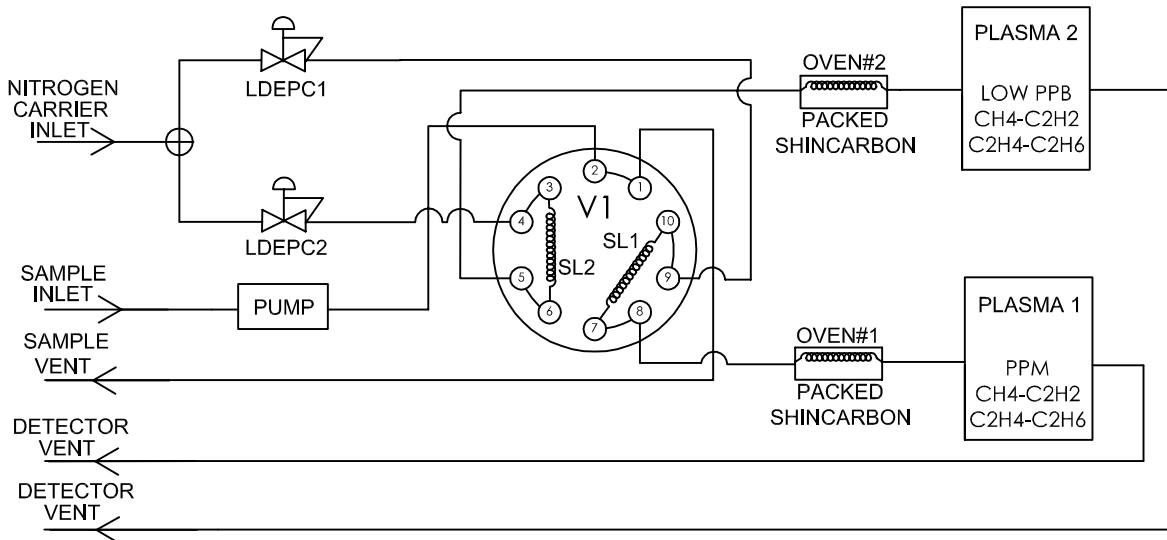

MultiDetek-2 configuration diagram 1: Valve position OFF: Filling both sampling loops

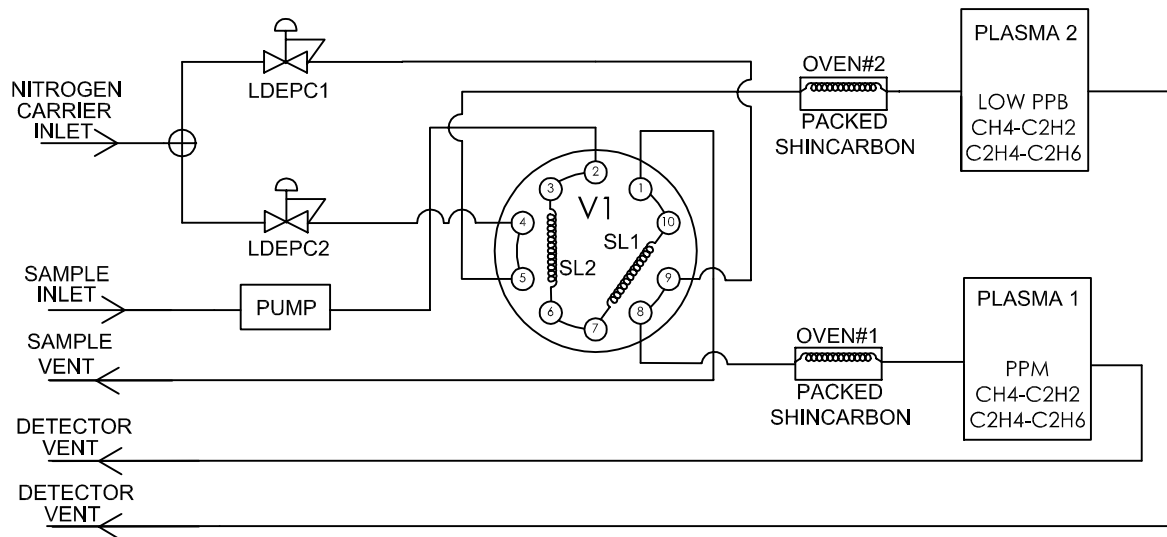


MultiDetek-2 configuration diagram 2: Valve position ON: Injecting both sampling loops in dual channels and running parallel analysis

A ten-port double injection valve is configured to inject both sampling loops at the same time through the dual channels. Each channel is configured with a Shincarbon packed column mounted in an isothermal or mini-programmable oven. The loop sizes and Plasma configurations allow a detection range going from 5ppb up to 3000ppm (other ranges are easily configurable depending on the requested application). The analysis time is speed up by using parallel chromatography technique and the possibility of using the LDetek mini-programmable ovens. This way, the high ppm and low ppb can be analyzed simultaneously to allow the full control of the process. The MultiDetek-2 will automatically select the appropriate channel depending on the sample impurity concentrations detected during the analysis.


The enhanced selectivity of the LDetek PlasmaDetek-E (patent pending) gives the possibility of using a single injection configuration. This easy to use technique improves the system performances, accelerates the analysis time and reduces the maintenance interventions.

Conventional solutions will tend to use an FID for such analysis. However, such technology requires complex and costly installation with air and fuel gas supplies. Moreover, the safety surrounding the use of an FID becomes complex. Other alternative solution to an FID is the use of a conventional HID or a PED that are non selective to hydrocarbons in CO₂ matrix. This solution will lead to the use of complex chromatography configuration with heartcut valves to remove the interference of CO₂ background gas over the hydrocarbons.

RESULTS:

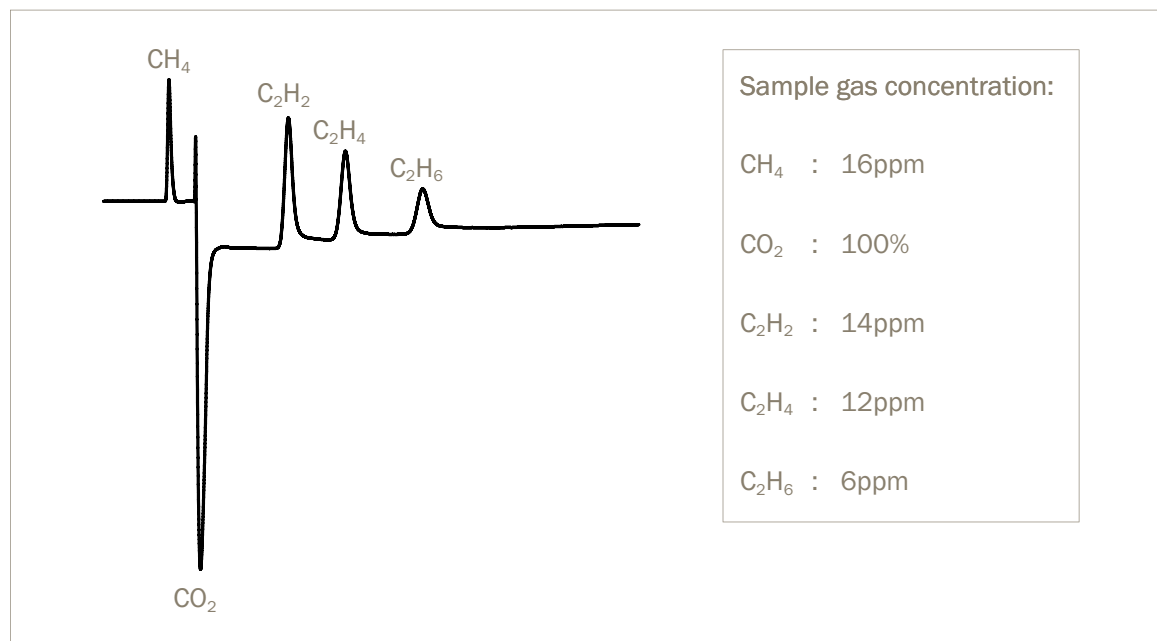

Chromatogram 1: Ppm hydrocarbon in pure CO₂ measured in MultiDetek-2 Channel #1

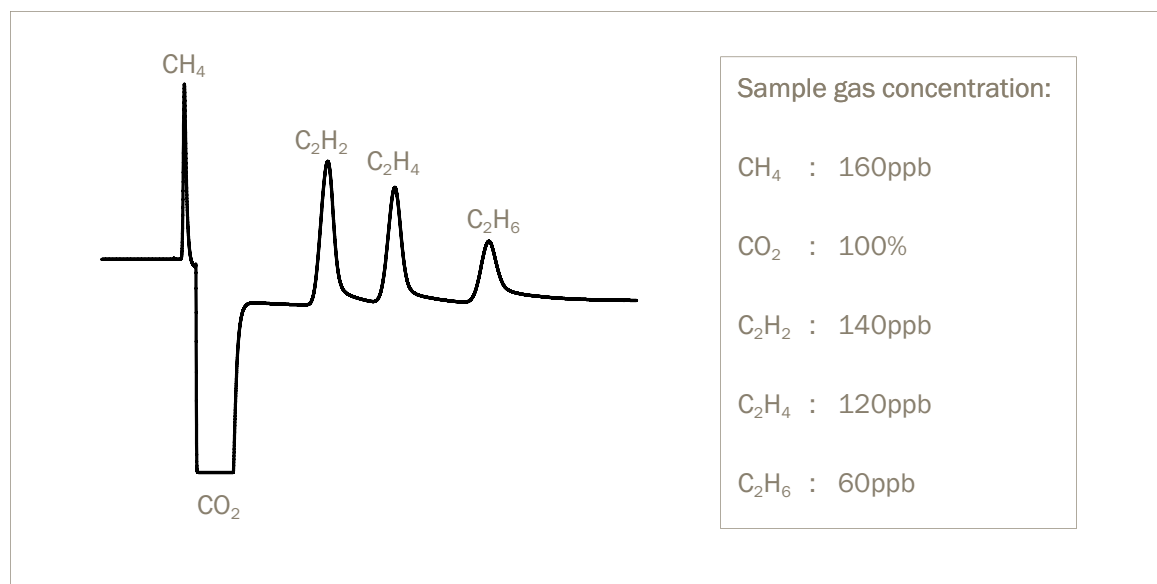

Chromatogram 2: Low ppb hydrocarbon in pure CO₂ measured in MultiDetek-2 Channel #2


CONCLUSION:

With its user-friendly interface and the simple configuration of this compact MultiDetek-2 GC, it is easy to use the instrument as a process control instrument that is a perfect fit for this Greenhouse application. Combined with the PlasmaDetek-E (patent pending) which is using a single Nitrogen source as carrier gas, this unique solution provides all the advantages to have a performing and reliable system for continuous monitoring of the CO₂ purity for Greenhouse.



3.0 APPLICATION NOTE

3.5 ELECTRONIC GASES & SEMICONDUCTOR

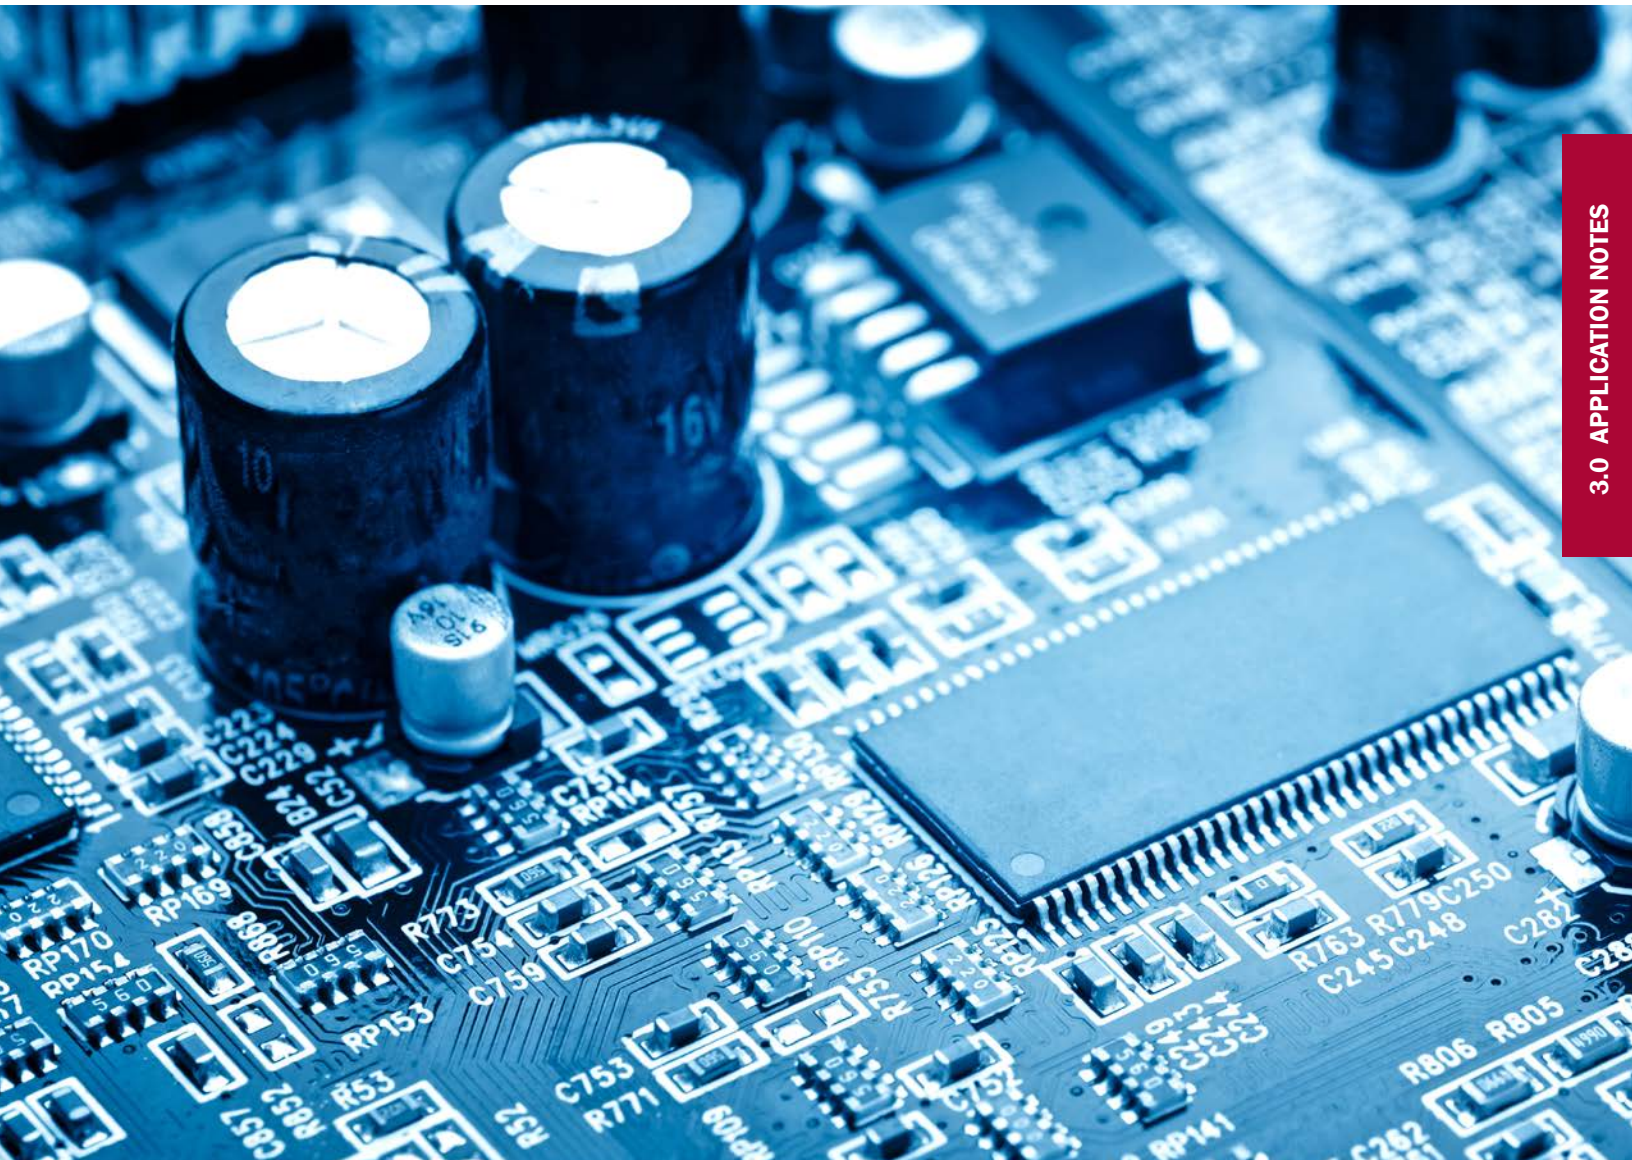

APPLICATION NOTE

LD15-02



Measurement of part per billion Ar and N2 in oxygen for semiconductor industry



MultiDetek2 ▲

The oxidation of silicon is a common and frequent step in the manufacture of integrated circuits (IC). The semiconductor industry requires the production of Ultra High Purity oxygen for the wafer production.


LDETEK SOLUTION:

The oxygen pipeline purity that goes to the semiconductor industry must be properly measured to ensure that there is no contaminant in it. It is critical and challenging to measure the ppb content of argon and nitrogen impurities in oxygen. The conventional technique used for such application is with a heated Oxy-Trap system combined with HID or conventional PED. Such technique requires a complex chromatography system with periodic Oxy-Trap regeneration with hydrogen. The operations of such system require a lot of maintenance and specialist interventions on a routine basis. The limitation of the lifetime of the trap reduces the continuous operation. Depending on the system condition, the Oxy-Trap has to be regenerated more or less once a week.

Our solution consists of eliminating all the consumables and ensuring continuous operation without maintenance and specialist intervention. Moreover, LDetek can also offer an all in one solution using the MultiDeteks-2 combined with the PlasmaDetek-E for monitoring the CO, CO2 and some hydrocarbons which are critical impurities to measure for semiconductor gases.

Measuring Ar in oxygen :

A first channel using a straight 10 port double injection diaphragm valve V1 combined with the LDetek unique ArgoTek packed column to separate part per billion argon from pure oxygen at an isothermal temperature of 45° Celsius with a carrier flow rate of 20-30sccm. The helium is used as carrier gas source. There is no need of cryogenic or Oxy-Trap system as commonly used. As simple as a basic injection through our ArgoTek packed column to conduct the accurate analysis of argon in oxygen.

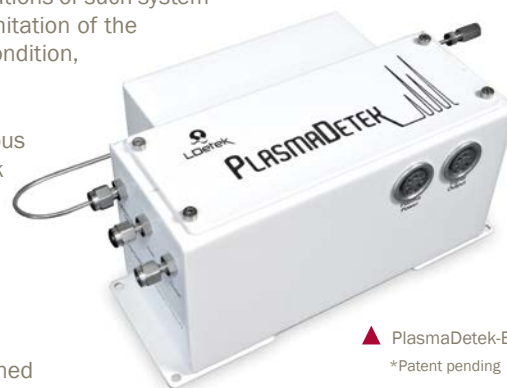


▲ PlasmaDetek-E
*Patent pending

Measuring N2 in oxygen :


A second channel still using the same straight diaphragm injection valve V1 is used to perform the analysis of N2 in oxygen with two packed molecular sieve columns combined with a Heartcut diaphragm valve V2. One more time, this configuration allows the measurement of N2 in oxygen without the use of a complex Oxy-Trap system. Both channels are selected accordingly at the right time with the selection diaphragm valve V3.

PlasmaDetek-E configuration for measuring Ar & N2 in oxygen :

The PlasmaDetek-E used for this system has a selective configuration to block the interference coming from the oxygen matrix. A specific optic circuit having its wavelength for measuring selectively the argon is mounted in the PlasmaDetek-E. Another specific optic circuit also having its wavelength for selectively measuring the N2 is in place. The appropriate optic circuit is automatically selected at the proper elution time to allow peak integration. The selectivity of the PlasmaDetek-2 for the Ar-N2 in oxygen gives the ability to have an easy to use system allowing quick analysis time even at ultra low concentration.

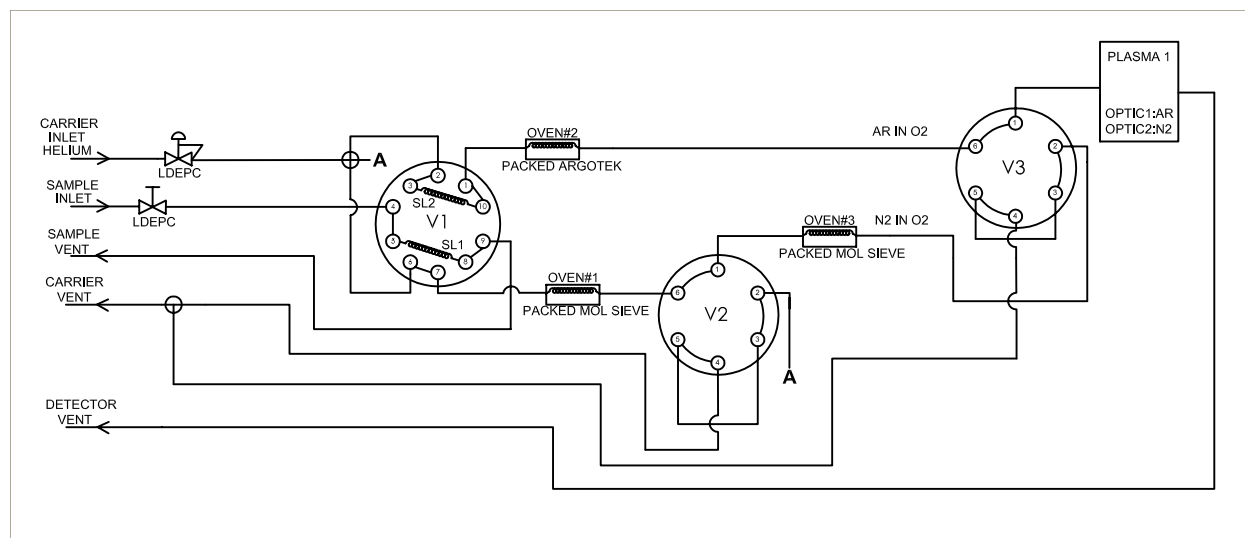

MultiDetek-2 configuration diagram 1: V1 position OFF: Filling loop #1 and injecting loop #2
V2 position OFF: Catch N2 peak from the first Packed Mol Sieve in Oven #1 to the second Packed Mol Sieve in Oven #2
V3 position OFF: Select channel #2 for Ar in O2 to the PED

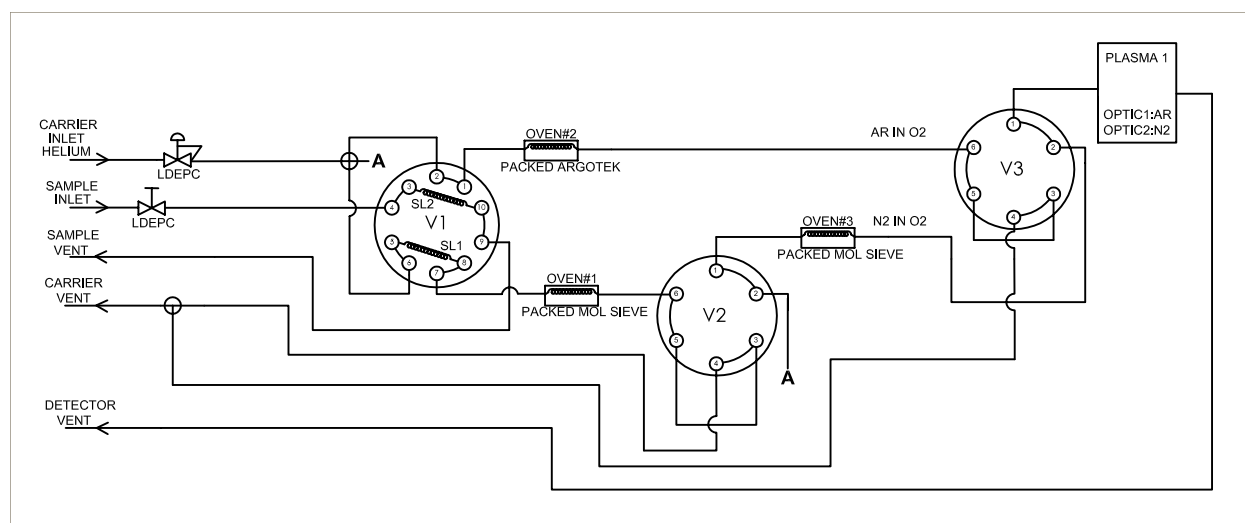


MultiDetek-2 configuration diagram 2: V1 position ON: Injecting loop #1 and filling loop #2
V2 position ON: Venting oxygen out of the system
V3 position ON: Select channel #1 for N2 in O2 to the PED

RESULTS: Linearity on a 0-10ppm range


Argon impurity

| DILUTED GAS (PPM) | CALCULATED VALUE (PPM) |
|-------------------|------------------------|
| 0.081 | 0.079 |
| 0.35 | 0.31 |
| 1.3 | 1.29 |
| 3.13 | 3.15 |
| 4.73 | 4.8 |
| 9.6 | 9.543 |

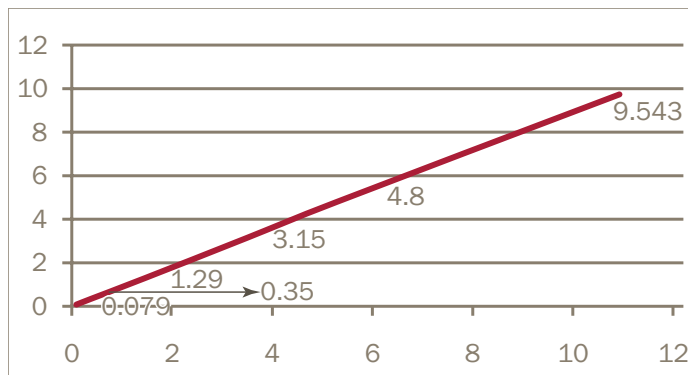


Nitrogen impurity


| DILUTED GAS (PPM) | CALCULATED VALUE (PPM) |
|-------------------|------------------------|
| 0.097 | 0.094 |
| 0.53 | 0.518 |
| 1.4 | 1.336 |
| 3.36 | 3.21 |
| 5.07 | 4.938 |
| 10.3 | 10.395 |

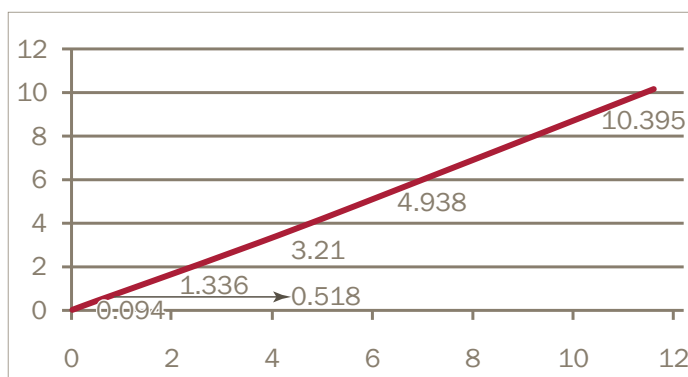


LOW PPB CHROMATOGRAM EXAMPLES:

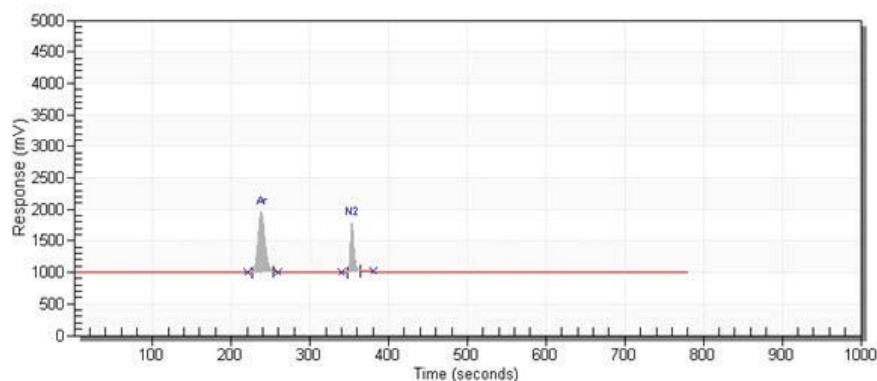

Chromatogram 1:
61ppb Ar & 77ppb N2 in pure oxygen

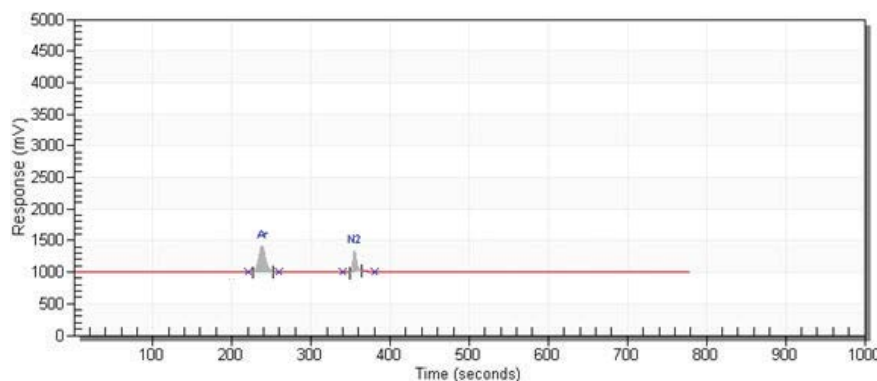

Chromatogram 2:
30ppb Ar & 38ppb N2 in pure oxygen

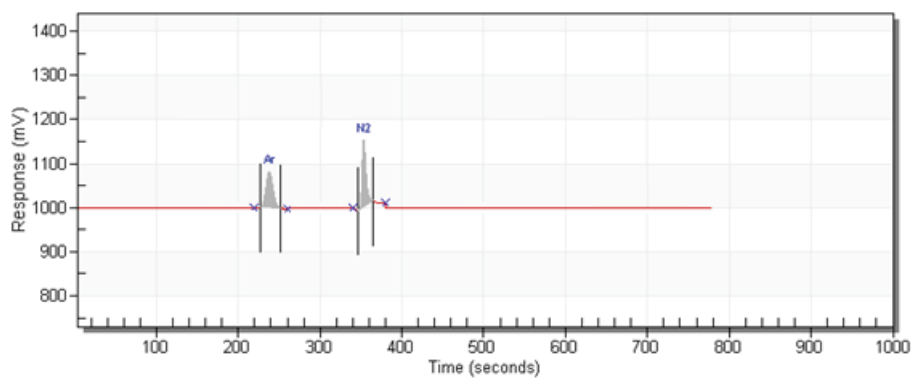

LDL calculation

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|----------------|---------------|-------------|--------|----------------|
| Ar | 3ppb | 95 mV | 1.5 mV | 0.1 ppb |
| N ₂ | 3.8ppb | 156 mV | 2.7 mV | 0.2 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

CONCLUSION:

With its user friendly interface and the simple configuration of this compact MultiDetek-2 GC, it is easy to use the instrument as a process control analyser that is a perfect fit for this semiconductor application. The enhanced sensitivity and selectivity of the PlasmaDetek-E allows extreme low limit of detection. Combined with the LDetek exclusive ArgoTek column, it makes this system perfectly suitable for semiconductor industry.

APPLICATION NOTE

LD15-04



Measurement of silane purity in electronic gases industry using PlasmaDetek-E and MultiDetek2



▲ PlasmaDetek-E
*Patent pending

▲ MultiDetek2

Silane (SiH_4), more properly known as monosilane and alternately called silicon tetrahydride or silicane, is a highly flammable and hazardous chemical compound containing silicon (87.45%) and hydrogen (12.55%). With silicon comprising 87.45% of its content by weight, pure silane is a primary source of high-purity silicon for use in industry. It is a critical gas in the manufacture of semiconductor devices, display panels and other electronic devices. The analysis of ultra low part per billion of permanent gases in silane is required for measuring the silane purity. The use of the LDetek compact & industrial MultiDetek2 GC combined with the PlasmaDetek-E is the perfect fit for this domain of application.

LDETEK SOLUTION:

Handling highly flammable gases like silane requires a high level of safety and this is what LDetek offers with its built-in sample purging and monitoring system inside the MultiDetek2 compact GC. This system consists of 4 steps of safety:


Step 1: The sample gas flow path external to the purge box is fully welded offering no possibility of leakage.

Step 2: A selection valve (V1) is mounted before the diaphragm valves used for filling the sampling loops in the system. That selection valve (V1) is configured to allow silane to go to the sampling loops only for a predetermined period of time, just before the start of each

analysis. The short period of time is configured in the factory and depends on the system configuration. The rest of the time, the selection valve (V1) is switched to a purge gas, which is normally the same gas type as the carrier gas of the system for purging the sampling loops. In the eventuality of leakage on the sampling loops or on the injection diaphragm valves, the reduced period of time introducing silane in the injection valves combined with the low pressure operation and small volume will avoid any potential hazardous situation.

Step 3: A sealed purge box containing the sample flow electronic pressure controller (LDEPC2) and the diaphragm selection valve (V1) is mounted in the MultiDetek2 chassis. That box is normally purged with the same gas type as the carrier gas used for the system. That environment requires low purge flow rate of about 10-30 sccm through a fixed orifice depending on the system configuration. The box is fully ambient air free and the system is ready to use after a short period of about 20-30 minutes depending on the system configuration. This waiting period is only required for initial start-up since once the MultiDetek2 has carrier flow going in it, the box is continuously on purge. Having a box fully purged with UHP carrier gas eliminates the ignition risk in potential presence of silane. A 1psig relief valve (RV) is mounted on the box to build up a minimum sealing pressure and to maintain a constant purge with the carrier gas.

Step 4: The sealed purge box is continuously monitored using a micro PED (PLASMA2) to selectively measure trace N2 to ensure there is no air contamination in the sealed box to avoid the ignition in the potential presence of silane. If trace of air is measured in the purge box by the micro PED (PLASMA2), then an alarm is activated to shut off the flow of silane gas inside the MultiDetek2. The shut-off valve must be mounted external to the MultiDetek2 chassis. The feedback signal controlling the shut off valve comes from the MultiDetek2. It is required to maintain the sample gas pressure coming to the shut-off valve below 10psig to minimize the risk of ignition.

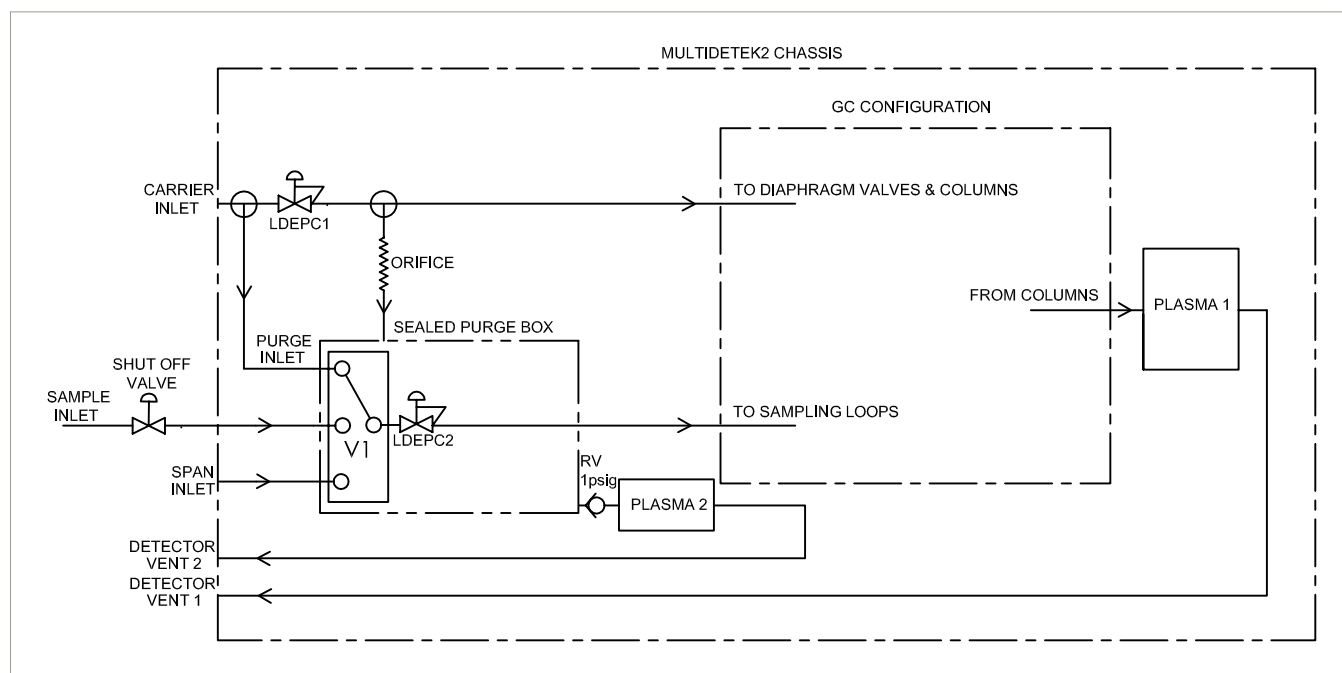

The flow type selected by the selection valve (V1) is controlled with the electronic flow controller (LDEPC2) to ensure a stable and constant flow rate whichever the selected gas type.

The GC configuration for this application is configured with Stainless Steel purge diaphragm valves and MXT column types. At the end of the GC configuration, a PlasmaDetek-E detector is configured to selectively measure the impurities requested. Multiple channels can be configured depending on the application. For this application note, the analysis of H₂-O₂-N₂-CH₄-CO is measured through channel #1 and the CO₂ through channel#2. Both channels are combined together and go in the PlasmaDetek2 detector. The highly sensitive PlasmaDetek-E allows good detection limit, what is required for silane purity.

RESULTS:

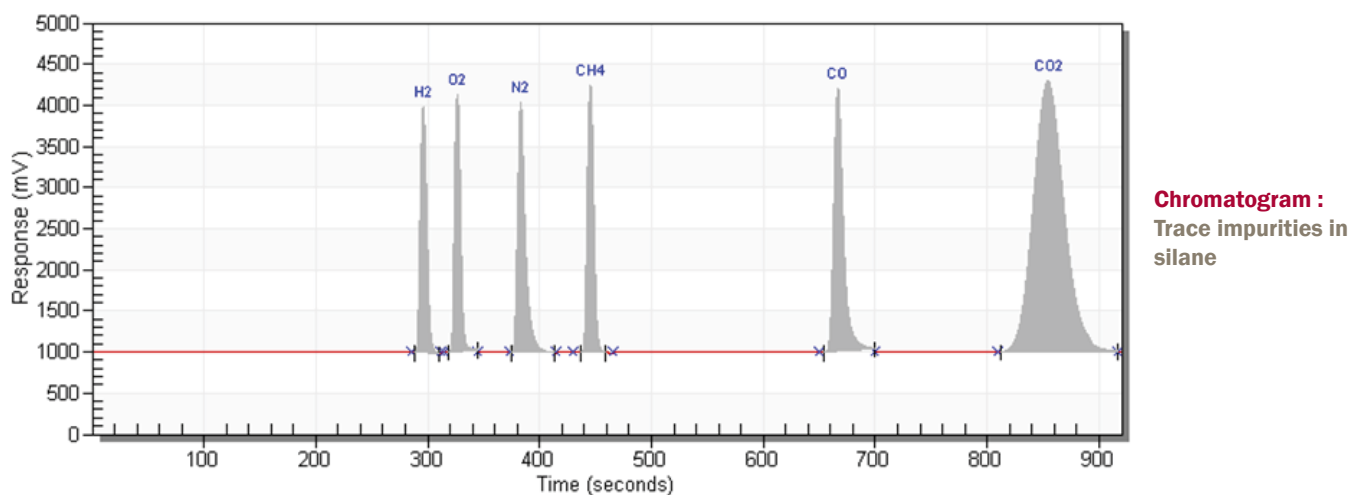


Chart : LDL calculation:

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------------|---------------|-------------|-------|----------------|
| H ₂ | 808 ppb | 2995 mV | 3 mV | 2.5 ppb |
| O ₂ | 810 ppb | 3220 mV | 3 mV | 2 ppb |
| N ₂ | 810 ppb | 3095 mV | 2 mV | 1.5 ppb |
| CH ₄ | 810 ppb | 3335 mV | 3 mV | 2 ppb |
| CO | 820 ppb | 3297 mV | 4 mV | 3 ppb |
| CO ₂ | 820 ppb | 3380 mV | 3 mV | 2 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

CONCLUSION:

The PlasmaDetek-E and the MultiDetek2 combined with the highly safe continuous monitoring sampling system allow the measurement of silane purity with reduced risk. The N₂ monitoring of the purge box is essential to ensure there is no ignition risk inside the MultiDetek2.

The measurement of trace of impurities can be performed with a relatively short analysis time, and can offer very low limit of detection what is required for silane purity.

APPLICATION NOTE

LD16-03



Measurement of part per billion H₂-NMHC-CH₄-N₂-CO₂-CO for semiconductor gases



▲ MultiDetek2

▲ PlasmaDetek2
patented

It is well known in the semiconductor industry that measuring part per billion of permanent gases in ultra high purity gases as Helium, Argon, Oxygen, Nitrogen and Hydrogen is required. Such measurement ensures quality of the product.

LDETEK SOLUTION:

Using the PlasmaDetek2 (PED) and the MultiDetek2 (GC), analyses of part per billion below 1ppb level become feasible all in one chassis. The analyses of the impurities H₂-Ar-N₂-CH₄-CO-CO₂-NMHC at concentration going down to single-digit ppb can be performed in multiple gas backgrounds. This application note will show the results obtained with a MultiDetek2 GC system having multiple configurations.

The MultiDetek2 system detection technology is based on the enhanced plasma emission detector (PlasmaDetek2). The specific configuration of the plasma detector that was used, allows a selective and sensitive detection of the desired impurities and blocks the undesired interference gases. Last years long-term work on the new patented plasma technology used for low ppb detection gives the ability to detect single-digit ppb down to 0.100ppb. It offers the capacity of measuring the complete gas matrix that appears on chart 1, all in one compact industrial GC chassis without the use of any traps as commonly installed by other GC manufacturers.

This document demonstrates the performances of the system by offering chromatograms, charts and graphs all obtained at low ppb concentration to show the real peak shapes and results. For more details about trace ppb Ar-N₂ as impurity, please refer to the application note LD15-02 that gives additional information.

BACKGROUND GASES

IMPURITIES

| CONFIGURATION NAME | RANGE | H2 (LDL) | NMHC (LDL) | CH4 (LDL) | N2 (LDL) | CO2 (LDL) | CO (LDL) |
|--------------------|----------|----------|------------|-----------|----------|-----------|----------|
| Helium | 0-500ppb | 0.350ppb | 0.400ppb | 0.300ppb | 0.100ppb | 0.300pb | 0.300ppb |
| Argon | 0-500ppb | 0.350ppb | 0.400ppb | 0.300ppb | 0.100ppb | 0.300pb | 0.300ppb |
| Oxygen | 0-500ppb | 0.350ppb | 0.550ppb | 0.400ppb | 0.200ppb | 0.400pb | 0.400ppb |
| Hydrogen | 0-500ppb | X | 0.400ppb | 0.400ppb | 0.200ppb | 0.400pb | 0.400ppb |
| Nitrogen | 0-500ppb | 0.350ppb | 0.400ppb | 0.400ppb | X | 0.400pb | 0.400ppb |

Chart 1: MultiDetek2 multiple configuration capabilities


RESULTS:

The results have been demonstrated using the most complicated configuration, which is Oxygen purity analyses. The chromatograms and results have been obtained by measuring different concentrations between 0ppb and 150ppb for the different impurities. It shows and defines the stability, the accuracy, the LDL and the linearity of such system.

ACCURACY AND STABILITY:

The accuracy is demonstrated using 3 different concentrations in the range of 0-500ppb for which ten consecutive cycles have been performed. The delta of the minimum and maximum concentrations measured for the ten consecutive cycles is calculated for each impurity. The accuracy is obtained by dividing the delta on the average results. The accuracy results must be within +/- 0.250ppb or +/-10% of the measured value.

The results indicated on the chromatograms 1, 2, 3 combined with the charts 2, 3, 4 and the figures 1, 2, 3 show well how to interpret the results.

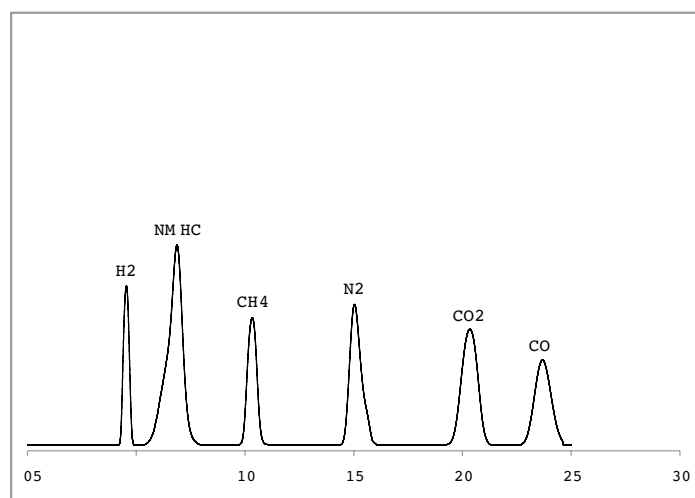


Chromatogram 1:
One chromatogram example of low ppb trace impurities used for accuracy and stability calculation. Sample gas concentration appears in chart2.

| IMPURITIES | MD2 RESULTS PPB (MIN) | MD2 RESULTS PPB (MAX) | MD2 RESULTS PPB (AVG) | MD2 RESULTS PPB (DELTA) | ACCURACY (%) |
|--------------------------|--------------------------|--------------------------|--------------------------|----------------------------|-----------------|
| Hydrogen | 111.509 | 112.417 | 111.963 | 0.908 | +/- 0.4 |
| Non methane hydrocarbons | 129.010 | 129.400 | 129.205 | 0.390 | +/- 0.15 |
| Methane | 87.502 | 87.762 | 87.632 | 0.260 | +/- 0.15 |
| Nitrogen | 124.064 | 124.672 | 124.368 | 0.608 | +/- 0.25 |
| Carbon dioxide | 84.140 | 84.682 | 84.411 | 0.542 | +/- 0.32 |
| Carbon monoxide | 95.182 | 96.089 | 95.635 | 0.907 | +/- 0.47 |

Chart 2: Accuracy & stability (Results are dependent on the system conditions and can vary)

| | H2 | NMHC | CH4 | N2 | CO2 | CO |
|----|---------|---------|--------|---------|--------|--------|
| 1 | 112.417 | 129.104 | 87.753 | 124.279 | 84.360 | 95.329 |
| 2 | 112.230 | 129.097 | 87.762 | 124.232 | 84.484 | 95.569 |
| 3 | 111.997 | 129.287 | 87.752 | 124.159 | 84.484 | 95.889 |
| 4 | 112.232 | 129.334 | 87.618 | 124.409 | 84.682 | 95.603 |
| 5 | 112.230 | 129.248 | 87.620 | 124.064 | 84.544 | 96.089 |
| 6 | 111.753 | 129.236 | 87.608 | 124.140 | 84.484 | 95.754 |
| 7 | 111.997 | 129.166 | 87.584 | 124.223 | 84.360 | 95.329 |
| 8 | 112.334 | 129.050 | 87.573 | 124.223 | 84.182 | 95.493 |
| 9 | 112.223 | 129.010 | 87.614 | 124.279 | 84.140 | 95.603 |
| 10 | 111.509 | 129.078 | 87.554 | 124.198 | 84.192 | 95.352 |
| 11 | 111.639 | 129.124 | 87.590 | 124.249 | 84.293 | 95.182 |
| 12 | 111.889 | 129.312 | 87.548 | 124.223 | 84.199 | 95.320 |
| 13 | 112.140 | 129.375 | 87.531 | 124.672 | 84.199 | 95.569 |
| 14 | 112.124 | 129.400 | 87.502 | 124.559 | 84.178 | 95.651 |

Figure 1: Results of ten consecutive cycles used for accuracy and stability calculation

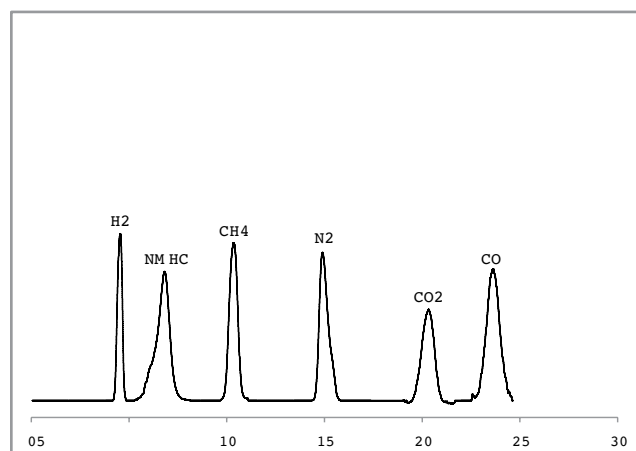

Chromatogram 2: One chromatogram example of low ppb trace impurities used for accuracy and stability calculation. Sample gas concentration appears in chart3.

| IMPURITIES | MD2 RESULTS PPB (MIN) | MD2 RESULTS PPB (MAX) | MD2 RESULTS PPB (AVG) | MD2 RESULTS PPB (DELTA) | ACCURACY (%) |
|--------------------------|--------------------------|--------------------------|--------------------------|----------------------------|-----------------|
| Hydrogen | 37.726 | 38.686 | 38.206 | 0.960 | +/- 1.25 |
| Non methane hydrocarbons | 24.927 | 25.526 | 25.226 | 0.599 | +/- 1.19 |
| Methane | 36.472 | 37.150 | 36.811 | 0.678 | +/- 0.92 |
| Nitrogen | 36.728 | 37.100 | 36.914 | 0.372 | +/- 0.50 |
| Carbon dioxide | 26.103 | 26.729 | 26.416 | 0.626 | +/- 1.18 |
| Carbon monoxide | 35.845 | 36.943 | 36.394 | 1.098 | +/- 1.50 |


Chart 3: Accuracy & stability (Results are dependent on the system conditions and can vary)

Historic Values

| | H2 | NMHC | CH4 | N2 | CO2 | CO |
|----|--------|--------|--------|--------|--------|--------|
| 1 | 38.686 | 25.526 | 37.149 | 36.728 | 26.477 | 36.773 |
| 2 | 38.562 | 25.358 | 37.031 | 36.821 | 26.544 | 36.821 |
| 3 | 38.526 | 25.216 | 37.150 | 36.658 | 26.456 | 36.730 |
| 4 | 38.531 | 25.280 | 37.107 | 36.730 | 26.103 | 36.651 |
| 5 | 38.646 | 25.328 | 37.081 | 36.845 | 26.244 | 36.556 |
| 6 | 38.187 | 25.092 | 36.990 | 36.992 | 26.434 | 36.773 |
| 7 | 38.659 | 25.150 | 36.958 | 36.996 | 26.283 | 35.951 |
| 8 | 38.642 | 25.045 | 36.773 | 36.920 | 26.578 | 35.874 |
| 9 | 38.415 | 24.927 | 36.651 | 36.939 | 26.729 | 36.587 |
| 10 | 37.726 | 24.992 | 36.556 | 36.869 | 26.662 | 36.839 |
| 11 | 38.173 | 25.076 | 36.504 | 36.951 | 26.453 | 36.943 |
| 12 | 38.291 | 25.135 | 36.501 | 36.917 | 26.529 | 36.032 |
| 13 | 37.833 | 25.198 | 36.472 | 37.083 | 26.246 | 35.845 |
| 14 | 38.321 | 25.276 | 36.594 | 37.100 | 26.171 | 35.917 |

More... On Chart... Ok Delete Cancel

Figure 2: Results of ten consecutive cycles used for accuracy and stability calculation

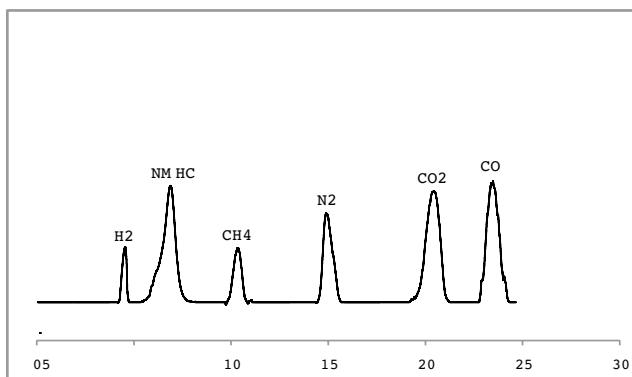

Chromatogram 3: One chromatogram example of low ppb trace impurities used for accuracy and stability calculation. Sample gas concentration appears in chart4.

| IMPURITIES | MD2 RESULTS PPB (MIN) | MD2 RESULTS PPB (MAX) | MD2 RESULTS PPB (AVG) | MD2 RESULTS PPB (DELTA max-min) | ACCURACY (%) |
|--------------------------|--------------------------|--------------------------|--------------------------|------------------------------------|-----------------|
| Hydrogen | 7.079 | 8.051 | 7.565 | 0.972 | +/- 6.42 |
| Non methane hydrocarbons | 8.985 | 9.235 | 9.110 | 0.250 | +/- 1.37 |
| Methane | 5.721 | 6.517 | 6.119 | 0.796 | +/- 6.50 |
| Nitrogen | 6.895 | 7.703 | 7.299 | 0.808 | +/- 5.53 |
| Carbon dioxide | 5.648 | 6.302 | 5.975 | 0.654 | +/- 5.47 |
| Carbon monoxide | 3.708 | 4.528 | 4.118 | 0.820 | +/- 9.95 |

Chart 4: Accuracy & stability (Results are dependent on the system conditions and can vary)

Historic Values


| | H2 | NMHC | CH4 | N2 | CO2 | CO |
|----|-------|-------|-------|-------|-------|-------|
| 1 | 7.469 | 9.170 | 5.721 | 7.547 | 5.747 | 4.215 |
| 2 | 7.703 | 9.171 | 5.825 | 7.568 | 5.694 | 4.314 |
| 3 | 8.051 | 9.154 | 6.172 | 7.549 | 5.754 | 4.528 |
| 4 | 7.783 | 9.124 | 6.169 | 7.703 | 5.932 | 4.463 |
| 5 | 8.012 | 9.077 | 6.257 | 7.700 | 6.104 | 4.386 |
| 6 | 7.789 | 9.020 | 6.266 | 7.687 | 6.302 | 4.388 |
| 7 | 7.606 | 8.985 | 5.823 | 7.682 | 6.176 | 4.275 |
| 8 | 7.343 | 9.026 | 6.311 | 7.642 | 6.062 | 4.056 |
| 9 | 7.403 | 9.071 | 6.309 | 7.522 | 5.862 | 4.068 |
| 10 | 7.162 | 9.140 | 6.334 | 7.426 | 5.848 | 4.077 |
| 11 | 7.123 | 9.229 | 6.517 | 7.547 | 5.648 | 4.143 |
| 12 | 7.079 | 9.235 | 6.234 | 7.091 | 5.660 | 3.708 |
| 13 | 7.703 | 9.164 | 6.344 | 7.011 | 5.709 | 4.234 |
| 14 | 7.364 | 9.098 | 6.373 | 6.895 | 6.200 | 4.364 |

More... On Chart... Ok Delete Cancel


Figure 3: Results of ten consecutive cycles used for accuracy and stability calculation

LOWER DETECTION LIMIT (LDL):

The limit of detection is identified by running an analysis below 5ppb of each impurity to identify the peak response height. Then, noise baseline identification is performed by running a cycle without valve actuation and measuring the noise level during the integration time of each impurity. The limit of detection (LDL) for each impurity is the relation between the peak response at a value below 5ppb and three times the noise level identified with baseline analysis. The results indicated on the chromatograms 4 & 5 combined with the chart 5 show well the performance of the system.

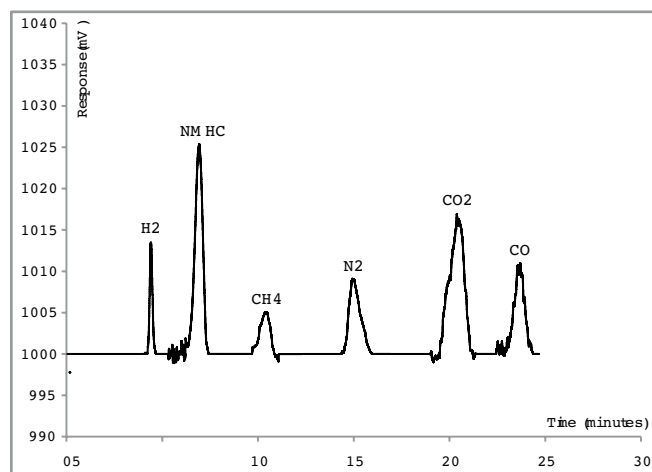

Chromatogram 4: One chromatogram example of low ppb trace impurities used for LDL calculation. Sample gas concentration appears in chart5.

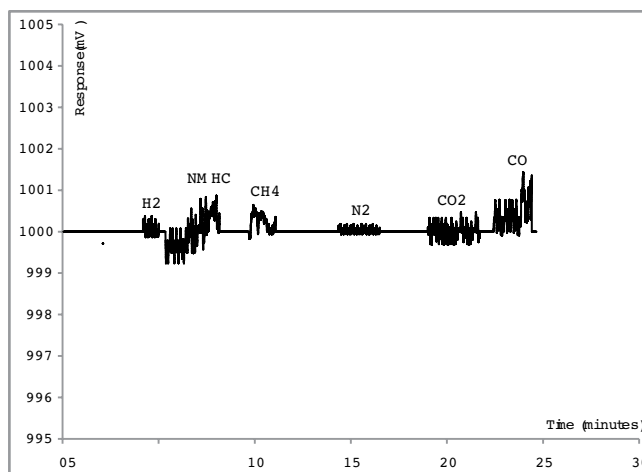




Chromatogram 5: Baseline noise analysis used for LDL calculation

| IMPURITIES | SAMPLE CONCENTRATION | RESPONSE (MV) | NOISE (MV) | 3X NOISE (MV) | LDL (PPB) (3X NOISE) |
|--------------------------|----------------------|---------------|------------|---------------|----------------------|
| Hydrogen | 3.1 | 13.49 | 0.48 | 1.44 | 0.331 |
| Non methane hydrocarbons | 3.2 | 25.34 | 1.47 | 4.41 | 0.556 |
| Methane | 0.9 | 5.01 | 0.74 | 2.22 | 0.398 |
| Nitrogen | 2.1 | 9.06 | 0.23 | 0.69 | 0.160 |
| Carbon dioxide | 2.3 | 16.93 | 0.76 | 2.28 | 0.309 |
| Carbon monoxide | 1.0 | 11 | 1.42 | 4.26 | 0.387 |




Chart 5: LDL calculation (results are dependent on the system conditions and can vary)

LINEARITY :

The linearity is calculated by running a minimum of 10 cycles at four different concentrations between 0 and 500ppb. The average of the results of the 10 cycles is used to generate the calculated values which are compared to a linear trend in relation to the known concentration values. The graphs 1-2-3-4-5 and 6 show well the good linearity results for each impurity.

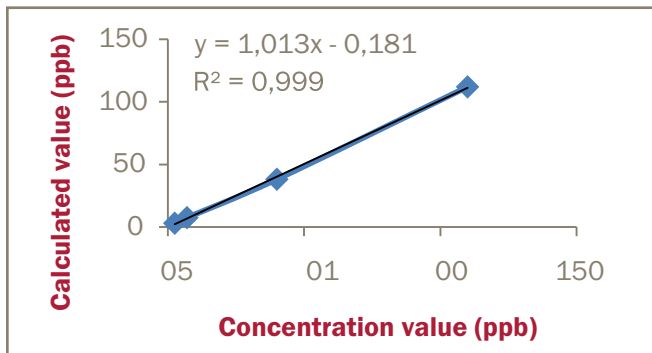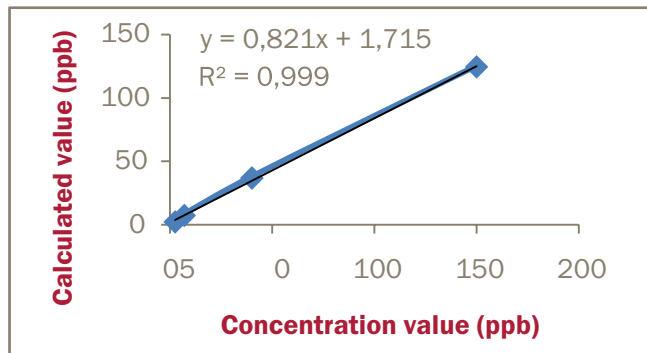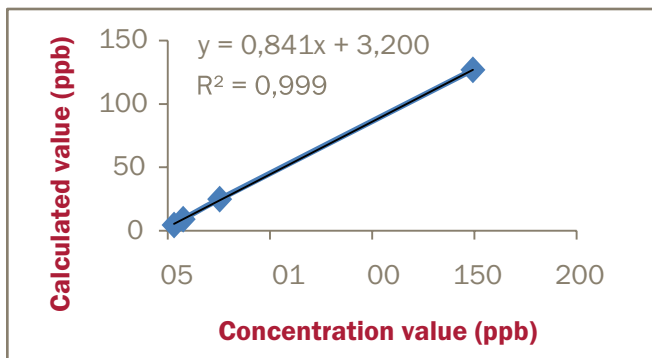Graph 1: H_2 peak linearityGraph 4: N_2 peak linearity

Graph 2: NMHC peak linearity

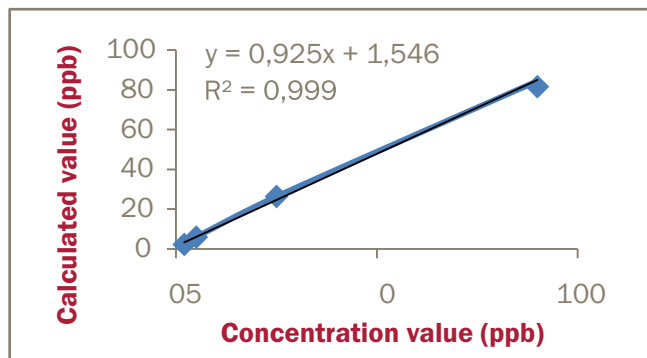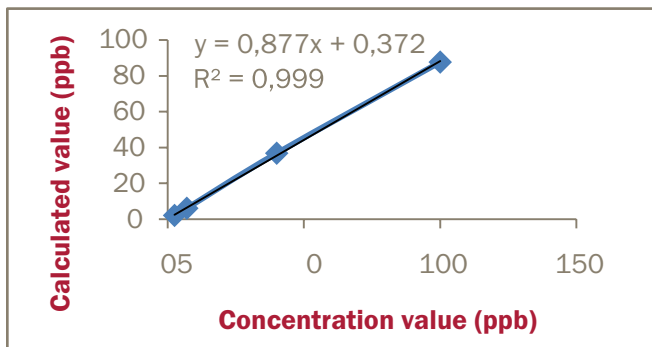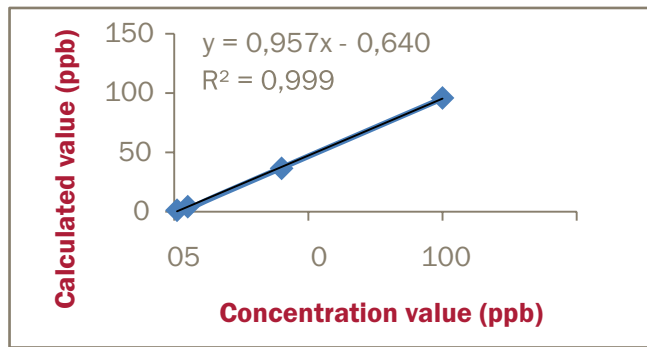Graph 5: CO_2 peak linearityGraph 3: CH_4 peak linearity

Graph 6: CO peak linearity

CONCLUSION:

Combined with the patented PlasmaDetek2, the compact, industrial and rack mount GC MultiDetek2 is a great instrument when analysis of low ppb is required. This compact system is able to manage multiple background gases in a single 6U chassis. No need of extra trap system. With its industrial design, the MultiDetek2 can manage all standard industrial communication protocols and remotely control the streams with communication with high purity LDGSS stream selector. Its remote access also gives the ability to easily support the instrument from distance. Many more features are available in this system what makes it ideal for the semiconductor market.

APPLICATION NOTE

LD18-01



Measurement of trace impurities in Germane (GeH₄) for electronic gas industry using PlasmaDetek2 and MultiDetek2



▲ MultiDetek2

▲ PlasmaDetek2
patent US 9,310,308 B2

LDETEK SOLUTION:

Handling highly flammable gas like germane (GeH₄) requires a high level of safety and it is what LDetek offers with its built-in sample purging and monitoring system inside the MultiDetek2 compact GC. This system consists of 4 steps of safety:

Step 1: The sample gas flow path external to the purged box is fully welded offering no possibility of leakage.

Step 2: A selection valve is mounted before the diaphragm valves used for filling the sampling loops in the system. That selection valve is configured to allow GeH₄ going to the sampling loops only for a pre determined period of time just before to start each analysis. The short period of time is configured in factory and is dependant to the system configuration. The rest of the time, the selection valve is switched on a purged gas which is normally the same gas type that the carrier gas of the system for purging the sampling loops. In the eventuality of leakage on the sampling loops or on the injection diaphragm valves, the reduced period of time introducing GeH₄ in the injection valves combined with the low pressure operation and small volume will avoid any potential hazardous situation.

Step 3: A sealed purge box containing the sample flow electronic pressure controller and the diaphragm selection valve is mounted in the MultiDetek2 chassis. That box is normally purged with the same gas type that the carrier gas used for the system. That environment requires low purge flow rate of about 10-30sccm through a fix orifice depending of the system configuration. The box is fully ambient air free and the system is ready to use after a short period of about 20-30minutes depending of the system configuration. This waiting period is only requires for initial start up since once the MultiDetek2 has carrier flow going in it, the box is continuously on purge. Having a box fully purged with UHP carrier gas eliminates the ignition risk in potential presence of GeH₄. A 1psig relief valve (RV) is mounted on the box to build up a minimum sealing pressure and to maintain a constant purge with the carrier gas.

Step 4: The sealed purge box is continuously monitored using a micro PED (PLASMA2) to selectively measure trace N₂ to ensure there is no air contamination in the sealed box to avoid the ignition in potential presence of GeH₄. If trace of air is measured in the purged box by the micro PED, then an alarm is activated to shut off the flow of GeH₄ gas inside the MultiDetek2. The shut off valve must be mounted external to the MultiDetek2 chassis. The feedback signal controlling the shut off valve comes from the MultiDetek2. It is requires to maintain the sample gas pressure coming to the shut off valve below 10psig to minimize the risk of ignition.

The flow type selected by the selection valve is controlled with the electronic flow controller to ensure a stable and constant flow rate whichever the gas type selected.

The GC configuration for this application is configured with Stainless Steel purged diaphragm valves and MXT column types. At the end of the GC configuration, the PlasmaDetek-2 detector is configured to selectively measure the impurities requested. Multiple channels can be configured depending of the application. For this application note, the MultiDetek2 GC is configured as follow:

Trace impurities C₂H₂-C₂H₄-C₂H₆ → is measured through channel #1


Trace impurities Ar → is measured through channel #2

Trace impurities CO-CO₂ → is measured through channel #3

Trace impurities H₂-O₂-N₂-CH₄ → is measured through channel #4

RESULTS:

Chromatograms : Trace impurities in GeH₄

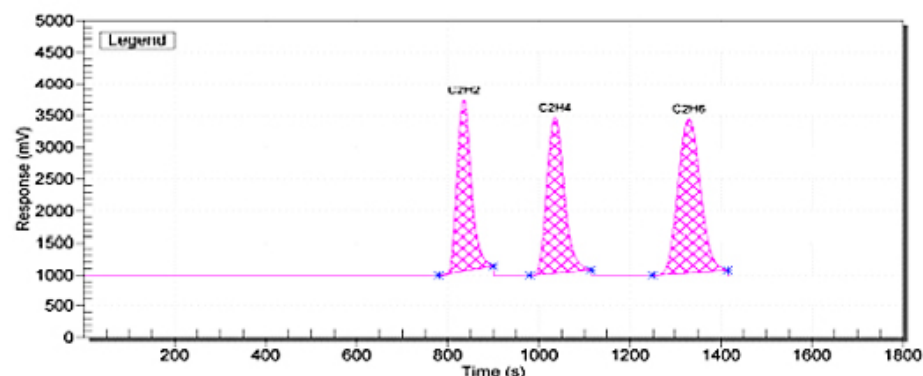

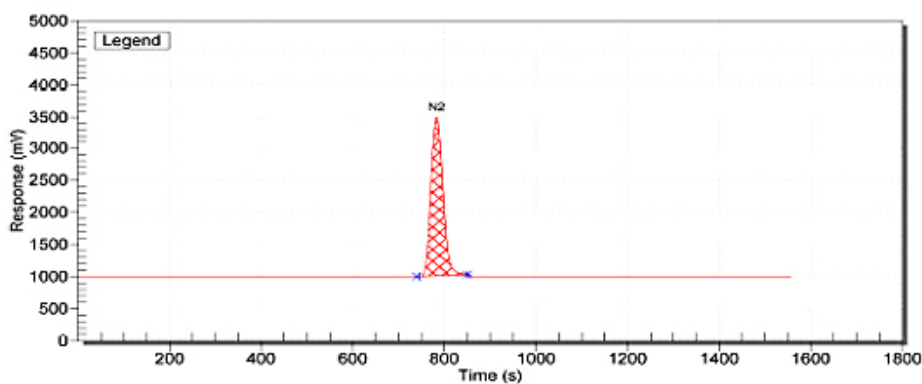
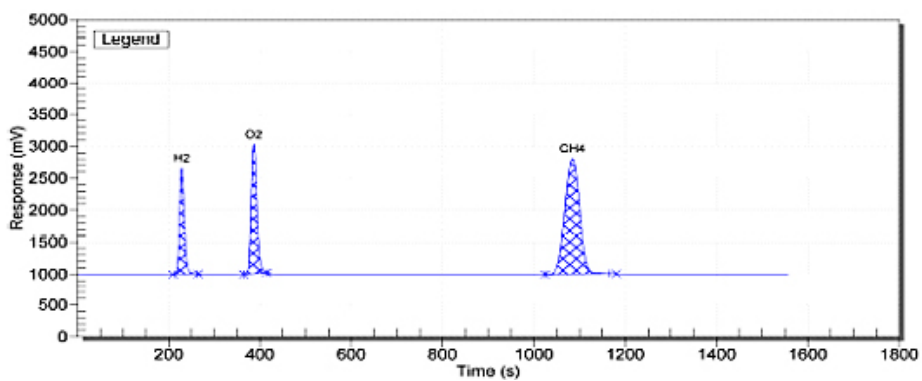
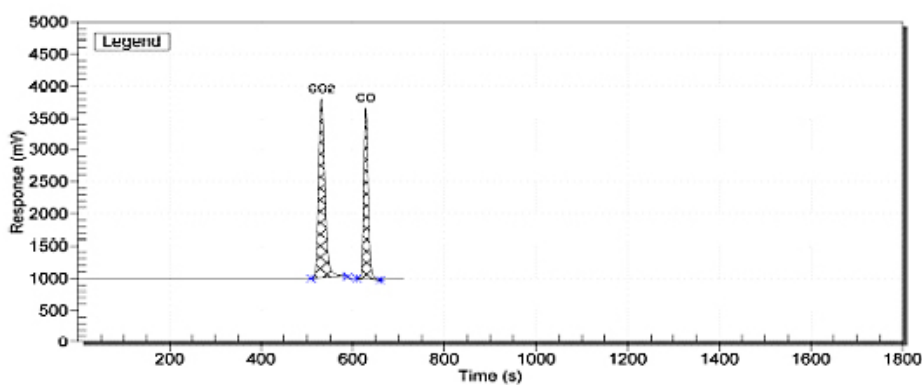
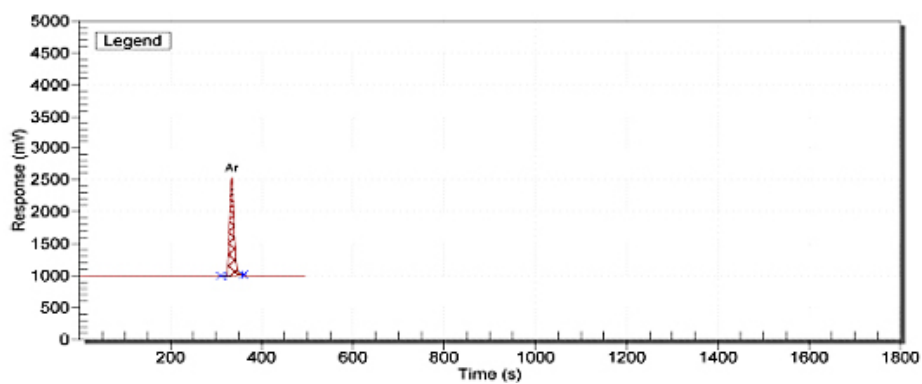


CHART: RESULTS, RESPONSE AND LDL CALCULATION

| COMPONENTS | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|------------|---------------|-------------|--------|----------------|
| C2H2 | 5.2 ppm | 2720 mV | 2.8 mV | 0.016 ppm |
| C2H4 | 4.9 ppm | 2495 mV | 2.8 mV | 0.016 ppm |
| C2H6 | 4.9 ppm | 2433 mV | 2.8 mV | 0.017 ppm |
| Ar | 3.1 ppm | 1544 mV | 1.1 mV | 0.006 ppm |
| CO2 | 4.7 ppm | 2802 mV | 2.1 mV | 0.010 ppm |
| CO | 4.6 ppm | 2705 mV | 2.1 mV | 0.010 ppm |
| H2 | 3.9 ppm | 1701 mV | 2.6 mV | 0.018 ppm |
| O2 | 4.1 ppm | 2065 mV | 2.6 mV | 0.015 ppm |
| CH4 | 3.6 ppm | 1789 mV | 2.6 mV | 0.016 ppm |
| N2 | 3.7 ppm | 2505 mV | 0.7 mV | 0.003 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic condition

CONCLUSION:

The PlasmaDetek2 and the MultiDetek2 combined with the highly safe continuous monitoring sampling system allows the measurement of GeH4 purity with reduced risk. The N2 monitoring of the purged box is essential to ensure there is no ignition risk inside the MultiDetek2.


The trace impurities measurement can be realized with a relatively short analysis time and can offer very low limit of detection of the measured impurities what is required for GeH4 purity analysis.

APPLICATION NOTE

LD18-02



Measurement of part per billion H₂-CO-N₂-CH₄-CO₂ in UHP gases for semiconductor

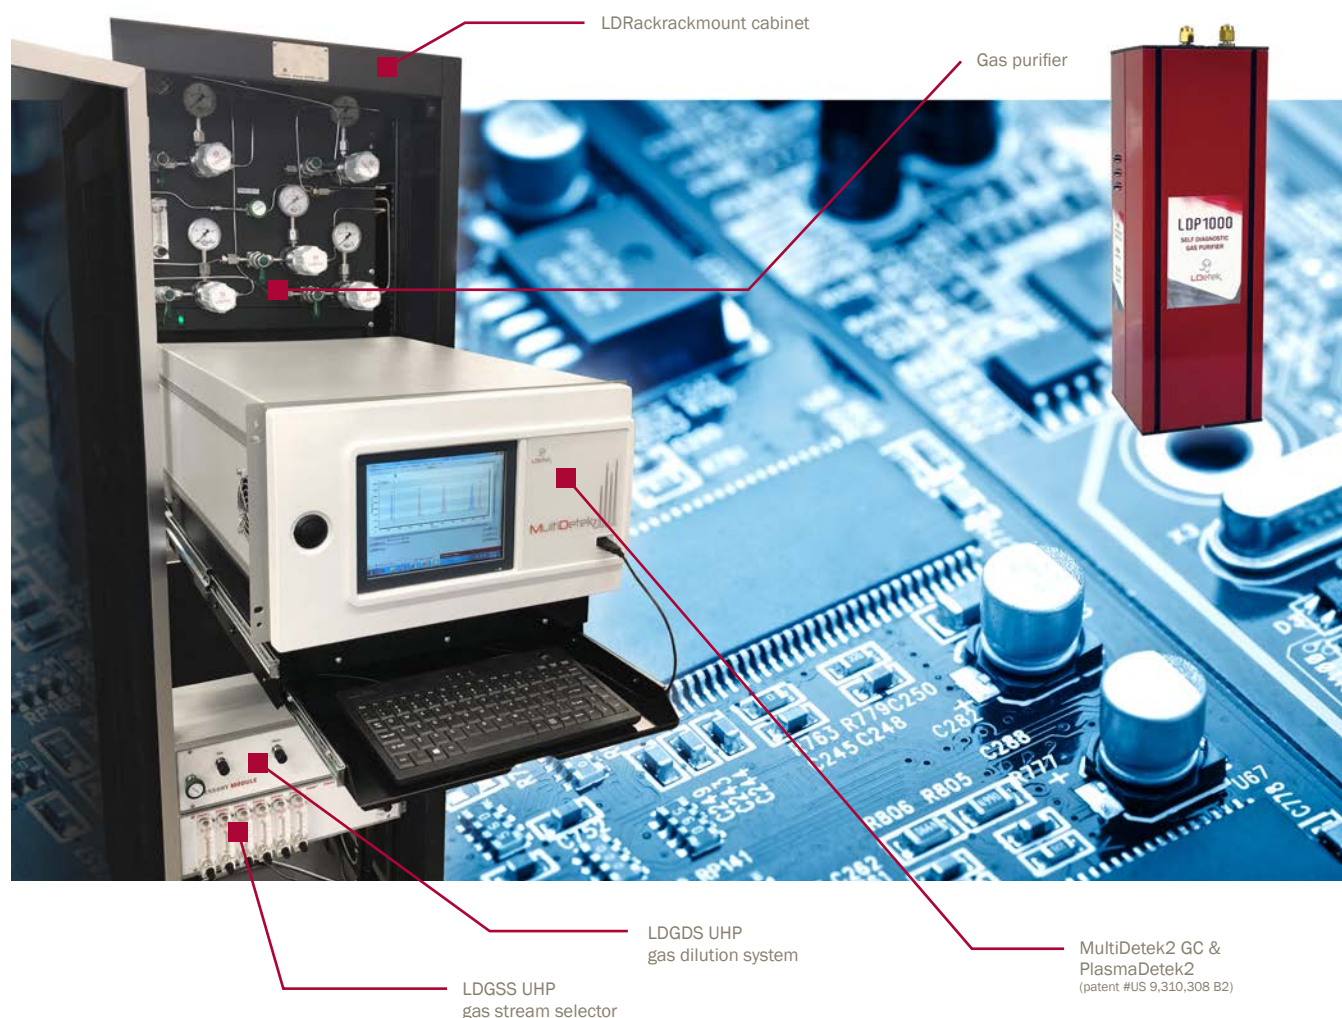

It is well known in the semiconductor industry that measuring part per billion of permanent gases in ultra high purity gases as Helium, Argon, Oxygen, Nitrogen and Hydrogen is required. Such measurement ensures quality of the product.

LDETEK SOLUTION:

Using the PlasmaDetek2 (PED) and the MultiDetek2 (GC), analyses of part per billion below 1ppb level become feasible all in one enclosure. The analyses of trace sub ppb impurities of H₂-Ar-N₂-CH₄-CO-CO₂-NMHC can be performed in multiple gas backgrounds. This application note will show the results obtained for sub ppb trace H₂-CO-N₂-CH₄-CO₂ in Argon-Helium-Oxygen.

The MultiDetek2 system detection technology is based on the enhanced plasma emission detector (PlasmaDetek2). The specific configuration of the plasma detector that was used, allows a selective and sensitive detection of the desired impurities and blocks the undesired interference gases. Last years long-term work on the patented plasma technology used for low ppb detection gives the ability to detect single-digit ppb down to 0.100ppb. It offers the capacity of measuring the complete gas matrix that appears on chart 1, all in one compact industrial GC chassis without the use of any traps and/or FID as commonly installed by other GC manufacturers.

This document demonstrates the performances of the system by offering chromatograms all obtained at low ppb concentration to show the real peak shapes and results in an industrial environment. For more details about other UHP gases application notes for SEMI , please refer to the application note LD15-02 and LD16-03 that give additional information.

| BACKGROUND GASES | | IMPURITIES | | | | | |
|--------------------|----------|----------------------|------------|-----------------------|----------------------|-----------------------|----------|
| CONFIGURATION NAME | RANGE | H ₂ (LDL) | NMHC (LDL) | CH ₄ (LDL) | N ₂ (LDL) | CO ₂ (LDL) | CO (LDL) |
| Helium | 0-500ppb | 0.350ppb | 0.400ppb | 0.300ppb | 0.100ppb | 0.300pb | 0.300ppb |
| Argon | 0-500ppb | 0.350ppb | 0.400ppb | 0.300ppb | 0.100ppb | 0.300pb | 0.300ppb |
| Oxygen | 0-500ppb | 0.350ppb | 0.550ppb | 0.400ppb | 0.200ppb | 0.400pb | 0.400ppb |
| Hydrogen | 0-500ppb | X | 0.400ppb | 0.400ppb | 0.200ppb | 0.400pb | 0.400ppb |
| Nitrogen | 0-500ppb | 0.350ppb | 0.400ppb | 0.400ppb | X | 0.400pb | 0.400ppb |


Chart 1: MultiDetek2 multiple configuration capabilities

RESULTS:

The results demonstrated have been performed in a real industrial environment. The chromatograms and results have been obtained by measuring different concentrations between 0ppb and 100ppb for the different impurities. It shows and defines the stability, the accuracy, and the LDL.

Our tests have been performed using our LDGDS gas dilution system to generate real low ppb concentrations. Our LDL results are based on real dilutions and not based on a signal to noise ratio.


CHROMATOGRAM AT 100PPB

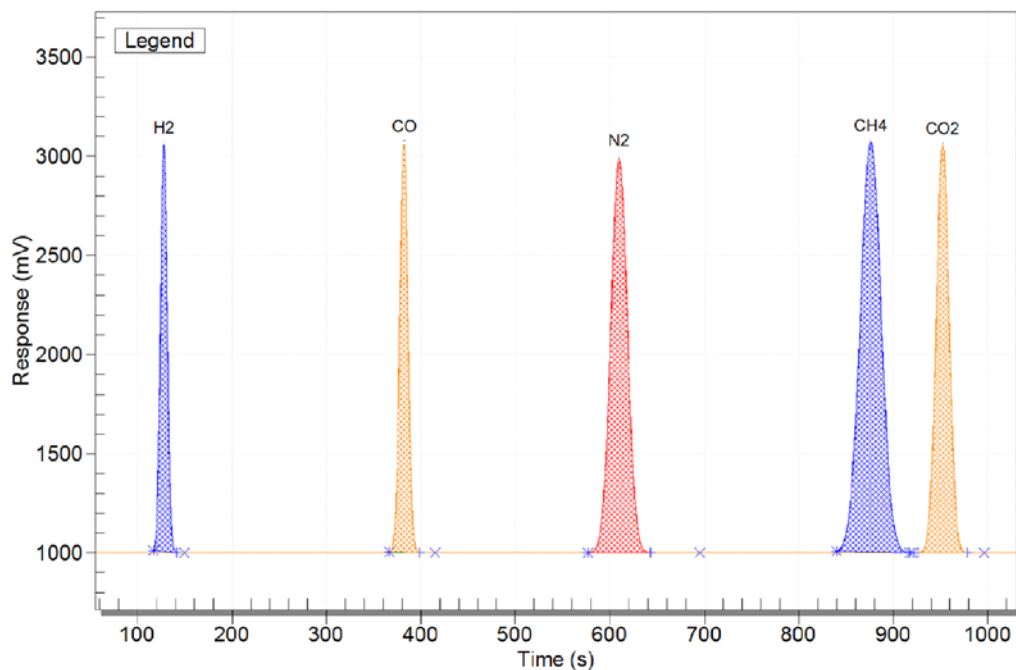

STABILITY/ACCURACY CHART AT 100PPB

| 100ppb | H2 | CO | N2 | CH4 | CO2 |
|----------------------------|---------|---------|---------|---------|---------|
| sam, 24 mars 2018 09:19:01 | 100.057 | 99.980 | 100.157 | 100.135 | 100.439 |
| sam, 24 mars 2018 09:35:15 | 100.165 | 99.960 | 100.169 | 100.074 | 100.400 |
| sam, 24 mars 2018 09:53:39 | 100.132 | 100.056 | 100.199 | 100.079 | 100.517 |
| sam, 24 mars 2018 10:12:03 | 100.110 | 100.164 | 100.219 | 100.111 | 100.500 |
| sam, 24 mars 2018 10:28:01 | 100.094 | 100.116 | 100.239 | 100.114 | 100.424 |
| sam, 24 mars 2018 10:46:25 | 100.116 | 100.069 | 100.330 | 100.217 | 100.361 |
| sam, 24 mars 2018 11:04:49 | 100.209 | 100.060 | 100.381 | 100.275 | 100.471 |
| sam, 24 mars 2018 11:23:14 | 100.276 | 100.012 | 100.217 | 100.296 | 100.488 |
| sam, 24 mars 2018 11:39:14 | 100.250 | 100.051 | 100.275 | 100.345 | 100.546 |
| sam, 24 mars 2018 11:57:36 | 100.236 | 100.127 | 100.252 | 100.320 | 100.589 |
| min | 100.057 | 99.960 | 100.157 | 100.074 | 100.361 |
| max | 100.276 | 100.164 | 100.381 | 100.345 | 100.589 |
| diff | 0.219 | 0.204 | 0.224 | 0.271 | 0.228 |
| avg | 100.165 | 100.060 | 100.244 | 100.197 | 100.474 |


CHROMATOGRAM AT 25PPB

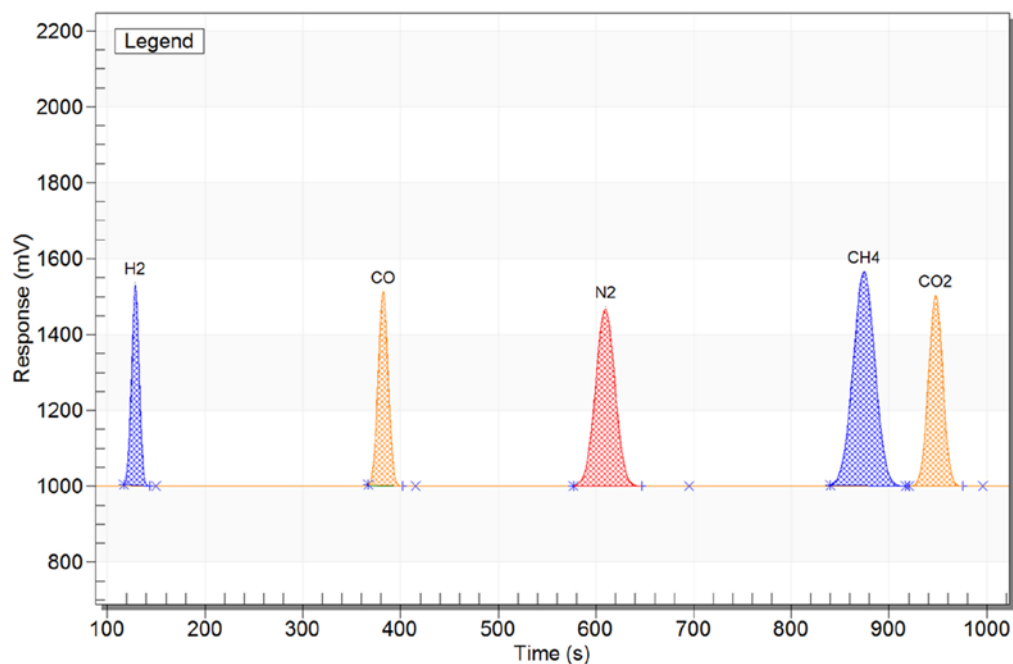

STABILITY/ACCURACY CHART AT 25PPB

| 25ppb | H2 | CO | N2 | CH4 | CO2 |
|----------------------------|--------|--------|--------|--------|--------|
| lun, 19 mars 2018 19:33:30 | 26.431 | 28.258 | 23.472 | 25.897 | 24.918 |
| lun, 19 mars 2018 19:49:30 | 26.427 | 28.350 | 23.295 | 25.889 | 24.966 |
| lun, 19 mars 2018 20:07:53 | 26.349 | 28.178 | 23.403 | 26.019 | 25.157 |
| lun, 19 mars 2018 21:41:40 | 26.511 | 28.144 | 23.519 | 26.096 | 24.971 |
| lun, 19 mars 2018 21:57:36 | 26.520 | 28.324 | 23.457 | 25.844 | 25.030 |
| lun, 19 mars 2018 22:15:59 | 26.665 | 28.475 | 23.351 | 25.974 | 25.074 |
| lun, 19 mars 2018 22:34:21 | 26.521 | 28.361 | 23.383 | 26.153 | 25.042 |
| lun, 19 mars 2018 22:50:29 | 26.520 | 28.431 | 23.363 | 25.981 | 24.959 |
| lun, 19 mars 2018 23:08:54 | 26.539 | 28.457 | 23.369 | 26.003 | 25.074 |
| lun, 19 mars 2018 23:27:17 | 26.477 | 28.155 | 23.319 | 26.037 | 25.215 |
| min | 26.349 | 28.144 | 23.295 | 25.844 | 24.918 |
| max | 26.665 | 28.475 | 23.519 | 26.153 | 25.215 |
| diff | 0.316 | 0.331 | 0.224 | 0.309 | 0.297 |
| avg | 26.496 | 28.313 | 23.393 | 25.989 | 25.041 |


CHROMATOGRAM AT 4PPB

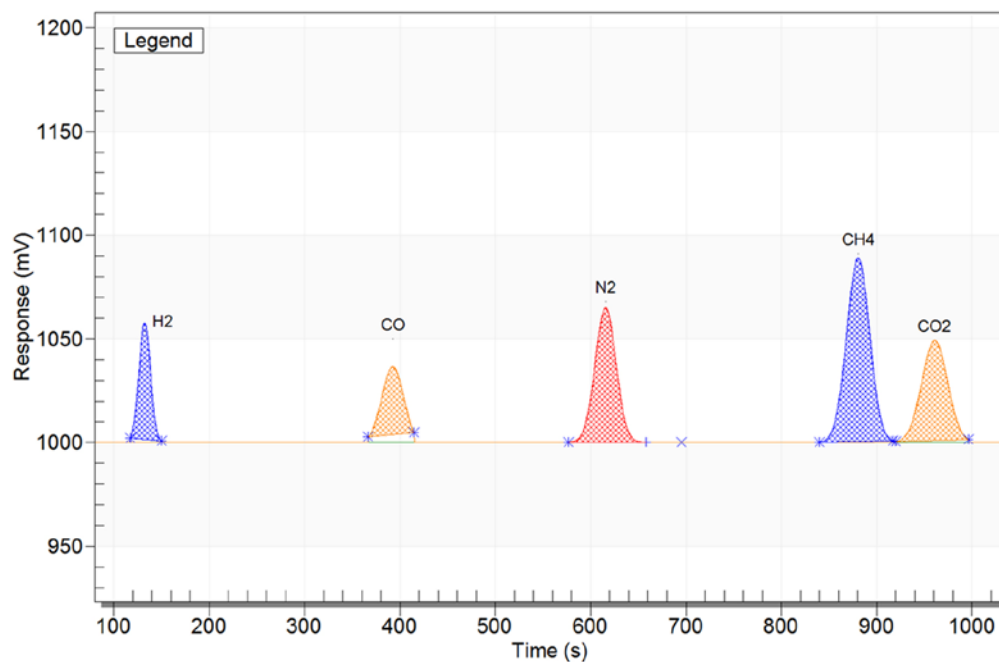

STABILITY/ACCURACY CHART AT 4PPB

| 4ppb | H2 | CO | N2 | CH4 | CO2 |
|----------------------------|-------|-------|-------|-------|-------|
| dim, 25 mars 2018 12:53:16 | 4.393 | 3.870 | 3.869 | 4.567 | 4.359 |
| dim, 25 mars 2018 13:11:40 | 4.377 | 3.918 | 3.869 | 4.561 | 4.383 |
| dim, 25 mars 2018 13:27:42 | 4.402 | 3.921 | 3.864 | 4.589 | 4.321 |
| dim, 25 mars 2018 13:46:05 | 4.389 | 4.070 | 3.861 | 4.593 | 4.283 |
| dim, 25 mars 2018 14:04:29 | 4.396 | 3.915 | 3.860 | 4.617 | 4.395 |
| dim, 25 mars 2018 14:20:29 | 4.409 | 3.879 | 3.864 | 4.617 | 4.323 |
| dim, 25 mars 2018 14:38:53 | 4.397 | 3.935 | 3.857 | 4.634 | 4.243 |
| dim, 25 mars 2018 14:57:19 | 4.388 | 3.978 | 3.865 | 4.620 | 4.443 |
| dim, 25 mars 2018 15:13:18 | 4.379 | 4.091 | 3.865 | 4.638 | 4.421 |
| dim, 25 mars 2018 15:31:18 | 4.386 | 3.900 | 3.867 | 4.683 | 4.255 |
| min | 4.377 | 3.870 | 3.857 | 4.561 | 4.243 |
| max | 4.409 | 4.091 | 3.869 | 4.683 | 4.443 |
| diff | 0.032 | 0.221 | 0.012 | 0.122 | 0.200 |
| avg | 4.392 | 3.948 | 3.864 | 4.612 | 4.343 |


CHROMATOGRAM AT 1PPB

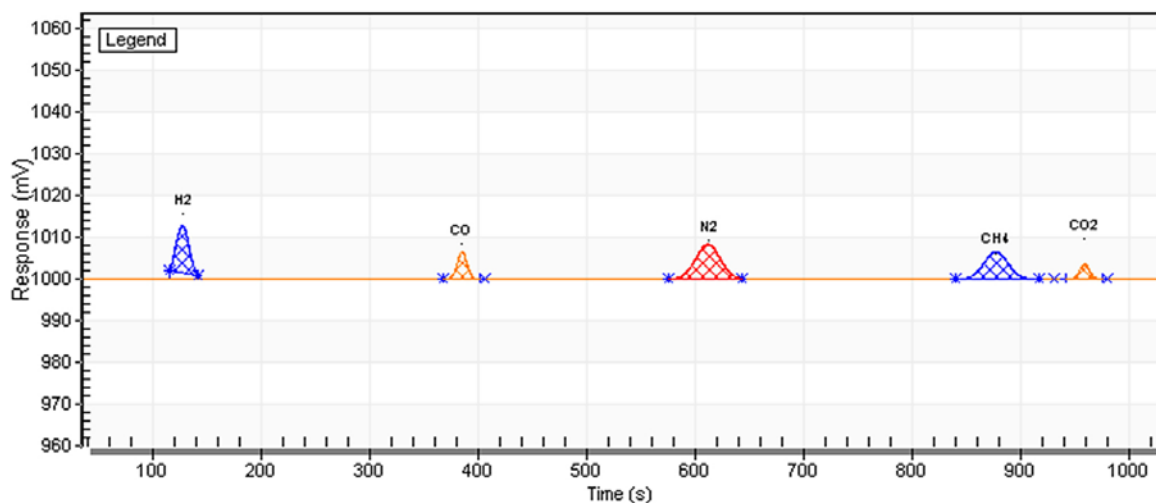

STABILITY/ACCURACY CHART AT 1PPB

| 1 ppb | H ₂ | CO | N ₂ | CH ₄ | CO ₂ |
|----------------------------|----------------|-------|----------------|-----------------|-----------------|
| mer, 28 mars 2018 08:06:07 | 1,004 | 0,896 | 1,085 | 1,048 | 1,067 |
| mer, 28 mars 2018 08:27:42 | 0,983 | 0,888 | 1,011 | 1,046 | 1,062 |
| mer, 28 mars 2018 08:49:04 | 0,971 | 0,875 | 1,016 | 1,048 | 1,065 |
| mer, 28 mars 2018 09:10:17 | 0,970 | 0,891 | 1,100 | 1,045 | 1,067 |
| mer, 28 mars 2018 09:28:38 | 0,962 | 0,896 | 1,098 | 1,047 | 1,063 |
| mer, 28 mars 2018 09:46:42 | 0,982 | 0,895 | 1,050 | 1,037 | 1,065 |
| mer, 28 mars 2018 10:04:57 | 0,980 | 0,885 | 1,052 | 1,043 | 1,063 |
| min | 0,962 | 0,875 | 1,011 | 1,037 | 1,062 |
| max | 1,004 | 0,896 | 1,100 | 1,048 | 1,067 |
| diff | 0,042 | 0,021 | 0,089 | 0,011 | 0,005 |
| avg | 0,979 | 0,889 | 1,059 | 1,045 | 1,065 |

CHROMATOGRAM WITH UHP PURIFIED HELIUM

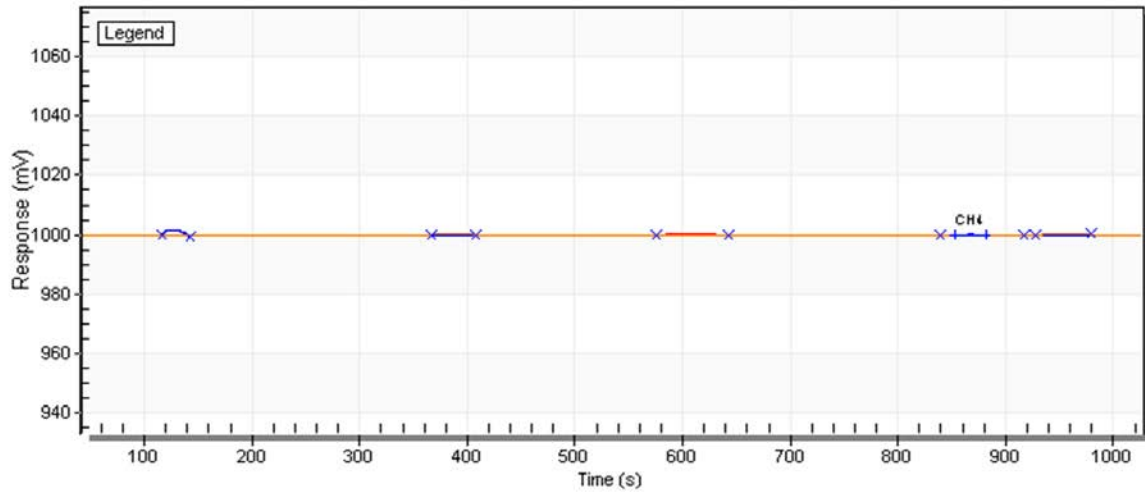


STABILITY/ACCURACY CHART WITH UHP PURIFIED HELIUM

| Pure Helium | H2 | CO | N2 | CH4 | CO2 |
|----------------------------|-------|-------|-------|-------|-------|
| mar, 27 mars 2018 18:42:26 | <LDL | <LDL | <LDL | <LDL | <LDL |
| mar, 27 mars 2018 19:00:49 | <LDL | <LDL | <LDL | <LDL | <LDL |
| mar, 27 mars 2018 19:16:51 | <LDL | <LDL | <LDL | <LDL | <LDL |
| mar, 27 mars 2018 19:35:14 | <LDL | <LDL | <LDL | <LDL | <LDL |
| mar, 27 mars 2018 19:53:37 | <LDL | <LDL | <LDL | <LDL | <LDL |
| mar, 27 mars 2018 20:09:43 | <LDL | <LDL | <LDL | <LDL | <LDL |
| mar, 27 mars 2018 20:28:05 | <LDL | <LDL | <LDL | <LDL | <LDL |
| min | 0,000 | 0,000 | 0,000 | 0,000 | 0,000 |
| max | 0,000 | 0,000 | 0,000 | 0,000 | 0,000 |
| diff | 0,000 | 0,000 | 0,000 | 0,000 | 0,000 |
| avg | 0,000 | 0,000 | 0,000 | 0,000 | 0,000 |

LDL value set at 0.5ppb

CHROMATOGRAM WITH UHP PURIFIED ARGON

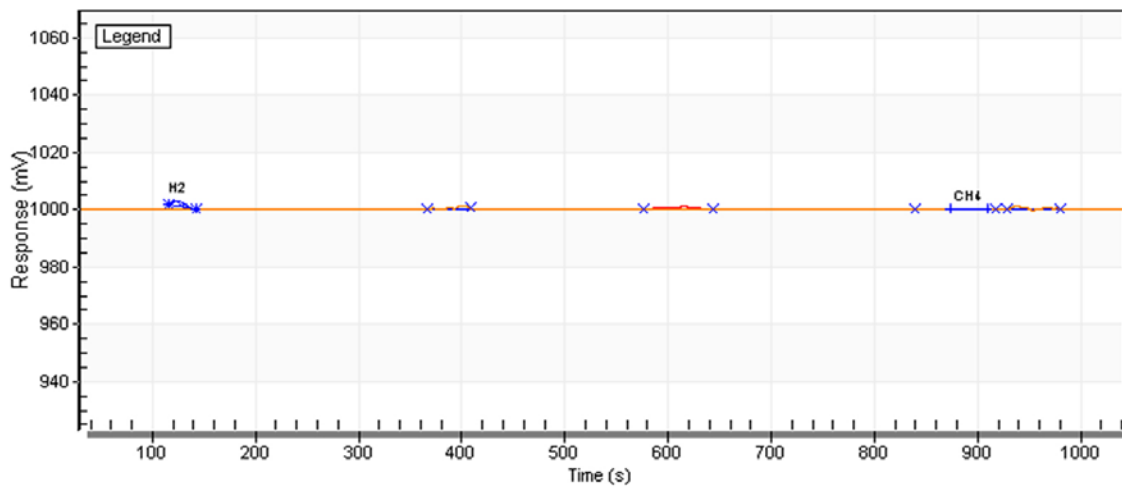

STABILITY/ACCURACY CHART WITH UHP PURIFIED ARGON

| Pure Argon | H2 | CO | N2 | CH4 | CO2 |
|---------------------------|-------|-------|-------|-------|-------|
| Mon, 26 Mar 2018 18:32:46 | <LDL | <LDL | <LDL | <LDL | <LDL |
| Mon, 26 Mar 2018 18:51:08 | <LDL | <LDL | <LDL | <LDL | <LDL |
| Mon, 26 Mar 2018 19:07:09 | <LDL | <LDL | <LDL | <LDL | <LDL |
| Mon, 26 Mar 2018 19:25:32 | <LDL | <LDL | <LDL | <LDL | <LDL |
| Mon, 26 Mar 2018 19:43:57 | <LDL | <LDL | <LDL | <LDL | <LDL |
| Mon, 26 Mar 2018 20:02:19 | <LDL | <LDL | <LDL | <LDL | <LDL |
| Mon, 26 Mar 2018 20:18:21 | <LDL | <LDL | <LDL | <LDL | <LDL |
| min | 0,000 | 0,000 | 0,000 | 0,000 | 0,000 |
| max | 0,000 | 0,000 | 0,000 | 0,000 | 0,000 |
| diff | 0,000 | 0,000 | 0,000 | 0,000 | 0,000 |
| avg | 0,000 | 0,000 | 0,000 | 0,000 | 0,000 |

LDL value set at 0.5ppb

CONCLUSION:

Our complete cabinet integration with our MultiDetek2 (GC), PlasmaDetek2 (PED), LDGSS gas stream selector, LDGDS gas dilution system and our LDP1000 carrier gas purifier are all perfectly designed and approved for the UHP semiconductor applications. With the results demonstrated, we can clearly see our systems is capable of generating and detecting very clear peaks at sub ppb concentrations. Don't hesitate to contact LDetek if more informations are required.

APPLICATION NOTE

LD19-02



Measurement of trace impurities in high purity Nitrogen trifluoride (NF₃) for electronic gas industry using PlasmaDetek2 and MultiDetek2 GC



The analysis of high purity nitrogen trifluoride is commonly used for the electronic market in the plasma etching of silicon wafers for the production of liquid crystal displays.

LDETEK SOLUTION:


The GC configuration for this type of application is generally configured with coated stainless steel purged diaphragm valves and coated MXT columns to improve the performances of the system. At the end of the GC configuration, the PlasmaDetek-2 detector is configured to selectively measure the impurities requested. Multiple channels can be configured depending of the application. For this application note, the MultiDetek2 GC is configured with 4 channels merging in the PED detector.

- ▶ **Trace H₂-Ar+O₂-N₂-CO impurities** measured with channel #1
- ▶ **Trace SF₆ impurities** measured with channel #2
- ▶ **Trace CO₂-N₂O impurities** measured with channel #3
- ▶ **Trace CH₄-CF₄ impurities** measured with channel #4

RESULTS:


Chromatogram : Trace CO₂-H₂-N₂-CO-CH₄ impurities in NF₃

| Peak | Unit | Calibration Value | Area Counts |
|-----------------|------|-------------------|-------------|
| CO ₂ | ppm | 5.00 | 89184 |
| H ₂ | ppm | 5.00 | 11170 |
| N ₂ | ppm | 5.00 | 22814 |
| CO | ppm | 5.00 | 96257 |
| CH ₄ | ppm | 5.00 | 64378 |

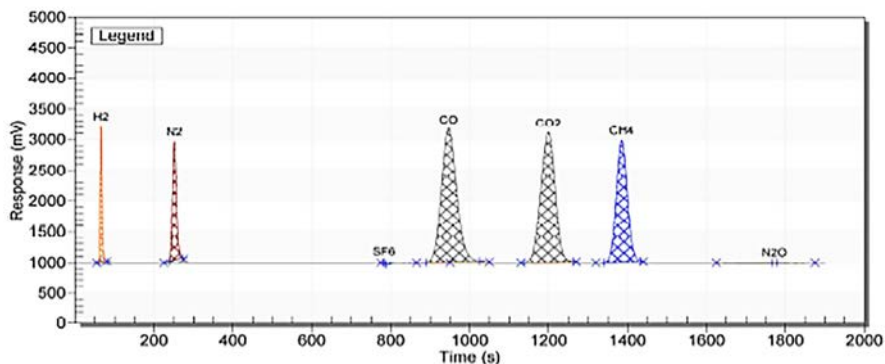


Chromatogram : Trace N₂O impurities in NF₃

| Peak | Unit | Calibration Value | Area Counts |
|------------------|------|-------------------|-------------|
| N ₂ O | ppm | 4.90 | 114967 |

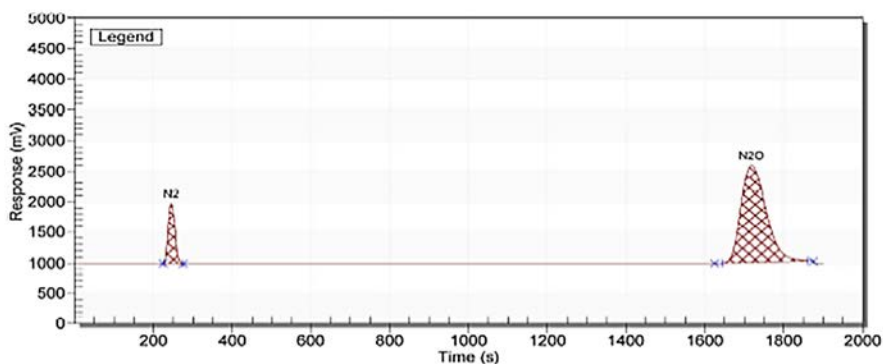


Chromatogram : Trace Ar+O₂ impurities in NF₃

| Peak | Unit | Calibration Value | Area Counts |
|-------------------|------|-------------------|-------------|
| Ar+O ₂ | ppm | 5.00 | 19120 |

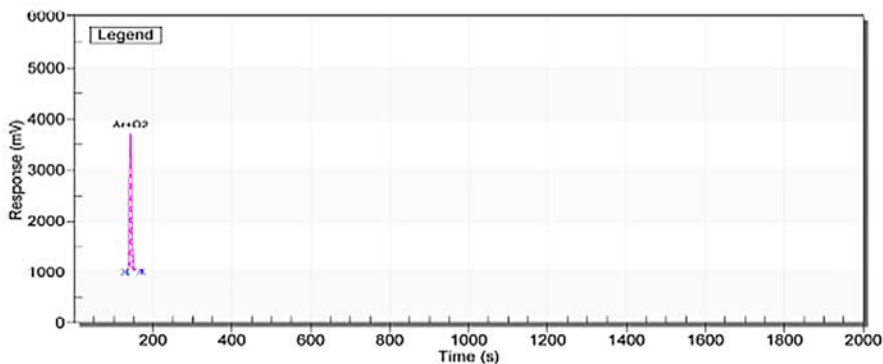

Chromatogram : Trace SF₆-CF₄ impurities in NF₃

| Peak | Unit | Calibration Value | Area Counts |
|-----------------|------|-------------------|-------------|
| SF ₆ | ppm | 5.00 | 99694 |
| CF ₄ | ppm | 5.00 | 100767 |

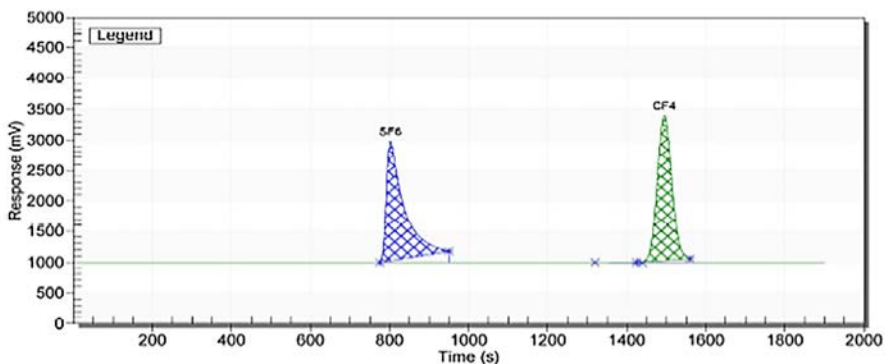


LIMIT OF DETECTION


| COMPONENTS | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|------------|---------------|-------------|--------|----------------|
| H2 | 0.27 ppm | 150 mV | 1.0 mV | 5.4 ppb |
| Ar+O2 | 0.61 ppm | 130 mV | 1.0 mV | 14.0 ppb |
| N2 | 0.46 ppm | 200 mV | 0.5 mV | 3.4 ppb |
| CO2 | 0.18 ppm | 93 mV | 1.9 mV | 11.0 ppb |
| CH4 | 0.18 ppm | 80 mV | 1.4 mV | 9.4 ppb |
| CO | 0.23 ppm | 105 mV | 2.3 mV | 15.0 ppb |
| N2O | 0.1 ppm | 34 mV | 2 mV | 17.6 ppb |
| SF6 | 1.5 ppm | 660 mV | 1 mV | 6.8 ppb |
| CF4 | 1.37 ppm | 700 mV | 3 mV | 17.6 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic condition


Channel 1 : 0.27ppm H2

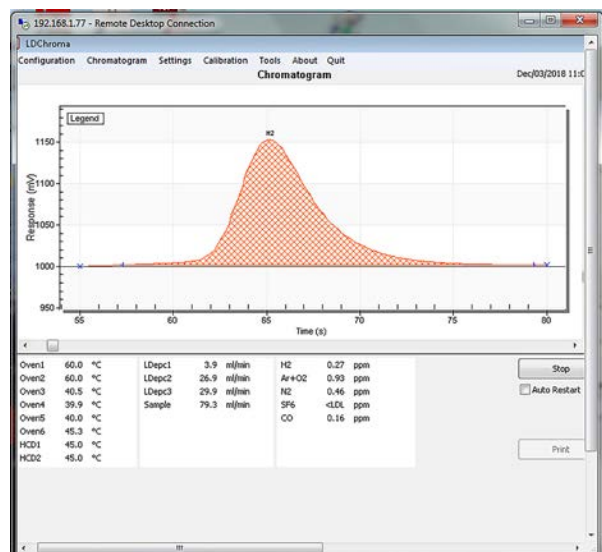


Channel 1 : 0.46ppm N2

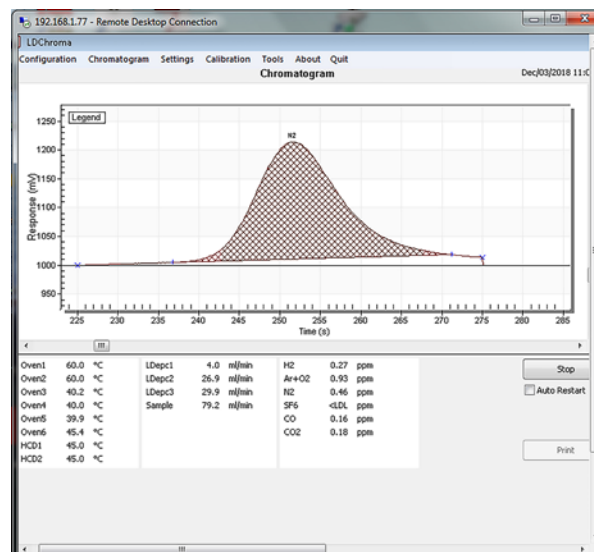


Channel 1 : 0.23ppm CO

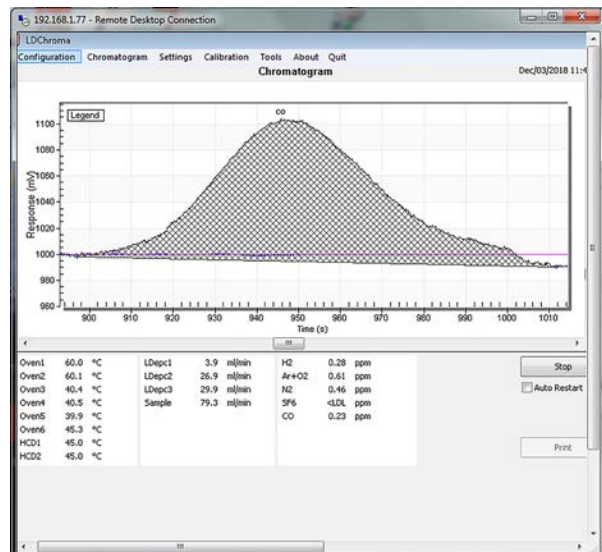


Channel 2 : 1.5ppm SF6

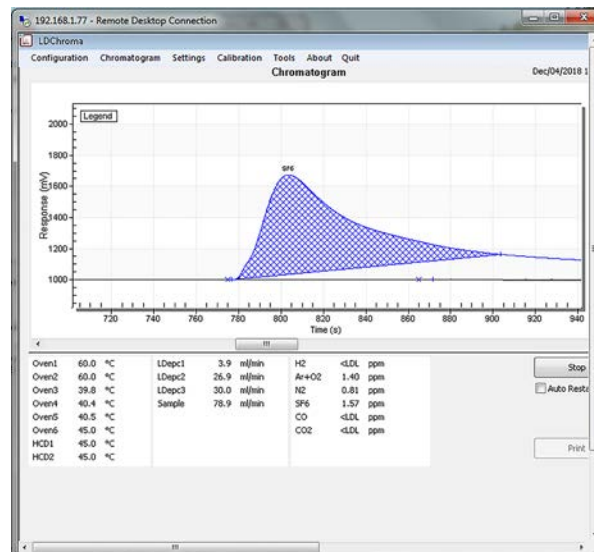


Channel 3 : 0.18ppm C02

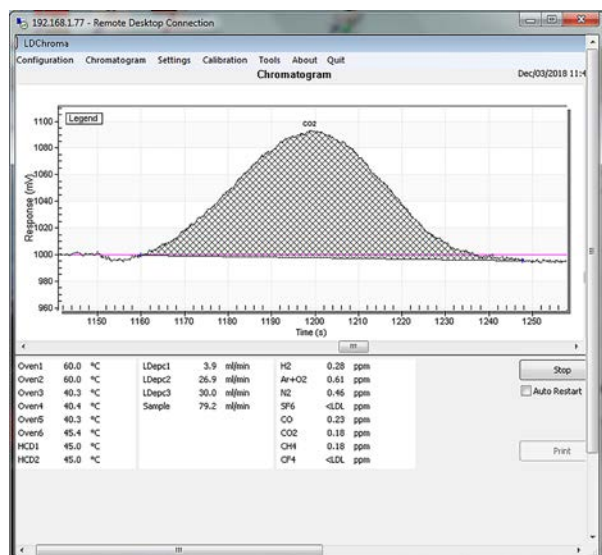


Channel 3 : 0.1ppm N20

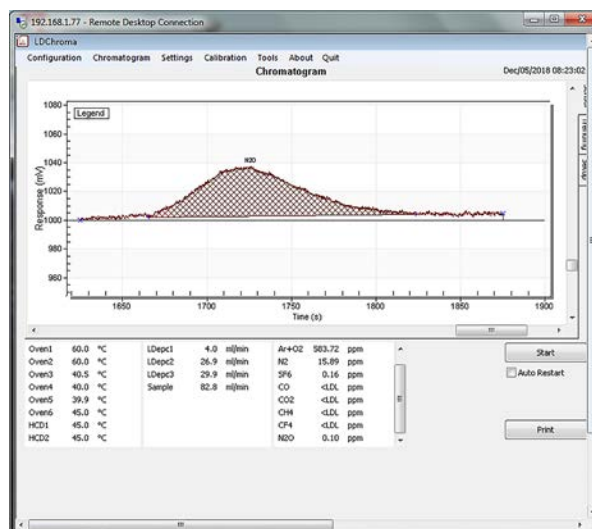

Channel 4 : 1.37ppm CF4

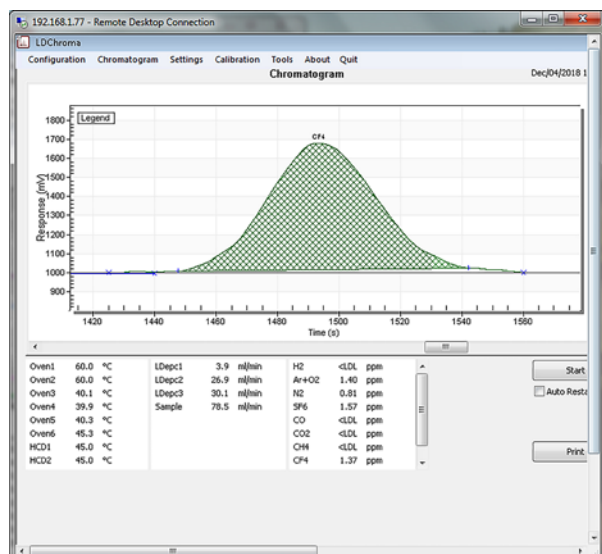

Channel 4 : 0.18ppm CH4

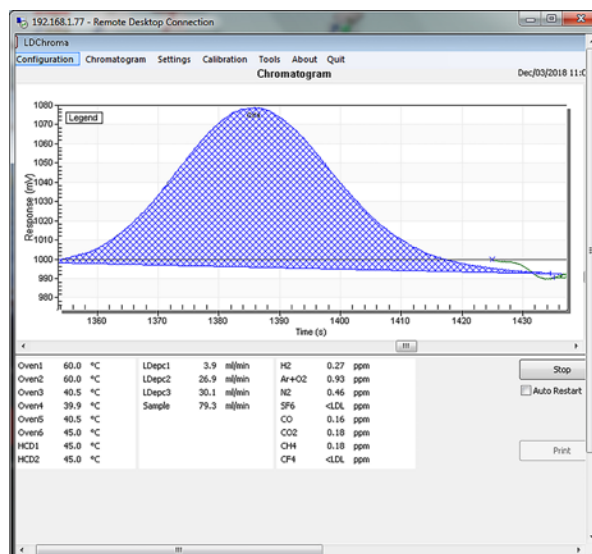

CONCLUSION:

The system is configured with the proper columns and valve configuration to get a quick analysis time and a robust configuration. The use of the PlasmaDetek2 offers a good selectivity for the detection allowing to get a relatively good short analysis time with good limit of detection.

APPLICATION NOTE

LD19-03



Measurement of trace impurities in high purity nitrous oxide (N₂O) for electronic gas industry using PlasmaDetek2 and MultiDetek2 GC



▲ MultiDetek2

▲ PlasmaDetek2
patent US 9,310,308 B2

Nitrous oxide (N₂O), often referred to as laughing gas, is used in the high-tech thin film industries of semiconductor and LCD display manufacturing. The primary application is the reaction with silane (SiH₄) or other silicon precursors to produce high-quality oxide films (SiO_x), which are used as electrical insulators in microelectronic transistors. N₂O is increasingly used to make thin-film oxides with other elements like titanium, aluminium, magnesium and zirconium. It is also used in the selective etching of semiconductor thin-films.

Nitrous oxide is a colourless, non-flammable gas at room temperature with a slightly sweet odour and taste and it is an oxidiser that can support combustion like oxygen. It is an electronic high-purity material produced from thermal decomposition of ammonium nitrate. Why is this gas used in electronics manufacturing? It is less reactive and therefore more selective, than oxygen. Often, this property is used to:


- ▶ **Control the amount of oxygen in a thin film**
- ▶ **Reduce the side oxidation reactions**
- ▶ **Selectively etch one thin film while allowing others to remain**

A addressable market than more than 10,000 metric tons N₂O continuously growing with the arrival of new higher-definition display technologies like ultra-high definition and OLED requiring higher amount of N₂O.

In addition to its use in electronics manufacturing, common applications of nitrous oxide are: anaesthetics, as food and beverage propellant (for whipped cream as example), as an industrial propellant and foaming agent and as a fuel oxidiser for rockets and race cars.

THE COMPLETE SOLUTION

This application note shows the configuration of a complete integrated system (LD rack mount cabinet).

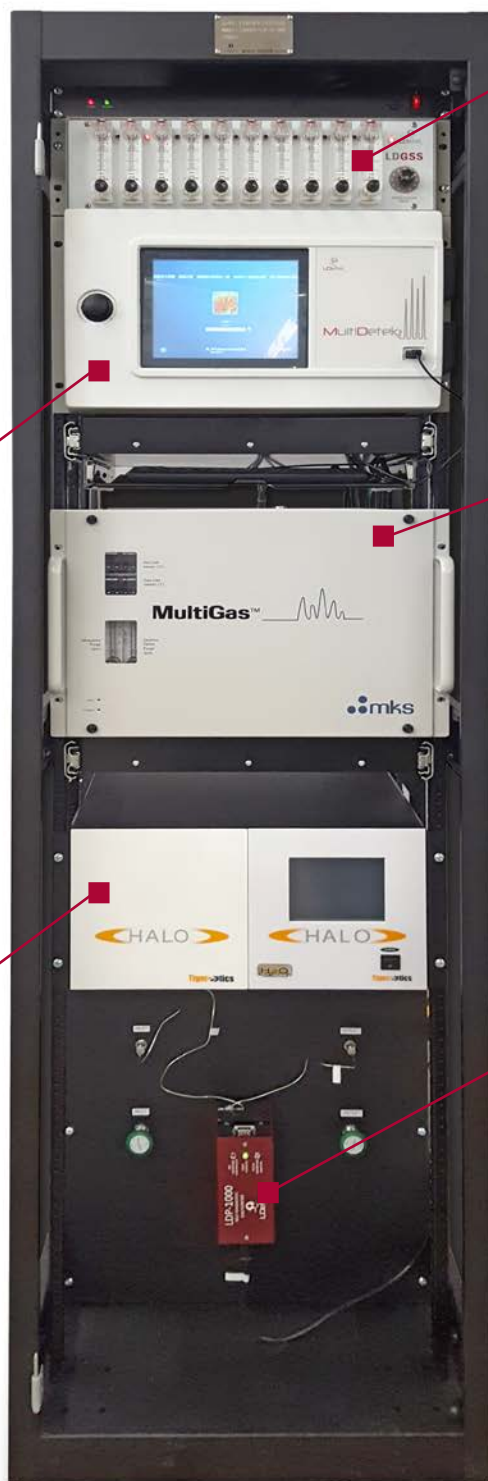

LDGSS

ultra high purity gas stream selector using stainless steel diaphragm valves for 10 streams.

MKS MULTIGAS

FTIR instrument for measuring ppb/ppm ammonia and NOx.

HEATED GAS PURIFIER

for generating grade 99.999999% UHP carrier gas for GC from Helium grade 99.999%

MULTIDETEK2

compact/industrial GC for measuring trace ppb/ppm impurities H₂-O₂-N₂-CH₄-CO-CO₂ with addition of Ar-Ne and addition of C₂H₂-C₂H₄-C₂H₆ all in one instrument using one type of sensor (PlasmaDetek2) with helium as carrier gas.


TIGER OPTICS

Halo instrument for measuring ppb/ppm trace H₂O.

RESULTS:


Chromatogram : Trace H2-O2-CH4 impurities in N2O

| Peak | Unit | Calibration Value | Area Counts |
|------|------|-------------------|-------------|
| H2 | ppm | 5.69 | 28374 |
| CH4 | ppm | 5.90 | 94297 |
| O2 | ppm | 4.94 | 35973 |

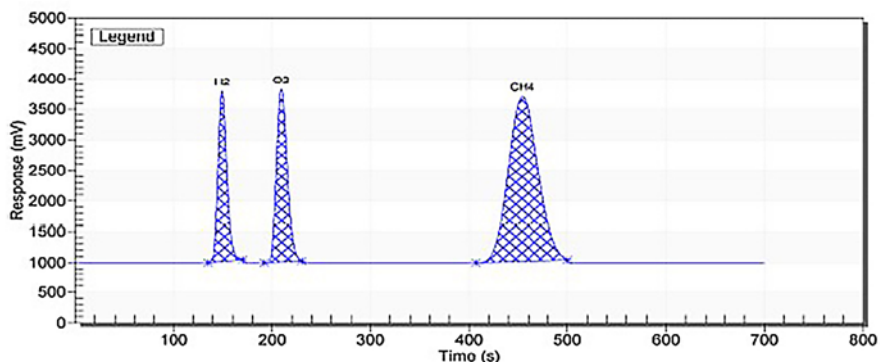


Chromatogram : Trace N2 impurities in N2O

| Peak | Unit | Calibration Value | Area Counts |
|------|------|-------------------|-------------|
| N2 | ppm | 5.36 | 39445 |

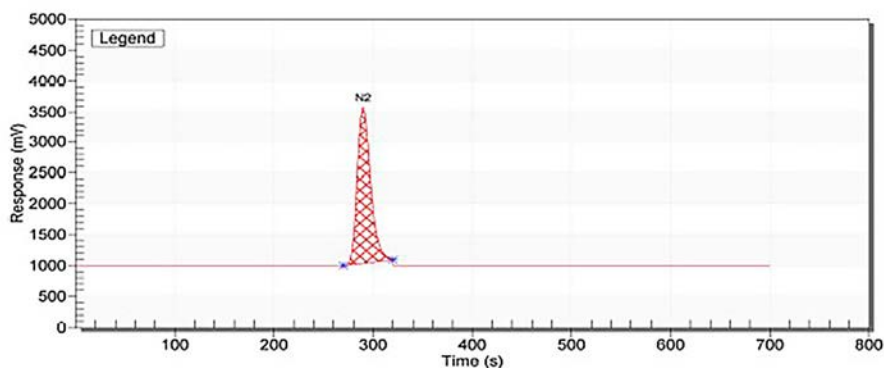


Chromatogram : Trace CO impurities in N2O

| Peak | Unit | Calibration Value | Area Counts |
|------|------|-------------------|-------------|
| CO | ppm | 5.32 | 34990 |

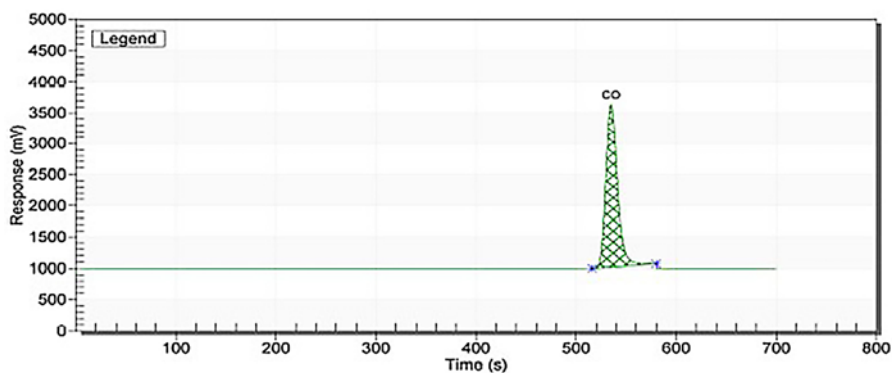


Chromatogram : Trace Ar impurities in N2O

| Peak | Unit | Calibration Value | Area Counts |
|------|------|-------------------|-------------|
| Ar | ppm | 4.65 | 31373 |

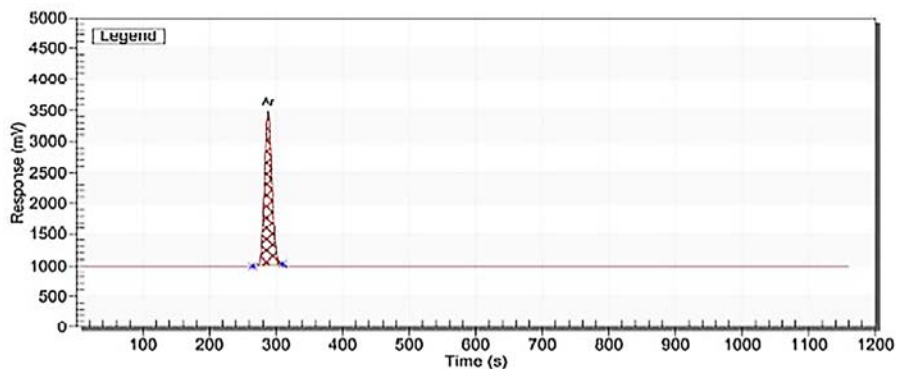


Chromatogram : Trace Ne impurities in N2O

| Peak | Unit | Calibration Value | Area Counts |
|------|------|-------------------|-------------|
| Ne | ppm | 4.86 | 9891 |

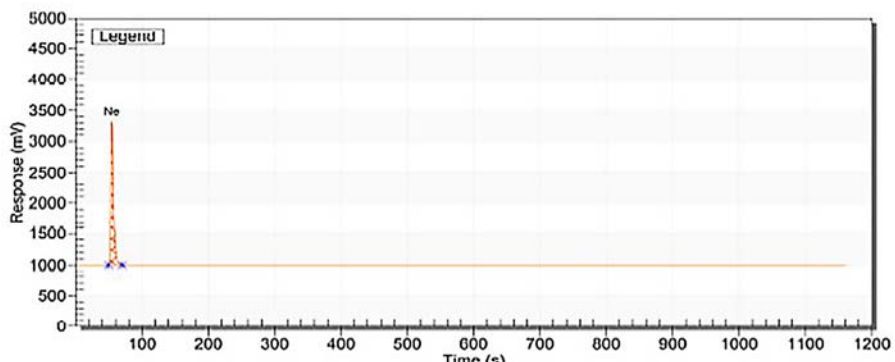**Chromatogram : Trace C2H2-C2H4-C2H6 impurities in N2O**

| Peak | Unit | Calibration Value | Area Counts |
|------|------|-------------------|-------------|
| C2H2 | ppm | 3.72 | 60461 |
| C2H4 | ppm | 4.62 | 107184 |
| C2H6 | ppm | 4.55 | 151170 |

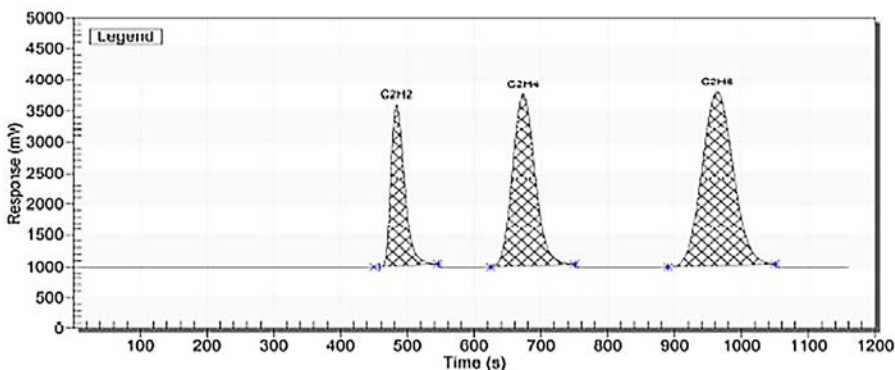
**LIMIT OF DETECTION**

| COMPONENTS | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|------------|---------------|-------------|--------|----------------|
| H2 | 0.05 ppm | 30 mV | 2.0 mV | 10 ppb |
| O2 | 0.053 ppm | 30 mV | 2.0 mV | 10.6 ppb |
| N2 | 0.05 ppm | 24 mV | 1.5 mV | 9.3 ppb |
| CH4 | 0.05 ppm | 33 mV | 2.0 mV | 9.0 ppb |
| CO | 0.05 ppm | 25 mV | 2.0 mV | 12.0 ppb |


Note: other LDL could be obtained with different injection volume and chromatographic condition

For the Idl of the impurities Ar-Ne-C2H2-C2H4-C2H6, they don't appear in the chart since the results are based on the O2 and CH4 which use the same sensor on the PlasmaDetek2. The Idl is then evaluate at 10ppb for Ar-Ne and 9ppb for C2s.


H2 : 0.05ppm

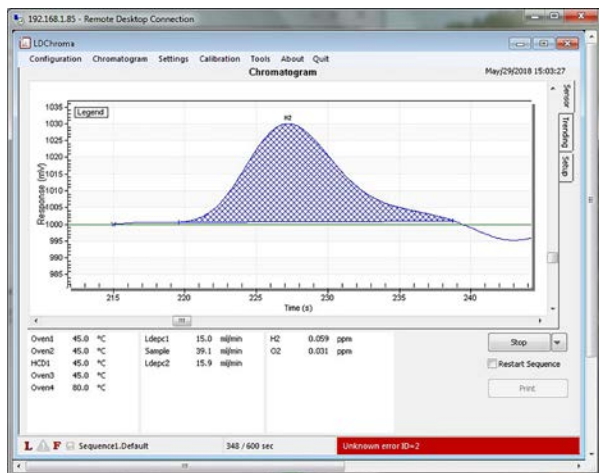


O2 : 0.053ppm

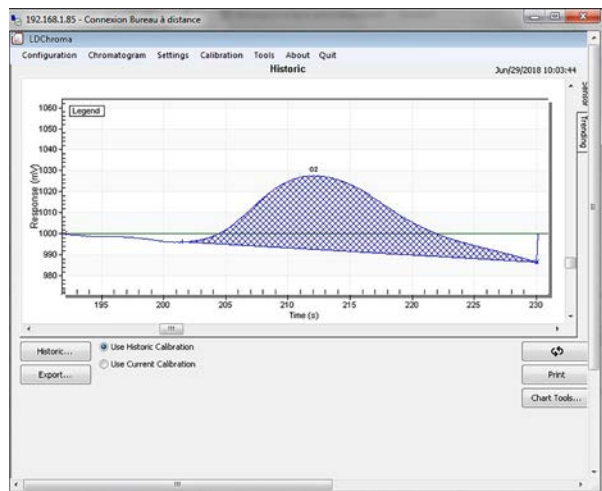


N2 : 0.05ppm

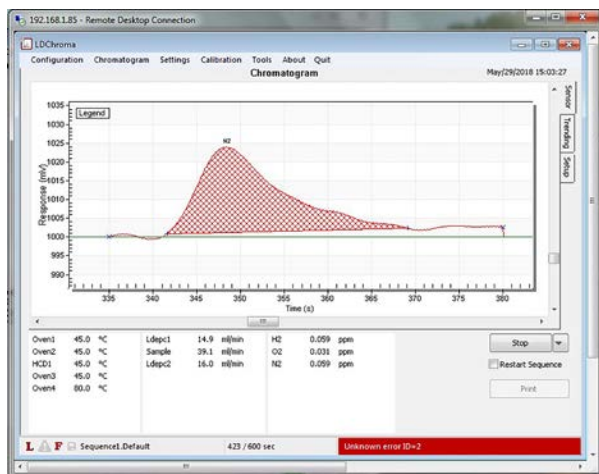

CH4 : 0.05ppm

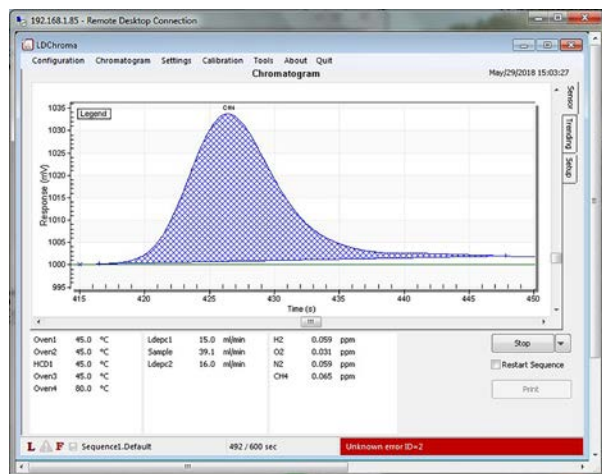

CO : 0.05ppm

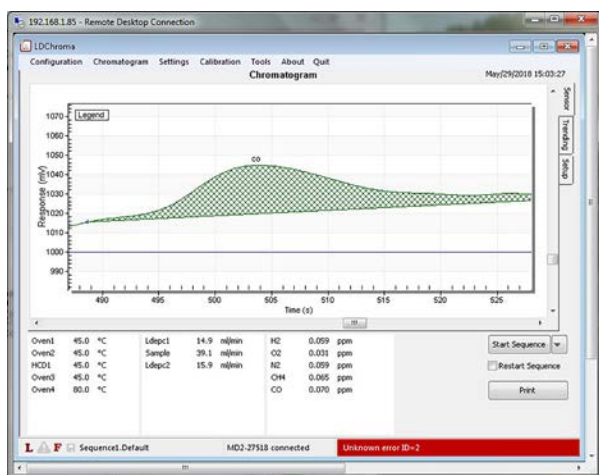


Repeatability to be at a value of $CV\% \times 3 < 5\%$ for a series of consecutive analysis at a fix concentration in a balance gas of nitrous oxide.


| COMPONENTS | Repeatability (CV% x 3) |
|------------|-------------------------|
| H2 | 1.64% |
| O2 | 0.73% |
| N2 | 1.56% |
| CH4 | 2.05% |
| CO | 1.66% |

For the repeatability of the impurities Ar-Ne-C2H2-C2H4-C2H6, they don't appear in the chart since the results are based on the O2 and CH4 which use the same sensor on the PlasmaDetek2. An evaluation of 0.73% for Ar-Ne and 2.05% for C2s is given.

Results (screenshot) of consecutive analysis at a fix concentration for H2-N2-CH4-CO impurities in balance N2O

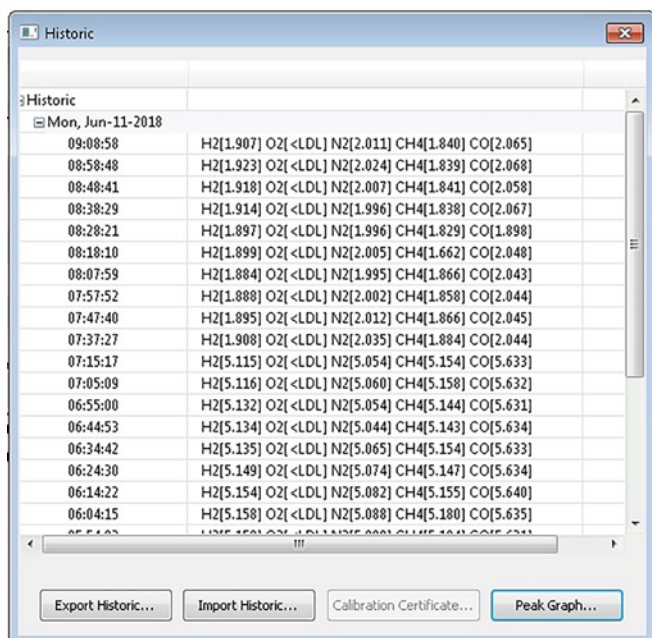

Results (screenshot) of consecutive analysis at a fix concentration for O2 impurity in balance N2O

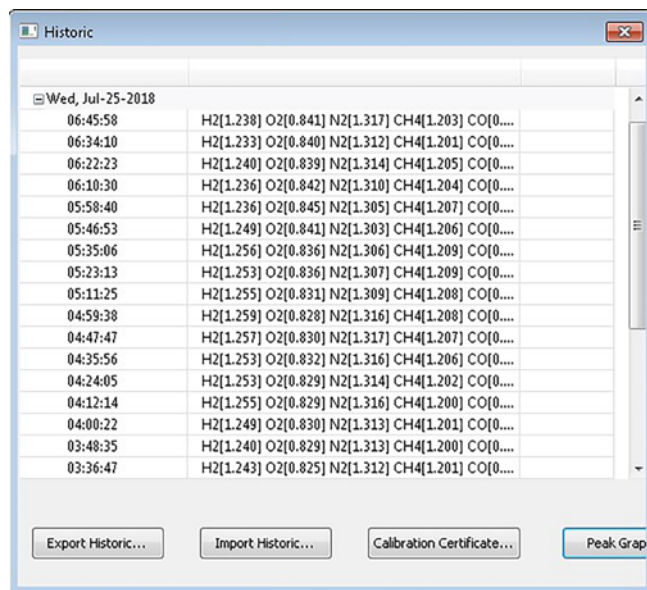

CONCLUSION:

Using one PlasmaDetek2 detector inside one unit MultiDetek2 GC, the analysis of trace ppb/ppm impurities H2-O2-N2-CH4-CO-CO2 with addition of Ar-Ne and addition of C2H2-C2H4-C2H6 have been measured. The analysis time for the impurities H2-O2-N2-CH4-CO-CO2 in UHP N2O was realized within 13 minutes. By adding the analysis of Ar-N2-C2H2-C2H4-C2H6 on top of the other impurities listed, the analysis time was realized in 20 minutes. The MultiDetek2 GC was configured with helium as carrier gas, stainless steel diaphragm valve and capillary MXT type columns to minimize the carrier flow consumption. The unit is using 4-20mA outputs for each impurity and also the Modbus protocol for transmitting the data's. The GC and the stream selector system LDGSS are both remotely controlled by the Ethernet port. Meaning that the calibration of the units can be performed remotely.

The complete integration of the system has been made inside a standard rackmount enclosure. The instruments from Tiger Optics and from MKS have been added for the analysis of H2O and NOx-NH3 respectively.

APPLICATION NOTE

LD20-02



MultiDetek2 gas chromatograph with PlasmaDetek2 detector uses for hydrogen isotopes separation and the analysis of impurities in Deuterium



▲ MultiDetek2

▲ PlasmaDetek2

LDetek SOLUTION:


The complex analysis of the impurities in a sample gas containing high purity deuterium (D₂) can be realized with our gas chromatograph model MultiDetek2. The detector uses for the trace impurities is the PlasmaDetek2, which is configured with its selective optics to obtain the best selectivity and sensitivity to the required impurities to measured. The requirements here was a range of 10ppm and 100ppm capable of detecting down to 10ppb limit of detection for each impurity. The GC has been coupled with our cryo system to realize the separation of the hydrogen isotopes without interference in a relative short analysis time.

Sample composition of deuterium (D₂):


| IMPURITIES | RANGE | SYSTEM LDL | SYSTEM LOQ |
|-----------------|-----------|------------|------------|
| O ₂ | 0-10 ppm | 10 ppb | 50 ppb |
| CH ₄ | 0-10 ppm | 10 ppb | 50 ppb |
| N ₂ | 0-10 ppm | 10 ppb | 50 ppb |
| CO | 0-10 ppm | 10 ppb | 50 ppb |
| CO ₂ | 0-10 ppm | 10 ppb | 50 ppb |
| NMHC | 0-10 ppm | 10 ppb | 50 ppb |
| H ₂ | 0-10 ppm | 10 ppb | 50 ppb |
| HD | 0-100 ppm | 10 ppb | 50 ppb |
| D ₂ | 100 % | — | — |

RESULTS

Chromatogram of trace ppm impurities O₂-CH₄-N₂-CO-CO₂-NMHC-H₂ in pure D₂ (deuterium)

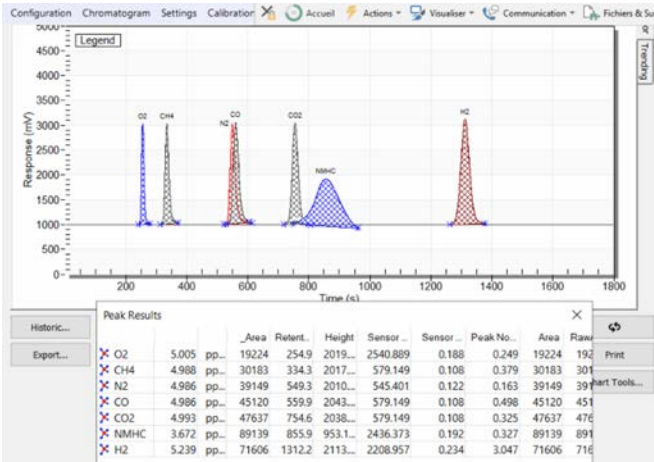

Chromatogram of trace ppm impurity HD (hydrogen deuteride) in pure D₂ (deuterium)

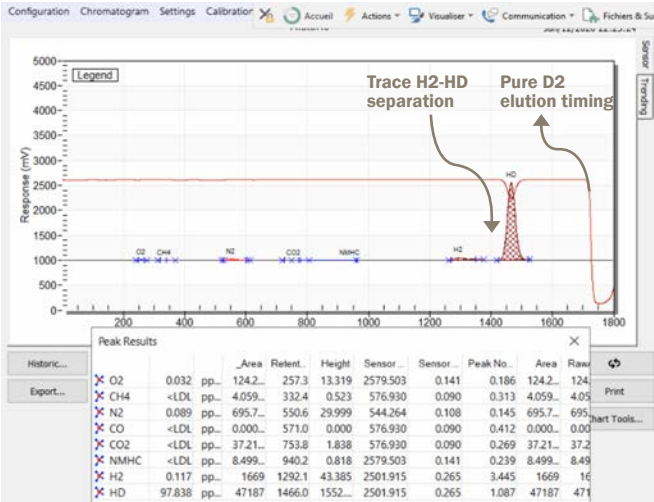

This chromatogram shows the good separation of the hydrogen isotopes H₂-HD-D₂ by using our PED detector combines with our MultiDetek2 cryo system.

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------------|---------------|-------------|---------|----------------|
| O ₂ | 5.005 ppm | 2019 mV | 1.3 mV | 9.66 ppb |
| CH ₄ | 4.988 ppm | 2017 mV | 1.2 mV | 8.90 ppb |
| N ₂ | 4.986 ppm | 2010 mV | 0.9 mV | 6.69 ppb |
| CO | 4.986 ppm | 2043 mV | 1.5 mV | 10.9 ppb |
| CO ₂ | 4.993 ppm | 2038 mV | 1.4 mV | 10.2 ppb |
| NMHC | 3.672 ppm | 953 mV | 0.9 mV | 10.4 ppb |
| H ₂ | 5.239 ppm | 2113 mV | 1.2 mV | 8.92 ppb |
| HD | 97.838 ppm | 1552 mV | 0.07 mV | 13.2 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic condition

CONCLUSION:

The MultiDetek2 gas chromatograph uses with the PlasmaDetek2 detector and the LDetek cryo column cooling system all in one unit can measured trace impurities in deuterium. The system is capable to achieve a full ppm range with 10ppb limit of detection. The separation of the hydrogen isotopes is easily realized by maintaining the micro packed column in a cryogenic environment. The system is rackmount and compact offering a full remote control. The industrial communication protocols are all built in and must simply be selected specifically for your requirements.

APPLICATION NOTE

LD20-03



MultiDetek2 gas chromatograph with PlasmaDetek2 detector uses for the analysis of semiconductor specialty gases as UHP Octafluorocyclobutane (C₄F₈)



Octafluorocyclobutane, or perfluorocyclobutane, C₄F₈, is a compound of carbon and fluorine used in the production and processing of semiconductor materials and devices, for example as a deposition gas and etchant. Production of such high purity specialty gas then requires a quality control analyser.

LDETEK SOLUTION:

Measuring the production quality of complex electronic specialty gases as C₄F₈ uses as etchant can be realized with our gas chromatograph MultiDetek2.

Our system uses PlasmaDetek2 (PED) as detection device to ensure good selectivity and sensitivity down to sub ppb level.


Multiple purged diaphragm valves ensure the leak integrity to keep the purity of the system in place for ppb detection. The column selection is adapted to CF gases to keep the reactivity and adsorption as low as possible to ensure the stability of the results. The complete flow path of the unit is coated with inert material to eliminate the reactivity for such complex electronic gas mixtures.

Sample composition of (C4F8):

| IMPURITIES | RANGE | SYSTEM LDL | SYSTEM LOQ |
|-------------------------------|-----------|------------|------------|
| C ₅ F ₈ | 0-100 ppm | 25 ppb | 75 ppb |
| C ₂ F ₆ | 0-100 ppm | 25 ppb | 75 ppb |
| C ₃ F ₈ | 0-100 ppm | 25 ppb | 75 ppb |
| CF ₄ | 0-100 ppm | 25 ppb | 75 ppb |
| CO ₂ | 0-100 ppm | 25 ppb | 75 ppb |
| C ₄ F ₆ | 0-100 ppm | 25 ppb | 75 ppb |
| C ₄ F ₈ | 100 % | — | — |

RESULTS

Chromatogram of trace ppm impurities C5F8, C2F6, C3F8, CF4, CO2 and C4F6 in Octafluorocyclobutane (C4F8) sample gas

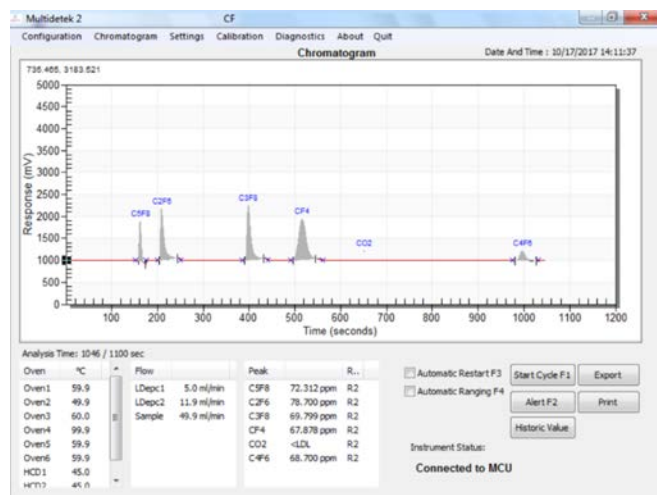

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-------------------------------|---------------|-------------|---------|----------------|
| C ₅ F ₈ | 72.312 ppm | 891 mV | 0.11 mV | 26.7 ppb |
| C ₂ F ₆ | 78.700 ppm | 1289 mV | 0.15 mV | 27.4 ppb |
| C ₃ F ₈ | 69.799 ppm | 1371 mV | 0.15 mV | 22.9 ppb |
| CF ₄ | 67.878 ppm | 960 mV | 0.11 mV | 23.3 ppb |
| C ₄ F ₆ | 68.700 ppm | 249 mV | 0.04 mV | 33.1 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic condition

CONCLUSION:

The MultiDetek2 gas chromatograph uses with the PlasmaDetek2 detector offers the requirements for such type of specialty gas application. The configuration with purged diaphragm valves combined with coated inert gas flow path and columns makes the system perfectly adapted for such specialty and complex gases. The system is rackmount and compact offering a full remote control. The industrial communication protocols are all built in and must simply be selected specifically for your requirements.



3.0 APPLICATION NOTE

3.6 NATURAL GAS



3.0 APPLICATION NOTES

APPLICATION NOTE

LD15-09



Measurement of THT in natural gas using MultiDetek2 and PlasmaDetek2



▲ MultiDetek2

▲ PlasmaDetek2

A quick analysis to trace tetrahydrothiophene (THT) in natural gas is required for controlling the amount of this odorant added in the natural gas. Due to its odor, the THT is used to detect any presence of gas leakage in natural gas distribution networks. The THT is composed of a five-membered ring containing four carbon atoms and a sulfur atom. It is also known as thiophane or thiolane. The THT is generally used in mixtures containing tert-Butylthiol (TBM) which is an organosulfur compound with the formula $(CH_3)_3CSH$. In the presence of TBM in natural gas, it is required to measure its concentration at low ppb/ppm because of its strong odor that causes nausea. The permissible exposure limit (PEL) is in the range of 500ppb and it is the reason why a highly sensitive detection system is required for measuring both THT and TBM in natural gas.

LDETEK SOLUTION:

The use of a highly sensitive detection system (PlasmaDetek2) combined with a compact GC system (MultiDetek2) are required for such type of analysis where sensitivity, robustness and speed are necessary. The figure 1 shows the easy to operate 2-valve/2-column configuration used to achieve a quick analysis of THT at low ppb/ppm concentration with no interference from other gases present in natural gas. This type of configuration is straight and ensures a good stability of the measurement over time. The valves, tubing, fittings are made of coated stainless steel to ensure repeatability and durability of the system. The robustness of the injection and detection system makes this solution maintenance free on long-term operation.

According to the minimum detection limit that is required, the analysis time can vary. The figure 2 shows a chromatogram of such system having a limit of detection fixed at 31ppb. Analysis time is then fixed below 4 minutes, what is the average time generally required for this type of measurement. If quicker analysis time is requested, the system parameters can be easily modified to achieve lower cycle time analysis. That generally consists of sampling loop volume and system gain reduction to achieve a higher ppb detection limit.

The PED detection system can be configured either with Helium or Argon as carrier gas depending of the sensitivity requested. It is a unique carrier gas source with low gas consumption for cost saving.

The analysis of tert-Butylthiol (TBM) can be added in the same MultiDetek2 compact GC still using PlasmaDetek2 (PED) as the detection system.

With its built in industrial PC, the MultiDetek2 offers all the conventional communication protocols (analog output, Modbus, Profibus, RS232), data storage disk and alarms contacts required for a process GC.

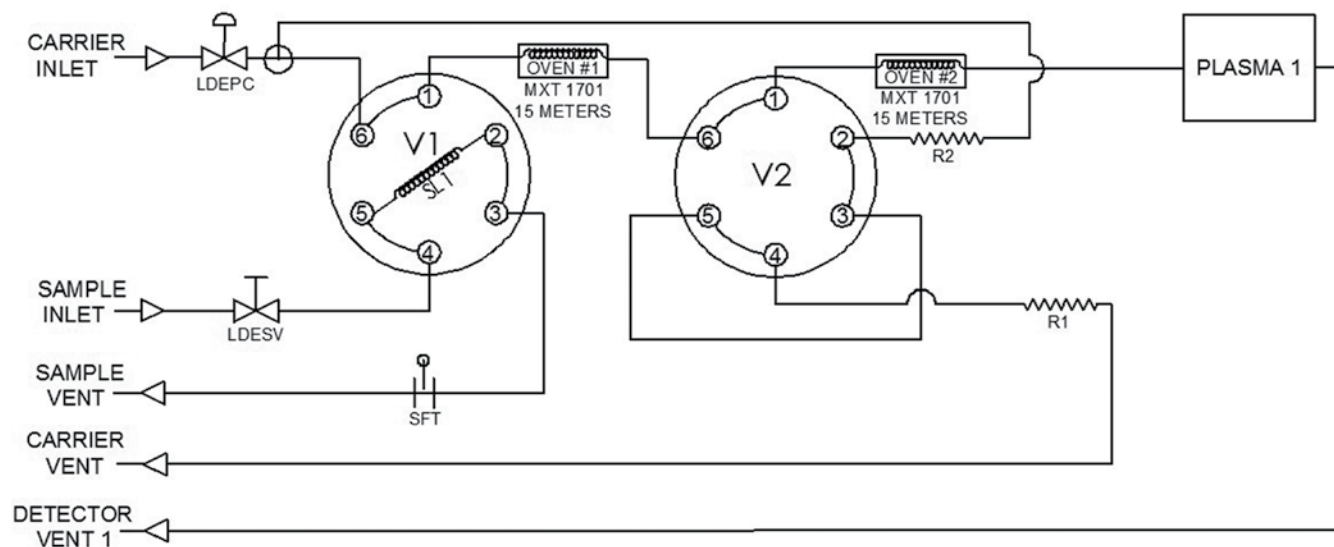


Figure 1: Application hardware configuration

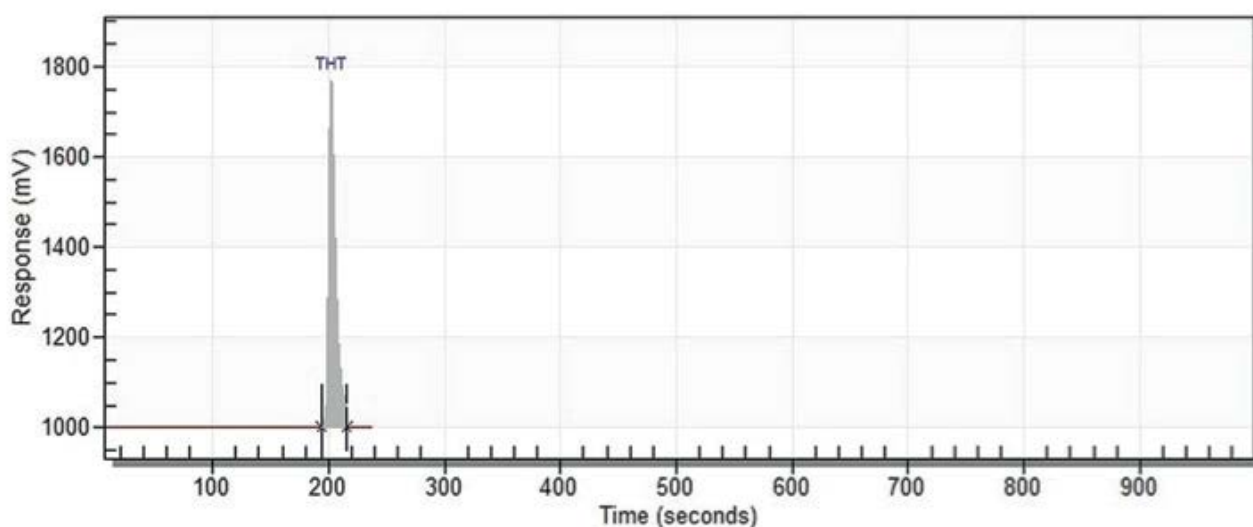


Figure 2: Chromatogram showing a standard gas containing 9.25ppm THT

Based on noise to ratio, LDL is calculated as follows:

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------|---------------|-------------|-------|----------------|
| THT | 9.257 ppm | 1780 mV | 2 mV | 0.031 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

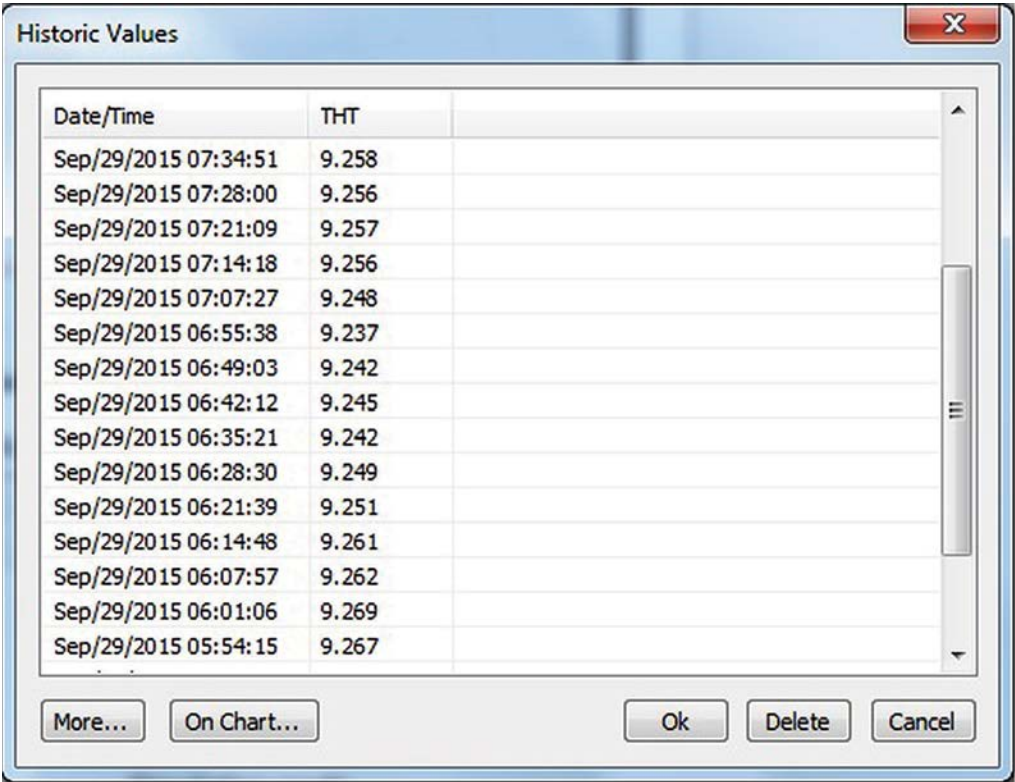


Figure 3: Historic values chart showing repeatability results better than 1% of reading

CONCLUSION:

Using a solution combining the PlasmaDetek2 and MultiDetek2 is the best way to achieve sensitivity, robustness and speed in an industrial compact system. This is exactly what is required from the natural gas industry.

APPLICATION NOTE

LD19-01



Measurement of THT-TBM odorants in natural gas using the MultiDetek 2 and PlasmaDetek 2



The quick analysis of trace tetrahydrothiophene (THT) in LNG is required for controlling the amount of this odorant added in the natural gas. The THT is used for his smell to detect any presence of gas leakage in natural gas distribution network. The THT is generally used in mixture containing tert-Butylthiol (TBM) which is an organosulfur compound. In presence of TBM in natural gas, it is required to measure its concentration at low ppb/ppm because of its strong odor that causes nausea. The permissive expose limit (PEL) is in the range of 500ppb and it is the reason why highly sensitive detection system is required for both measuring THT and TBM in natural gas. This application note is the continuity of the previous app. Note LD15-09.


LDETEK SOLUTION:

The use of a highly sensitive detection system (PlasmaDetek2) combined with a compact GC system (MultiDetek2) are required for such type of analysis where sensitivity, robustness and speed are necessary. With its built in industrial PC, the MultiDetek2 offers all the conventional communication protocols (analog output, Modbus, Profibus, RS232/RS485), data storage capability and alarm contacts required for a process GC.


In this application note, the results of the performance are demonstrated for the quick analysis of sub ppb/ppm detection of THT and TBM in LNG. The representation of few chromatograms, the linearity, the repeatability and the limit of detection well demonstrated the capability for such type of application. One detector PlasmaDetek2 has been used. The two channels are configured with coated diaphragm valves and coated MXT capillary columns to optimize the sensitivity and the analysis time. Both channels merge together in the same PED for an optimal selectivity. By this configuration, there is no interference from any hydrocarbons presence in the sample gas.

RESULTS:


Chromatogram for 11.9ppm THT

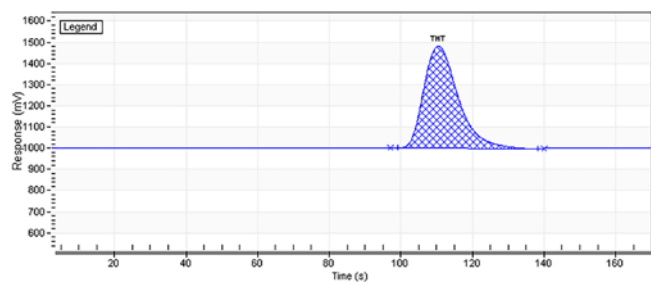


Chromatogram for 5.3ppm THT

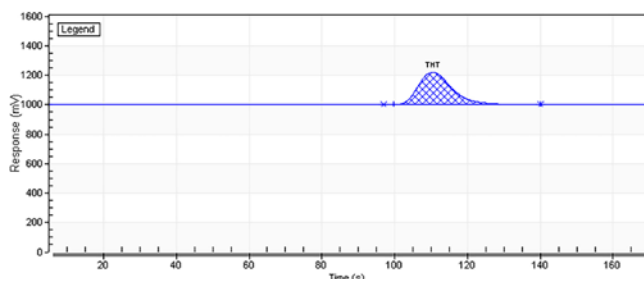

Chromatogram for 2.9ppm THT

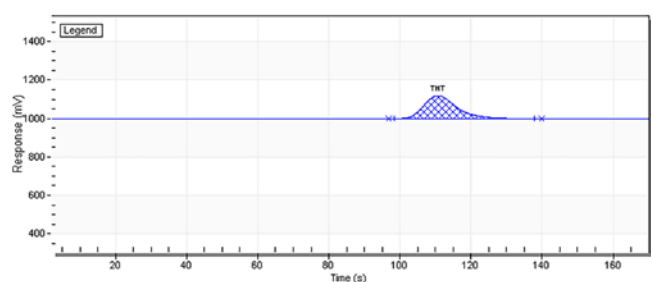


Chromatogram for 1.2ppm THT

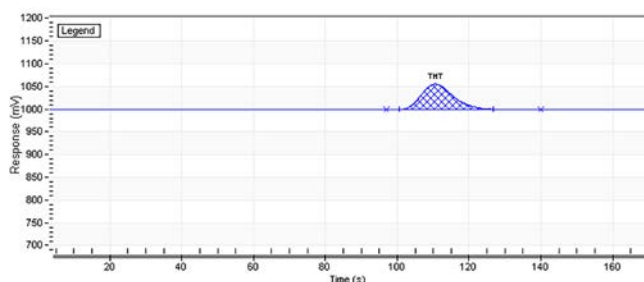





Based on the 4 chromatograms for THT, the linearity is as follow :

| Impurity : THT | |
|-------------------|--------------------------|
| Concentration | |
| ppm from dilution | Peak height(mV) from MD2 |
| 11.9 | 480 |
| 5.3 | 225 |
| 2.9 | 112 |
| 1.2 | 51 |
| 0 | 0 |

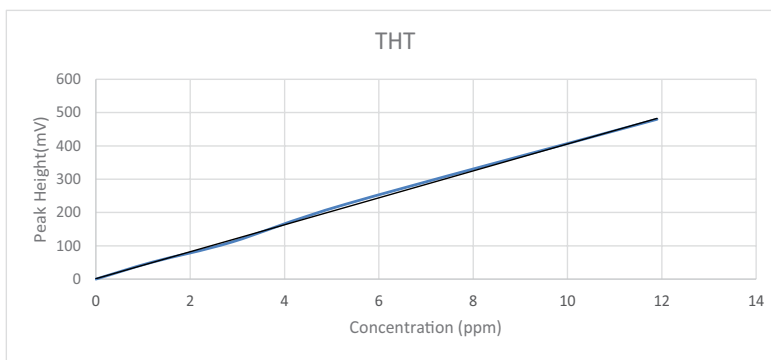


| | | |
|-----------------------------------|--------|----------|
| Coefficient correlation (R^2) | 0.9990 | Accepted |
|-----------------------------------|--------|----------|

R^2 for 5 points within the range must be between 0.998-1.00 to be accepted

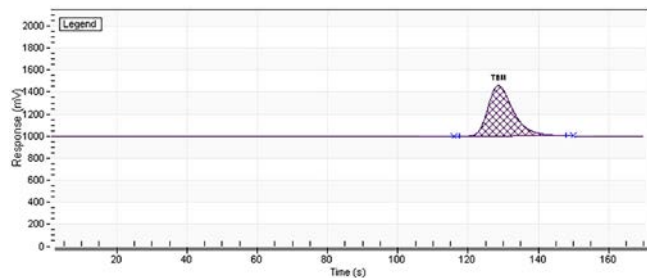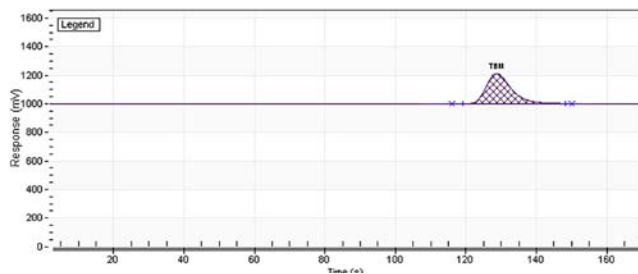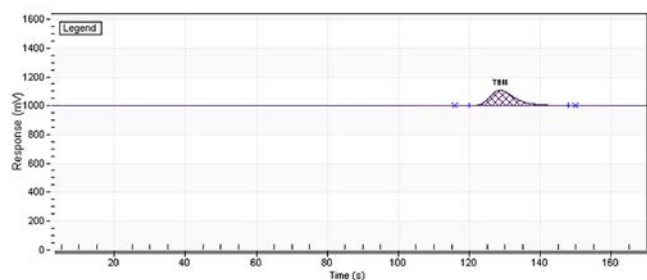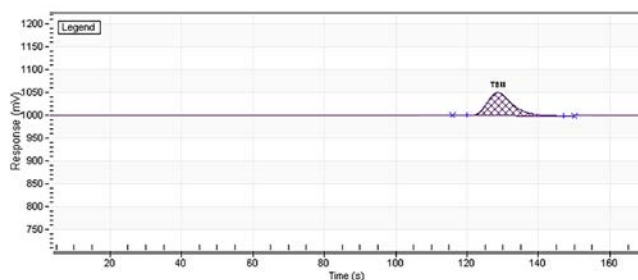Chromatogram for 11.3ppm TBM**Chromatogram for 5.4ppm TBM****Chromatogram for 2.8ppm TBM****Chromatogram for 1.4ppm TBM**

Based on the 4 chromatograms for TBM, the linearity is as follow :

| Impurity : TBM | |
|----------------------|-----------------------------|
| Concentration | |
| ppm from dilution | Peak height(mV) from MD2 |
| 11.3 | 455 |
| 5.4 | 225 |
| 2.8 | 120 |
| 1.4 | 51 |
| 0 | 0 |

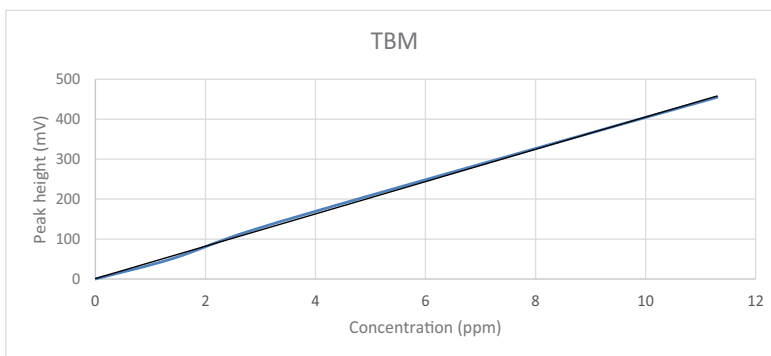

Coefficient correlation (R^2)

0.9991

Accepted

R^2 for 5 points within the range must be between 0.998-1.00 to be accepted

Repeatability for THT at a known concentration of 4.0 ppm in LNG.

| Start | stream | THT | THTbis | TBM1701 | TBM | TBMbis |
|------------------|--------|-----------|--------|---------|------|--------|
| 2019-03-12 04:00 | | 4.021 ppm | | | <LDL | |
| 2019-03-12 03:57 | | 3.942 ppm | | | <LDL | |
| 2019-03-12 03:54 | | 3.999 ppm | | | <LDL | |
| 2019-03-12 03:51 | | 4.117 ppm | | | <LDL | |
| 2019-03-12 03:48 | | 4.060 ppm | | | <LDL | |
| 2019-03-12 03:45 | | 3.980 ppm | | | <LDL | |
| 2019-03-12 03:42 | | 3.939 ppm | | | <LDL | |
| 2019-03-12 03:39 | | 4.005 ppm | | | <LDL | |
| 2019-03-12 03:36 | | 4.038 ppm | | | <LDL | |
| 2019-03-12 03:33 | | 4.077 ppm | | | <LDL | |
| 2019-03-12 03:30 | | 3.990 ppm | | | <LDL | |
| 2019-03-12 03:27 | | 4.090 ppm | | | <LDL | |
| 2019-03-12 03:24 | | 4.001 ppm | | | <LDL | |
| 2019-03-12 03:21 | | 3.988 ppm | | | <LDL | |
| 2019-03-12 03:19 | | 3.954 ppm | | | <LDL | |
| 2019-03-12 03:16 | | 4.027 ppm | | | <LDL | |
| 2019-03-12 03:13 | | 4.069 ppm | | | <LDL | |

For an 8 hours period, the repeatability is accepted at 2.16% for CV% x 3.

Repeatability for TBM at a known concentration of 5.2 ppm in LNG.

| Start | stream | THT | THTbis | TBM1701 | TBM | TBMbis |
|------------------|--------|------|--------|---------|-----------|--------|
| 2019-03-11 05:46 | | <LDL | | | 5.163 ppm | |
| 2019-03-11 05:43 | | <LDL | | | 5.176 ppm | |
| 2019-03-11 05:40 | | <LDL | | | 5.201 ppm | |
| 2019-03-11 05:37 | | <LDL | | | 5.137 ppm | |
| 2019-03-11 05:34 | | <LDL | | | 5.151 ppm | |
| 2019-03-11 05:31 | | <LDL | | | 5.188 ppm | |
| 2019-03-11 05:28 | | <LDL | | | 5.196 ppm | |
| 2019-03-11 05:25 | | <LDL | | | 5.173 ppm | |
| 2019-03-11 05:22 | | <LDL | | | 5.190 ppm | |
| 2019-03-11 05:19 | | <LDL | | | 5.204 ppm | |
| 2019-03-11 05:16 | | <LDL | | | 5.205 ppm | |
| 2019-03-11 05:14 | | <LDL | | | 5.199 ppm | |
| 2019-03-11 05:11 | | <LDL | | | 5.190 ppm | |
| 2019-03-11 05:08 | | <LDL | | | 5.145 ppm | |
| 2019-03-11 05:05 | | <LDL | | | 5.175 ppm | |
| 2019-03-11 05:02 | | <LDL | | | 5.199 ppm | |
| 2019-03-11 04:59 | | <LDL | | | 5.177 ppm | |


For an 8 hours period, the repeatability is accepted at 1.05% for CV% x 3.

Based on noise to ratio, LDL is calculated as follow :


| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------|---------------|-------------|-------|----------------|
| THT | 3.91ppm | 164mV | 0.4mV | 28.7ppb |
| TBM | 5.17ppm | 208mV | 0.3mV | 22.3ppb |

Note: other LDL could be obtained with different injection volume and chromatographic condition

3.91 ppm of THT measured in **channel 1**

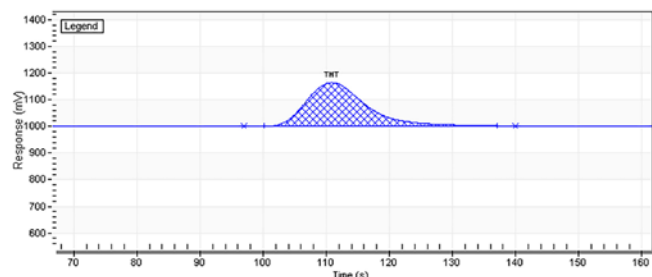

5.17ppm of TBM measured in **channel 2**

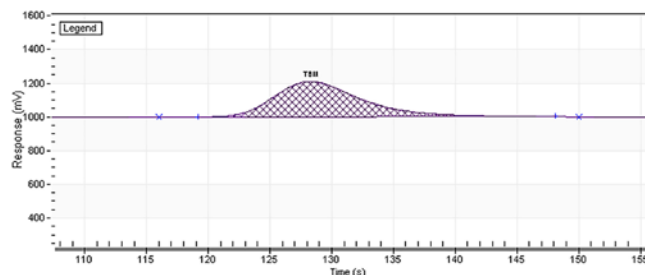

CONCLUSION:

Using a solution combining the PlasmaDetek 2 and MultiDetek 2 is the best way to achieve sensitivity, selectivity, simplicity, robustness and speed in an industrial compact system. Our solution can be used in safe zone or hazardous area. A purged version of the MultiDetek2 gas analyser is available to meet the ATEX and IECEx requirements if an ex proof solution is required.

APPLICATION NOTE

LD19-04



Measurement of sulfurs & mercaptans combined with THT-TBM in natural gas using the MultiDetek2 and PlasmaDetek2



▲ MultiDetek2

▲ PlasmaDetek2
patent US 9,310,308 B2

Natural gas is colourless and odourless in its most pure form. When extracted, it can contain sulphur compounds such as sulfurs and Mercaptans that when in the presence of moisture can produce sulphuric acid that can degrade the pipeline. So for reasons of public safety as well as pipeline integrity, there is a need to measure and control precisely the level of odorant species in natural gas:

- ▶ **Adjust the amount of sulphur molecules in the gas**
- ▶ **Control of odorant passivation**
- ▶ **Aids in detection of leaks**

This application note is the continuity of the previous app. note LD15-09 and LD19-01 where the description of the method for the detection of THT and TBM is demonstrated.

LDETEK SOLUTION:

The use of a highly sensitive detection system (PlasmaDetek2) combined with a compact GC system (MultiDetek2) is able to analyse sulfurs, mercaptans, Diethyl sulfide (DES), Dimethyl sulfide (DMS), Dimethyl disulfide (DMDS), THT and total sulphur directly without convertor. With its built in industrial PC, the MultiDetek2 offers all the conventional communication protocols (analog output, Modbus, Profibus, RS232/RS485), data storage capability and alarm contacts required for a process GC. Complete remote control of the system can be performed from the Ethernet connection available on every unit.

Our solution can be used in safe zone with our 6U standard 19" rackmount enclosure or in hazardous area with our IP66 rated 316SS wall mount purged enclosure 30"(762mm)deep x 57"(1447mm) height x 38"(965mm) width. An X-purge controller is installed to create a constant positive flow of air inside the enclosure, thus making a positive pressure inside enclosure. The purge is set to prevent toxic fumes from going inside the instrument in case of hazardous leakage.

The X-purge controller located on the top of the purged SS enclosure is configured to control the purging time requires prior to apply power to the instrument and hardware inside the box. It is also used for monitoring the purge pressure and flow rate inside the purged enclosure. In case of low purge pressure and/or flow rate, the power is shutoff instantly.

An extra safety pneumatic Swagelok VCR shut-off valve is mounted externally to the purged box on the sample inlet line to ensure the sample flow will but shut off in case of air supply pressure drops.


Internal temperature is monitored and controlled with a Vortex cooling system in case the unit isn't mounted in an air conditioned shelter. Our ATEX and IECEx solutions are certified by CSA following the standard II 2G Ex e mb ib pxb IIC T* Gb.

In this application note, the results of the performance are demonstrated for the analysis of sub ppb/ppm detection of COS-SO2-DES-DMDS-CS2-EM-DMS in natural gas. The representation of calibration chromatograms, the repeatability and the limit of detection well demonstrated the capability of our system for such type of application. One detector PlasmaDetek2 has been used. The multi channels of the MultiDetek2 GC are configured with coated diaphragm valves and coated metalized capillary columns to optimize the sensitivity and the carrier flow consumption. All channels merge together in the same PED for an optimal selectivity. More than one PED detector can be installed to allow parallel analysis and then reducing the analysis time when required. By this configuration, there is no interference coming from the other impurities present in the natural gas.

RESULTS:


Chromatogram for 10.28ppm COS in natural gas

| Peak | Unit | Calibration Value | Area Counts |
|------|------|-------------------|-------------|
| COS | ppm | 10.28 | 9607 |

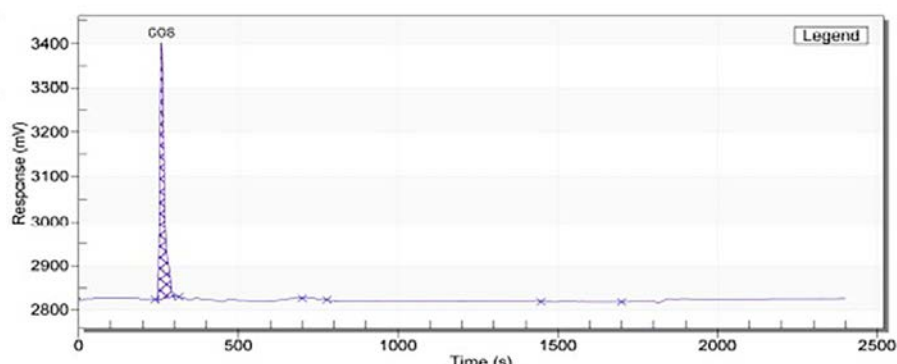


Chromatogram for 9.91ppm SO2 in natural gas

| Peak | Unit | Calibration Value | Area Counts |
|------|------|-------------------|-------------|
| SO2 | ppm | 9.91 | 5388 |

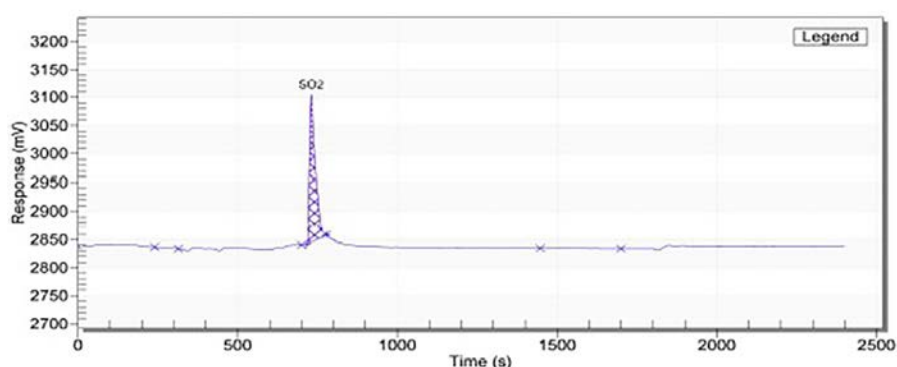


Chromatogram for 10.23ppm CS2-EM-DMS in natural gas

| Peak | Unit | Calibration Value | Area Counts |
|------------|------|-------------------|-------------|
| CS2-EM-DMS | ppm | 10.23 | 28361 |

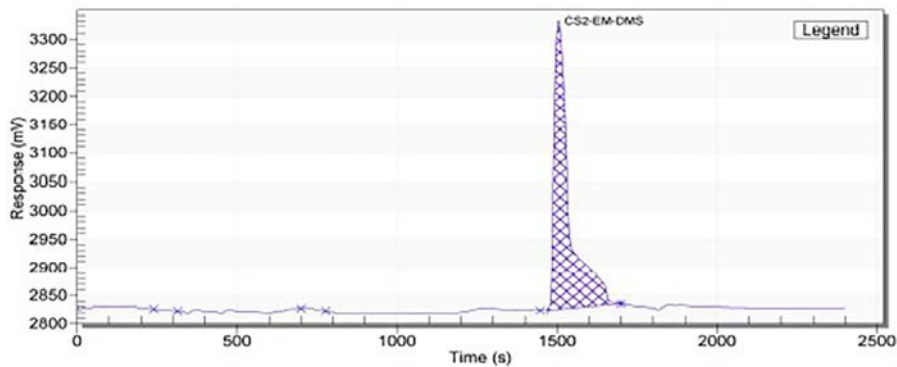

Chromatogram for 10.09ppm DES and 9.79ppm DMDS in natural gas

| Peak | Unit | Calibration Value | Area Counts |
|------|------|-------------------|-------------|
| DES | ppm | 10.09 | 16864 |
| DMDS | ppm | 9.79 | 14983 |

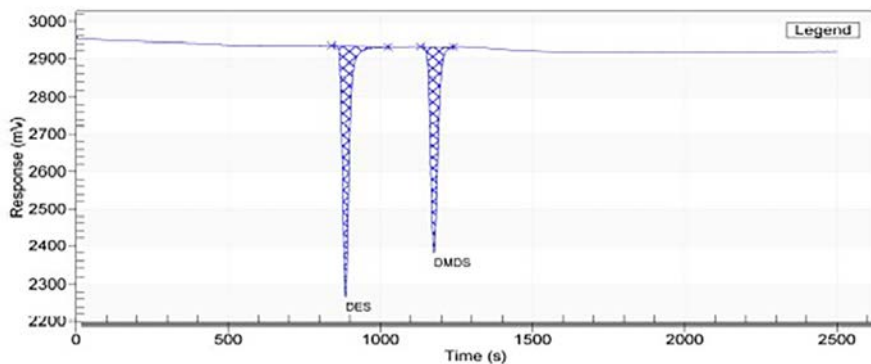

Repeatability to be at a value of $CV\% \times 3 < 5\%$ for a series of consecutive analysis at a fix concentration in a balance gas of natural gas.

COMPONENTS

Repeatability (CV% x 3)

| | |
|------|-------|
| DES | 3.99% |
| DMDS | 1.69% |
| COS | 4.66% |
| SO2 | 3.83% |
| CS2 | 2.45% |
| EM | 2.45% |
| DMS | 2.45% |

Results for THT and TBM are documented in our application note LD19-01.

Results (screenshot) of consecutive analysis at a fix concentration of 2.25ppm for DES and 2.10ppm for DMDS impurities in balance natural gas

| Historic | |
|------------------|--|
| istoric | |
| Thu, Aug-17-2017 | |
| 13:56:24 | COS[<LDL] SO2[<LDL] DES[2.284] DMDS[2.119] |
| 13:34:32 | COS[<LDL] SO2[<LDL] DES[2.253] DMDS[2.126] |
| 13:12:39 | COS[<LDL] SO2[<LDL] DES[2.207] DMDS[2.113] |
| 12:50:47 | COS[<LDL] SO2[<LDL] DES[2.274] DMDS[2.099] |
| 12:28:52 | COS[<LDL] SO2[<LDL] DES[2.290] DMDS[2.096] |
| 12:07:00 | COS[<LDL] SO2[<LDL] DES[2.257] DMDS[2.103] |
| 11:45:08 | COS[<LDL] SO2[<LDL] DES[2.243] DMDS[2.091] |
| 11:23:14 | COS[<LDL] SO2[<LDL] DES[2.260] DMDS[2.091] |
| 11:01:21 | COS[<LDL] SO2[<LDL] DES[2.231] DMDS[2.090] |
| 10:30:23 | COS[<LDL] SO2[<LDL] DES[2.224] DMDS[2.088] CS2-EM-DMS[<... |

Results (screenshot) of consecutive analysis at a fix concentration of 2.10ppm for COS impurity in balance natural gas

| Historic | |
|------------------|---|
| Historic | |
| Mon, Aug-21-2017 | |
| 08:01:30 | COS[2.157] SO2[<LDL] |
| 07:44:38 | COS[2.166] SO2[<LDL] |
| 07:25:37 | COS[2.137] |
| 06:45:19 | COS[2.117] SO2[<LDL] DES[<LDL] DMDS[<LDL] CS2-EM-DMS[<... |
| 06:05:00 | COS[2.100] SO2[<LDL] DES[<LDL] DMDS[<LDL] CS2-EM-DMS[<... |
| 05:24:42 | COS[2.081] SO2[<LDL] DES[<LDL] DMDS[<LDL] CS2-EM-DMS[<... |
| 04:44:24 | COS[2.049] SO2[<LDL] DES[<LDL] DMDS[<LDL] CS2-EM-DMS[<... |
| 04:04:05 | COS[2.021] SO2[<LDL] DES[<LDL] DMDS[<LDL] CS2-EM-DMS[<... |
| 03:23:46 | COS[2.016] SO2[<LDL] DES[<LDL] DMDS[<LDL] CS2-EM-DMS[<... |
| 02:43:26 | COS[1.986] SO2[<LDL] DES[<LDL] DMDS[<LDL] CS2-EM-DMS[<... |

Results (screenshot) of consecutive analysis at a fix concentration of 1.50ppm for SO2 impurity in balance natural gas

| Timestamp | COS | SO2 | DES | LDL | DMS | CS2-EM-DMS |
|-----------|------|---------|------|------|------|------------|
| 07:19:58 | <LDL | [1.476] | <LDL | <LDL | <LDL | <LDL |
| 06:39:39 | <LDL | [1.519] | <LDL | <LDL | <LDL | <LDL |
| 05:59:19 | <LDL | [1.507] | <LDL | <LDL | <LDL | <LDL |
| 05:18:59 | <LDL | [1.471] | <LDL | <LDL | <LDL | <LDL |
| 04:38:40 | <LDL | [1.488] | <LDL | <LDL | <LDL | <LDL |
| 03:58:19 | <LDL | [1.479] | <LDL | <LDL | <LDL | <LDL |
| 03:18:00 | <LDL | [1.482] | <LDL | <LDL | <LDL | <LDL |
| 02:37:40 | <LDL | [1.499] | <LDL | <LDL | <LDL | <LDL |
| 01:57:20 | <LDL | [1.495] | <LDL | <LDL | <LDL | <LDL |
| 01:17:00 | <LDL | [1.471] | <LDL | <LDL | <LDL | <LDL |

Results (screenshot) of consecutive analysis at a fix concentration of 1.55ppm for CS2-EM-DMS impurities in balance natural gas


| Timestamp | COS | SO2 | DES | LDL | DMS | CS2-EM-DMS |
|-----------|------|------|------|------|------|------------|
| 16:23:39 | <LDL | <LDL | <LDL | <LDL | <LDL | [1.571] |
| 14:20:59 | <LDL | <LDL | <LDL | <LDL | <LDL | [1.580] |
| 13:40:39 | <LDL | <LDL | <LDL | <LDL | <LDL | [1.563] |
| 13:00:20 | <LDL | <LDL | <LDL | <LDL | <LDL | [1.554] |
| 12:20:00 | <LDL | <LDL | <LDL | <LDL | <LDL | [1.588] |
| 11:39:40 | <LDL | <LDL | <LDL | <LDL | <LDL | [1.560] |
| 10:53:10 | <LDL | <LDL | <LDL | <LDL | <LDL | [1.605] |
| 10:12:50 | <LDL | <LDL | <LDL | <LDL | <LDL | [1.604] |
| 09:32:30 | <LDL | <LDL | <LDL | <LDL | <LDL | [1.597] |
| 08:52:08 | <LDL | <LDL | <LDL | <LDL | <LDL | [1.596] |

Based on noise to ratio, LDL is calculated as follow :


| COMPONENTS | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|------------|---------------|-------------|--------|----------------|
| DES | 2.28 ppm | 164 mV | 0.4 mV | 16.7 ppb |
| DMS | 2.11 ppm | 128 mV | 0.2 mV | 9.9 ppb |
| COS | 2.15 ppm | 252 mV | 0.3 mV | 7.7 ppb |
| SO2 | 1.47 ppm | 47 mV | 0.2 mV | 18.8 ppb |
| CS2 | 1.57 ppm | 198 mV | 0.4 mV | 9.5 ppb |
| EM | 1.57 ppm | 198 mV | 0.4 mV | 9.5 ppb |
| DMS | 1.57 ppm | 198 mV | 0.4 mV | 9.5 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic condition


DES : 2.25 ppm

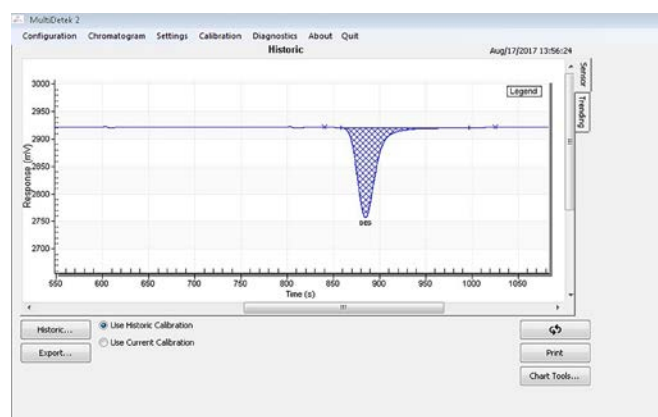


DMS : 2.11 ppm

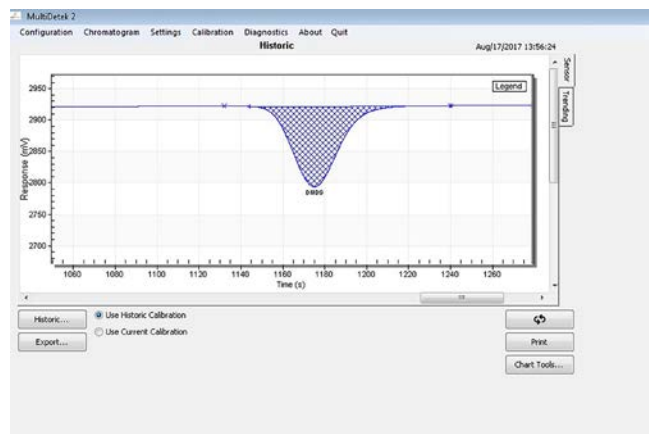


COS : 2.15 ppm

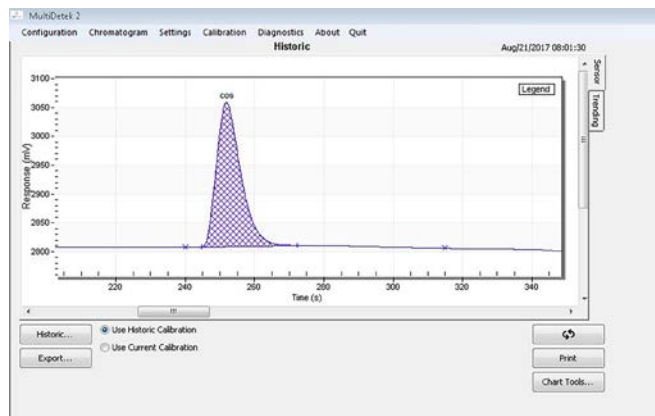

S02 : 1.47 ppm

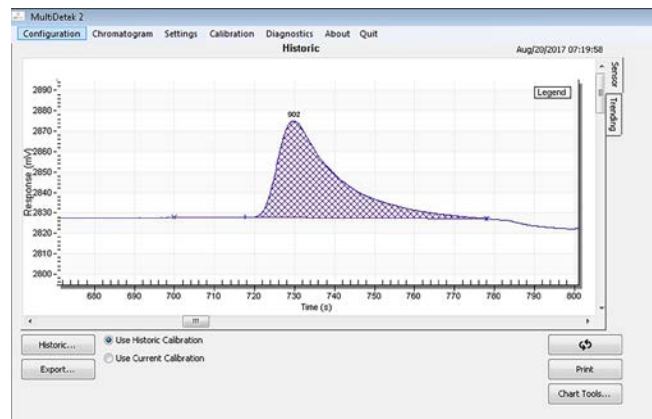

CS2-EM-DMS : 1.57 ppm

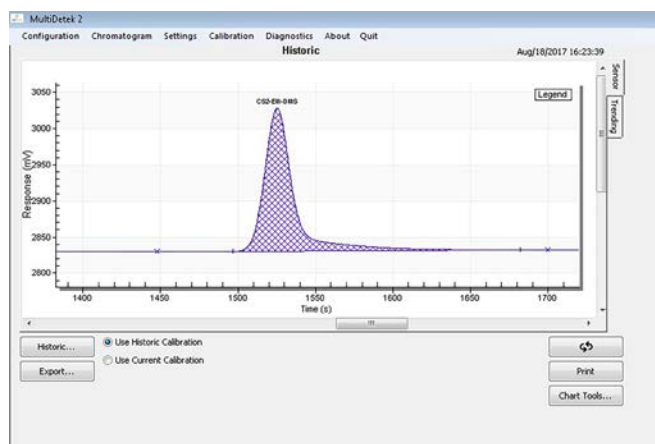

CONCLUSION:

Our MultiDetek2 GC coupled with our PlasmaDetek2 selective detector can together in one rackmount instrument measured sulfurs, mercaptans and THT-TBM in natural gas. It allows measuring all these impurities in LNG without the use of multiple detectors and accessories. The GC only requires a constant source of helium carrier gas being configured for minimum flow consumption using coated metalized capillary columns. The same instrument configuration can be used in the industry for pipeline and storage quality control. As well as process monitoring for natural gas extraction, landfill or biogas and also for delivery station for non-odorized gas as aerosol application. As describes, our instrument can be used in safe zone with its standard rackmount enclosure or in hazardous area using our wall mount IP66 rated 316 SS ATEX/IECEx certified X-purged solution.



3.0 APPLICATION NOTE

3.7 ENERGY



APPLICATION NOTE

LD16-04



Sulfur Hexafluoride (SF₆) purity analysis using the MultiDetek 2 and PlasmaDetek 2



▲ MultiDetek2

▲ PlasmaDetek2

SF₆ is used in the electrical industry as a gaseous dielectric medium for high-voltage circuit breakers, switchgear and other electrical equipment. Due to its high electrical insulation properties, it is often used for replacing oil filled circuit breakers. The sulfur hexafluoride is an expensive gas and it also has been identified as the most potent greenhouse gas. A SF₆ purity monitoring instrument is then required in the electrical industry to prevent failures, extend equipment life, reduces equipment cost and increase safety.

LDETEK SOLUTION:

Using the compact MultiDetek2 combined with the robust PlasmaDetek2 detector, this application note shows our solution for measuring impurities in SF₆ to ensure good operations of electrical equipment. The system has been configured with two channels both merging in the PlasmaDetek2 detector.

The first channel is used for measuring O₂-N₂-CO using a porous polymer Q type pre column combined with a Mol Sieve separation column. The pre column is mounted on a 10 port injection/back flush diaphragm valve to flush out the SF₆. The second column allows the separation of O₂-N₂ and CO.

The second channel is used for CF₄ analysis. This channel is also mounted with a 10 port injection/back flush diaphragm valve with two Porapak Q type columns. The pre column is used to flush out the SF₆ and the second column for separation of CF₄ from other impurities. This channel can also allow the analysis of CO₂ and SOF₂.

RESULTS:

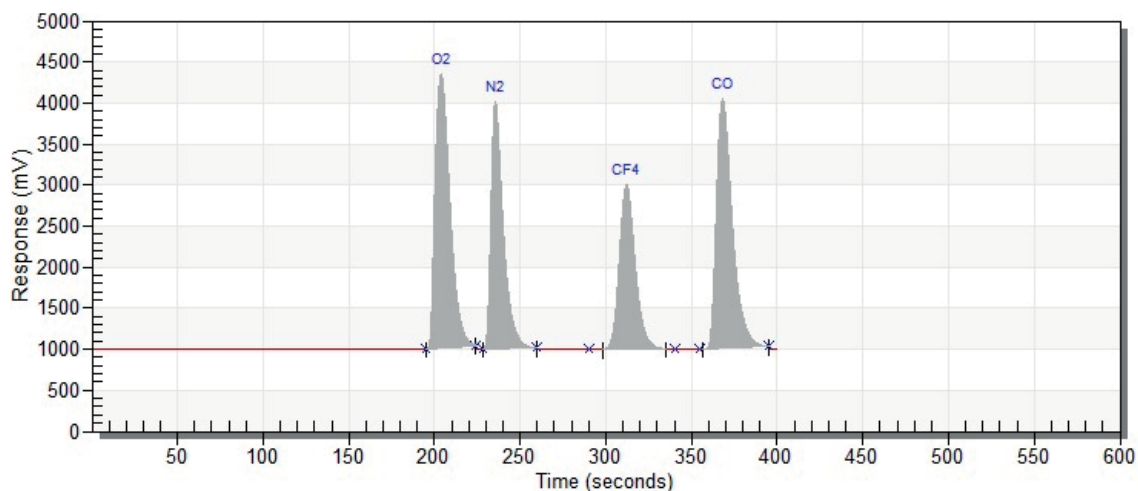


Figure 1: Chromatogram of trace impurities in balance SF6

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------------|---------------|-------------|--------|----------------|
| O ₂ | 1701 ppm | 4425 mV | 2 mV | 2.3 ppm |
| N ₂ | 1446 ppm | 4101 mV | 0.2 mV | 0.6 ppm |
| CF ₄ | 64 ppm | 3055 mV | 10 mV | 0.6 ppm |
| CO | 196 ppm | 4170 mV | 5 mV | 0.7 ppm |

Note: other LDL could be obtained with different injection volume and chromatographic conditions

Figure 2: LDL based on 3 times noise ratio

CONCLUSION:

Using a solution combining the PlasmaDetek 2 and the MultiDetek 2 is the best way to achieve sensitivity, robustness and speed in a compact GC system for sulfur hexafluoride purity analysis for the energy market.



3.0 APPLICATION NOTE

3.8 FOOD AND BEVERAGE



3.0 APPLICATION NOTES

APPLICATION NOTE

LD16-12



Trace impurities in Carbon Dioxide for beverage and food packaging industry



▲ MultiDetek2

▲ PlasmaDetek2

With regards to the beverage industry, the dissolved Carbon Dioxide which is used as carbonic acid gives a pleasantly acidic flavour and a nice mouth-feel when drinking. When it is not present, the drinks taste flat. Being used in many different fields of food and beverage, the CO₂ quality management is essential to meet the market requirements.

The CO₂ is produced from different techniques such as fermentation, combustion, ammonia/hydrogen production and others. It is required by the industry, especially for bottlers to control the supply chain by monitoring the CO₂ purity allowing maintenance of the product quality.

LDETEK SOLUTION:

Using the PlasmaDetek2(PED) plasma detector and the MultiDetek2 compact gas chromatograph, the analysis of the most critical trace impurities in carbon dioxide can be achieved in one unit with a single detection technology (PED).

By default, the configuration has 3 channels to cover the analysis of Benzene, Acetaldehyde, Nitrogen and Carbon Monoxide. If additional options for the analysis of Methanol, Sulfurs and Hydrocarbons are required, then channels 4, 5 and 6 are added in the same instrument.

Channel#1: 0-100ppb Benzene

Channel#2: 0-1000ppb Acetaldehyde

Channel#2: 0-120ppm Nitrogen & 0-10ppm Carbon Monoxide

Also integrated inside the MultiDetek2, a dilution system allows generating for a span calibration gas at ppb level for the low concentration impurities. This option gives you the capacity to use a standard certified calibration gas at higher concentrations, which is usually lower in cost and easier to get, also that generates a low ppb calibration gas. The dilution system is designed for low gas consumption, high accuracy/stability and is automatically handled by the interface during span calibration process.

For multiple streams requirement, the LDGSS high purity stream selector system can be combined with the MultiDetek2 to offer all the flexibility to switch streams and even run stream sequences analysis as required.

RESULTS:

The results show the performances of the system for a standard configuration used to measure Benzene, Acetaldehyde, Nitrogen and Carbon Monoxide in Carbon Dioxide.

It displays details about the calibration chromatogram, some examples of low ppb chromatograms for each impurity, the IdI chart for noise/response calculation, the stability and the linearity curves.

SPAN CALIBRATION CHROMATOGRAM:

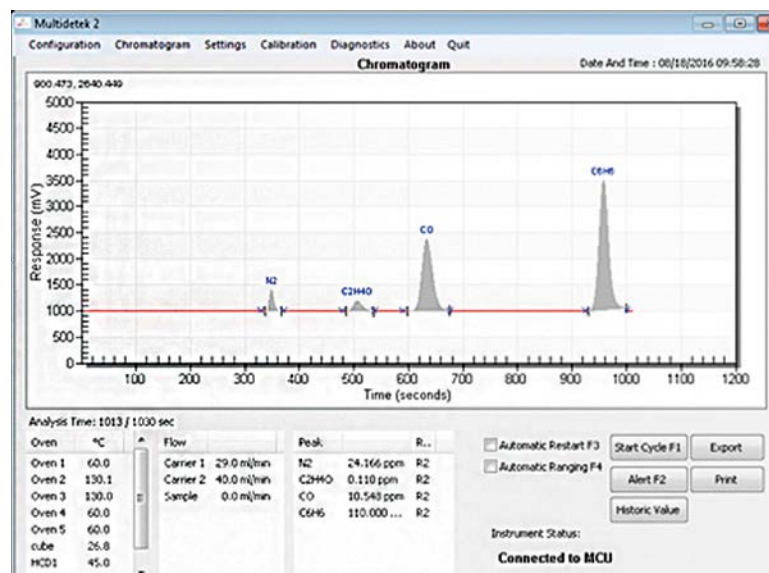


Figure 1:
Chromatogram of a gas mixture containing 24ppm nitrogen, 110ppb acetaldehyde, 10.5ppm carbon monoxide and 110ppb benzene in a balance gas carbon dioxide.

LOW PPB CHROMATOGRAM:

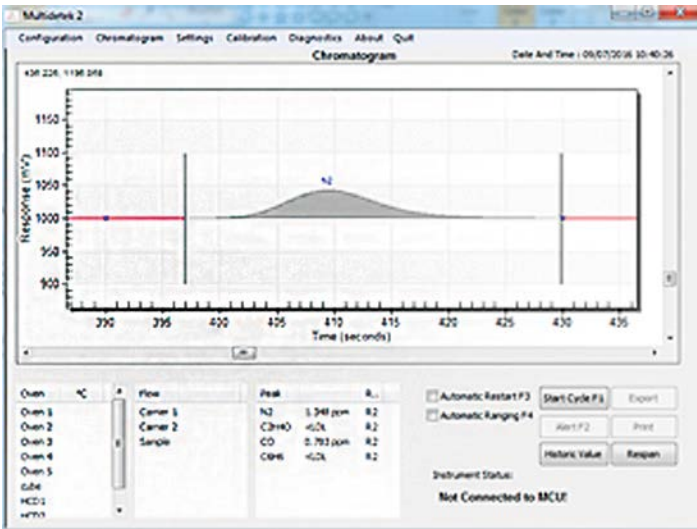


Figure 2:
Chromatogram of 1348 ppb Nitrogen in
Carbon dioxide

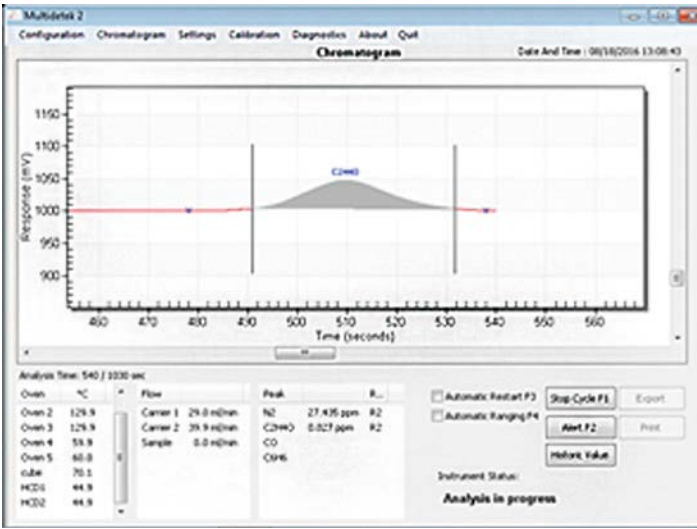


Figure 3:
Chromatogram of 27ppb Acetaldehyde in
Carbon dioxide

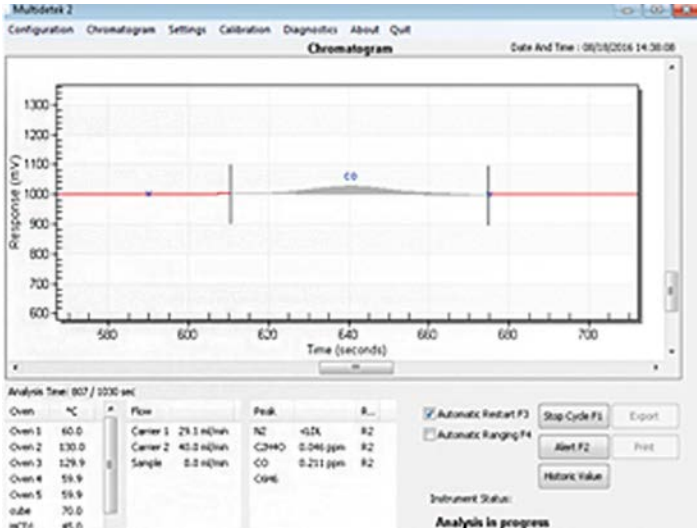


Figure 4:
Chromatogram of 211ppb Carbon monoxide in
Carbon dioxide

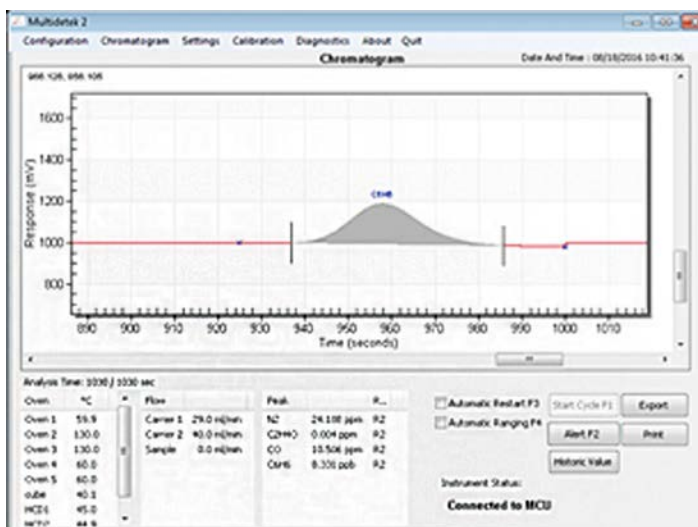


Figure 5:
Chromatogram of 8.331ppb Benzene in Carbon dioxide

LDL calculation

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|-----------------|---------------|-------------|--------|----------------|
| Nitrogen | 1348 ppb | 49.3 mV | 0.2 mV | 16.4 ppb |
| Acetaldehyde | 27 ppb | 49.1 mV | 1.1 mV | 1.8 ppb |
| Carbon monoxide | 211 ppb | 35.4 mV | 1.6 mV | 28.6 ppb |
| Benzene | 8.331 ppb | 215.7 mV | 2.1 mV | 0.243 ppb |


Note: other LDL could be obtained with different injection volume and chromatographic conditions

STABILITY:

| Date/Time | N2 | C2H4O | CO | C6H6 |
|----------------------|--------|-------|--------|--------|
| Aug/18/2016 08:07:47 | 24.596 | 0.783 | 10.601 | 57.229 |
| Aug/18/2016 07:50:32 | 24.678 | 0.783 | 10.601 | 57.165 |
| Aug/18/2016 07:33:17 | 24.606 | 0.784 | 10.597 | 57.110 |
| Aug/18/2016 07:16:00 | 24.588 | 0.784 | 10.615 | 57.026 |
| Aug/18/2016 06:58:45 | 24.579 | 0.784 | 10.613 | 57.102 |
| Aug/18/2016 06:41:29 | 24.617 | 0.783 | 10.613 | 56.838 |
| Aug/18/2016 06:24:13 | 24.768 | 0.782 | 10.617 | 56.933 |
| Aug/18/2016 06:06:57 | 24.742 | 0.781 | 10.617 | 56.960 |
| Aug/18/2016 05:49:41 | 24.627 | 0.780 | 10.601 | 56.890 |
| Aug/18/2016 05:32:25 | 24.720 | 0.780 | 10.599 | 56.752 |
| Aug/18/2016 05:15:10 | 24.687 | 0.780 | 10.599 | 56.860 |
| Aug/18/2016 04:57:54 | 24.762 | 0.780 | 10.596 | 56.920 |
| Aug/18/2016 04:40:38 | 24.797 | 0.780 | 10.599 | 56.879 |
| Aug/18/2016 04:23:22 | 24.827 | 0.780 | 10.599 | 57.006 |
| Aug/18/2016 04:06:06 | 24.728 | 0.780 | 10.604 | 56.974 |

Figure 6:
The results show the stability over a period of 15 consecutive cycles. The units for nitrogen, acetaldehyde and carbon monoxide are ppm and the unit for benzene is ppb


LINEARITY:

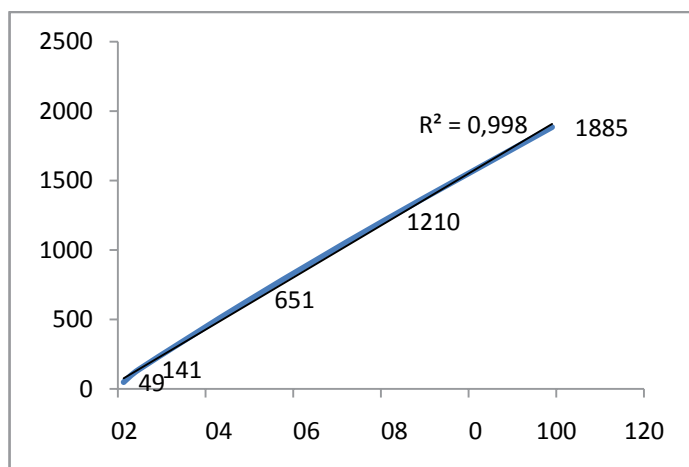

N2 CONCENTRATION N2 RESPONSE

| | |
|------------|---------|
| 1.348 ppm | 49 mV |
| 4.856 ppm | 141 mV |
| 30.518 ppm | 651 mV |
| 60.6 ppm | 1210 mV |
| 99 ppm | 1885 mV |


Figure 7:
Impurity : nitrogen

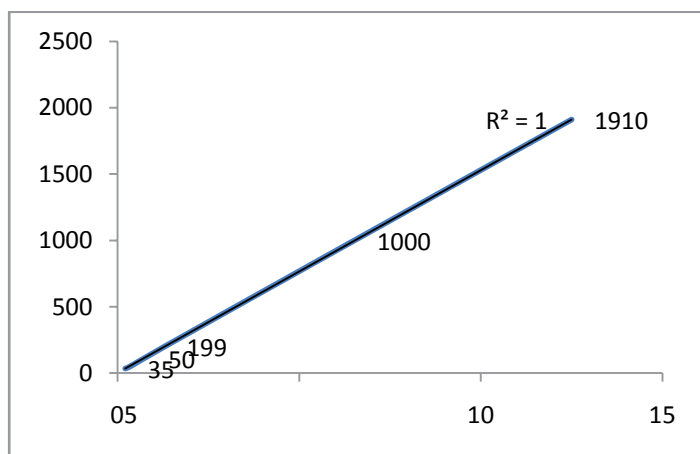

CO CONCENTRATION CO RESPONSE

| | |
|-----------|---------|
| 0.211 ppm | 35 mV |
| 0.343 ppm | 50 mV |
| 1.285 ppm | 199 mV |
| 6.521 ppm | 1000 mV |
| 12.5 ppm | 1910 mV |


Figure 8:
Impurity : carbon monoxide

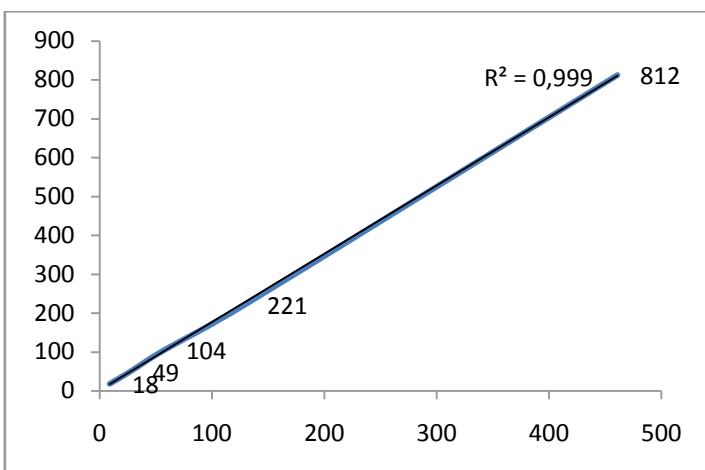

ACETALDEHYDE CONCENTRATION ACETALDEHYDE RESPONSE

| | |
|---------|--------|
| 9 ppb | 18 mV |
| 27 ppb | 49 mV |
| 57 ppb | 104 mV |
| 129 ppb | 221 mV |
| 461 ppb | 812 mV |

Figure 9:
Impurity : acetaldehyde

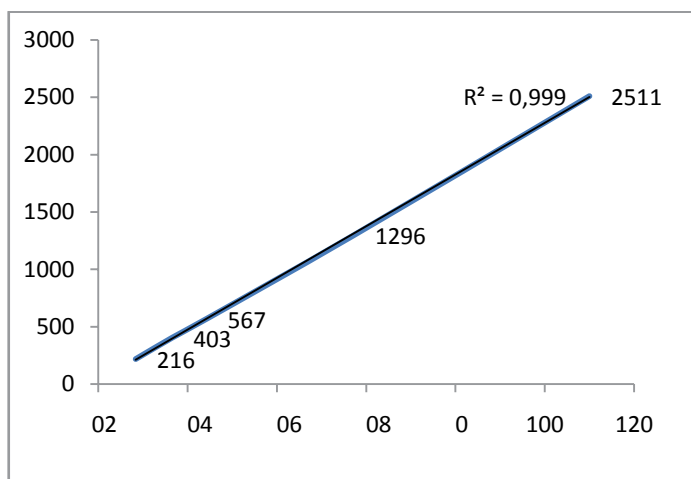

| BENZENE CONCENTRATION | BENZENE RESPONSE |
|--------------------------|------------------|
| 8.331 ppb | 216 mV |
| 16.532 ppb | 403 mV |
| 24.212 ppb | 567 mV |
| 57.158 ppb | 1296 mV |
| 110 ppb | 2511 mV |

Figure 10:
Impurity : benzene

CONCLUSION:

Our solution detects traces of gas impurities required by the food and beverage industry for Carbon Dioxide. The complete spectrum analysis can be covered with one single MultiDetek2 unit using the PlasmaDetek2 detection technology. It can detect sub ppb concentrations that are required for this type of application. It combines the analysis of different gas types that are usually very difficult to do with the same instrument. The MultiDetek2 offers a solution with an integrated PC interface that offers standard communication protocols compatible with all market standards.

APPLICATION NOTE

LD17-02



Gas analysis for wineries



In the wineries for proper wine production, inert gases like nitrogen, carbon dioxide and argon are used for sparging, blanketing as counter-pressure to move wine(usually from barrels), as well as to flush transfer lines and tanks prior to moving wine or juice. Sparging involves the introduction of a stream of very fine gas bubbles to help add or remove dissolved Oxygen or CO₂. Blanketing partially-filled tanks attempts to maintain an inert gas layer above the wine/ juice surface in the hope of minimizing wine/air contact. The main reason for the use of inert gassing is to prevent the growth of aerobic microorganisms in the wine. The gas chromatography is a well known analysis technique to ensure the measurement of the purity and to control the production of wine to achieve the best quality.

LDETEK SOLUTION:

Using the PlasmaDetek2(PED) plasma detector and the MultiDetek2 compact gas chromatograph, the analysis of the most critical impurities in carbon dioxide, nitrogen and argon used in wine production can be achieved with a single unit.

The configuration uses one channel for trace analysis of O₂-N₂-CO₂-Ethanol with the PlasmaDetek2(PED) optimized for low concentrations. The second channel is configured with a conventional TCD optimized for high concentrations in % for O₂-N₂-CO₂-Ethanol. This dual detectors configuration allows covering a wide analysis range.

- **Channel#1:** Trace O₂-N₂-CO₂-Ethanol
- **Channel#2:** % O₂-N₂-CO₂-Ethanol

Since the sample volume and pressure for this type of application is limited, the MultiDetek2 is equipped with a mini pump that sucks the right amount of sample to fill the sampling loops correctly prior to run the analysis. The parameters can be adjusted by the user easily from the software interface depending of the sample line selected. The sample collection system is designed(leak free) for low O₂-N₂ analysis performances without air contamination.

The advantages of our solution over standard chromatograph systems is based on the use of Argon as carrier gas with the PlasmaDetek2. It allows an easy GC configuration that can measure O₂-N₂ with a single column configuration, having low operating cost and getting good sensitivity at ppb level. This isn't feasible with standard ionisation detector because of the use of Helium as carrier gas, the O₂ analysis becomes not possible and the operating cost are higher.

RESULTS


The results show the performances of the system for each pre configured method used to measure impurities in each sample type.

Method #1 is configured and calibrated for trace (Ar+O2)-CO2-ethanol in sample gas nitrogen.

Method #2 is configured and calibrated for trace N2-CO2-ethanol in sample gas argon.


Method #3 is configured and calibrated for percent (Ar+O2)-N2-ethanol in sample gas carbon dioxide.

Span calibration chromatogram for Nitrogen method:

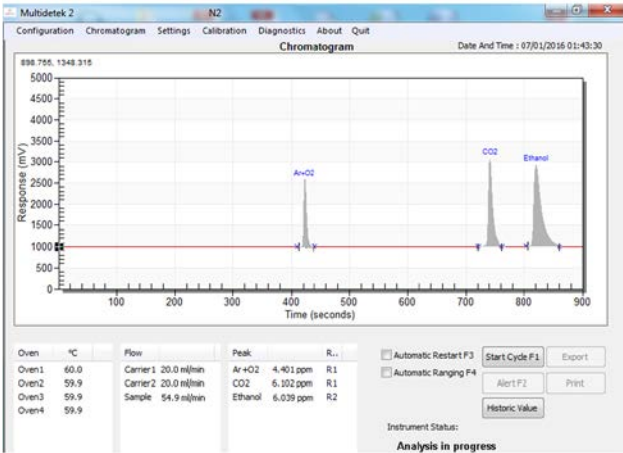


Chromatogram of a gas mixture containing 4.4ppm O2, 6.1ppm CO2 and 6.0ppm ethanol in a balance gas Nitrogen.

Span calibration chromatogram for Argon method:

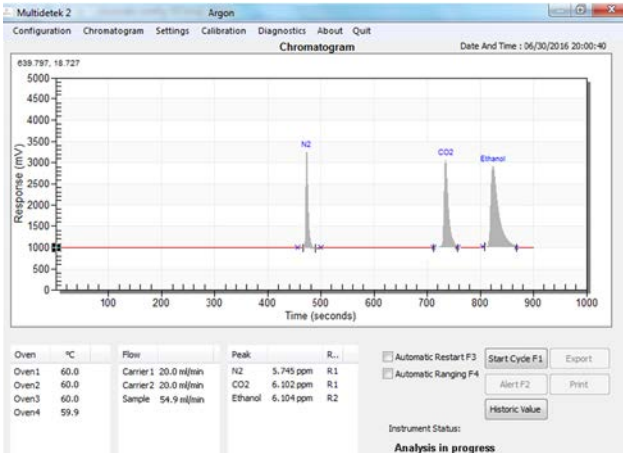

Chromatogram of a gas mixture containing 5.7ppm N2, 6.1ppm CO2 and 6.1ppm ethanol in a balance gas Argon.

Span calibration chromatogram for Carbon dioxide method:

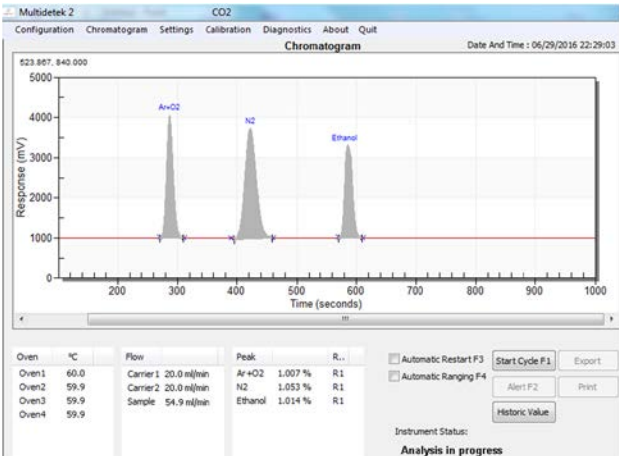

Chromatogram of a gas mixture containing 1% O2, 1% N2 and 1% ethanol in a balance gas Carbon dioxide.

CONCLUSION:

Our solution combines our PlasmaDetek2 for low ppb/ppm concentrations and a TCD for the percent concentrations. Having this dual detectors configuration, a wide range of analysis can be covered. The MultiDetek2 is configured with multiple methods depending of the requirements. It is easy for the user to simply load the proper method for his requirement. On request, additional impurities and methods can be added to the same system.

Our solution is robust and perfectly adapted for the gas analysis used in the wine production sector.

APPLICATION NOTE

LD17-04



Trace impurities in Carbon Dioxide for beverage and food packaging industry



▲ MultiDetek2

▲ PlasmaDetek2

With regards to the beverage industry, the dissolved Carbon Dioxide which is used as carbonic acid gives a pleasantly acidic flavour and a nice mouth-feel when drinking. When it is not present, the drinks taste flat. Being used in many different fields of food and beverage, the CO₂ quality management is essential to meet the market requirements.

The CO₂ is produced from different techniques such as fermentation, combustion, ammonia/hydrogen production and others. It is required by the industry, especially for bottlers to control the supply chain by monitoring the CO₂ purity allowing maintenance of the product quality.

LDETEK SOLUTION:

Following the application note LD16-12 this application note shows another configuration of the MultiDetek2 with PlasmaDetek2 also related to the beverage industry where the analysis of different components in carbon dioxide is realized.

This configuration has 3 channels to cover the analysis of benzene, hydrogen sulfide, nitrogen and oxygen. Additional channels can be added if analysis of more components is required. All the components are measured with one type detector PED using Helium as carrier gas.

- ▶ **Channel#1:** 0-1000ppb benzene
- ▶ **Channel#2:** 0-1000ppb hydrogen sulfide
- ▶ **Channel#3:** 0-10ppm oxygen and nitrogen

A FID analyser LD2000 is added to this solution for measuring THC on a scale of 0-10ppm

A TCD binary gas analyser LD8000 is added for measuring 98-100% CO₂ purity

A dewpoint meter LD500 is added for the analysis of moisture on a 0-10ppm scale

LDRACK CABINET:


All the instruments are integrated in the LDrack cabinet. A multiple streams selector system LDGSS selects the right gas lines for analysis. The stream selector can be controlled locally or remotely with the MultiDetek2 interface. The complete solution is configured with coated stainless steel tubing to ensure stability of the system. It reduces the risk of surface absorption, especially for the sulfur components.



RESULTS:

The results show the performances of the MultiDetek2 system for a standard configuration used to measure oxygen, nitrogen, benzene and hydrogen sulfide in Carbon Dioxide. The Idl and repeatability results are demonstrated.

Analysis of a gas mixture containing a certified concentration of trace O2-N2-C6H6-H2S-H2O in balance gas CO2

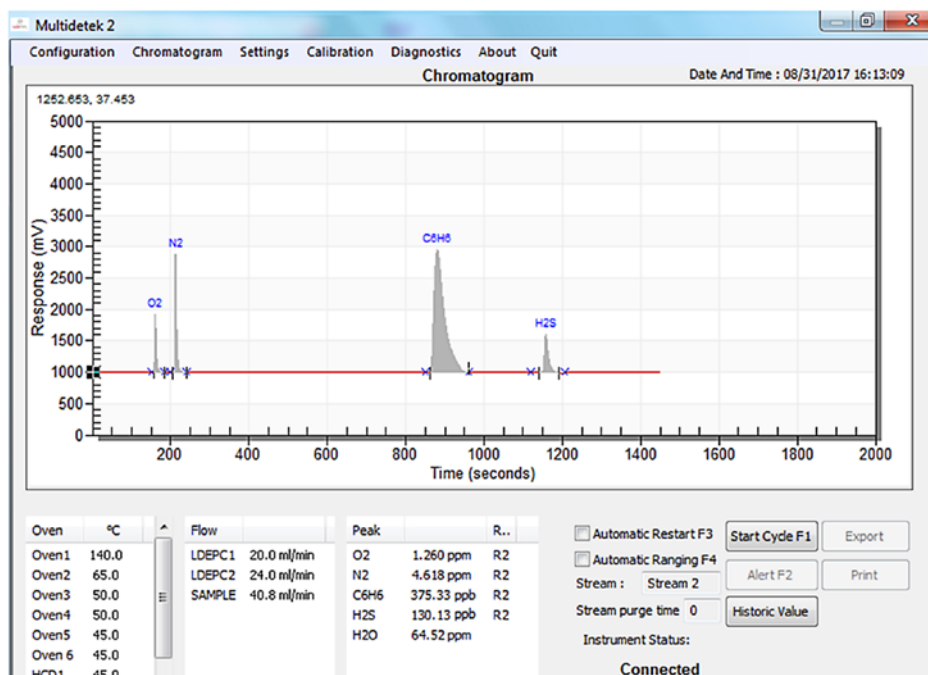

LDL:

| COMPONENT | CONCENTRATION | PEAK HEIGHT | NOISE | LDL (3X NOISE) |
|------------------|---------------|-------------|---------|----------------|
| Oxygen | 1.260 ppm | 987 mV | 4.2 mV | 16.0 ppb |
| Nitrogen | 4.618 ppm | 1961 mV | 2.9 mV | 20.4 ppb |
| Benzene | 375.33 ppb | 1987 mV | 12.6 mV | 7.14 ppb |
| Hydrogen sulfide | 130.13 ppb | 611 mV | 12.9 mV | 8.24 ppb |

Note: other LDL could be obtained with different injection volume and chromatographic condition

REPEATABILITY:

The results below show the repeatability for each component. Three times of the percentage of coefficient of variation (3*CV %) for each component must be smaller than 5% to meet the requirements.

$$s = \sqrt{\frac{1}{N-1} \sum_{i=1}^N (x_i - \bar{x})^2}$$

| COMPONENT | CV (%) | CV% x 3 < 5% |
|------------------|--------|--------------|
| Oxygen | 0.95 | 2.85 |
| Nitrogen | 0.66 | 1.98 |
| Benzene | 1.02 | 3.06 |
| Hydrogen sulfide | 0.74 | 2.22 |

Component : O2

| Historic Values | | | | |
|----------------------|-------|-------|-------|--|
| Date/Time | O2 | N2 | C6H6 | |
| Jun/20/2017 07:53:23 | 4.132 | 3.380 | <LDL | |
| Jun/20/2017 07:35:37 | 4.126 | 3.388 | <LDL | |
| Jun/20/2017 07:17:51 | 4.114 | 3.380 | <LDL | |
| Jun/20/2017 07:00:05 | 4.142 | 3.400 | <LDL | |
| Jun/20/2017 06:42:19 | 4.179 | 3.406 | <LDL | |
| Jun/20/2017 06:24:33 | 4.197 | 3.432 | <LDL | |
| Jun/20/2017 06:06:47 | 4.211 | 3.435 | <LDL | |
| Jun/20/2017 05:49:01 | 4.244 | 3.444 | 0.068 | |
| Jun/20/2017 05:31:15 | 4.246 | 3.442 | <LDL | |
| Jun/20/2017 05:13:29 | 4.230 | 3.433 | <LDL | |
| Jun/20/2017 04:55:43 | 4.213 | 3.414 | <LDL | |
| Jun/20/2017 04:37:57 | 4.218 | 3.428 | 0.089 | |
| Jun/20/2017 04:20:11 | 4.229 | 3.453 | <LDL | |
| Jun/20/2017 04:02:25 | 4.222 | 3.447 | <LDL | |
| Jun/20/2017 03:44:39 | 4.203 | 3.444 | <LDL | |

Component : N2

| Historic Values | | | | |
|----------------------|-------|-------|-------|--|
| Date/Time | O2 | N2 | C6H6 | |
| Jun/20/2017 07:53:23 | 4.132 | 3.380 | <LDL | |
| Jun/20/2017 07:35:37 | 4.126 | 3.388 | <LDL | |
| Jun/20/2017 07:17:51 | 4.114 | 3.380 | <LDL | |
| Jun/20/2017 07:00:05 | 4.142 | 3.400 | <LDL | |
| Jun/20/2017 06:42:19 | 4.179 | 3.406 | <LDL | |
| Jun/20/2017 06:24:33 | 4.197 | 3.432 | <LDL | |
| Jun/20/2017 06:06:47 | 4.211 | 3.435 | <LDL | |
| Jun/20/2017 05:49:01 | 4.244 | 3.444 | 0.068 | |
| Jun/20/2017 05:31:15 | 4.246 | 3.442 | <LDL | |
| Jun/20/2017 05:13:29 | 4.230 | 3.433 | <LDL | |
| Jun/20/2017 04:55:43 | 4.213 | 3.414 | <LDL | |
| Jun/20/2017 04:37:57 | 4.218 | 3.428 | 0.089 | |
| Jun/20/2017 04:20:11 | 4.229 | 3.453 | <LDL | |
| Jun/20/2017 04:02:25 | 4.222 | 3.447 | <LDL | |
| Jun/20/2017 03:44:39 | 4.203 | 3.444 | <LDL | |

Component : C6H6

| Historic Values | | | | |
|----------------------|-------|-------|---------|--|
| Date/Time | O2 | N2 | C6H6 | |
| Jun/22/2017 07:31:16 | 0.235 | 0.721 | 217.452 | |
| Jun/22/2017 07:11:09 | 0.237 | 0.721 | 216.403 | |
| Jun/22/2017 06:51:02 | 0.238 | 0.722 | 216.805 | |
| Jun/22/2017 06:30:55 | 0.237 | 0.782 | 216.725 | |
| Jun/22/2017 06:10:48 | 0.237 | 0.718 | 212.256 | |
| Jun/22/2017 05:50:41 | 0.239 | 0.728 | 213.026 | |
| Jun/22/2017 05:30:34 | 0.238 | 0.722 | 214.129 | |
| Jun/22/2017 05:10:27 | 0.234 | 0.729 | 217.782 | |
| Jun/22/2017 04:50:20 | 0.236 | 0.735 | 214.711 | |
| Jun/22/2017 04:30:13 | 0.239 | 0.739 | 214.861 | |
| Jun/22/2017 04:10:06 | 0.240 | 0.746 | 214.218 | |
| Jun/22/2017 03:49:59 | 0.241 | 0.753 | 213.506 | |
| Jun/22/2017 03:29:52 | 0.239 | 0.739 | 208.152 | |
| Jun/22/2017 03:09:45 | 0.239 | 0.777 | 207.693 | |
| Jun/22/2017 02:49:38 | 0.236 | 0.736 | 208.471 | |

Component : H2S

| Historic Values | | | | | |
|----------------------|-------|-------|---------|-------|--|
| Date/Time | O2 | N2 | H2S | C6H6 | |
| Jul/03/2017 06:48:40 | <LDL | 0.021 | 200.383 | <LDL | |
| Jul/03/2017 06:28:33 | 0.011 | 0.030 | 199.310 | 0.057 | |
| Jul/03/2017 06:08:26 | <LDL | <LDL | 199.189 | 0.089 | |
| Jul/03/2017 05:48:19 | <LDL | <LDL | 201.363 | 0.065 | |
| Jul/03/2017 05:28:12 | <LDL | <LDL | 202.909 | <LDL | |
| Jul/03/2017 05:08:05 | <LDL | <LDL | 201.060 | <LDL | |
| Jul/03/2017 04:47:58 | <LDL | <LDL | 200.999 | <LDL | |
| Jul/03/2017 04:27:51 | 0.007 | 0.020 | 202.269 | 0.403 | |
| Jul/03/2017 04:07:44 | <LDL | 0.030 | 200.069 | <LDL | |
| Jul/03/2017 03:47:37 | 0.009 | 0.030 | 199.016 | <LDL | |
| Jul/03/2017 03:27:30 | 0.007 | 0.030 | 199.152 | <LDL | |
| Jul/03/2017 03:07:23 | <LDL | <LDL | 199.657 | <LDL | |
| Jul/03/2017 02:47:16 | <LDL | <LDL | 197.671 | <LDL | |
| Jul/03/2017 02:27:09 | 0.001 | 0.019 | 196.237 | <LDL | |
| Jul/03/2017 02:07:02 | <LDL | <LDL | 193.154 | <LDL | |

CONCLUSION:

Our solution combining multiple LDetek instruments to achieve the complete carbon dioxide analysis all in one cabinet well demonstrated the capabilities to meet the food and beverage industry requirements. Have a look at our complementary application note LD16-012 that demonstrates other capabilities and results related to this market.



3.0 APPLICATION NOTE

3.9 PHARMACEUTICAL AND MEDICAL



3.0 APPLICATION NOTES

APPLICATION NOTE

LD20-01



MultiDetek2 gas chromatograph uses for medical & pharmaceutical applications



▲ MultiDetek2

LDETEK SOLUTION:

Our medical gas analysers control safety and quality of production, according to the European Pharmacopeia norms.


LDetek provides different GC configurations using the MultiDetek2 gas chromatograph where different detectors as our TCD and/or our FID can be mounted in.

Various applications possible :


- ▶ **Nitrous Oxide:** Analysis of ppm CO by FID & ppm CO₂ by TCD inside the same unit
- ▶ **Carbon dioxide:** Analysis of ppm CO by FID
- ▶ **Nitrogen:** Analysis of % N₂ by TCD (% O₂ optional)
- ▶ **Nitric Oxide :** Analysis of ppm N₂-CO₂-N₂O by TCD

RESULTS - NITROGEN ASSAY

Chromatogram of UHP Nitrogen

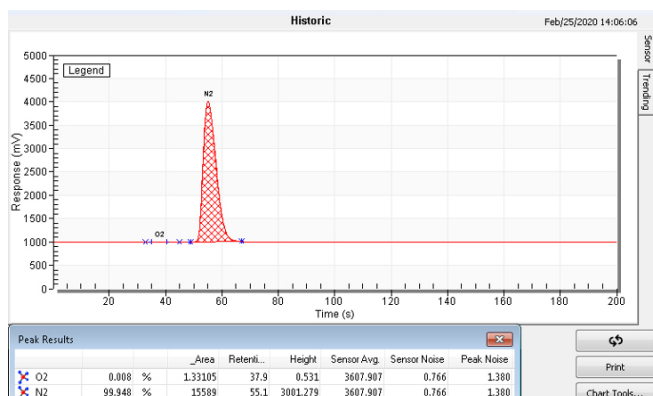

Chromatogram of a gas mixture containing 3% Oxygen & 97% Nitrogen

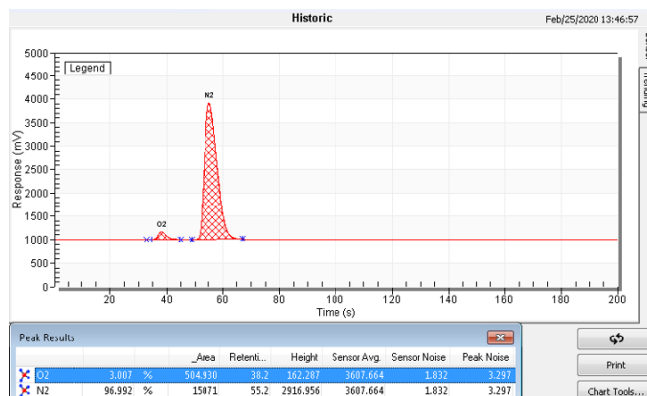

Where innovation leads to success


www.ldetek.com

10 consecutive analyses to demonstrates a quick overview of the stability


| Start | O2 | N2 |
|------------------|---------|----------|
| 2020-02-21 11:47 | 3.007 % | 97.024 % |
| 2020-02-21 11:46 | 3.009 % | 97.030 % |
| 2020-02-21 11:44 | 3.004 % | 97.038 % |
| 2020-02-21 11:42 | 3.007 % | 97.047 % |
| 2020-02-21 11:40 | 3.008 % | 97.045 % |
| 2020-02-21 11:39 | 3.002 % | 97.047 % |
| 2020-02-21 11:37 | 3.004 % | 97.031 % |
| 2020-02-21 11:35 | 3.008 % | 97.034 % |
| 2020-02-21 11:33 | 3.008 % | 97.033 % |
| 2020-02-21 11:32 | 3.007 % | 97.021 % |
| 2020-02-21 11:30 | 3.015 % | 97.000 % |

RESULTS - NITRIC OXIDE ASSAY

Chromatogram of a gas mixture
containing 3000ppm N2-CO2-N2O in a balance of Nitric Oxide

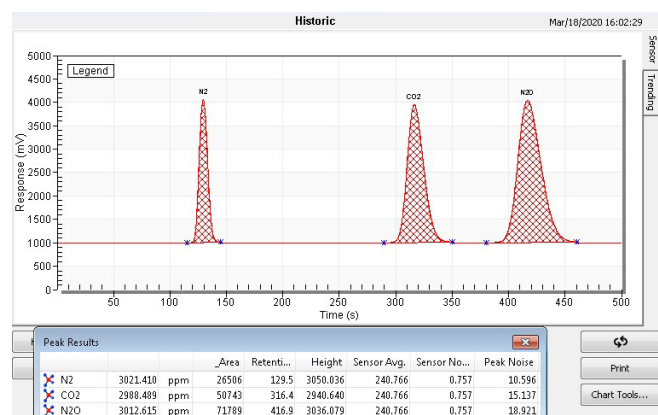

Chromatogram of a gas mixture
containing 1500ppm N2-CO2-N2O in a balance of Nitric Oxide

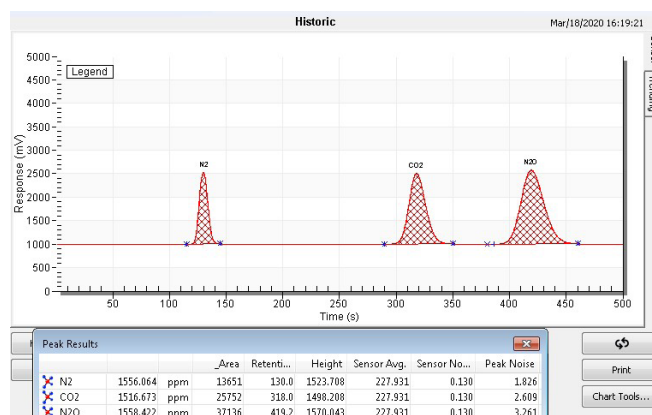

CONCLUSION:

With its combination of the TCD and the FID, the MultiDetek2 can be configured adequately for the European pharmacopeia norms. Our system is compact and offer the performances required by this medical market. The platform offers a touchscreen panel PC with date storage disk and remote-control platform.



3.0 APPLICATION NOTE

3.10 DESIGN REPORTS



3.0 APPLICATION NOTES

LD8000



TRACE NITROGEN IN ARGON OR HELIUM ANALYZER

DESIGN REPORT v2



The need of trace nitrogen in argon or helium analysis in the industry is not something new. Many instruments have been and still are on the market to achieve such measurement for different type of applications. The most popular use is without any doubt in air separation industry for the production of argon.

The demand and the production of gas more and more pure require good analytical instrumentations. It is even more the case for the measurement of nitrogen. Small leakage, dead volume, change in temperature, bad accuracy, etc can all cause big headaches.

In this document, information about the design of the LDetek LD8000 trace nitrogen in argon or helium analyzer will be described to explain how we achieve such good performance. Those results are also described to show that the LD8000 is now the solution for any applications that require such measurement.

ANALYZER COMPONENTS

PLASMA EMISSION DETECTOR (PED):

Detection principle

The LD8000 is using a Plasma Emission Detector where the principle is based on a spectroscopic emission cell. This is actually not a new technique, but the unique design of LDetek in terms of frequency, intensity as well as the mechanical and electrodes conception make the system very stable and efficient.

A luminous phenomenon, called electroluminescence, is created and is used as emission technique to quantify the nitrogen analyte. A plasma is created with the argon or helium flowing in the cell and when concentration of nitrogen changes, spectral lines emission change as well. The light is then directed in an optical filter that will discriminate the spectral lines. At the end, a photo-diode will convert light to current to make a proportional electric signal of nitrogen in the sample.

With its unique design, LDetek achieves unsurpassed performance that provides now a reference trace nitrogen in argon or helium analyzer.

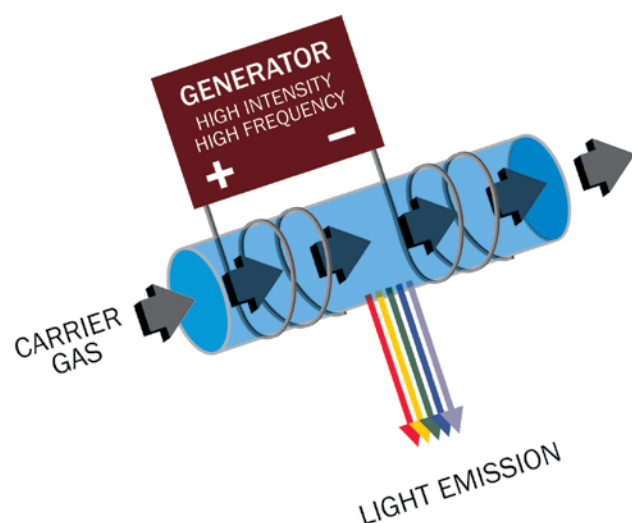


Figure 1: Plasma detector principle

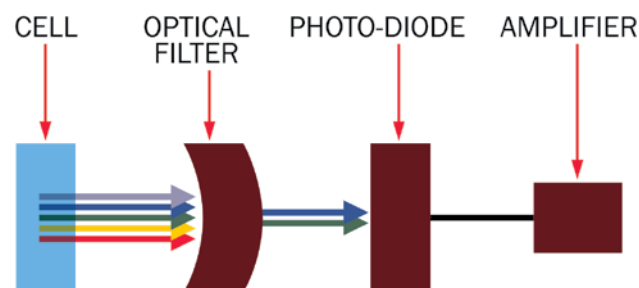


Figure 2: Light to current transformation

Plasma Cell

The cell of the PED is generally made of quartz. The material used has strong UV transmission properties. It is also durable, inert and heat resistant.

LDetek plasma detector has a specific cell design that provides a stable plasma. This unique conception will help getting low noise and good sensitivity when nitrogen is flowing in the detector along with the argon or helium. The wall cell design made of quartz combined with specific electrodes shape and inlet/outlet flow path configuration are some of the key parameters that give the performance of a PED.

Plasma Generator

The plasma generator is also quite important. Its specific voltage, frequency and current make the glow discharge in the cell very stable. The combination of the cell design and generator is critical in such application. LDetek has developed a perfect combination to get a stable light emission from the plasma. The components of the generator are well proven to be efficient and resistant over the years.

The generator is also based on a duty cycle controlled system that extends lifetime of the cell. The cell is put ON and OFF on a specific frequency and period to help the system to give the performance desired as well as decreasing the degradation of the detector.

Optical Filter and photo-diode

Optical filter is made specifically for LDetek specifications with properties to avoid interferences, temperature drift, loss of sensitivity and wavelength shifting over time. The wavelength, size, transmission lines and material are all critical characteristics that need special care to obtain such good performances.

The photo-diode will then convert the light out of the filter to current that is proportional of the amount of nitrogen in the sample. An electronic circuit designed by LDetek is then used for precision treatment of analog signal coming out of the photodiode.

Even if it sounds straightforward, LDetek has a unique way to install and align all items together. LDetek established rigorous procedures in a way to achieve high and same performances for each unit.



Figure 3: Plasma Detector module in the LD8000

FLOW CONTROL:

Flow management in such analyzer is critical in terms of dead volume and leakage. It is important to have a flow control device that will not introduce air and dead legs in the system. The LD8000 has an operating range as low as 0-1 ppm with a few ppb as detection limit. Conventional Mass Flow Controllers (MFC) is not suitable for such analysis. Since air is made of 78% of nitrogen, the chance to have some nitrogen introduced in the system with MFC is too high.

LDetek has designed its own flow control system to avoid air infiltration by the flow control device. The instrument can work with a flow as low as 25 cc/min and have a quick response time without apparition of dead volume.

Micro-Valve

LDetek have worked to develop a valve that meets the performances requirement. This miniature valve has a very small orifice size and offers ultra low flow rate. Since the LD8000 can work on relatively low flow, this valve design does not introduce delay or drifting problems.

Standard valves (figure 5) introduce "spikes" in the reading caused by dead volume located inside the valve. Measuring in so low concentration can be a big problem when having nitrogen released after calibration or upset condition in the sample.

With the LDetek micro-valve performance (figure 6), this problem is avoided and stable reading is obtained after any changes of concentration.

The inlet pressure can range from low as 4 PSIG to 30 PSIG without reading fluctuation. With an optional pump offered by LDetek, the instrument could work in even lower pressure.

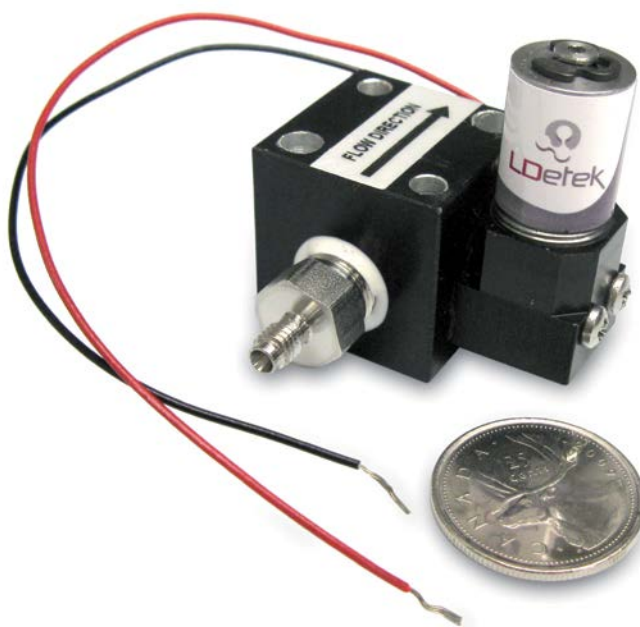


Figure 4: Micro-Valve for sample control

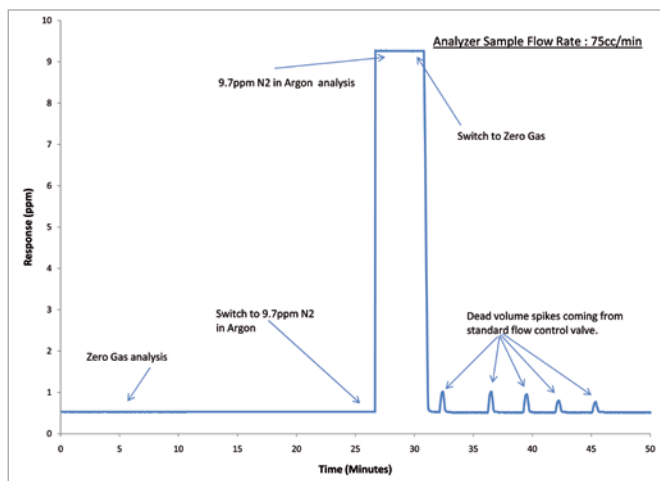


Figure 5: Standard valve performance

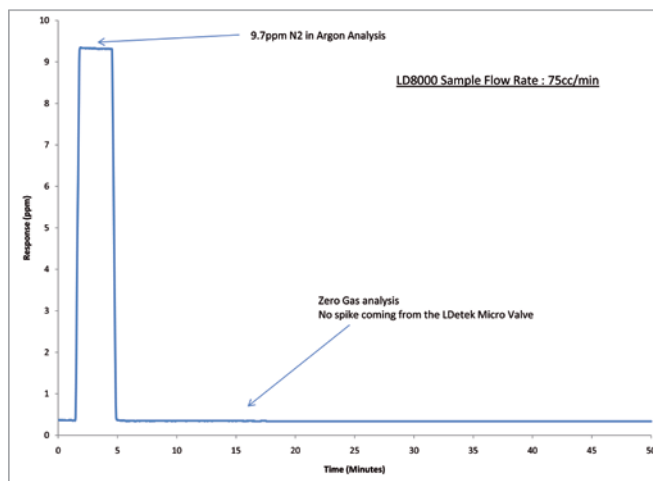


Figure 6: LDetek valve performance

Flow Transducer

The flow transducer is the biggest source of contamination for such analyzer. To avoid any problem with such device, the transducer is installed at the end of the flow path after the detector and is connected to the microcontroller unit to give information to the micro-valve to control a stable flow.

So why not using a MFC after the detector? That would avoid any chance of contamination or leakage? Actually, the PED must work at atmospheric pressure and it must not be pressurized. Since the PED is a cell made of quartz, it can break with a backpressure coming from the vent. Furthermore, you want to keep a constant pressure in the detector to get a stable plasma.

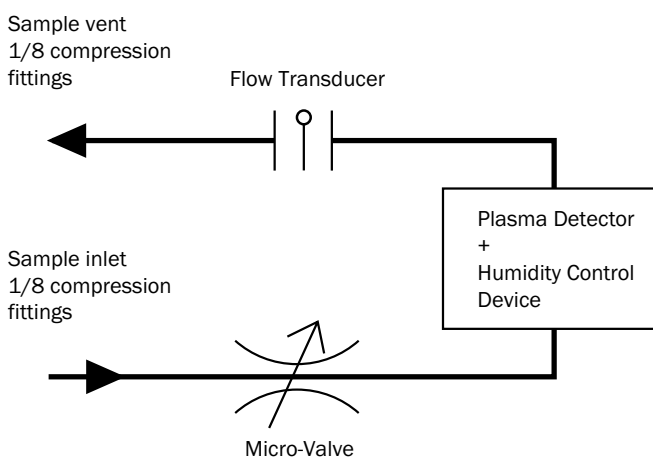


Figure 7: Flow path of the LD8000

NO NEED OF ZERO CALIBRATION GAS:

An option is available that avoids the need of a pure reference gas to make the zero calibration. The LD8000 can be designed in a way that components are added inside the analyzer to generate zero gas.

Only the sample gas is connected to the instrument and zero calibration can be achieved. A valve's system is used to change the flow path to the detector. During zero calibration, the sample goes to a small gas purifier to get pure argon or helium.

There is no consumable in such configuration. Since the integrated gas purifier is used only during zero calibration and the valve system isolates it, the lifetime of the purifier is extended. Such system will save the needs of pure argon supply, gas regulator, piping, external purifier, bypass valve for the purifier, etc. The payback is quite evident!

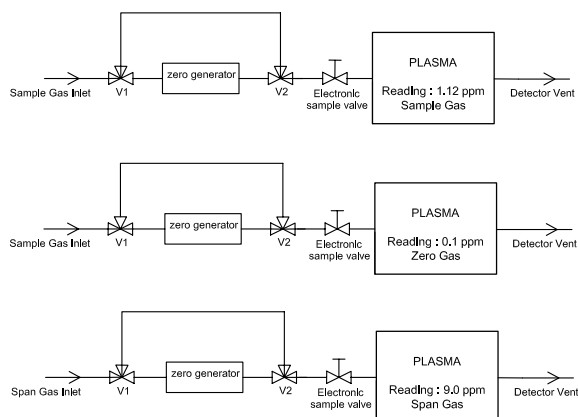


Figure 8: LD8000 with integrated zero calibrator

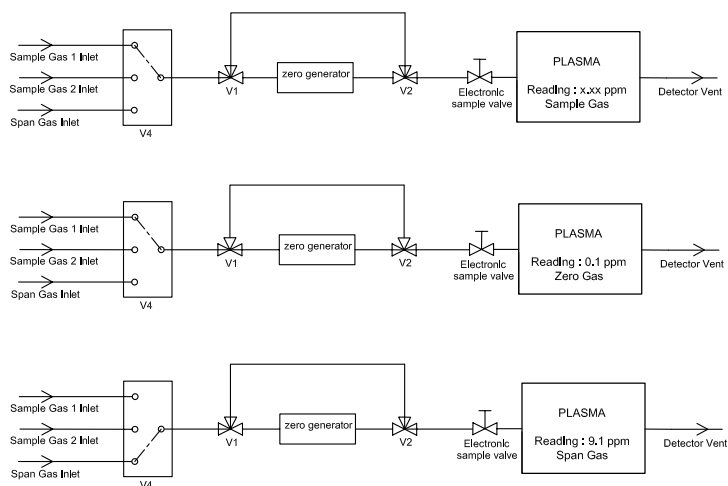


Figure 9: LD8000 with integrated zero calibrator & stream selector

HUMIDITY CONTROL DEVICE (HCD):

Moisture is the worst « enemy » of nitrogen in the plasma. First of all, its emission wavelength is closed to nitrogen and some interference can occur. Furthermore, the level of energy available in the plasma is more consumed by H₂O than N₂. That reduces the light intensity of nitrogen ending by a loss of sensitivity.

In each LD8000, a Humidity Control Device is included in the detector module. This device introduces a constant amount of H₂O and other chemical vapors compounds in the detector to stabilize the influence of the moisture on the measurement of N₂. With the combination of the moisture trap installed outside of the cabinet on the sample line, the analyzer becomes stable at any variation of humidity in the sample.

MAINTENANCE ? :

No maintenance is required in the analyzer. The detector is a non-depleting type device as well as the other components inside the cabinet. Same for the flow control system, however if a defective part needs to be changed, no need to change a complete and expensive flow module or MFC (Mass Flow Controller). You can replace only the micro-valve or transducer.

The unit has been designed in a way to make life easier if parts need to be changed. No need to send back the instrument to factory. Any kind of parts, including the detector module, can be replaced on site by a technician.

The moisture trap installed outside the analyzer should be replaced or regenerated every year to get the best performance in stability and accuracy of the LD8000.

ANALYZER PERFORMANCE

The design of the LD8000 brings outstanding performances for the market demand. Even if this analyzer is used for ppm measurement, we get stability, accuracy and noise level for ppb analysis. With the design described above, some tests have been done to show the performances in different situations. Those performances have been tested with argon sample, since it is the most popular application on the market.

RESPONSE TIME:

The LD8000 has a fast response time to ensure a good purity control in the different applications of such analysis. However, such good result is always dependant of the installation along with the instrument. The stream selector system is critical to be able to achieve such good response time. We strongly suggest to use the LDGSS from LDetek which has been designed specifically for such application.

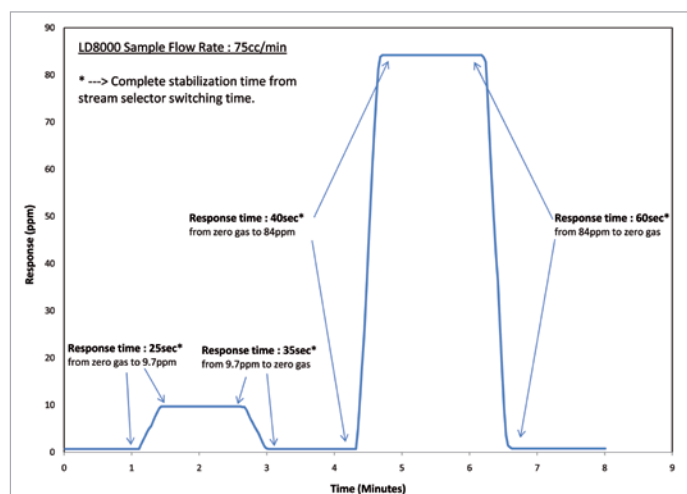


Figure 10:
*LD8000 Reponse time

NOISE:

The electronic for the acquisition of the detector has been designed to avoid any noise that could influence the reading of the analyzer. But more importantly, the design of the detector itself is very important to minimize the noise as much as possible. The position of the optical filter along with the photo-diode is critical to get the specification of the LD8000. Bad response of those components means electrical gain increase to achieve the measurement desired and at the same time the noise level will be amplified. When mounting the detector, special care is done by LDetek specialist.

The amplifier board used to manage the signal from the photo-diode was also particularly well designed. This board takes very low voltage to amplify it on a scale up to 0-10 volts.

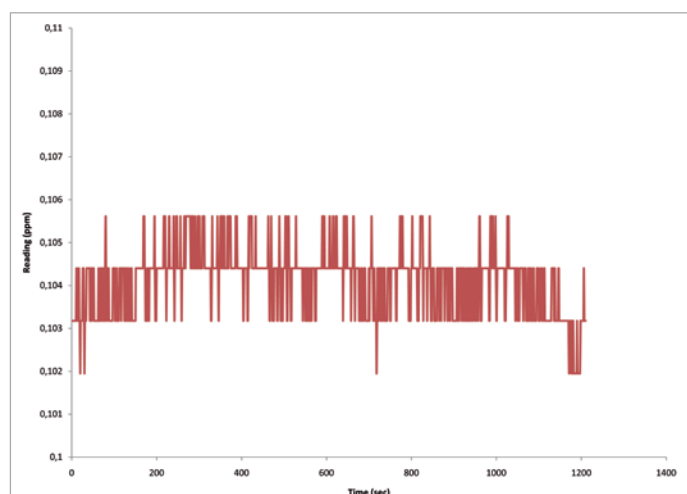


Figure 11:
*Noise level acquired on the analog output
with a sample gas of about 0.104 ppm

*Note: This result has been obtained in LDetek facilities with the LDGSS stream selector device with a well purged system according to LDetek standard methods.

STABILITY:

Stability of the analyzer has been evaluated through a few hours period. Temperature variation has been caused to show the stability of the reading even with an unstable temperature environment. Those variations have been done on the analyzer itself and not on the whole system installation which can be different from site to site.

With a deviation of 4.4 Celsius (31.6 to 36 degrees) on a 36 hours period, the reading has moved down from 300 ppb to 280 ppb. This slight variation gives a 4.5 ppb / Celsius change. Considering that most of the installations are temperature controlled, no temperature effect will be observed. Moreover, the resolution of the analyzer is 10 ppb and slight temperature variation will not be seen by the software reading.

Stability has been evaluated on a 24 hours basis with stable environment (figure 13). The drift observed is less than 2 ppb.

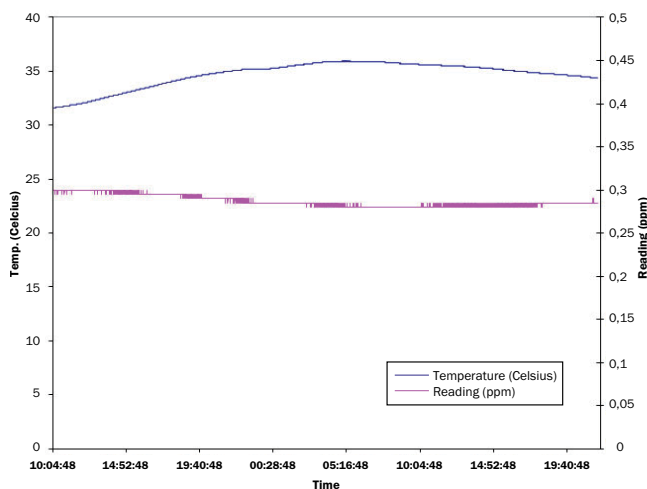


Figure 12: *Signal versus temperature

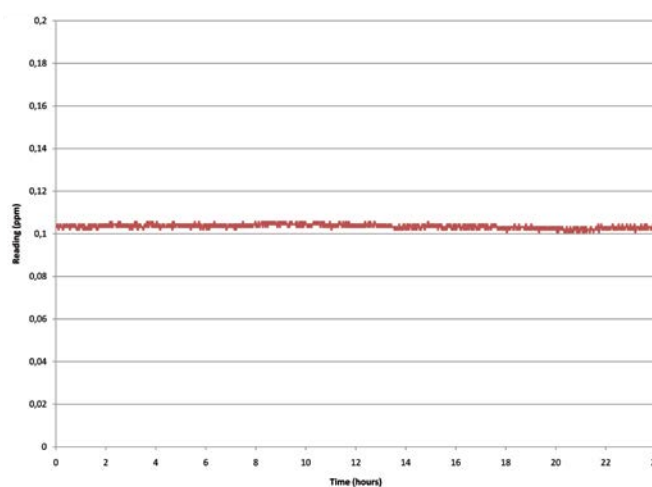


Figure 13: *24 hours stability on stable environment

LINEARITY AND ACCURACY:

Special care has been made on the linearity of the system. Knowing that existing instruments on the market do not offer linearity on the complete range of 0-100 ppm, LDetek has improved its detection system to be sure that working and calibrating the instrument on the range 0-100 ppm will offer the best performance.

On figures 14, calibration of the instrument has been done with a zero gas going through the LDP1000 gas purifier and the same dilution system for the different concentrations measured.

We have also made step changes in low concentration to show the accuracy of the instrument. Figure 15 demonstrates that a 10 ppb step change is easily detectable by the LD8000. Measuring pure gas on the range 0-1 ppm is more and more popular and such performance is appreciated from gas producers.

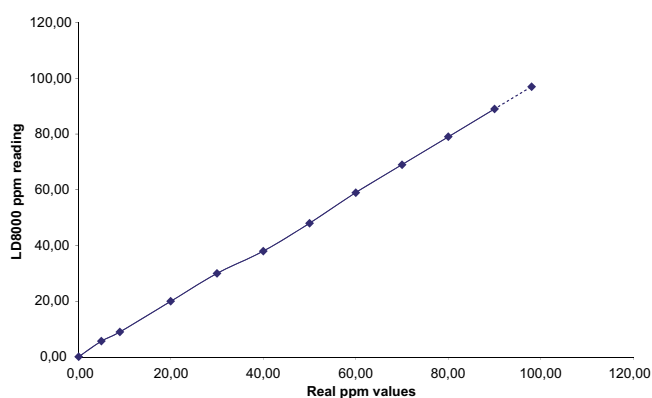


Figure 14: *LD8000 linearity on 0-100 ppm range

*Note: This result has been obtained in LDetek facilities with the LDGSS stream selector device with a well purged system according to LDetek standard methods.

DETECTION LIMIT:

Referring to the noise of the LD8000 from figure 11, we get maximum 3.6 ppb peak to peak. Using the standard deviation method, we have used 15 consecutive points where we get the maximum peak to peak noise. Five times the standard deviation gives a LDL of 4.4 ppb.

This kind of instrument is mostly used for concentration higher than 100 ppb. The LDL is low enough for all Air Separation Unit or glove box application.

If LDL lower than that is required, LDetek is manufacturing the LD8000-Plus, which is the ppb version of the trace Nitrogen analyzer. We can detect lower than 1 ppb with signal to noise ratio very low. Please contact factory.

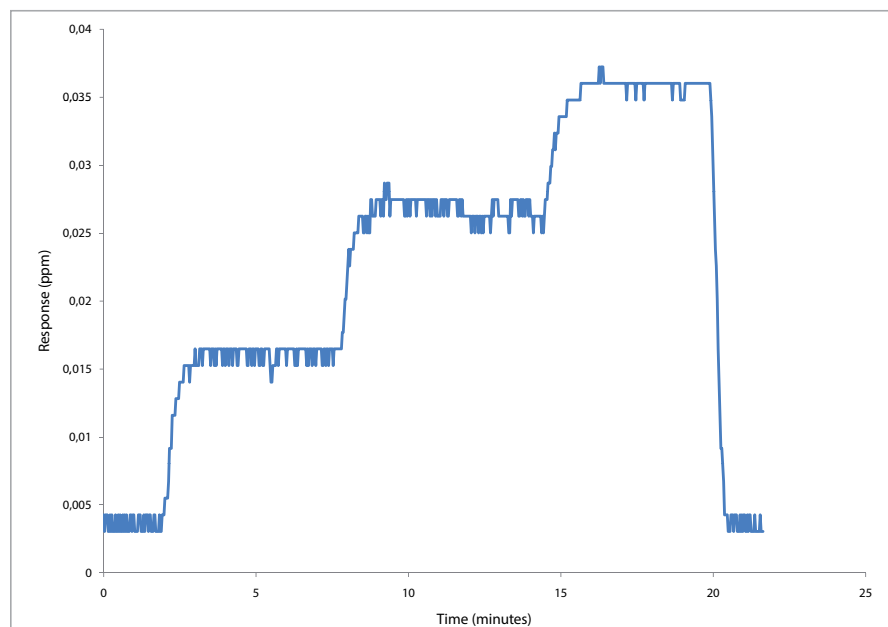


Figure 15:
*10 ppb concentration step changes

*Note: This result has been obtained in LDetek facilities with the LDGSS stream selector device with a well purged system according to LDetek standard methods.

CONCLUSION:

LDetek has put a lot of effort and time to introduce on the market a trace nitrogen in argon or helium analyzer with outstanding performances. We are proud to offer a reliable instrument that has been carefully designed with specialists having over ten years experience in trace nitrogen measurement and plasma emission detector.

For more information, comments or questions, don't hesitate to contact LDetek (info@ldetek.com).

APPLICATION NOTE

LD12-05



IMPROVING GAS CHROMATOGRAPH MEASUREMENTS WITH THE USE OF THE LDP1000 GAS PURIFIER

When measuring low level of impurity by gas chromatography, the carrier gas quality is quite important. Since the carrier gas is the reference gas for the device, good precaution to provide pure carrier is required. Using a grade 5 (99.999% pure) or grade 6 (99.9999%) is not enough in some cases. Even more, it is well known that many problems can simply come from the use of a bad quality gas cylinder or leakage on pressure regulator after cylinders manipulation. By using the LDP1000, it gives the certitude it catches all impurities coming from the carrier gas lines although you have sources of contamination.

The LDP1000 purifies noble gases, nitrogen or hydrogen at level that give the best reference for any gas chromatograph and GC/MS. It's non-evaporable zirconium-based getter alloy is contained in a 316L Stainless Steel bloc to ensure high purity and safe operating mode. It removes impurities down to ppt level (total impurities).

LDP1000 DESIGN:


The LDP1000 gas purifier is designed to be used with any noble gases, nitrogen or hydrogen. Its changeable getter gives the possibility to avoid changing the whole unit but only the consumable parts inside. That is a cost effective solution for long term use.

Having an accurate temperature control for such purifier is critical. The LDP1000 is based on a microcontroller unit that regulates the temperature of the getter to ensure stability on the purity and maximum purification. An over temperature protection is also in place to ensure safety of the unit.

Its mechanical design allows to use it on a table in a laboratory as well as in the industry with its holding plates. The bypass plate option gives also the necessary installation for maintenance purpose to avoid contamination and flow shutdown to the gas chromatograph.

AMBIENT VS HEATED PURIFIERS:

Since the entirety of the alloy volume is used, the heated LDP1000 adds to the purifier capacities and life time in comparison to any conventional ambient purifiers and/or traps. Heating the alloy makes the impurity molecules diffuse into the bulk of the getter particles instead of only relying on surface absorption like ambient purifiers. Moreover, the LDP1000 technology has the capacity to remove nitrogen, hydrogen and methane in noble gases.

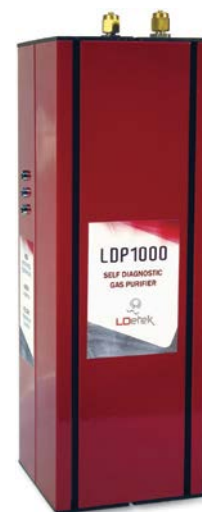

LDP1000
gas purifier

CONTAMINATION INFLUENCE:

It is well known that a contaminated carrier gas in a gas chromatograph has a big impact on the stability, sensitivity and performances of the system. Picture 1 shows the impact on the nitrogen reading while having a contaminated carrier gas.

Having a carrier gas contaminated, but less than the sample gas to measure, we lose sensitivity by the amount of the contamination. From the picture 1, we clearly see that we lose about 50% response with a sample/contamination ratio of 2. That affects significantly the detection limit of the system.


It is even worse when the contamination is higher than the sample to measure. Since the sample is more pure than the carrier gas, you get a negative peak for the impurity. The measurement is completely erroneous and cannot be used.

The LDP1000 ensures that the carrier gas of the system is at its best purity you can get. This way, the gas chromatograph can have the best performances for all its measurements.


Referring to picture 2, the impact of bad carrier quality on a gas chromatograph system is clearly demonstrated. The chromatograms used to do the demonstration are the same that the ones used in picture 1 which are contaminated with different level of air.

The noise level increases with the level of air contamination. That makes the signal/noise ratio lower. That has also a direct impact on the performances of the system by degrading the columns stability and separation. It can even lead to capillary column destruction.

Having the LDP1000 installed on gas chromatograph keeps the system stable and extends the lifetime of the whole system hardware by removing any trace of particles and air contaminants.

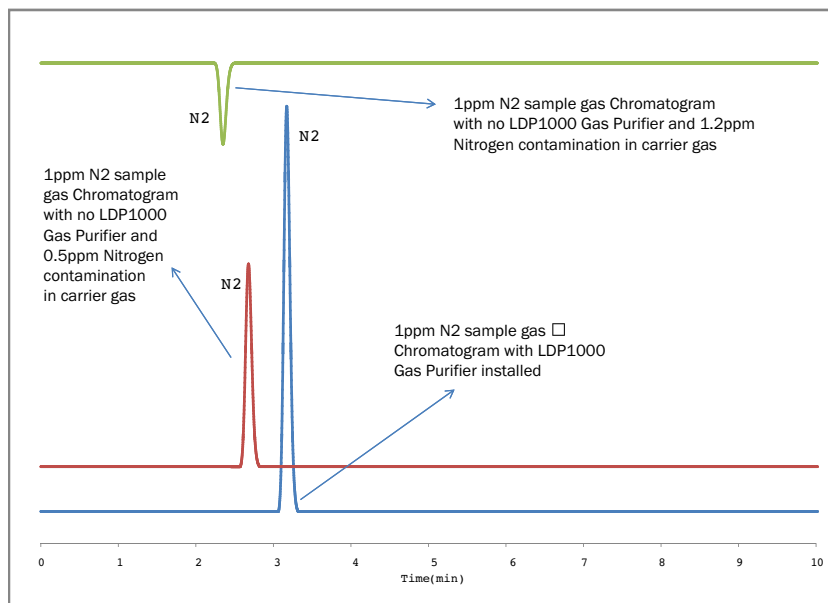

Picture 1: N₂ contamination influence

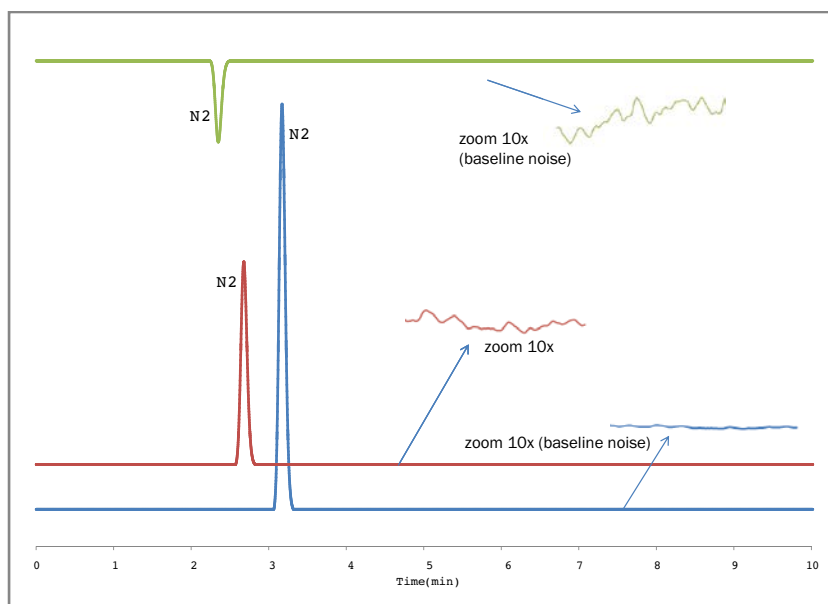


Picture 2: Contamination influence on noise level

TWO BEDS OF PURIFICATION:

To ensure high purity, the LDP1000 noble gas version has two beds of purification. The first stage has an elevated temperature grabbing all components except some low level hydrogen. At this temperature, some H₂ can be released from this bed. The amount of H₂ can be as high as a few hundreds ppb with the use of one stage of purification only.

By having a second bed of purification operating at a different temperature, the hydrogen out of the first stage can then be totally trapped.

Both bed temperatures are controlled by a microprocessor ensuring stability and efficiency of the purifier.

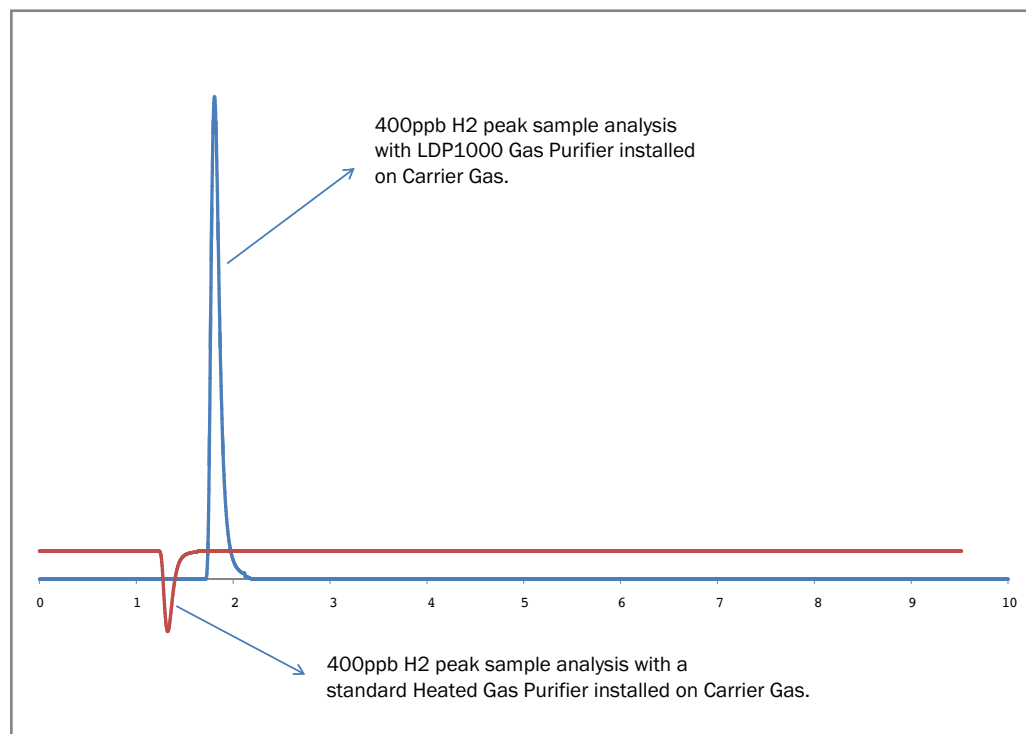

Picture 3: Hydrogen influence on measurement with different purifiers

Having H₂ released from the first bed could influence your H₂ measurement considerably. Such phenomenon is known in the gas chromatography industry when measurement of low level hydrogen is necessary. A part of the hydrogen comes from the cracking of methane and non-methane hydrocarbons. The cracked by-products are then sorbed by the getter. However, the sorption capacity for H₂ isn't high enough caused by high temperature which makes some low level hydrogen come out of the getter.

Picture 3 shows the effect of H₂ presence coming out of a purifier in the carrier gas when only one stage of purification is used. Then, if the sample gas is more pure than the carrier gas, you will reduce sensitivity and even get negative reading for hydrogen in some cases, as illustrated on picture 3. With its two beds of purification, the LDP1000 removes completely the presence of H₂ in the carrier which is ideal for low measurement.

LEDS INDICATION & RS232 COMMUNICATION:

The LDP1000 has intelligent features to be able to monitor some information:



- **Green LED**

Indicates that the LDP1000 is powered ON

- **Yellow LED**

Indicates if one of the beds has a temperature deviation

- **Red LED**

Indicates that the lifetime of the purifier has expired.
Getter needs to be replaced.

Picture of the LDP1000 LED

Those indications are very useful to know that your system is fully working or the purifier is not the cause of any performance issue you can have with your gas chromatograph. The diagnostic and control of those LED's is fully managed by the microcontroller and the different sensors in place.

A RS-232 serial port is also installed by default on the LDP1000. This feature gives the possibility to monitor the temperature of the 2 beds of purification. This is very useful for troubleshooting the device.

CONCLUSION:

With the LDP1000, the carrier gas quality becomes indisputable. With its specific mechanical and electrical design, the gas purity level has never been so good and stable. It is a must for the gas chromatography and GC/MS industry. Moreover, with its changeable getter, this may be the last gas purifier you will ever buy. The LDP1000 is the cost effective solution you need.

LD2000



TRACE TOTAL HYDROCARBONS ANALYZER

DESIGN REPORT




Measuring total hydrocarbons is required in the air separation industry for quality control of the gas produced. The series LD2000 is an online analyzer using a flame ionization detector especially designed for this application. This document will demonstrate the performances of the unit.

ANALYZER COMPONENTS

FLAME IONIZATION DETECTOR (FID)

DETECTION PRINCIPLE

It is well known that due to its relatively good sensitivity to most organic compounds, the FID is a good detector for measuring the level of THC in different sample gases. The principle is based on the creation of carbon atoms (ions) formed during the combustion of the organic compounds burned by a hydrogen flame.

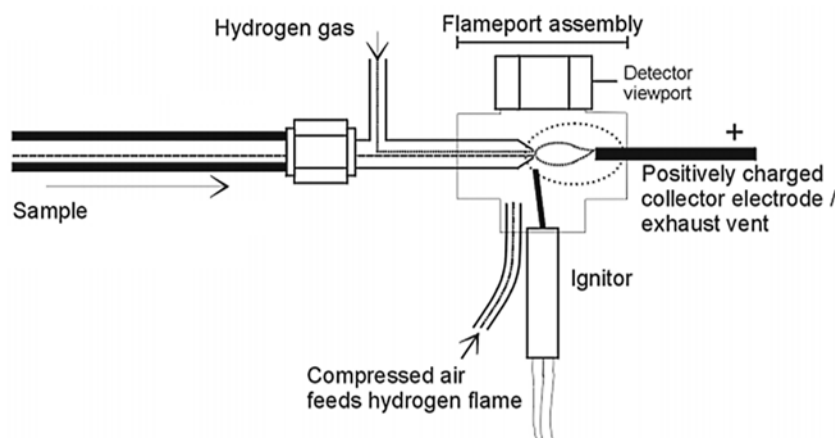

AMPLIFIER

The signal on the collector is amplified with our multi-stage amplifier which has been designed to satisfy the different ranges required. Different sample rates are adjustable to optimize the sensitivity of the signal.

FLOW CONTROL

The sample flow is controlled with the LDetek electronic proportional valve to ensure stability. Concerning air and fuel, the flow control is adjusted with a stainless-steel mini pressure regulator. A safety shutoff valve is installed on the hydrogen gas line to close the fuel when the flame goes off.

FEATURES

The unit offers all the industrial communication protocols with alarms for data/results collection.

MAINTENANCE

It is recommended to replace the hydrocarbon traps for air/fuel once a year to ensure integrity of the flame by avoiding any trace of hydrocarbons coming from the feeding gases. Depending on the carbon level, the FID collector and ignitor are to be replaced every 2 to 3 years to avoid any lack of sensitivity.

ANALYSER PERFORMANCES

RESPONSE TIME

The response time of the unit is demonstrated on the figure 1. Upfront and down front time is of 60-90 seconds depending on the concentration and also the sampling system design. Such response time satisfies the requirements.

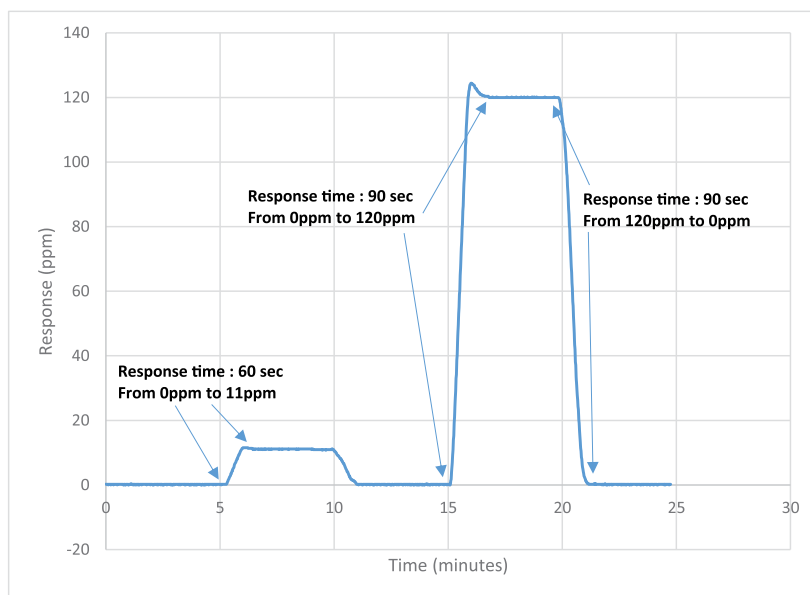


Figure 1

LINEARITY/ACCURACY/REPEATABILITY

The linearity curve of the analyser (figure 2) is 0.99 and has been performed using 13 points diluted at different concentrations between 0-560ppm. The same span bottle has been used for the dilution and the calibration to avoid concentration shifting due to different bottle certifications.

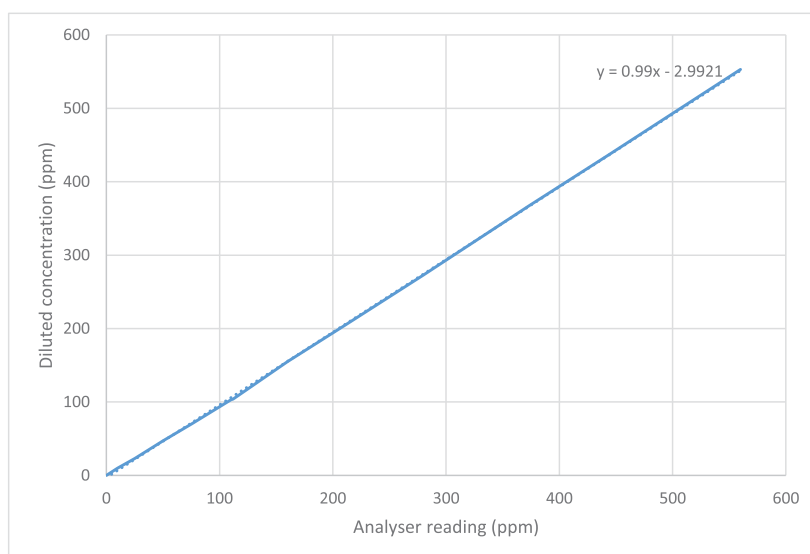


Figure 2

The accuracy error is +/-1% of full scale. The figure 3 shows the % error for 13 points diluted at different concentrations between 0-560ppm and measured on a 1000ppm scale.

The repeatability error is +/-1% of full scale in a stable environment.

| Diluted concentrations *(ppm) | Analyser reading (ppm) | Accuracy (% of scale) |
|-------------------------------|------------------------|-----------------------|
| 0 | 0 | 0 |
| 10 | 10 | 0 |
| 25 | 23 | 0.2 |
| 50 | 47 | 0.3 |
| 75 | 70 | 0.5 |
| 110 | 103 | 0.7 |
| 112 | 104 | 0.8 |
| 160 | 155 | 0.5 |
| 210 | 204 | 0.6 |
| 280 | 273 | 0.7 |
| 373 | 367 | 0.6 |
| 444 | 437 | 0.7 |
| 560 | 553 | 0.7 |

Figure 3

*The dilution system and the certified bottle combined together may give an additional source of error of +/- 1% depending on the conditions.

DETECTION LIMIT (LDL) AND NOISE

Referring to the figure 4, the peak to peak noise level is 50ppb based on the 40 minutes period. A factor of 2 times the noise level is applied to give an LDL of 100ppb.

To demonstrate the response limit, some concentration step changes of 200-250ppb have been done. The figure 4 well shows the performances of the unit on its 10ppm range.

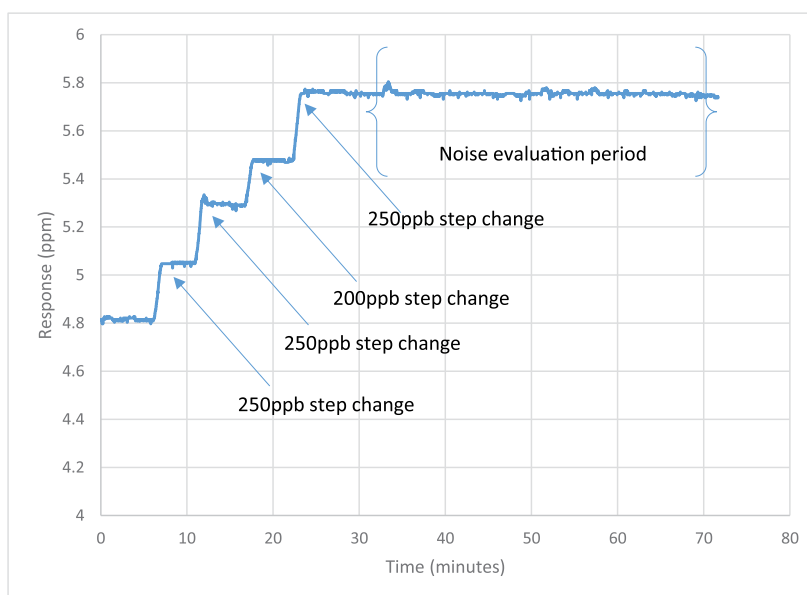


Figure 4

STABILITY/DRIFT

Running on a 4 days period at a concentration of 22ppm on a scale of 100ppm in a stable environment, the instrument reading delta shows 1.9ppm which is in the specification of +/-2% of full scale for a one-week period in stable conditions.

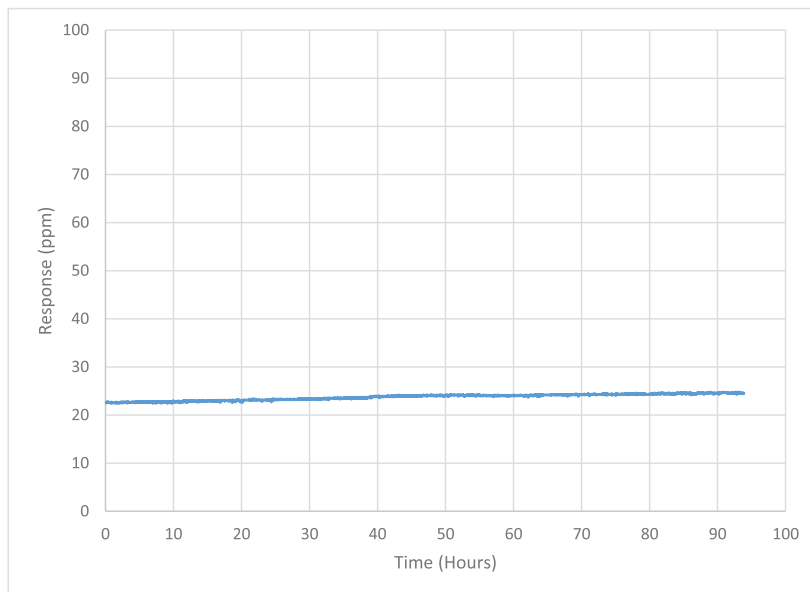


Figure 5

MULTIDETEK2 GC



WITH INTEGRATED MODULE FOR TRACE MOISTURE ANALYSIS

DESIGN REPORT



The Advanced Quartz Crystal Microbalance sensor from Michell Instruments is now integrated inside the MultiDetek2 GC to provide reliable, fast and accurate measurement of trace moisture content in a variety of applications where keeping moisture to a minimum is of critical importance.

The analyzer provides consistently accurate measurements of trace moisture. This consistency is achieved using a self-calibration system, which adjusts the sensor with reference to an internal moisture generator. The moisture generator is supplied with a calibration traceable to NPL and NIST, so long term stability of its measurements is guaranteed.

Having such module inside a GC allows to combine multiple impurities analysis with trace moisture inside the same instrument.

DETECTION PRINCIPLE

Sensor: Quartz crystal microbalance

A quartz crystal is sensitised with a thin film of hygroscopic material.

- ▶ Water molecules are adsorbed into the hygroscopic layer deposited on the surface.
- ▶ The change in mass modifies, in a very precise and repeatable manner, the oscillation frequency.
- ▶ The moisture concentration is measured as a change in the oscillation.
- ▶ The change in the oscillation is evaluated by switching the gas inside the sensor and by measuring the response delta. For sampling response, the sensor is balanced between a dry gas source and the sample source. The difference is then calculated. The same principle is applied for the span gas calibration. However, this time the comparison is between a dry gas and a source of wet gas. A cycling time of 30 seconds on each gas is used to compare the response delta.

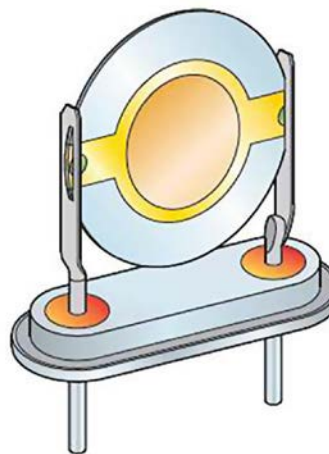
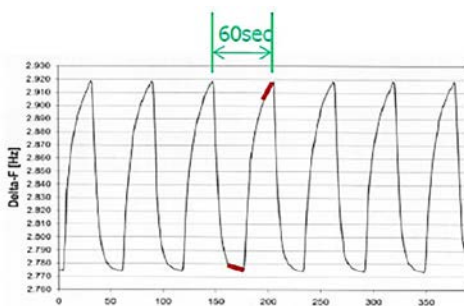


Figure 1:
Quartz crystal sensor

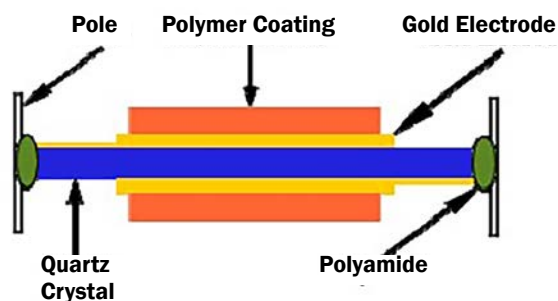


Figure 2: Quartz crystal principle

$$\text{Measurement } \Delta f = \text{primary } \Delta f_{\text{sample}} - \text{primary } \Delta f_{\text{dry}}$$

- 30/30 sec measurement cycle
- Non-equilibrium for fast response
- Self-cancelling effect for contamination

- ▶ The dry gas comes from the carrier gas source of the GC. The sensor is supplied by a known Helium or Argon or Nitrogen grade 5.0 carrier source going through a heated gas purifier model LDP1000 series. This combination generates a gas purity of 8N. By using this technique, the dry gas source contains less than 10ppb H₂O what is ideal as zero gas reference.
- ▶ The wet gas comes from a certified water filled permeation tube heated at a controlled temperature of 45 Celsius. It generates


a stable amount of moisture used for span calibration. The moisture generator is made of coated stainless steel to reduce the surface absorption of water molecules and then keep the moisture rate very stable and accurate.

- ▶ The flow inside the module is controlled and maintained by a network of calibrated orifices. All flow passageways upfront the sensor are less than 0.030"ID, all coated with an inert coating to accelerate the response/purge time and improve the performances of the system.

FLOW DIAGRAM


Sampling position:

The V4 diaphragm valve switch between sample gas and dry gas every 30 seconds. The response delta between the dry gas and the sample gas is then measured at the quartz crystal module (QCM). The flow rate inside the sensor is stabilized at 100sccm by the flow orifice R11 mounted at the outlet of the sensor. Two balanced flow orifices R8-R10 keep an equal flow rate of 100sccm to be sure the system stays in equilibrium even with valve switching. This technique ensures the system stabilizes very quickly. This sampling position is the normal running mode and a refreshed reading is proceeding every 60 seconds.

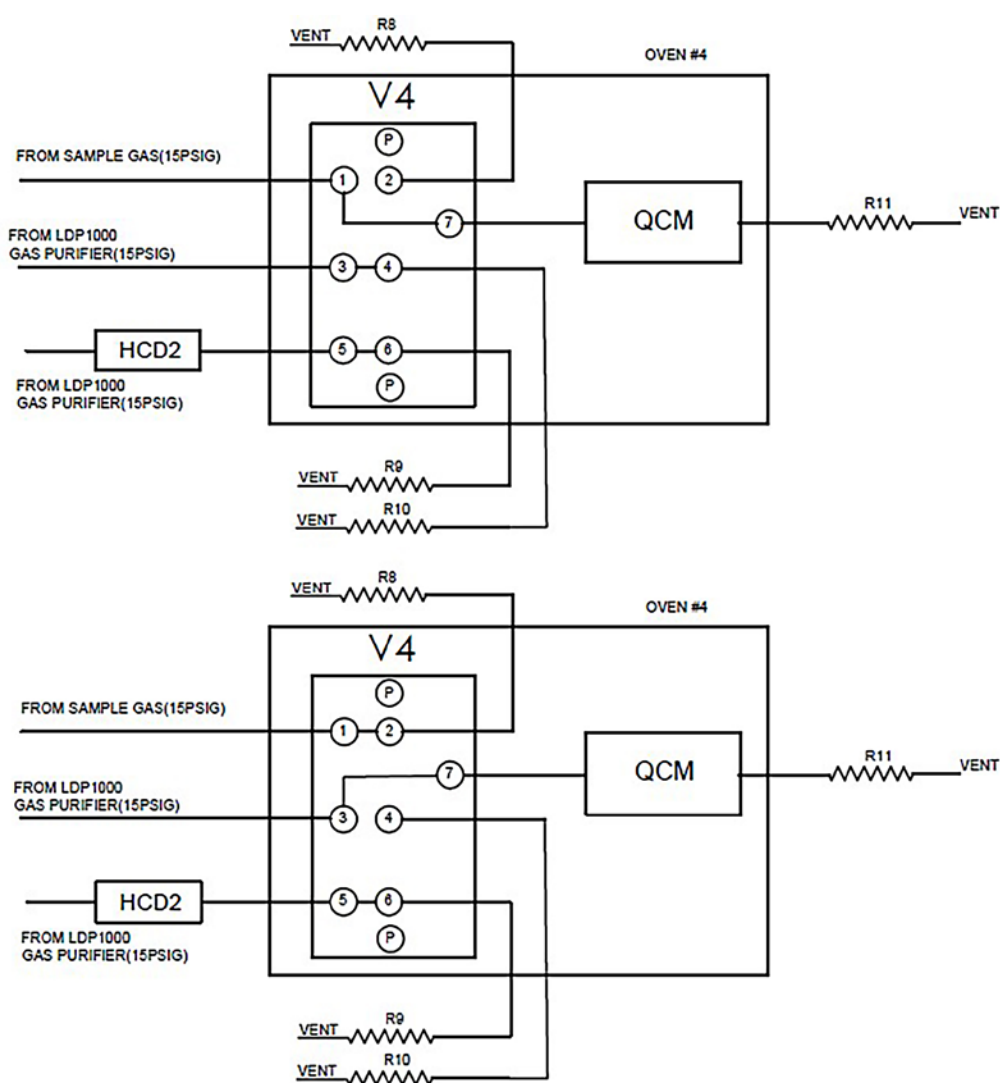


Span calibration position:

The V4 diaphragm valve switch between the dry gas and the wet gas every 30 seconds. This position is used for span calibration purpose. The span calibration frequency depends of the requirements but is generally required every 2 weeks for check spot. During this process, the V4 valve switches every 30 seconds to compare the response delta between the wet gas to the dry gas. Again, the flow is balanced with R9-R10 flow orifices. The humidity control device (HCD2) is continuously kept under a fix flow rate at a stable temperature of 45 Celsius in an inert coated controlled environment. The permeation device generates a certified and known moisture ppb rate. The concentration generated depends on the application, but is generally 500ppb. Having the calibration performed at the bottom of the scale increase the accuracy of the system in the most critical reading region.

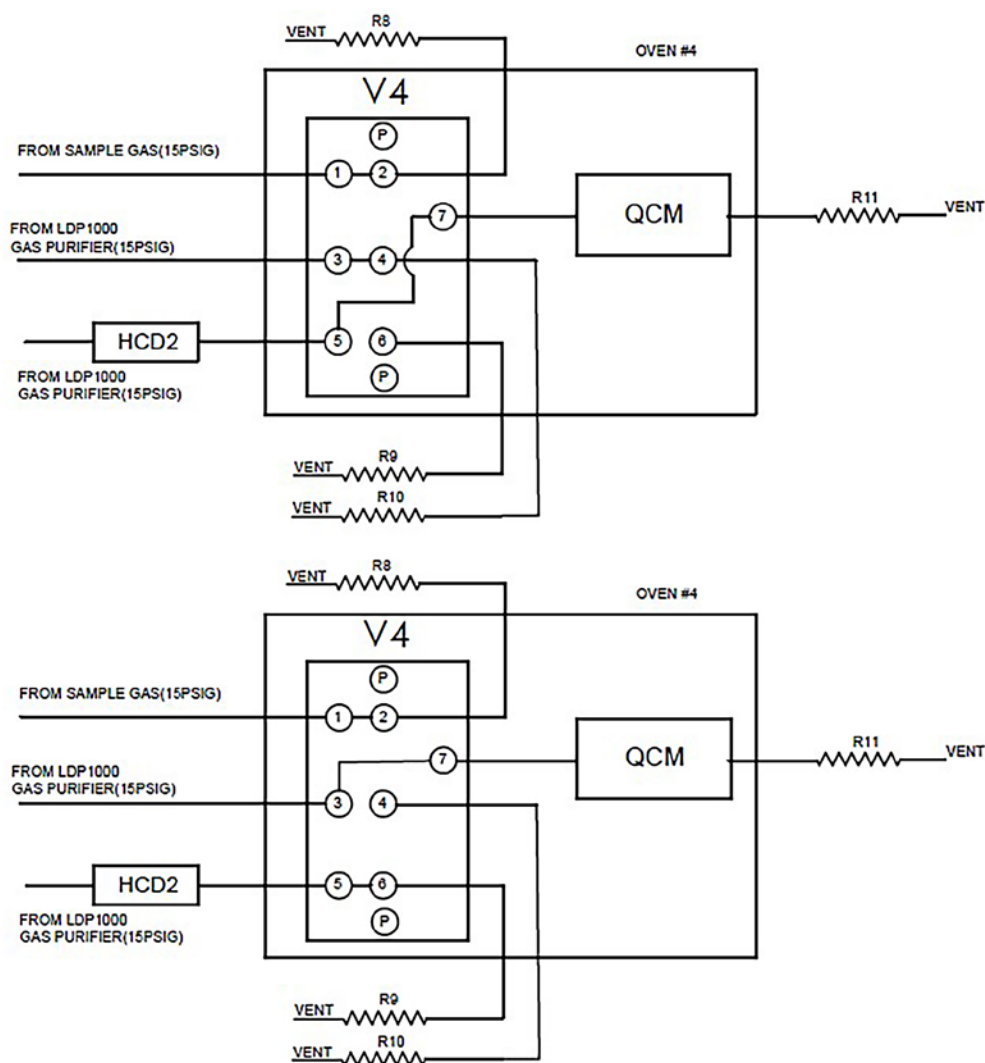

MODULE ASSEMBLY

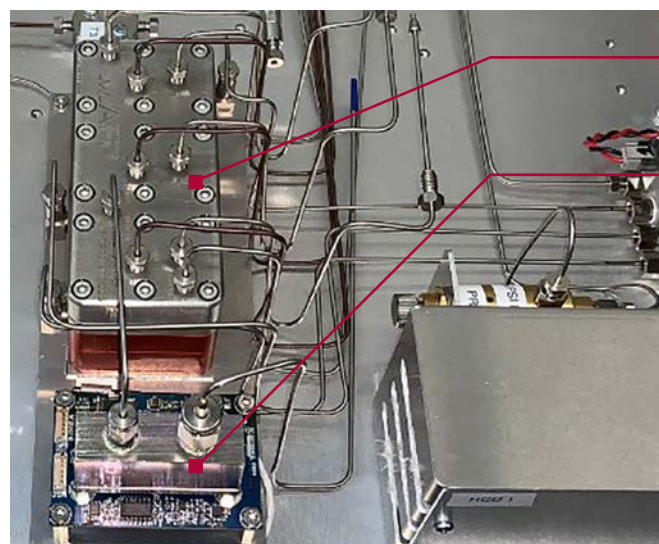


3 streams, inert coated stainless-steel diaphragm valve with sample bypass and purge

Trace moisture sensor (quartz crystal microbalance)

*All flow passageways to the sensor are made of stainless steel inert coated with an ID of 0.030"

Moisture generator (certified permeation tube) maintained at a fixed temperature

Solenoid valve and manifold to actuate the diaphragm valve

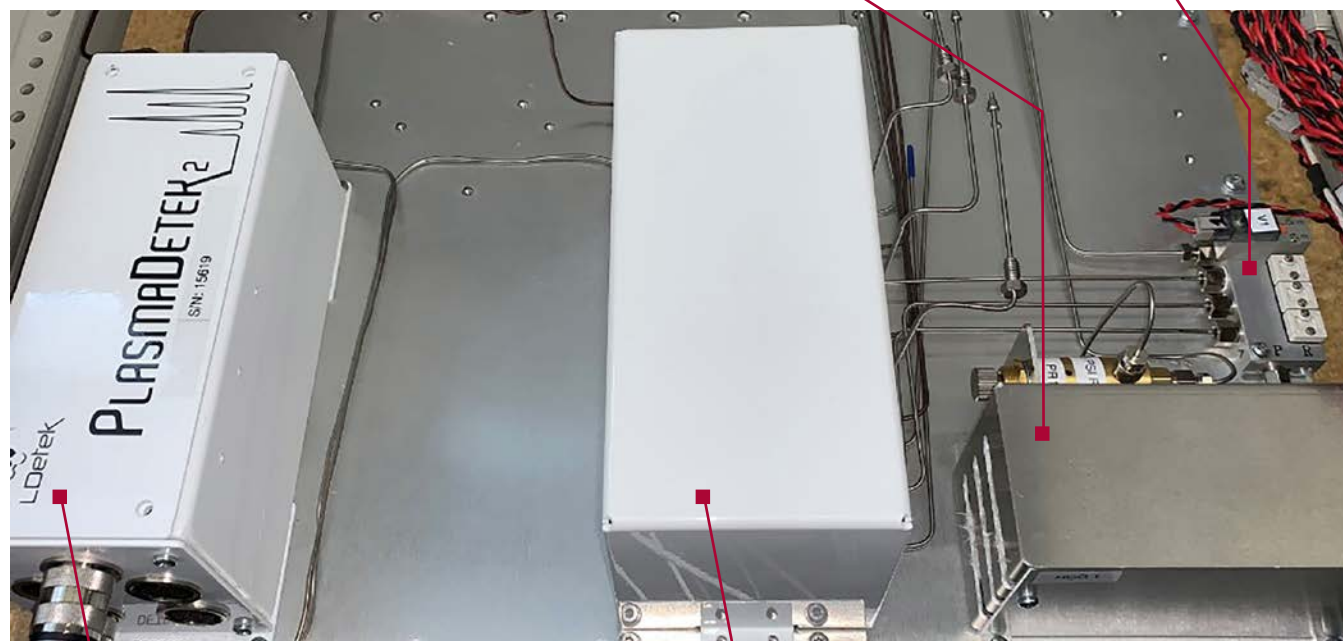

PED sensor integrated inside the same GC unit to allow other impurities analysis in one GC

Temperature controlled module for the sensor and the valve assembly




MAINTENANCE

The system is built to be resistant and simple of operation with minimum interventions. A routine maintenance interval every 5 years for replacing the moisture generator, the gas purifier and the diaphragm of the valve is required. The unit has been designed in a way that replacing those components is very easy. In addition to that, the 5 years period is very long what is appreciated to keep the maintenance tasks at its minimum. These tasks are at the same frequency that the ones required inside the GC. So, a GC check can be done every 5 years for all modules together.

ANALYSER PERFORMANCES


RESPONSE TIME

Different steps of 1ppm, 5ppm and 10ppm have been tested to demonstrate the response time at different concentrations. The response time either on upfront or down end steps remains at about 4-5 minutes. The readings are updated every 60 seconds. The flow path design having low internal volume (0.030"ID) and the purged diaphragm valve makes the system being very quick to respond. On top of that, the system is coated with an inert coating to keep the surface absorption as low as possible to avoid signal drifting. Also, no flow control hardware has been mounted inline with the sensor. The system is configured with bypass flow controller to avoid response delay normally caused by residual dead volume in a standard flow controller.

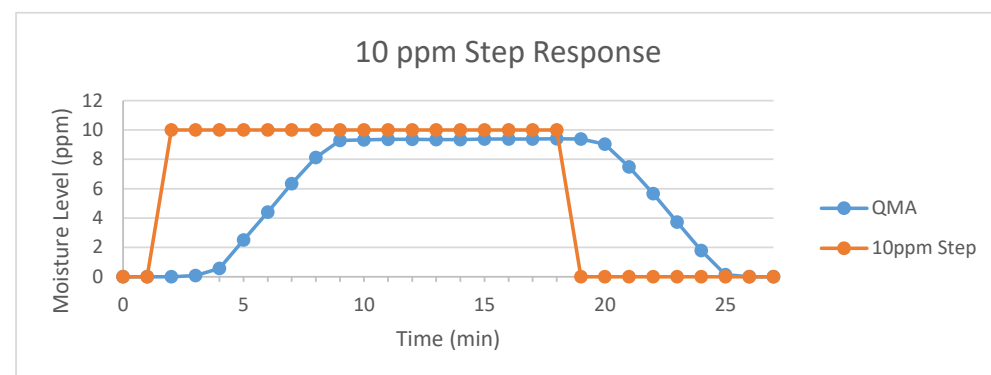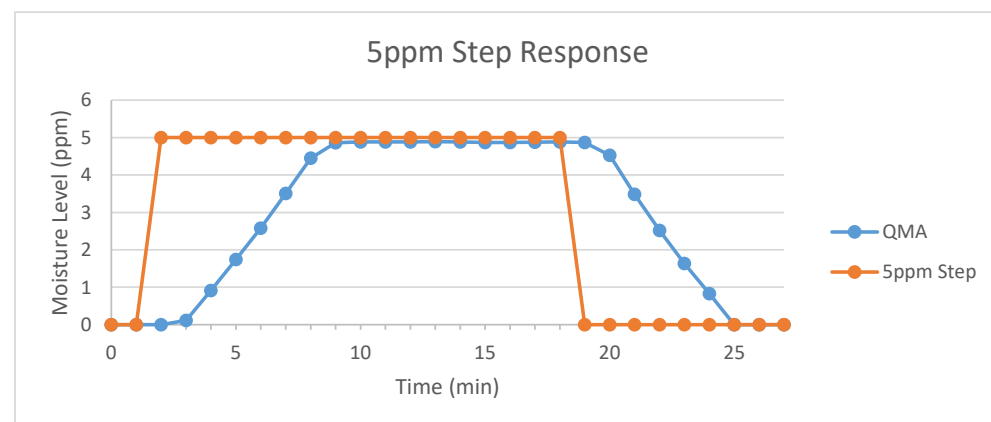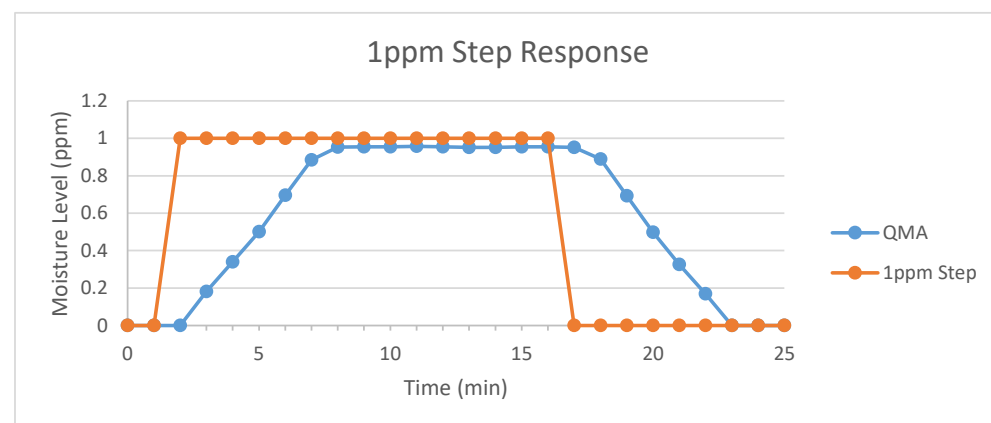

LINEARITY/ACCURACY/REPEATABILITY

The system is fully linear due to the linearization rectification of every sensor. Each system is characterized in function of its full range to ensure the respond is linear. A series of multiple points at different concentration within the scale are performed.

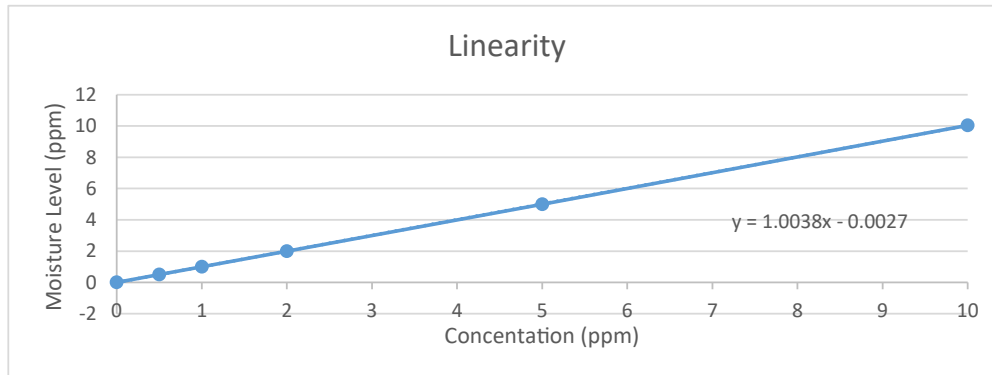


The accuracy error is +/-1% of the scale. In this instance, the table below shows the % error for 6 points diluted at different concentrations between 0-10ppm.

The repeatability error is +/-1% of the scale in a stable environment.

| Diluted concentrations *(ppm) | Analyser reading (ppm) | Accuracy (% of scale) |
|-------------------------------|------------------------|-----------------------|
| 0 | 0 | 0 |
| 0.5 | 0.505 | +0.05 |
| 1 | 1.004 | +0.04 |
| 2 | 1.999 | -0.01 |
| 5 | 5.04 | +0.04 |
| 10 | 10.042 | +0.42 |

DETECTION LIMIT (LDL) AND NOISE

Multiple steps at a concentration of 25ppb of moisture have been performed to demonstrate the lowest detection limit (LDL). The steps are repeatable and clearly show a good response. Considering a maximum noise level equivalent to 0.002ppm(2ppb) at a concentration of 0.2ppm(200ppb) represented by the zoom section, then 5 times this noise level brings the Idl at a value of 10ppb.

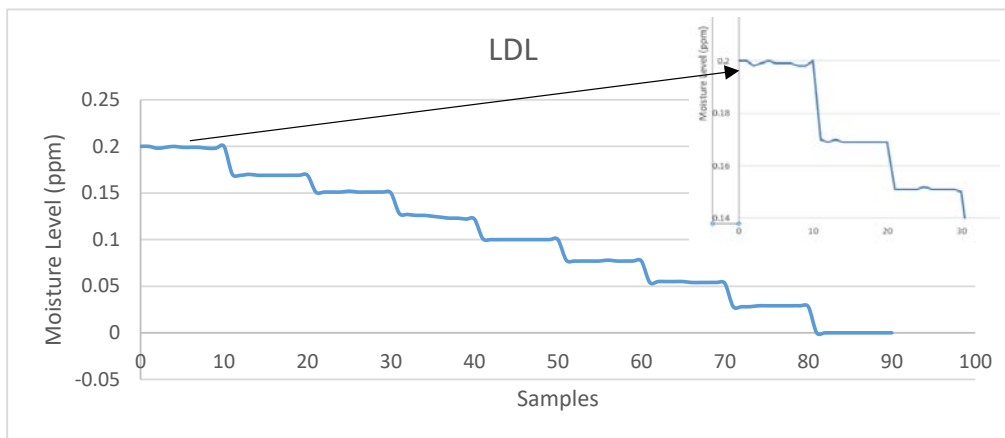


STABILITY/DRIFT

Stability/drift

To evaluate the stability and drift of the unit, a gas bottle containing 8.5ppm moisture in a balance of helium has been connected as sample gas. The system was offering a stability of better than +/- 2% on 24 hours+ period.

8.61ppm (maximum reading) - 8.50ppm (reference value) = 0.11ppm (+1.1%)

8.5ppm (reference value) - 8.44ppm (minimum reading) = 0.06ppm (-0.6%)

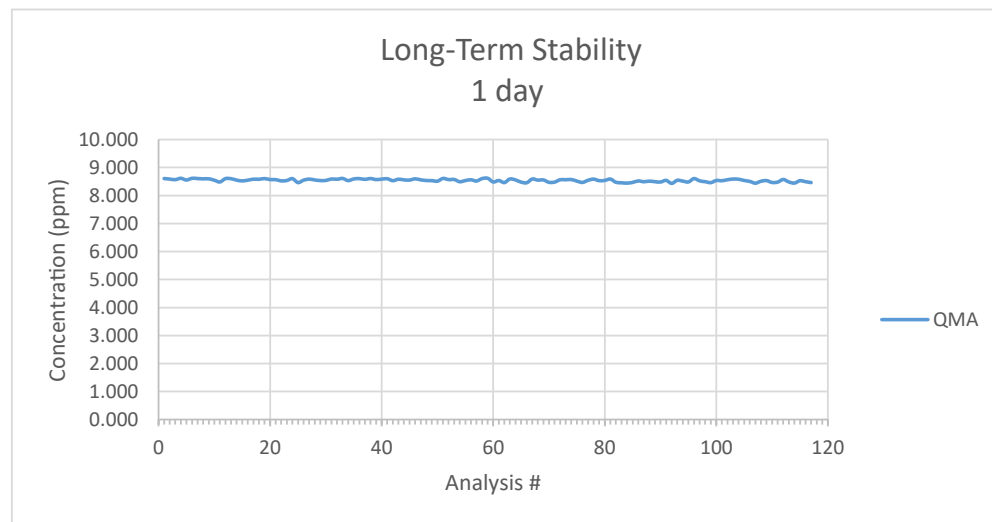

CONCLUSION

LDetek is proud to be the first GC manufacturer capable of bringing an innovative and highly performant trace moisture module inside its gas chromatograph MultiDetek2 series. Its presence in LDetek 's portfolio offers the market the possibility to combine many impurities measured by gas chromatography along with an integrated online trace moisture module inside one instrument.

LD8000-MULTIGAS



CONFIGURED FOR CRYOGENIC HELIUM APPLICATION

DESIGN REPORT



▲ LD8000 MultiGas

▲ PlasmaDetek2

This technical document follows the application note LD16-06 on the use of LD8000-Multigas for the quality control of helium used in cryogenic stations.

The measurement of the trace impurities N₂-O₂-H₂O-CnHm in a helium or argon matrix can be carried out with a PED type detector (PlasmaDetek2) US patent 9,310,308 B2 integrated into an instrument of the LD8000-Multigas type. This technology is based on cold micro-plasma excited at high voltage / frequency in a helium atmosphere and allowing the selective measurement of each component at a precise optical wavelength. The optical circuit is composed of photodiodes and interference filters combined with an amplification system for converting the measured photons into voltage. All signal processing is then redirected to a microcontroller.

Several variants and options on this device are possible depending on the needs of the customer. In this document, we will explain three types of assemblies possible for applications in a helium matrix.

Figure 1 shows an installation where the required measurement must be configured for the following ranges (low to high ppm configuration):

| IMPURITIES | N ₂ | O ₂ | H ₂ O | CnHm |
|------------|----------------|----------------|------------------|----------|
| Range | 0-300 ppm | 0-50 ppm | 0-100 ppm | 0-30 ppm |

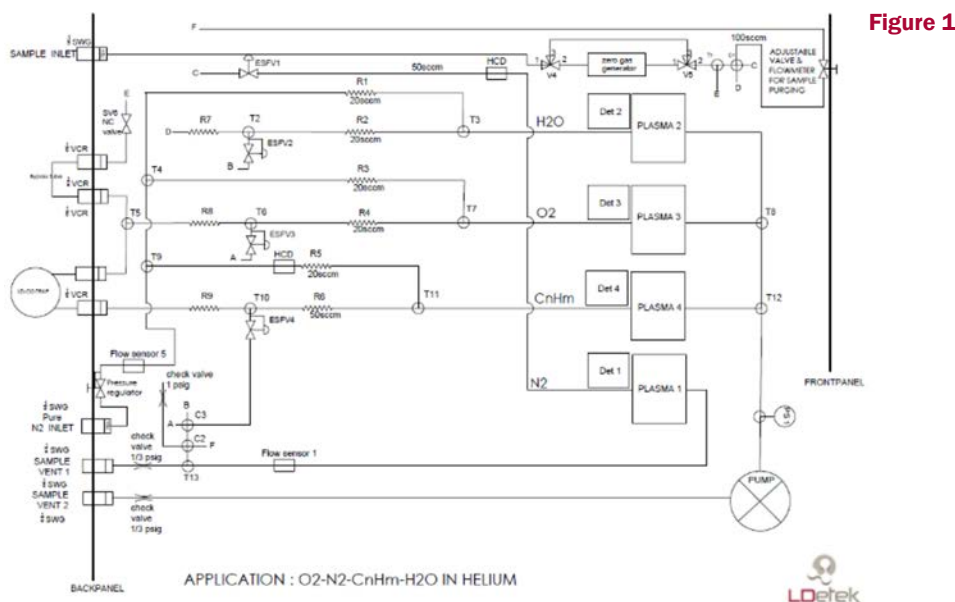


Figure 1

Figure 1 demonstrates an instrument configured as follows:

- Four plasma detectors have been installed in the instrument for N₂-O₂-H₂O-CnHm measurement. Each detector is configured with a narrow optical interference filter providing an optical response specific to the measured impurity. Each plasma is a monolithic structure made of quartz through which a pipe allows a linear gas flow. Through this linear flow, a scanning by an electric discharge is applied. This discharge is called "dielectric" because these electrodes are mounted externally of the quartz assembly. This ensures the inertia of the block internally being in contact with the gas. The discharge is said to be alternative to a specific high frequency and voltage.
- The N₂ doping input is required since the trace measurement of N₂ can reach 300ppm. The N₂ doping is then applied to the PEDs used for H₂O-O₂-CnHm measurement to eliminate the interference from the nitrogen beyond 10ppm. The nitrogen flow is generally controlled to the same value as the helium sample flow. We therefore speak of a ratio of 50% He / N₂. Figure 1 shows a value of 20sccm for 20sccm nitrogen. Total nitrogen consumption for the instrument is therefore 60ml/min. The nitrogen flow rate is controlled by static orifices pre-adjusted to a defined pressure. To ensure the stability of the nitrogen flow, a mini pressure regulator is mounted on the instrument as well as a pressure flow sensor. This assembly ensures the stability of the nitrogen flow rate which is very important for maintaining the N₂-He mixture equilibrium in the plasmas.
- A vacuum pump is required at the PED output used with N₂ / He mixture to allow the excitation of the PEDs performing the O₂-H₂O-CnHm measurement. The same pump is therefore common to the three PEDs. By this output, the measured flow is generally around 120 ml/min of a mixture of 50% He / N₂. The 2nd output, this one without a vacuum pump, is specific to the PED for N₂ measurement. The flow of helium on this output is 50ml/min from the PED for the measurement of N₂, and 3 x 50ml / min being the bypass flow rates of the 3 sample regulators for the O₂-H₂O-CnHm PEDs. To these flow rates, is added the bypass flow at the inlet of the device serving to purge the line upstream of the instrument generally set at 100 ml/min. The total flow of clean helium that can therefore be recovered by the customer is around 300ml / min. Consequently, it is a total flow rate of 300ml / min + 60ml / min, i.e. 360ml / min of helium that is consumed. It is therefore possible to recover more than 83% of the helium consumed by the instrument. A system of "check valve" out of the PED was set up to recover helium without the risk of pressurization of the PEDs. The internal pressure PED is therefore limited to 1/3psig avoiding any risk of rupture of the quartz.

4. A zero-gas free system is installed to generate ultra high purity gas by flowing through a heated purifier and to do a zero calibration. It simply allows to use the sample gas of the customer and to purify it generating the 8.0 grade Helium (i.e., 99.999999%) having maximum impurity level of 10ppb. This purification allows to avoid a bad zero calibration and negative readings on the “process” gas of the customer. Moreover, there is no need for installation of an extra ultra-purity gas bottle with an external purification system, which is generally required by our competitors.
5. Each PED has its own electronic flow control by pressure flow regulator to ensure stability of reading regardless of the inlet pressure fluctuation. All flow controllers are “bypassed” to prevent contamination of the sample and ensure the best possible response time at a small flow rate. Generally, systems measuring N₂-O₂-H₂O must operate at a high rate to allow a good sweep and dilution of the contamination to minimize drift and long response time. Thanks to our ‘bypass’ design, we can afford to keep small flows and limit the waste of Helium being generally very expensive.
6. An O₂ trap with VCR connections is installed on the CnHm PED to eliminate oxygen interference on the CnHm measurement. This trap is composed of activated copper powder.
7. Humidity interference is removed by HCDs (H₂O permeation tubes) installed on N₂-CnHm PEDs. Providing a stable concentration of moisture to the N₂-CnHm plasmas, they are saturated with water, removing the interference caused by moisture in the sample. If the presence of moisture in the sample is above 10-20ppm, then a second trap, this time to capture moisture, is required. It is also with VCR connections, consists of molecular sieve 3A. When it is not required, a simple “bypass” is mounted on the instrument.
8. A software protection system against carbon deposits in the PEDs allows them to go out when the CnHm measurement rises above 3ppm (adjustable parameter). By cutting the excitation of the N₂-O₂-H₂O PEDs during high CnHm measurements, it is possible to prevent the degradation of the PEDs caused generally by the creation of carbon deposits on the walls of the monolithic quartz block.
9. In this configuration, by using the nitrogen doping for the O₂ measurement, the nitrogen level is saturated and any form of interference from the N₂ concentrations is avoided. In addition, the installation of optional moisture trap allows to eliminate any interference on O₂ measurement from H₂O concentrations. The O₂ measurement shielded by its selective optical spectrum combined with N₂ doping and H₂O blocking by a trap can be used to compensate the N₂ measurement. This compensation is done at the software level by an algorithm.
10. The tubing and fittings in contact with the line used for the H₂O measurement are treated with a water-repellent inert coating to minimize surface absorption and provide better temperature stability and response time.

INTERFERENCE SUPPRESSION SYSTEM:

The protection system of the PEDs in the presence of too high hydrocarbon measurements, combined with O₂-H₂O trap networks and the humidity and nitrogen dosing system allows the LD8000-Multigas to remove interferences between the impurities. This is a unique LDetek practice, allowing accuracy and prolonged lifetime of the detector.

In order to protect the H₂O and O₂ traps, they are isolated by a “ shut off ” valve when the N₂ measurement rises above 200ppm (adjustable parameter). The logic behind this protection is based on the fact that if the N₂ measurement rises to a high level, then there is a strong possibility that it is an air infiltration and the same fact increases the O₂-H₂O concentrations. So, as long as the N₂ measurement remains high, a protection preventing the sample from going to the O₂-H₂O traps remains activated.

Table of effects caused by interferents*:**

| SAMPLE* | 10 PPM N ₂ O ₂ CH ₄ H ₂ O | 10 PPM N ₂ | 5 PPM N ₂ | 10 PPM O ₂ | 10 PPM N ₂ O ₂ CH ₄ |
|------------------|---|-----------------------|----------------------|-----------------------|--|
| N ₂ | 10 ppm | 10 ppm | 5 ppm | 0 ppm | 10 ppm |
| O ₂ | 10 ppm | 0 ppm | 0 ppm | 10 ppm | 10 ppm |
| CnHm | 10 ppm | 0 ppm | 0 ppm | 0 ppm | 10 ppm |
| H ₂ O | 10 ppm | 0 ppm | 0 ppm | 0 ppm | 0 ppm |

*The balance of the sample is helium.

*** Other combinations have been tested successfully, so have not been presented in this table. Only critical interference has been presented in this table.

MAINTENANCE:

Frequency 12-18 months:

Regeneration of O₂ and H₂O traps depending on the contents present in the sample.

Frequency 2-3 years:

Replacement of the vacuum pump.

Frequency 4-5 years:

Replacement of the HCD (permeation tube) normally performed at the same time as the replacement of the internal mini-purifier as well as the external compact purifier required for nitrogen dosing.

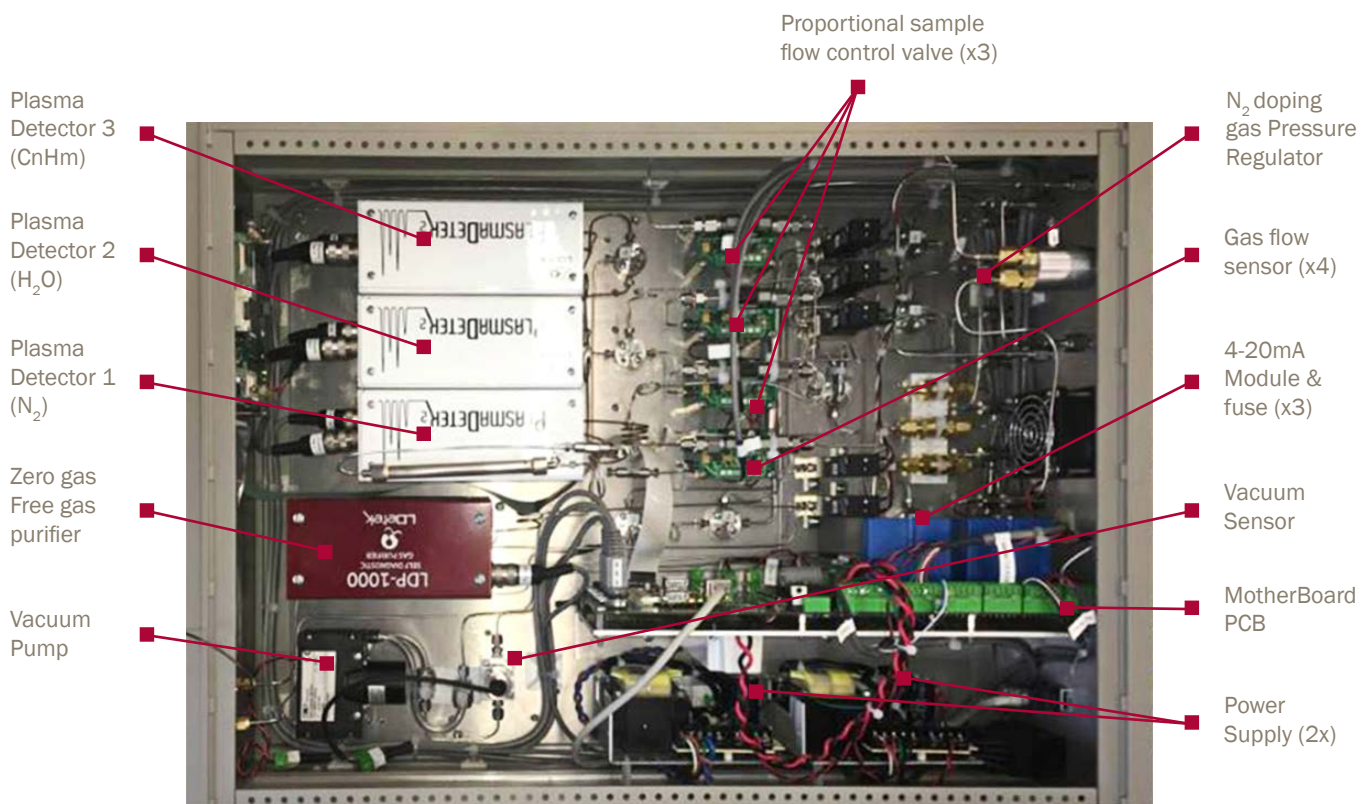


Photo 1

Photo of a configuration based on Figure 1 but for N₂-CnHm-H₂O measurements without O₂ measurement. Other configurations are based on the same mounting but with slightly different module layouts to accommodate the same 4U rack mount cabinet.

Conclusion on the configuration of Figure 1:

This is the most complete configuration of all. It shows no interference between the components to be measured as shown in the table. In addition, this configuration can cover the full range from low ppb / ppm to higher ppm. It is therefore the most robust, stable and precise solution for this type of application.

Figure 2 shows an installation where the required measurement must be configured for the following ranges (low ppm configuration only):

| IMPURITIES | N ₂ | O ₂ | H ₂ O | CnHm |
|------------|----------------|----------------|------------------|----------|
| Range | 0-10 ppm | 0-10 ppm | 0-10 ppm | 0-10 ppm |

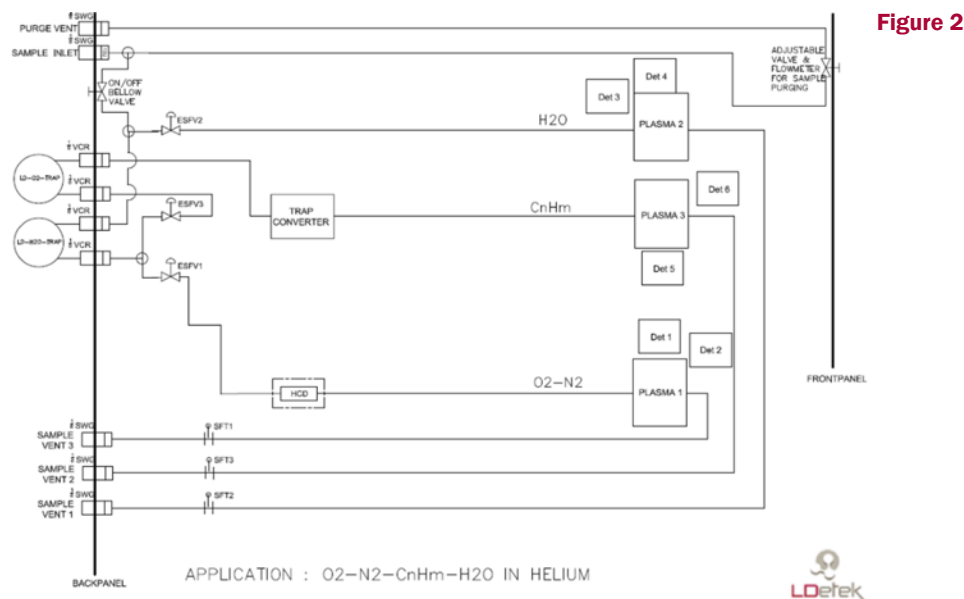


Figure 2 demonstrates an instrument configured as follows:

- Three plasma detectors have been installed in the instrument, respectively for the N₂ / O₂-H₂O-CnHm measurement. Each detector is configured with a narrow interference optical filter providing an optical response specific to the measured impurity. Each plasma is a monolithic structure made of quartz through which a pipe allows a linear gas flow. Through this linear flow, a scanning by an electric discharge is applied. This discharge is called "dielectric" because these electrodes are mounted externally of the quartz assembly. This ensures the inertia of the block internally being in contact with the gas. The discharge is said to be alternative to a specific high frequency and voltage.
- Nitrogen doping is not required because the N₂ range is below 10ppm and the interference caused by nitrogen on O₂-CnHm-H₂O measurements is limited.
- A vacuum pump is not required at the PED output for the same reason as indicated in point 1.
- Each PED has its own electronic flow control regulated by a proportional microvalve with minimal internal volume. The reading of the flow is made by mass sensors installed at the outlet of the PEDs to avoid any form of contamination and additional volume in front of the detector. Our design allows the use of small flow since no bulky flow control element is installed upstream of the detectors. All tubing is made of 1 / 16"OD stainless steel to minimize purge volumes. A water-repellent "coating" is applied for the plasma pipes used for H₂O measurement to reduce surface absorption. The flow rates at the outlet of each PED are respectively 50 ml / min for a total of 150 ml / min. If this flow rate is combined with the flow rate at the inlet, which is generally adjusted to 100 ml / min, the total flow rate of the instrument is thus 250 ml / min. All this flow can be recovered because it has not been contaminated by the instrument.
- Moisture interference is removed by installing HCD (H₂O permeation tube) on PED O₂ / N₂. Providing a stable concentration of moisture to the O₂ / N₂ plasma, it is saturated with water, removing the interference caused by moisture in the sample. If the presence of moisture in the sample is above 5-10ppm, then a second trap, this time to capture moisture is required. It consists of molecular sieve 3A and has VCR fittings. When it is not required, a simple "bypass" is mounted on the instrument.

6. A software protection system against carbon deposits at the PEDs allows them to go out when the CnHm measurement rises above 3ppm (adjustable parameter). By cutting the excitation of the N₂ / O₂-H₂O PEDs during high CnHm measurements, it is possible to prevent the degradation of the PEDs generally caused by the creation of carbon deposits on the walls of the monolithic quartz block.

7. In this configuration where the plasma nitrogen dosage is not used, it should not be surprising that O₂-H₂O traps should be used at a lower concentration to eliminate interference than we see in a platform where the nitrogen dosage is in place. This phenomenon is caused by the equilibrium of the species inside the plasma, offering a different mode of operation. It is also for the same reason that in this configuration under Helium plasma only, we use a system of "trap converter" which consists of a mini plasma allowing the carbon to decompose thus allowing the PED CnHm to measure a "by-product" from the carbon decomposition. This allows a more selective measurement of hydrocarbons and at the same time avoids the CnHm PED to make carbon deposits on these walls since the carbons remain in the space of the trap converter system protecting the plasma used to measure the CnHm.

8. In this configuration, each PED contains an additional optical circuit, selective to the N₂ measurement. This allows leak diagnosis in each channel.

INTERFERENCE SUPPRESSION SYSTEM:

The protection system of the PEDs in the presence of too high hydrocarbon measurements, combined with O₂-H₂O trap networks, moisture metering system and carbon converter allows the LD8000-Multigas to minimize the interferences between the impurities. This is a unique LDetek practice, allowing accuracy and prolonged lifetime of the detector.

Table of effects caused by interferences*:**

| SAMPLE* | 10 PPM N ₂ O ₂ CH ₄ H ₂ O | 10 PPM N ₂ | 5 PPM N ₂ | 4 PPM O ₂ | 10 PPM N ₂ O ₂ CH ₄ |
|------------------|---|-------------------------------|-------------------------------|-------------------------------|--|
| N ₂ | 10 ppm | 10 ppm | 5 ppm | -2 ppm** (display = 0 ppm) | 10 ppm |
| O ₂ | 10 ppm | -3 ppm** (display = 0 ppm) | -2 ppm** (display = 0 ppm) | 4 ppm | 10 ppm |
| CnHm | 10 ppm | 0 ppm | 0 ppm | 0 ppm | 10 ppm |
| H ₂ O | 10 ppm | +0.2 ppm** | +0.1 ppm** | +0.2 ppm** | +0.5 ppm** |

* The sample balance is helium

** Approximate measurement based on laboratory tests

*** Other combinations have been successfully tested, so they are not presented in this table. Only critical interference is shown in this table.

MAINTENANCE:

Frequency 12-18 months:

Regeneration of the O₂ and H₂O traps according to the contents present in the sample.

Frequency 4-5 years:

HCD (permeation tube) replacement.

Conclusion on the configuration of Figure 2:

This is the simplest and cheapest configuration of all, but it presents some interference between the compounds to be measured as shown in the table. On the other hand, these interferences can be negligible according to the needs and the application of the customers.

Figure 3 shows an installation where the required measurement must be configured for the following ranges (so-called low to medium ppm configuration):

| IMPURITIES | N ₂ | O ₂ | H ₂ O | CnHm |
|------------|----------------|----------------|------------------|----------|
| Range | 0-20 ppm | 0-20 ppm | 0-20 ppm | 0-20 ppm |

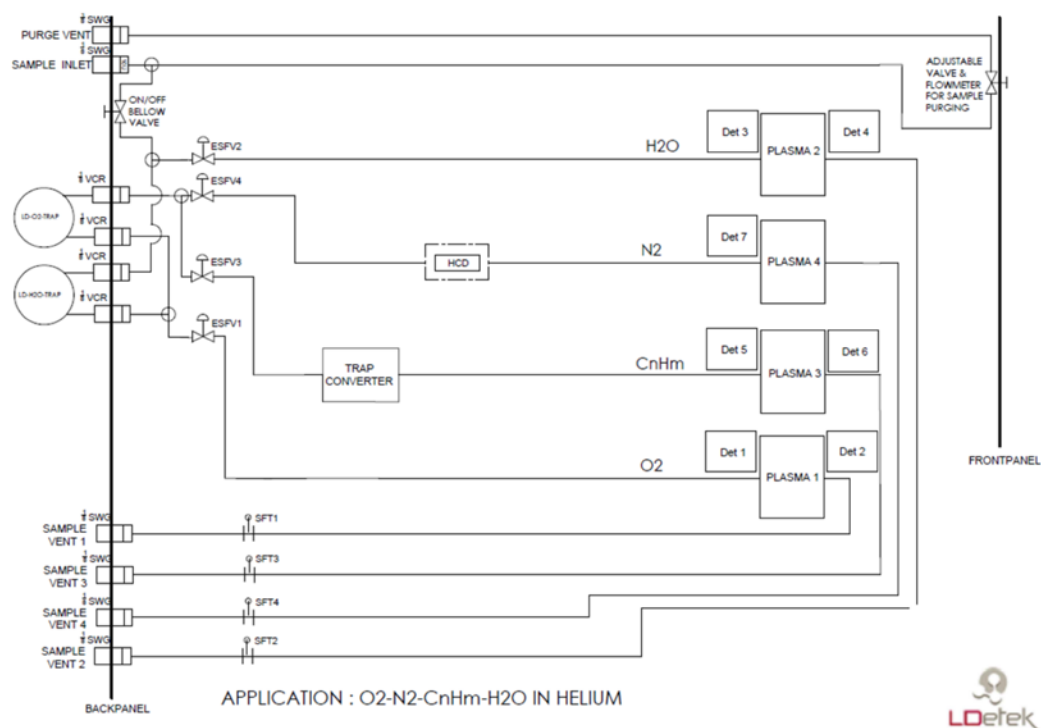


Figure 3

Figure 3 demonstrates an instrument configured as follows:

1. This configuration is similar to the one described in Figure 2. However, it allows to cover a so-called average measurement range, i.e. to go up to 20ppm ranges. To enable this, a plasma specifically configured for N₂ measurement has been added behind the H₂O and O₂ traps allowing to obtain a measurement without interference of nitrogen. In this configuration, the shielded nitrogen measurement is used to apply compensation to the O₂ measurement.

INTERFERENCE SUPPRESSION SYSTEM:

The protection system for PEDs in the presence of excessively high hydrocarbon measurements, combined with O₂-H₂O trap networks, moisture metering system and carbon converter allows the LD8000-Multigas to eliminate interference between the impurities. This is a unique LDetek practice, allowing accuracy and prolonged lifetime of the detector.

Table of effects caused by interferences*:**

| SAMPLE* | 10 PPM N₂ O₂ CH₄ H₂O | 10 PPM N₂ | 5 PPM N₂ | 10 PPM O₂ | 10 PPM N₂ O₂ CH₄ |
|------------------|---|-----------------------------|----------------------------|-----------------------------|--|
| N ₂ | 10 ppm | 10 ppm | 5 ppm | 0 ppm | 10 ppm |
| O ₂ | 10 ppm | 0 ppm | 0 ppm | 10 ppm | 10 ppm |
| CnHm | 10 ppm | 0 ppm | 0 ppm | 0 ppm | 10 ppm |
| H ₂ O | 10 ppm | +0.2 ppm** | +0.1 ppm** | +0.2 ppm** | +0.5 ppm** |

* The sample balance is helium

** Approximate measurement based on laboratory tests

*** Other combinations have been successfully tested, so they are not presented in this table. Only critical interference is shown in this table.

MAINTENANCE:

Frequency 12-18 months:

Regeneration of the O₂ and H₂O traps according to the contents present in the sample.

Frequency 4-5 years:

HCD (permeation tube) replacement.

Conclusion on the configuration of Figure 3:

This is the configuration that lies between the simplest and most complete configurations previously explained (Figures 1 and 2). It allows a little higher ranges measurement and interference minimization without the use of nitrogen doping. Depending on the needs and application, this configuration can be considered advantageous and is a good compromise between the two extremes.



4.0 TESTIMONIALS





ANALYSIS OF PERMANENT GASES IN DIFFERENT MATRIX USING PLASMADETEK

The goal of this application is to analyze permanent gases in different matrix used for electronic industry. The investigation of these impurities is important for gas providers to ensure the high purity of their products to their customers.

This analyzer has been configured with two independent channels, each one dedicated to one matrix. The system is based on a GC Clarus 580 from Perkin Elmer equipped with electronic pressure regulators. Two high quality 10 ports diaphragm valves with internal purge ensure sample injection directly on-column and matrix backflush. The precolumn is a semi-capillary Plot Q 30m x 530um column. The analytical column is a Molsieve 5A 30m x 530um column with a by-pass flow to elute CO₂. Two detectors Plasmadetek with two internal detectors each are used to quantify the components. The signal coming from each PED is sent to the acquisition software Totalchrom.

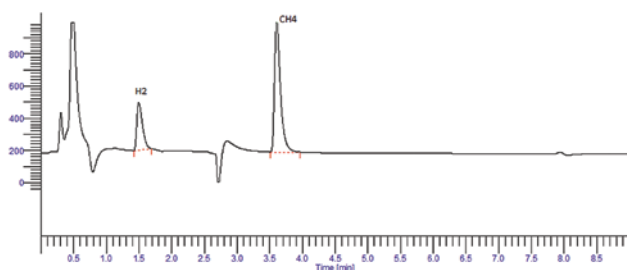


Figure 2

| COMPONENT | CONC. (PPM) | PEAK HEIGHT | NOISE | S/N | LOD (PPB) S/N=3 | LOQ (PPB) S/N=5 |
|-----------------|-------------|-------------|-------|-------|--------------------|--------------------|
| H ₂ | 5 | 296 | 0.02 | 14800 | 1.0 | 1.7 |
| CH ₄ | 5 | 808 | 0.02 | 40400 | 0.4 | 0.6 |
| CO ₂ | 5 | 223 | 0.02 | 11150 | 1.3 | 2.2 |
| N ₂ | 5 | 793 | 0.02 | 39650 | 0.4 | 0.6 |
| CO | 5 | 110 | 0.02 | 5500 | 2.7 | 4.5 |

Figure 4

The use of Plasmadetek in this system provides excellent results regarding sensibility and selectivity. The Plasmadetek is ideal for this kind of analyses because it can support high volume of sample injection and we can adjust Make Up gas flow to obtain a suitable chromatogram. The installation of Plasmadetek on a Clarus GC is easy and don't need physical modification of the GC. Its design is in full harmony with the GC whose all parts are accessible for an easy modification (figure 5).

One of the main advantages of Plasmadetek is that it is maintenance free, so that gives a robust system for long analyses sequences in the laboratory or for on-line measuring analyzers. The large range of concentrations (from ppb to %) and the available selectivity of Plasmadetek make this detector ideal to work in a lot of domains where GC is necessary.

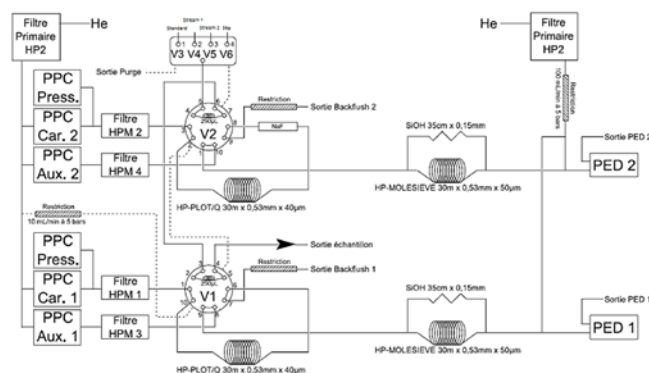


Figure 1

A 5 ppm standard of each permanent gas has been used to calibrate the system and determine LOQ for each component. The chromatograms shown below illustrate the results we can obtain from this configuration. The chromatogram in figure 2 is obtained with the detector optimized for H₂ and CH₄. The chromatogram in figure 3 is obtained with the detector optimized for N₂, CO and CO₂.

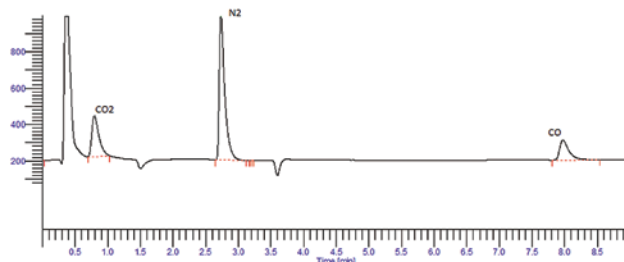


Figure 3




Figure 5

ANTELIA: 9 Chemin de la Brocardière, 69570 DARDILLY • contact@antelia.fr • Port +33 6 77 01 51 25 • Tel +33 4 72 17 82 10 • Fax +33 4 78 66 07 03

Application: Online analysis of four different streams. Monitoring nitrogen and impurities (H_2 , CH_4 , HCs, O_2 and CO_2) at low level in Helium matrix with the PlasmaDetek.



The online analysis controller software (SRA Prochem) manages and anticipates the selection of the next stream. Alarms are generated when impurities concentration becomes critical. Peak reproducibility using the complete system is close to 1% (RSD; n=5).

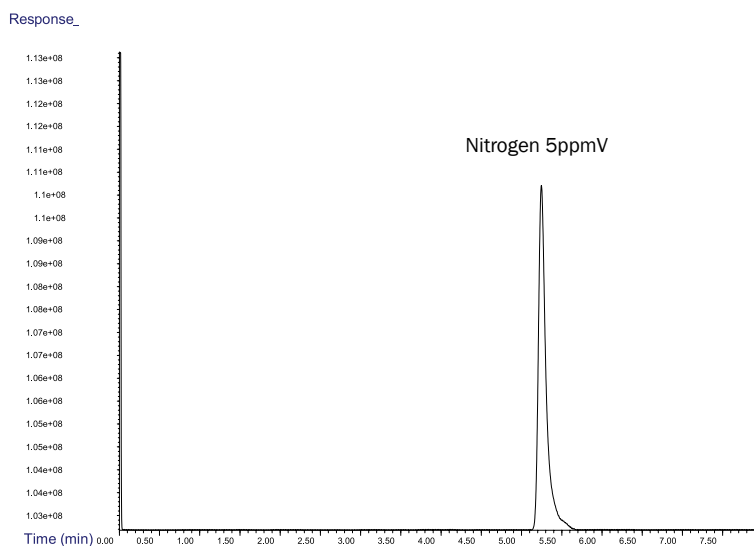

SRAINSTRUMENTS
150 rue des Sources
69280 Marcy l'Etoile
France

T : 04.78.44.29.47
F : 04.78.44.29.62
info@sra-instruments.com
www.sra-instruments.com

SA à Directoire et Conseil de surveillance
au capital de 150.000 €
RCS Lyon B 342 068 731
APE 4669B
SIRET: 342 068 731 00039
Code TVA FR 40342068731

 **Agilent Technologies**
Premier Solution Partner

Due to Helium shortage, gas suppliers see an increased request for alternative gases. Their clients demand high purity with exact specification for various applications like instrumental use and industrial production. Often PDD (Pulsed Discharge Detector) is used for measuring impurities in bulk gases. But in case of determining the purity of Argon, separation problems arise with this detector because Helium is used as carrier gas and the bulk Argon elutes close to Oxygen. The Plasmadetek-2 from LDetek offers the perfect solution here, since Argon is used as carrier gas, and therefore the bulk peak is not seen at all.

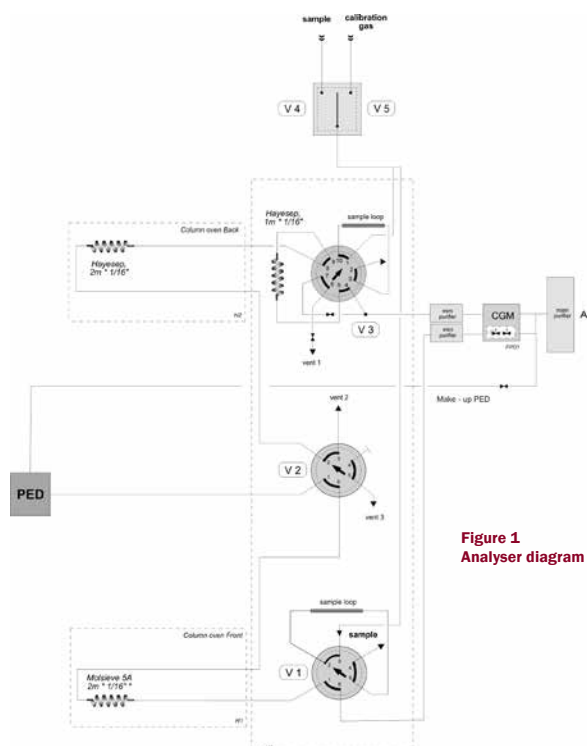


Figure 1
Analyser diagram

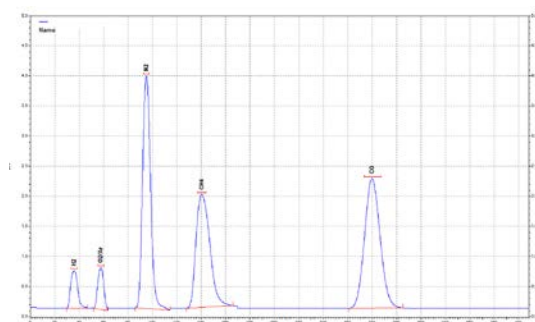


Figure 2
Chromatogram
Molsieve column

| Aqilent 35900E Inte... | H2 | O2/Ar | N2 | CH4 | CO |
|------------------------|-----------|-----------|------------|------------|------------|
| Sample ID | Area | Area | Area | Area | Area |
| molsieve testFATHel... | 203067.00 | 194281.00 | 1452795.00 | 1218724.00 | 1591571.00 |
| molsieve testFATHel... | 202392.00 | 195591.00 | 1452917.00 | 1219249.00 | 1590896.00 |
| molsieve testFATHel... | 205617.00 | 194085.00 | 1455726.00 | 1216440.00 | 1592798.00 |
| molsieve testFATHel... | 204789.00 | 195496.00 | 1455690.00 | 1223070.00 | 1582777.00 |
| molsieve testFATHel... | 205039.00 | 193859.00 | 1455817.00 | 1227535.00 | 1587183.00 |
| molsieve testFATHel... | 205447.00 | 195147.00 | 1455831.00 | 1220549.00 | 1584348.00 |
| molsieve testFATHel... | 205320.00 | 196256.00 | 1454897.00 | 1224674.00 | 1592919.00 |
| molsieve testFATHel... | 203894.00 | 195299.00 | 1455741.00 | 1226357.00 | 1573995.00 |
| molsieve testFATHel... | 206239.00 | 196406.00 | 1456723.00 | 1225968.00 | 1590468.00 |
| molsieve testFATHel... | 205231.00 | 194874.00 | 1457012.00 | 1227555.00 | 1587986.00 |
| Min: | 202392.00 | 193859.00 | 1452795.00 | 1216440.00 | 1573995.00 |
| Max: | 206239.00 | 196406.00 | 1457012.00 | 1227555.00 | 1592919.00 |
| Mean: | 204703.50 | 195129.40 | 1455314.90 | 1223012.10 | 1587494.10 |
| Std Dev: | 1211.05 | 867.00 | 1419.98 | 4022.07 | 5862.43 |
| %RSD: | 0.59 | 0.44 | 0.10 | 0.33 | 0.37 |

Figure 3 - Repeatability

Figure 1 shows a two-channel analyser with single Plasma Emission Detector. Valve V1 and Molsieve column analyse H₂, N₂, O₂, CH₄ and CO in Ar. A second channel around valve V3 is present for analysing CH₄, CO₂, N₂O and Ethane in Ar. For analysis of impurities in N₂, a fore-flush column switching option is added to this channel to vent the bulk N₂. Figure 2 shows the Molsieve chromatogram of an 11 ppm calibration standard. Figure 3 demonstrates the obtained repeatability, which is excellent. Valve V2 combines both channels to a single PlasmaDetect-2 detector, which contains up to four optical sensors for optimal sensitivity for each individual component, see figure 4. Figure 5 shows the integrated analyser using CompactGC^{4.0}.

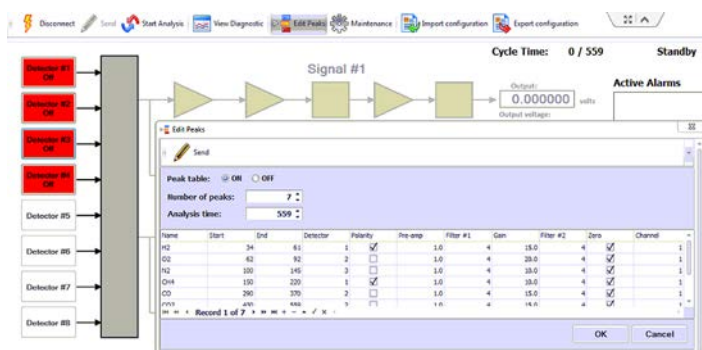


Figure 4 - programming 4 optical sensors in one PlasmaDetect-2 detector




Figure 5 - CompactGC^{4.0}

GLOBAL ANALYSER SOLUTIONS
P.O. Box 2148, 4800 CC Breda, The Netherlands
T: +31 (0)76 5411800 F: +31 (0)842 206757
info@gas-site.com www.gas-site.com




PARTNER

Antelia integrated PlasmaDetek series solutions in many GCs over the last years and is proud of its strong expertise for developing high performance applications. Antelia works with Perkin Elmer lab GC platform to develop their solutions. On top of that, Antelia also integrates PlasmaDetek on the compact GAS GC. Depending on the applications, Antelia uses the GAS compact series or the Perkin Elmer desktop GC.

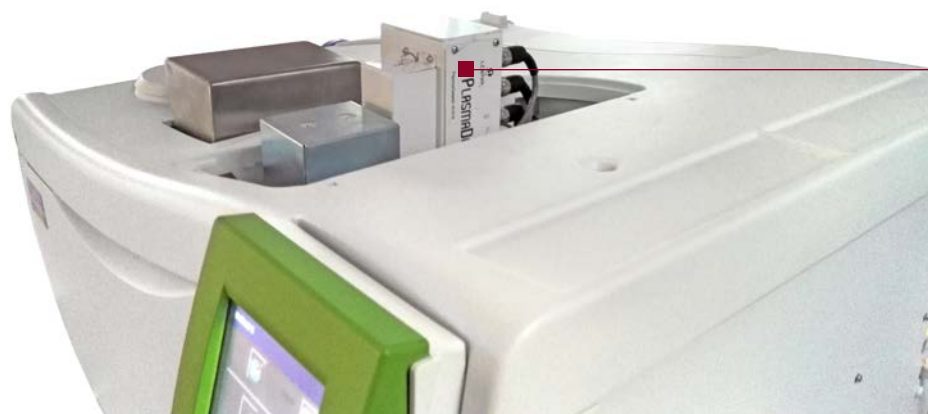

PlasmaDetek2(PED) mounted on the Clarus Perkin Elmer GC

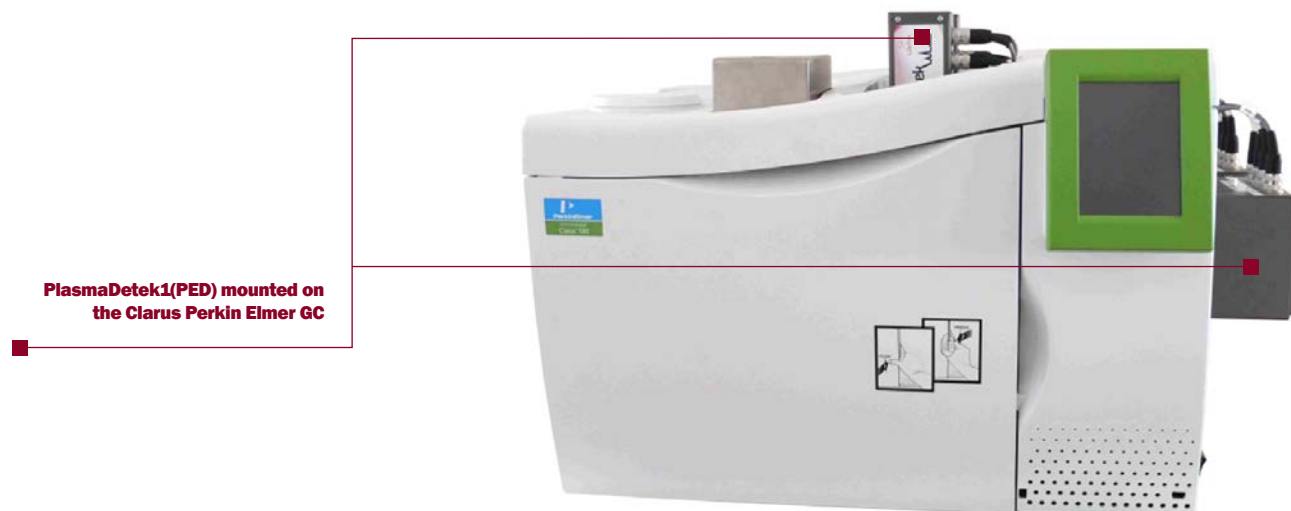

PlasmaDetek1(PED) mounted on the Clarus Perkin Elmer GC

ANTELIA: 9 Chemin de la Brocardière, 69570 DARDILLY • contact@antelia.fr • Port +33 6 77 01 51 25 • Tel +33 4 72 17 82 10 • Fax +33 4 78 66 07 03



CREATVAR
TECHNOLOGY CORP.

ANALYSIS OF TRACE IMPURITIES IN ELECTRONIC GRADE HYDROGEN USING AGILENT GC WITH PDHID AND PLASMADETEK 2



APPLICATION

Impurities(Ar-O₂-N₂-CH₄-CO-CO₂) analysis of electronic grade Hydrogen at 10 to 20ppb level with the PDHID and Plasmadetek 2.

This analyzer has been configured with two independent channels, front channel for impurities(Ar-O₂-N₂-CH₄-CO) measurement by PDHID and back channel for impurities(CO₂,n-C₂~4) measurement by PED. The system is based on a GC 6890N from Agilent equipped with electronic pressure control module. Two low leak rate 6 port and 4 port switching valves with Molsieve 5A column to perform bulk Hydrogen heart-cut technic and assure the baseline separation for Ar and O₂ in H₂ gas sample.



H2 Analyzer

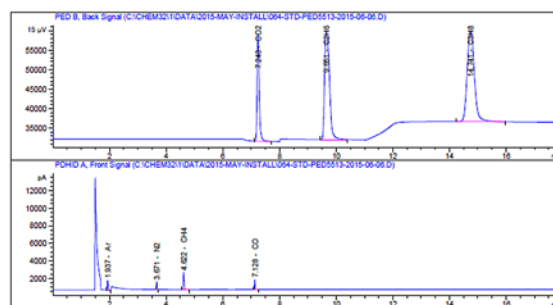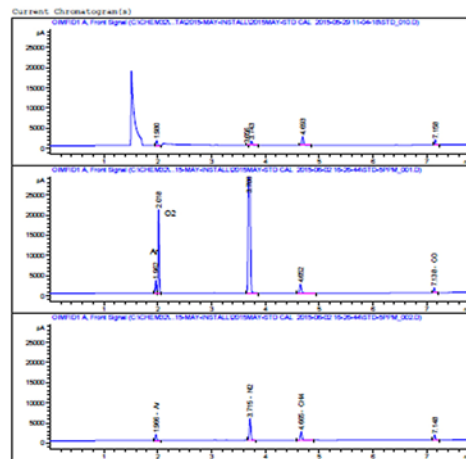

Signal 1: PED B, Back Signal

| RetTime [min] | Type | Area [15 μ V*s] | Amt/Area | Amount [ppm] | Grp | Name |
|------------------|------|------------------------|------------|-----------------|------|------|
| 7.243 | BB S | 1.44087e5 | 2.78998e-5 | 4.02000 | CO2 | |
| 9.651 | BB S | 3.36276e5 | 3.28599e-5 | 11.05000 | C2H6 | |
| 14.741 | BB | 4.07393e5 | 1.13159e-5 | 4.61000 | C3H8 | |

Signal 2: PDHID A, Front Signal

| RetTime [min] | Type | Area [pA*s] | Amt/Area | Amount [ppm] | Grp | Name |
|------------------|------|----------------|------------|-----------------|-----|------|
| 1.937 | BBA | 1860.75464 | 2.86443e-3 | 5.33000 | Ar | |
| 3.671 | BB | 1753.38501 | 3.59305e-3 | 6.30000 | N2 | |
| 4.622 | BB | 4349.97461 | 1.13334e-3 | 4.93000 | CH4 | |
| 7.128 | BB | 1978.74536 | 2.41567e-3 | 4.78000 | CO | |

| LDL CALCULATION | | | | |
|-----------------|-----------------------------|-------------|---------|-----------|
| COMPONENT | Standard Gas Conc. (ppm) | Peak Height | 3xNoise | MDL (ppb) |
| AR-PDDA | 5.33 | 1826.99624 | 0.3381 | 9.36858 |
| N2-PDDA | 6.3 | 794.99384 | 0.3381 | 2.679304 |
| CH4-PDDA | 4.93 | 1911.48582 | 0.3381 | 8.72009 |
| CO-PDDA | 4.78 | 1107.18896 | 0.3381 | 1.45966 |
| CO2-PEDB | 4.02 | 19544.75508 | 6.4824 | 1.33331 |
| C2H6-PEDB | 11.05 | 16159.39258 | 6.4824 | 4.43275 |
| C3H8-PEDB | 4.61 | 15624.92695 | 6.4824 | 1.91258 |



Copyright(C) 2008 CREATVAR TECHNOLOGY ALL Right Reserved
地址:807 高雄市三民區北平二街10號7F
Tel:07-3150125 Fax:07-3150025
www.cvtweb.com.tw



Agilent Technologies

Premier Solution Partner

PLASMADETEK2 (PED) MOUNTED ON DANI MASTER GC

APPLICATION SUMMARY

At Microbial Analytics Sweden AB we have investigated gases dissolved in water for over two decades. The water is collected from deep boreholes in solid rock and the gases are dissolved in the water under very high pressure. The background is that some of these gases might act as fuel for microorganisms; other gases indicate ongoing microbiological processes. It is important to investigate these mechanisms because they might endanger long-term storage of for instance spent nuclear fuel. Also, in a shorter time span other structures underground might be heavily corroded by such mechanisms.

SOLUTION

We have developed our own sampler design to collect and transfer the water pressurized to the laboratory. After extraction, we analyze the dissolved gases using several different gas chromatographs. The ranges of gases are the usual permanent gases, though present at unusual ratios and concentrations, as well as lighter hydrocarbons.

As a research institute it is important for us to keep the quality at a very high level. Because of this we have decided that all analytical results should be verified by multiple analyses on different gas chromatographs using alternative columns as well as alternative principles of detection.

Last year we decided to replace an older gas chromatograph that was set up with TCD detector as well as an FID detector and a methanizer. It was brought to our attention by the Swedish agent for PlasmaDetek2, Kovalent AB, that the plasma detector could be a useful alternative for the replacement instrument. Because of this we settled for the PlasmaDetek2 instead of the FID/methanizer setup on one channel in the new chromatograph, keeping TCD detection on the other channel.

For us this was a very fortunate decision since the PlasmaDetek2 has qualities difficult to obtain in other ways. Not only is it very easy to quantify carbon monoxide and

dioxide in the same run as the hydrocarbons without the need for a methanizer that has to be protected by switching valves. It is also possible to detect inert permanent gases in the same run. This is very much in line with our quality goals, to detect the analytes using different principles. Other instruments in our laboratory are still equipped with for instance FID detection and the results are compared, showing very good correlation.

Another positive effect was the ability to tune the sensitivity for different gases. In our samples we sometimes have to measure hydrogen at low concentration in the presence of comparatively high levels of neon. Chromatographic separation is possible, but not always optimal. Using the PlasmaDetek2, the sensitivity for hydrogen is much higher than for neon and the quantification gets a lot easier.

The PlasmaDetek2 (PED) detector has been a very positive experience for us!


RESULTS

The chromatogram below shows an example of analysis of a sample gas containing 0,10% of CO-CO₂-C₂H₂-C₂H₄-C₂H₆ and C₃ in balance nitrogen. The CH₄ is also measured in this application and the integration window appears at minute 5, but it is not present in the sample gas used for this analysis.


On the chromatogram, we can see that the CO peak is integrated in a slight drift that comes from the balance Nitrogen peak that elutes just before. The selectivity of the Plasmadetek2 (PED) for the CO measurement makes it suitable to measure it, even if the column used cannot separate N₂ from CO perfectly.

The C₂'s are also shown in a slight drift that comes from the temperature programming of the column. The peaks can be separated and integrated with success at any concentration.

The configuration of the system uses a single Carboxen 1010 column for the separation. The column temperature was programmed to allow the peaks having a late elution time to come earlier. The injection volume used was 100 micro liters.

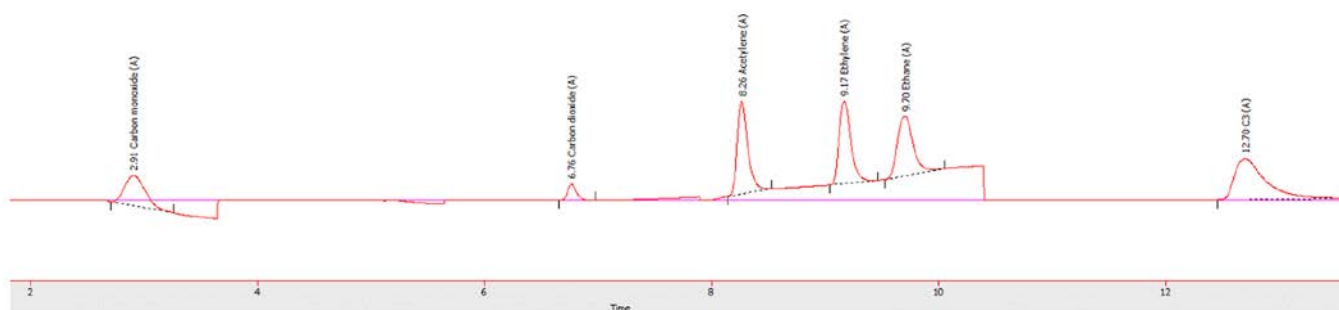

SYSTEM PICTURE

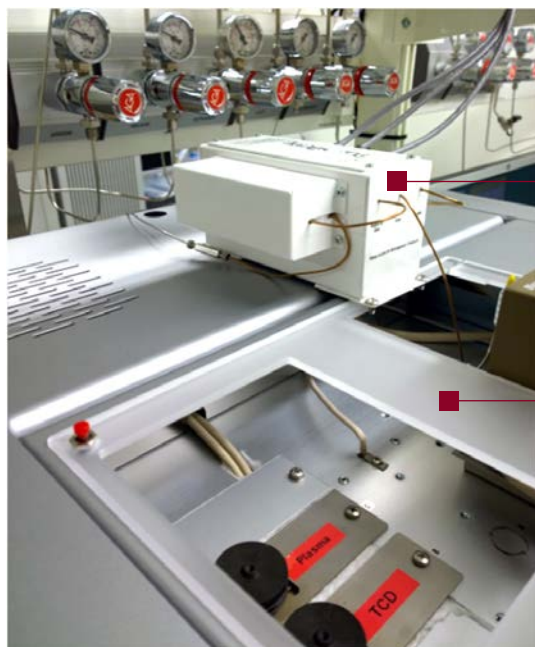

PlasmaDetek 2 (PED)



DANI Master GC

Koalent AB, Fältspatsgatan 6, 421 30 Västra Frölunda. Tel. +46 (0)31 709 81 80, e-post: koalent@koalent.se

APPLICATION SUMMARY

As part of a research project for measuring greenhouse gases in France, more precisely for the N₂O and CO₂ for multiple soil sample analysis having a wide range of concentrations, the use of the PlasmaDetek2 (PED) detector and the Agilent 7890 GC combined with the Headspace 111 auto sampler system have been used in this proposed solution.

CHALLENGE OF THE APPLICATION

The samples from different locations come in 40ml vials. More than 4000 samples have to be analyzed per campaign. The samples contain CO₂ concentrations ranging from 500ppm up to 80% and N₂O concentration from 300ppb up to 5000ppm. The system of detection must be able to cover each sample within 15 minute cycle time. Low and high concentrations are analyzed with the same system.


SOLUTION

System implementation comprises a Headspace setter 111 positions coupled to an Agilent 7890 gas chromatograph (GC) equipped with purged valves and connected to two types of detectors, one TCD for high levels of CO₂ in particular, and a PED (PlasmaDetek2 from LDetek) for traces of N₂O. The advantage of this notorious PED detector with respect to ECD detector, frequently encountered in this application, is the absence of radioactive source subject to a heavy administrative procedure and staff empowerment. The presence of these two sensors in the same instrument, allows analysis and quantification of high levels of CO₂ and very low levels of N₂O.


SYSTEM PICTURE



RESULTS

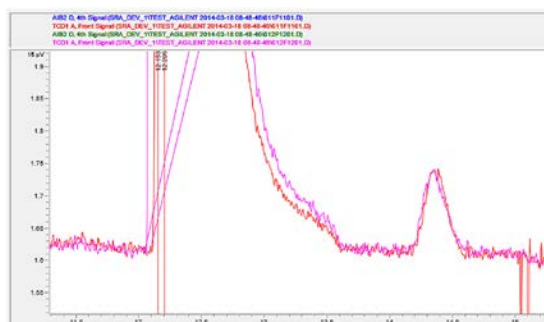

Chromatogram showing 80% CO₂ and 40ppm N₂O using TCD channel. This channel gives the ability to measure high concentration CO₂.

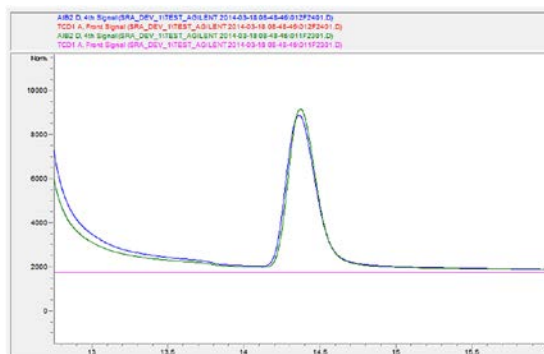

Chromatogram showing 40ppm N₂O using PED (PlasmaDetek2) channel. This channel is used for measuring low concentration N₂O.

HYDROGENICS

SHIFT POWER | ENERGIZE YOUR WORLD

Hydrogenics is a leading developer and manufacturer of hydrogen generation and hydrogen-based power systems. With a proven track-record of over 60-years of experience in fuel cell technology and innovation.

Hydrogenics helps companies reduce their footprint by reducing carbon emissions and producing clean renewable energy that can be sent back into the power grid. Hydrogenics super-dense PEM fuel cell allows for large-scale energy storage with unprecedented high-overload capability.

SOLUTION

The 1 MW pilot plant in Daesan Korea produces renewable electricity from unclean hydrogen and sends it back to the Korean power grid to be used for home and industry. Hydrogenics needed a company that offered advanced quality critical monitoring system and LDetek delivered with its turnkey solution cabinet system. The MultiDetek 2 checks the level of purity to ensure no contaminants in the hydrogen stream being delivered to the PEM fuel cell. LDetek provided a full system including cabinet, LDGSS (streams selector) and carrier gas purifier. As a company that values safety and reliability, Hydrogenics only chooses best-in-class partners, making LDetek an ideal choice to do business with.

INSTALLATION PICTURES



WWW.HYDROGENICS.COM

等离子体发射检测器在检测高纯氦气中 微量氖气的应用*

胡树国, 张体强

(中国计量科学研究院, 北京 100029)

摘要 采用等离子体发射检测器 (PED) 和氦离子放电检测器 (DID) 对重量法制备的氦气中微量氖气进行了检测, 对比了微量氖气在两种检测器上的灵敏度和重复性。结果显示, PED 对氖气的检测灵敏度较高, 氖气含量在 $0.03 \sim 0.3 \mu\text{mol/mol}$ 范围与响应值呈良好的线性关系, $r^2=1.000$, 检测限小于 1 nmol/mol , 测定结果的相对偏差小于 2% ($n=6$)。利用大气压离子质谱仪对检测限测试结果进行了验证。采用等离子体发射检测器检测氦气中微量氖气的方法, 可以降低微量氖气标准物质的定值不确定度, 为研制高准确度微量氖气标准物质奠定基础。

关键词 等离子体发射检测器; 高纯氦气; 微量氖气; 检测限; 气体标准物质

中图分类号: O657.3

文献标识码: A

文章编号: 1008-6145(2016)01-0078-03

Application of Plasma Emission Detector in Determination of Trace Neon in High Purity Helium

Hu Shuguo, Zhang Tiqiang

(National Institute of Metrology, Beijing 100029, China)

Abstract Trace neon in helium prepared by gravimetric method was determined by gas chromatography with plasma emission detector and discharge ionization detector. Sensitivity and repeatability of trace neon in different detector were compared. The results showed that the detection sensitivity of PED was higher, the linear range of neon was $0.03 \sim 0.3 \mu\text{mol/mol}$, the correlation coefficients (r^2) was 1.000, the detection limit was less than 1 nmol/mol , the RSD was less than 2% ($n=6$). By comparing the data of atmosphere pressure ion mass spectrometry, the reliability of the results was verified. The determination of trace neon in helium by plasma emission detector may decrease the uncertainty of neon reference material, which lays the foundation of development of high precision trace neon standard material.

Keywords plasma emission detector; high purity helium; trace neon; detection limit; gas standard material

氦气是主要的工业气体品种之一, 被广泛应用于军工、科研、石化、制冷、医疗、半导体、管道检漏、超导实验、金属制造、深海潜水、高精度焊接、光电子产品生产等。在实验室中, 氦气主要作为气相色谱仪、气体质谱仪等仪器的载气使用。在氦气应用领域中, 使用者对其纯度有着较高的要求, 氦气中杂质检测是判断氦气纯度的重要手段。国标 GB/T 4844-2011^[1] 中给出了 4 种不同纯度氦气中氖气、氢气、氩气、氧气、氮气、一氧化碳、二氧化碳、甲烷和水分共 9 种杂质含量的指标, 并建议除水分外, 其它 8 种组分可以利用氦放电离子化色谱法测定。在这 8 种杂质中, 氖气是比较特殊的一种气体, 通常不能通过纯化方法去除; 此外, 氖气电离能较高, 在氦离子放电色谱仪上的响应值低, 检测灵敏度不高, 在有些检测器仪器上, 甚至没有响应信号。

在研制高准确度氦气中微量氖气标准物质过程中, 需要准确定量高纯氦气中微量氖气, 氖气的检测限及其不确定度对标准物质的定值有很大影响, 因此选择合适的仪器定量检测氖气以及确定仪器的检测限是研制标准物质的关键。

蔡体杰^[2] 等对微量氖气的检测方法进行了总结。笔者实验室有两台不同原理的放电离子化色谱仪, 一台为放电离子化色谱仪 (检测器为氦离子放电检测器, DID), 另一台为脉冲放电氦离子化色谱仪 (检测器为脉冲放电氦离子检测器, PDHID)。配有 DID^[3] 或 PDHID^[4-5] 检测器的气相色谱仪主要用于高纯气体中杂质的分析和检测, 在标准物质研制及气体分析等领域有着广泛应用。通过使用两台

* 国家支撑计划项目 (2013BAK10B03)

联系人: 胡树国; E-mail: hushg@nm.ac.cn

收稿日期: 2015-10-20

色谱仪对微量氖气的检测发现,配有 DID 的色谱仪可以检测到高纯氦气中的氖气,而配有 PDHID 的色谱仪对氖气没有响应,这与文献中报道一致^[3]。除了上述常见的 DID 外,目前新购置了一台配有等离子体发射检测器 (PED) 的气相色谱仪。PED 是一种新型色谱检测器,其原理是在检测器的石英小池周围加以高频、高强度的电磁场,在高频、高强电磁场的作用下载气和杂质气体被电离为等离子体,等离子体具有较高的能量,样品进入检测器的石英小池之后,被等离子体电离并发出不同波长的光,主组分发出的光不能通过被检测组分的滤光片,这样就避免了主组分的干扰,光信号经光电二极管转化为电信号,因此 PED 检测器是一种选择性光谱检测器^[6]。

笔者利用配有 DID 和 PED 的气相色谱仪对重量法制备的 3 瓶氦气中微量氖气混合气进行了分析比较,结果发现 PED 对氖气的检测灵敏度较高。利用 3 瓶混合气的重量值和在 PED 上的响应值进行线性拟合,得到了微量氖气在 PED 上的检出限,并计算出检出限的不确定度。

1 实验部分

1.1 主要仪器与气体

氦放电离子色谱仪:592 型,美国 GOW-MAC 公司;

等离子体发射色谱仪: MULTIDETEK2 型,美国 LDetek 公司;

大气压离子质谱仪:APIX 8 Q 型,美国 Thermo Fisher 公司;

高纯氦气:纯度大于 99.999%,北京氦普北分工业气体有限公司;

高纯氖气:纯度大于 99.999%,北京首钢氧气厂;

氦气中微量氖气混合气体:氖气含量分别为 0.276 $\mu\text{mol/mol}$ (L0054012[#] 瓶), 0.101 $\mu\text{mol/mol}$ (305593[#] 瓶), 0.028 $\mu\text{mol/mol}$ (L0054174[#] 瓶)。

1.2 仪器工作条件

1.2.1 DID 色谱仪

色谱柱: 13X 分子筛柱 (3 m \times 3.2 mm); 柱温: 80 $^{\circ}\text{C}$; 检测器温度: 室温; 放电电压: 300 V。

1.2.2 PED 色谱仪

色谱柱: Argotek 柱 (2.4 m \times 3.2 mm); 柱温: 45 $^{\circ}\text{C}$; 检测器温度: 60 $^{\circ}\text{C}$; 增益值: 10。

1.2.3 大气压离子质谱仪

选择离子: 20; 放电电压: 1 200 V。

2 结果与讨论

2.1 氖气在 DID 和 FED 上响应比试验

选用同一瓶高纯氦气根据重量法原理^[7]利用微量转移技术^[8-9]制备 3 瓶氦气中氖气, 瓶号为 L0054174[#] (0.028 $\mu\text{mol/mol}$), 305593[#] (0.101 $\mu\text{mol/mol}$), L0054012[#] (0.276 $\mu\text{mol/mol}$)。分别采用 DID 检测器和 PED 检测器对稀释气 (高纯氦) 和制备的 3 瓶混合气进行分析, 结果见表 1。

表 1 稀释气和 3 瓶混合气中氖气在 DID 和 PED 上的响应 ($n=6$)

| 气体 | DID | | PED | |
|---------------------------|------------------------|-----------|------------------------|-----------|
| | 响应值/ (mV \cdot s) | RSD/ % | 响应值/ (mV \cdot s) | RSD/ % |
| 稀释气 (高纯氦气) | 0 | — | 0 | — |
| L0054174 [#] 混合气 | 0 | — | 381.8 | 2.0 |
| 305593 [#] 混合气 | 158.1 | 4 | 1 390.2 | 0.5 |
| L0054012 [#] 混合气 | 347.5 | 3 | 3 839.6 | 0.5 |

由表 1 可知, 对于 0.1 $\mu\text{mol/mol}$ 以上的微量氖气在 DID 和 PED 检测器上均有响应; 当氖气含量下降至 0.03 $\mu\text{mol/mol}$ 时, 在 DID 检测器上没有响应, 而在 PED 检测器上响应值仍较高, 如图 1 所示。

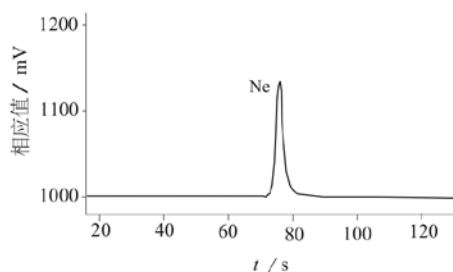


图 1 含量为 0.03 $\mu\text{mol/mol}$ 氖气在 PED 上的响应

2.2 线性方程

对于 DID 检测器, 由于低含量氖气混合气在 DID 上没有响应, 无法获得线性方程。利用表 1 中 PED 对混合气体的检测数据, 以氖气的含量 (X , $\mu\text{mol/mol}$) 为横坐标, 以响应值 (Y) 为纵坐标进行线性回归, 得回归方程为 $Y=13\,952.3419X-13.029\,0$, $r^2=1.000$ 。

2.3 检测器的重复性

从表 1 可以看出, 随着氦气中氖气含量的降低, 氖气在 DID 和 PED 上响应值的相对标准偏差逐渐增大。氖气在 DID 检测器上响应值的相对标准偏差明显大于 PED 检测器。原因可能是 DID 检测器需要通过提高放电电压才能实现检测氖气, 而提高放电电压将增大基线噪声; 另一方面, 低含量的氖气在 DID 上的响应值较小, 从而导致重复性变差。PED 检测器具有较高的灵敏度, 氖气含量大于 0.1 $\mu\text{mol/mol}$ 时, 其 6 次进样测定结果的相对标准偏

差为0.5%;氦气含量低于 $0.1\ \mu\text{mol/mol}$ 时,相对标准偏差为2.0%。

2.4 PED检测限的确定

用于制备微量氦气混合气的稀释气(高纯氦气)在PED检测器上没有响应,说明稀释气中的氦气含量低于PED仪器的检测限。当仪器响应值为零($Y=0$)时,可通过拟合的方程计算出 X 值为 $0.93\ \text{nmol/mol}$,由此推断氦气在PED上的检测限为 $1\ \text{nmol/mol}$ 左右。根据文献方法^[10]计算得检测限的标准不确定度为 $0.51\ \text{nmol/mol}$ 。

为进一步验证数据的准确性和可靠性,利用高灵敏度高的气压离子质谱仪^[11-12]对结果进行了核验,测试结果显示,稀释气中氦气杂质含量小于 $1\ \text{nmol/mol}$,这与PED检测器上得出的结论相一致。根据PED测试结果,可以给出用于制备3瓶混合气体的稀释气中氦气的含量小于 $1\ \text{nmol/mol}$,考虑到还有其它因素的影响,将PED对氦气检测限的不确定度扩大为 $1\ \text{nmol/mol}$ 。

假设研制 $1\ \mu\text{mol/mol}$ 的微量氦气标准物质,如果以DID色谱仪对稀释气中的氦气进行检测,以检测限 $30\ \text{nmol/mol}$ 作为不确定度,则由制备引入的相对不确定度至少为3%;而以PED检测限 $1\ \text{nmol/mol}$ 作为不确定度,引入的相对不确定度为0.1%。由此可见,氦气的检测限对于研制高准确度氦气中微量氦气标准物质非常重要。

3 结语

利用等离子发射检测器PED对3瓶重量法制

备的氦气中微量氦气混合气进行了检测,检测灵敏度较高。通过线性拟合,得出了PED对氦气的检测限及检测限的不确定度,为研制高准确度的微量氦气标准物质奠定了基础。配有PED新型检测器的气相色谱仪,在检测微量氦气方面与常规仪器相比具有较高的灵敏度,是目前检测氦气中微量氦气的理想仪器。

参考文献

- [1] GB/T 4844-2011 纯氦、高纯氦和超纯氦[S].
- [2] 蔡体杰,刘雅珍,张杨,等.关于氦离子化检测器气相色谱法分析氦中微量氦[J].低温与特气,2012(4): 85-91.
- [3] 李富勇,郭东方,金伟,等.气相色谱用氦等离子体离子化检测器研究进展[J].分析科学学报,2012(2): 279-284.
- [4] 胡树国,金美兰,盖良京.利用脉冲放电氦电离色谱检测高纯气体中微量无机杂质[J].计量技术,2007(6): 36-38.
- [5] 胡树国,韩桥,李春瑛.高纯甲烷纯气体中的杂质分析——CCQM K66国际比对[J].化学分析计量,2009,18(6): 67-69.
- [6] 黎文字,张晓红.等离子发射检测器(PED)及相关技术在气相色谱中的应用[J].低温与特气,2014,32(3): 48-54.
- [7] GB/T 5274-2008 气体分析校准用混合气体的制备称量法[S].
- [8] 胡树国,李佳.利用气体微量转移技术制备低含量R12气体标准物质[J].化学分析计量,2012(6): 67-69.
- [9] 胡树国,王德发,王哲.微量气体转移技术在重量法制备各气体标准物质中的应用[J].计量学报,2013(1): 72-75.
- [10] 刘渊,建华,王茂仁.直线拟合中的不确定度计算[J].物理与工程,2009,19(2): 25-27.
- [11] 张体强,胡树国,韩桥.大气压电离质谱及其用于超高纯气体分析研究进展[J].岩矿测试,2014,33(6): 775-781.
- [12] 张体强,胡树国,韩桥.大气压电离质谱在超高纯气体纯度分析中的应用[J].分析测试学报,2014,33(7): 854-858.

用技术革新破解食品安全难题

80后小伙陈建军开发一种试剂,在3~5 min内快速检测出食品中的农药、兽药、毒素、重金属含量,甚至能检测是否转基因。

食品安全大于天。蔬菜农残超标、肉里含有瘦肉精、奶里有三聚氰胺一波又一波的问题,让人觉得吃啥也不放心。与之相对应的,目前食品的国标检测方法成本高、周期长,基层食品安全监管部门很难用上。

陈建军从代理产品做起,2011年某知名火腿肠品牌被检出含有瘦肉精,引起轩然大波。瘦肉精其实主要有3种,使用最多的就是盐酸克仑特罗,其次是沙丁胺醇。陈建军说,他代理的产品检测速度快,价格适中,中标了沙丁胺醇检测项目,这次中标当年让他销售数百万元。但遗憾的是这个产品没有中标盐酸克仑特罗检测,原因是速度不够快。企业把猪肉放在生产线上,每次只停留1 min,当时只有一家企业的产品能1 min出结果。

2013年起,陈建军开始和华中农业大学专家合作开发转基因检测剂。由于检测准确度高、价格只有进口产品的60%,产品很快打开市场。不仅农业部门需要,一些大米加工企业也需要用它来鉴别原料米是否混有转基因。随后又与湖北一些高校开展产学研合作,研发出30多种自有品牌的检测试剂盒。

个人消费市场是陈建军的下一个目标。陈建军说:“我们刚刚研发出一种黄曲霉毒素的检测产品,如果投入市场,老百姓自己就可以在家里检测牛奶里的黄曲霉毒素是否超标,甚至可以检测饭馆里是不是用了地沟油”。黄曲霉毒素是一种食物霉变就可产生的致癌物质,变苦的坏瓜子、花生,里面都含有它。奶牛如果吃了霉变的饲料,牛奶里也可能残留黄曲霉毒素。

陈建军说,虽然我们不是权威的食品安全状况发布机构,但我们希望用自己的产品,帮助大家吃到放心的食品。

(人民日报)


PETROCHEMICAL
 FORMALDEHYDE
 ETHANE
 NITRIC OXIDE
 I-BUTENE
 HYDROGEN
 XENON
 NITROGEN
 CARBON MONOXIDE
 DIFLUOROETHANE
 METHYL CHLORIDE
 NITRIC DIOXIDE
 ARGON
 PROpane
 KRYPTON
 OXYGEN
 HELIUM
 NEON
 CARBON DIOXIDE
 N-BUTANE
 ETHYLENE
 TETRAFLUOROMETHANE
 ACETYLENE
 ISObutane
 ACETONE
 PHOSPHINE
 SILANE
 METHANE
 PROPYLENE
 SULFUR DIOXIDE
 HYDROGEN SULFIDE
 CARBONYL SULFIDE
 ARSINE
 ACETALDEHYDE
 AMMONIA
 SAFETY
 FOOD
 ENVIRONMENT
 MEDICINE
 INDUSTRIAL GASES
 GREENHOUSE GASES
 PHARMACEUTICAL
 HEALTH

IMPURITIES


Chromatograms #

| | |
|--|---|
| 1,3-Butadiene (1,3-C ₄ H ₆) | 73 |
| Acetaldehyde | 1-2-3-4-76 |
| Acetic acid | 5 |
| Acetylene (C ₂ H ₂) | 6-7-8-9-10-11-23-69-73-78-79-83-110-114 |
| Ammonia | 13-90 |
| Argon (AR) | 14-15-16-17-18-19-71-72-77-80-85-87-97-107-109-113 |
| Arsine | 20-21-22 |
| Benzene(C ₆ H ₆) | 76 |
| Butadiene (C ₄ H ₆) | 23 |
| Butane (C ₄ H ₁₀) | 23 |
| Butylene | 6-7-8 |
| Butylene (C ₄ H ₈) | 23 |
| c-2-Butane (C-2-C ₄ H ₈) | 73 |
| Carbon dioxide (CO ₂) | 1-24-25-26-27-64-65-30-19-31-32-33-23-34-35-36-37-66-67-71-73-74-75-78-79-80-81-82-83-84-90-96-99-100-105-111-115 |
| Carbon monoxide (CO) | 6-25-38-30-19-39-31-40-32-33-41-34-35-36-37-42-66-67-71-73-76-78-79-80-81-82-83-84-88-96-100-105-111-115 |
| Carbonyl sulfide | 5-43-44-45-46 |
| Ethane (C ₂ H ₆) | 6-7-8-9-10-23-69-73-78-79-110-114 |
| Ethanol (C ₂ H ₆ O) | 74 |
| Ethylene (C ₂ H ₄) | 6-7-8-9-10-23-69-73-78-79-83-110-114 |
| Fluorine | 87 |
| Formaldehyde | 3-4 |
| Formic acid | 5 |
| Freon11 | 83 |
| Freon113 | 83 |
| Freon12 | 83 |
| Freon13 | 83 |
| Freon22 | 83 |
| Helium | 38-87-91 |
| Hydrogen (H ₂) | 6-25-18-38-30-58-19-39-32-33-34-35-36-37-66-67-78-80-81-82-91-95-105-111-116 |
| Hydrogen sulfide | 5-43-44-45-46 |
| iso-Butane (i-C ₄ H ₁₀) | 73 |
| iso-Butylene (i-C ₄ H ₈) | 73 |
| iso-Pentane (i-C ₅ H ₁₂) | 73 |
| Krypton | 18-47-70-72-77-80-85-87 |
| Methane (CH ₄) | 6-25-7-10-26-27-48-38-30-58-19-39-31-40-32-49-33-19-23-34-35-36-37-66-67-68-69-71-73-75-78-79-80-82-83-88-95-103-105-111-116 |
| n-Pentane (N-C ₅ H ₁₂) | 73 |
| Neon (NE) | 18-19-77-85-112 |
| Nitrogen (N ₂) | 17-24-6-47-52-53-56-57-38-30-58-19-39-31-40-33-41-34-35-36-37-42-66-67-71-72-73-74-76-78-79-80-81-82-86-91-94-101-105-106-111-117 |
| Nitrous oxide (N ₂ O) | 11-27-48-54-49-23-5-75-81-83-106 |
| Non-methane hydrocarbons (NMHC) | 19-33-34-35-36-37-67-68-69-71-80-83-93-102 |
| Oxygen (O ₂) | 6-25-56-57-30-38-58-19-39-31-32-42-66-67-71-73-79-81-82-88-90-95-103-107-111-116 |
| Phosphine | 59-60-61 |
| Propane | 6-7-8-9-10-23 |
| Propylene | 6-7-8-9-10-23 |
| Sulfur hexafluoride (SF ₆) | 42-62-75-81-92-108 |
| t-2-butane (T-2-C ₄ H ₈) | 73 |
| Tetrafluoromethane (CF ₄) | 42-63-81-82-98-99-108 |
| Tetrahydrothiophene | 89 |
| Trichloroethane | 83 |
| Trichloroethylene | 83 |
| Water | 1-8-13-20-21-3-44-45-61-64-65 |
| Xenon (XE) | 70-77-80-85-88-104 |


CHROMATOGRAM #1

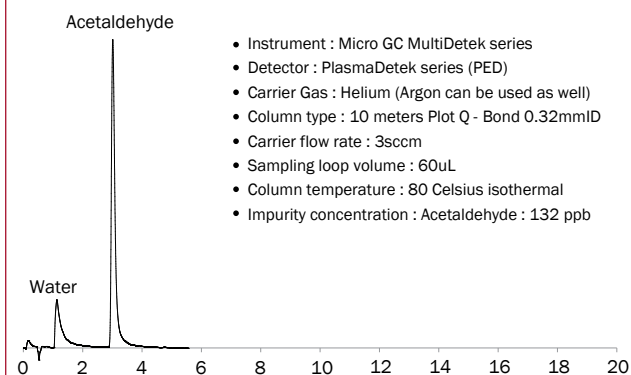


CHROMATOGRAM #2

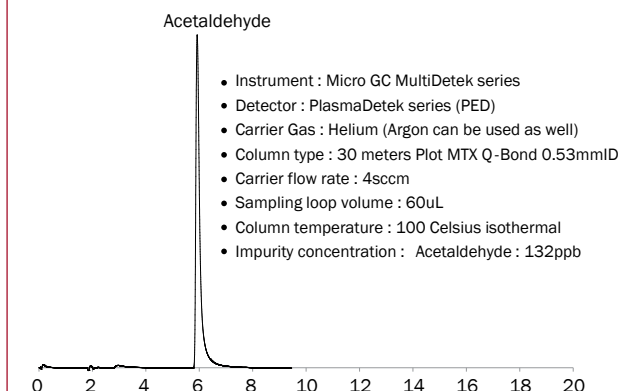


CHROMATOGRAM #3

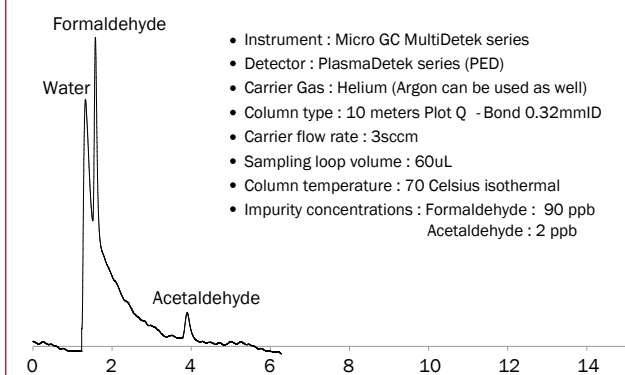


CHROMATOGRAM #4

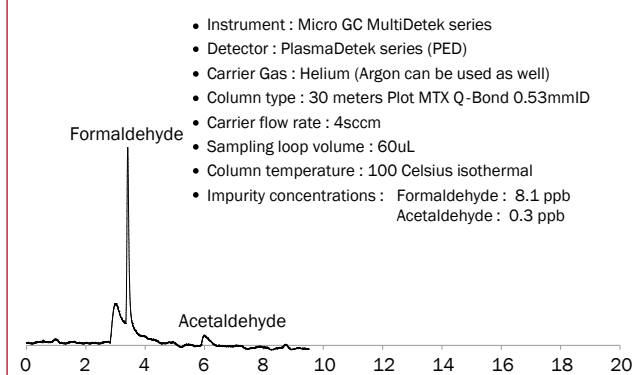


CHROMATOGRAM #5

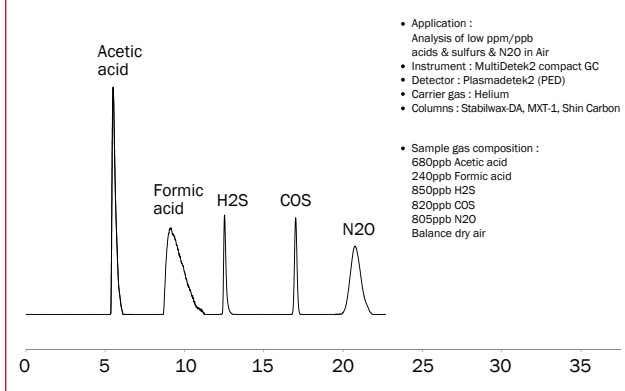


CHROMATOGRAM #6

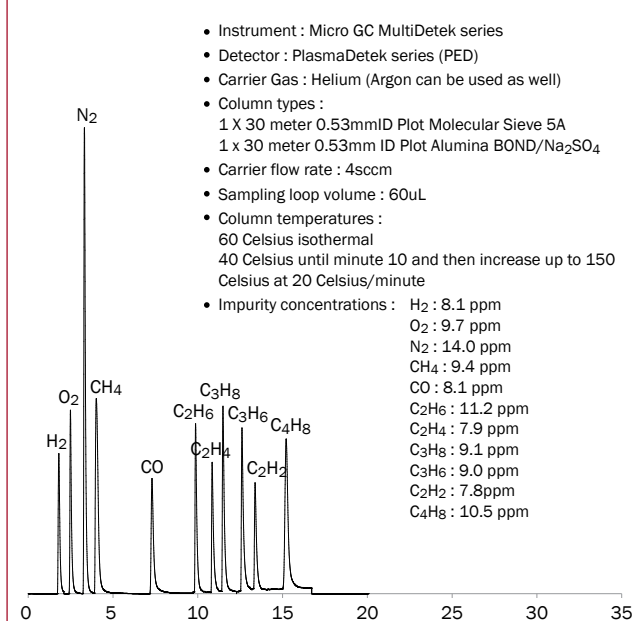


CHROMATOGRAM #7

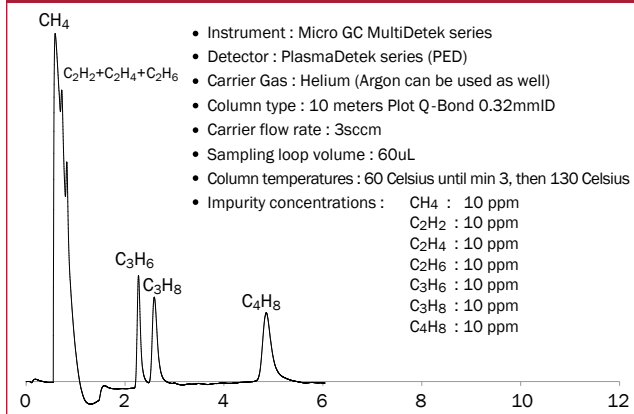


CHROMATOGRAM #8

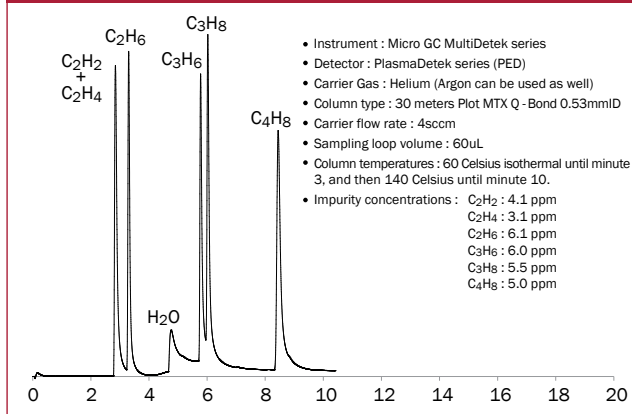


CHROMATOGRAM #9

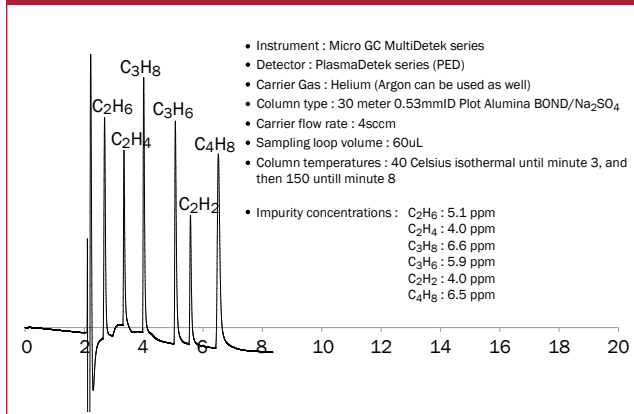


CHROMATOGRAM #10

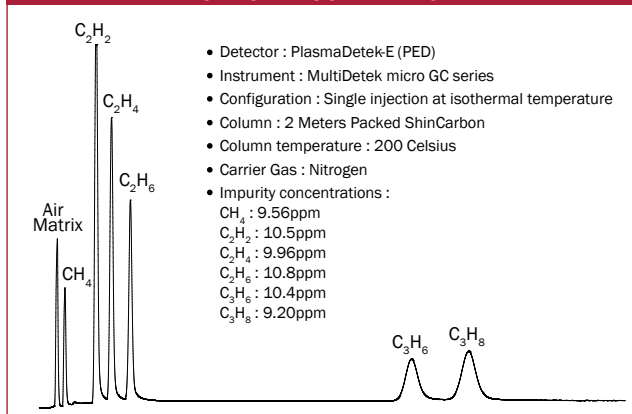


CHROMATOGRAM #11

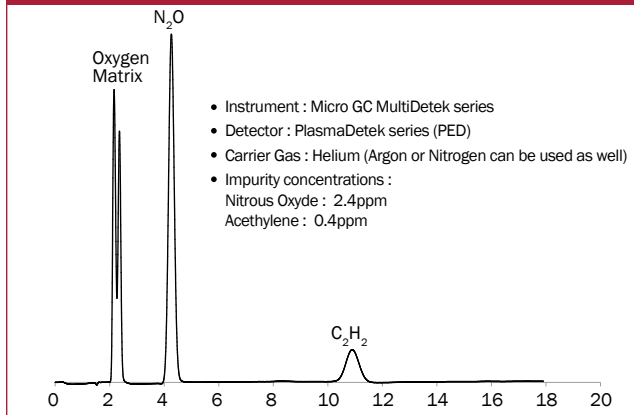


CHROMATOGRAM #13

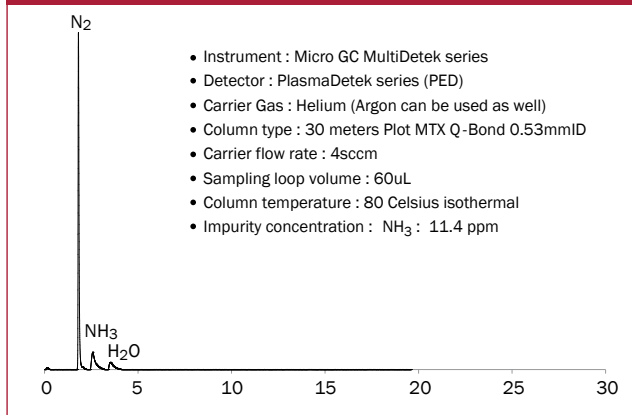


CHROMATOGRAM #14

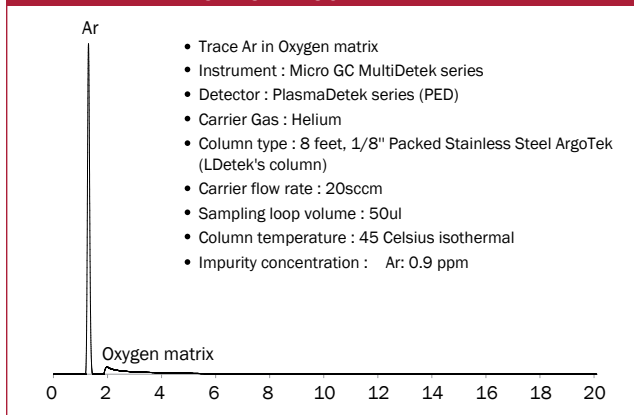


CHROMATOGRAM #15

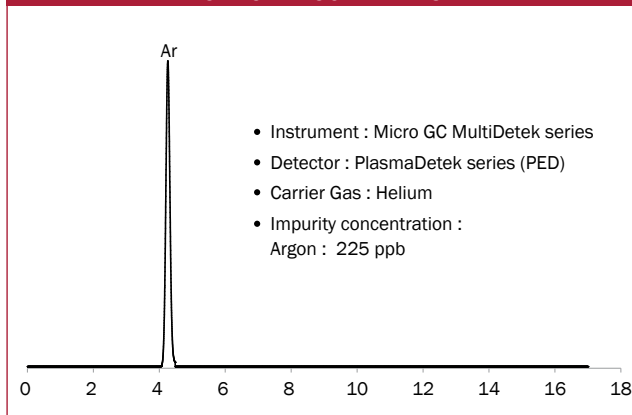


CHROMATOGRAM #16

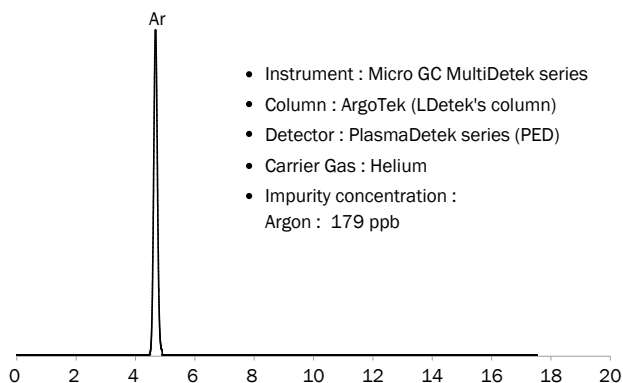


CHROMATOGRAM #17

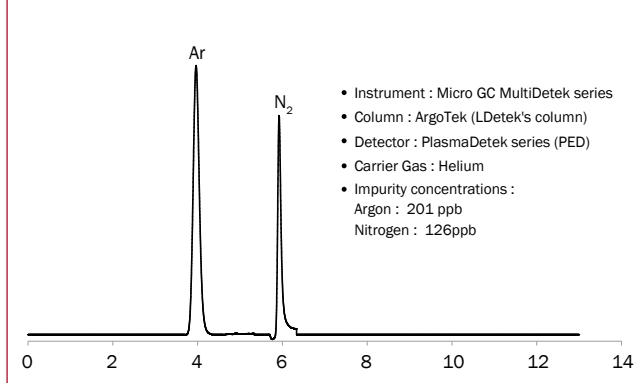


CHROMATOGRAM #18

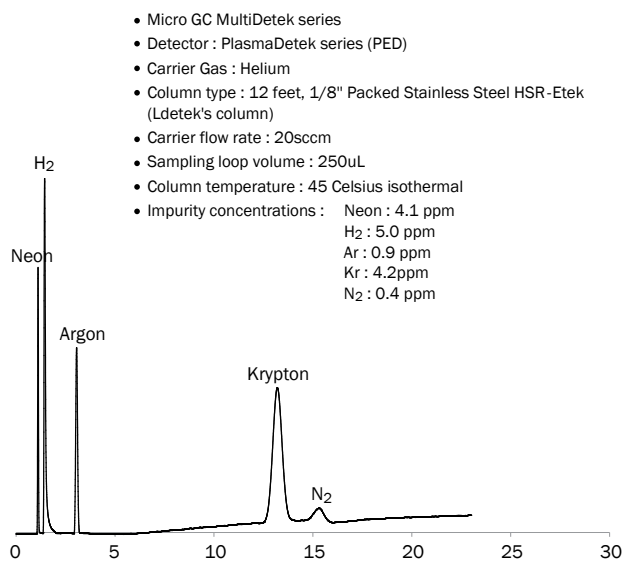


CHROMATOGRAM #19

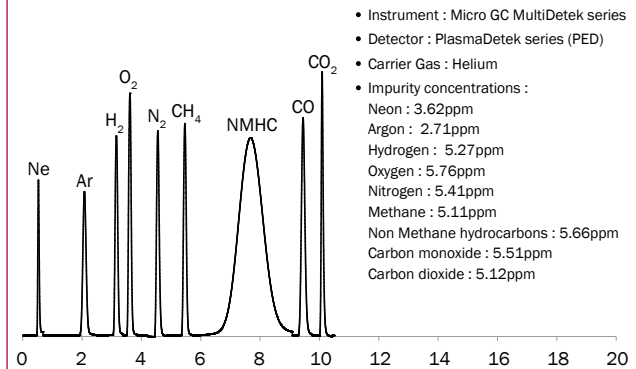


CHROMATOGRAM #21

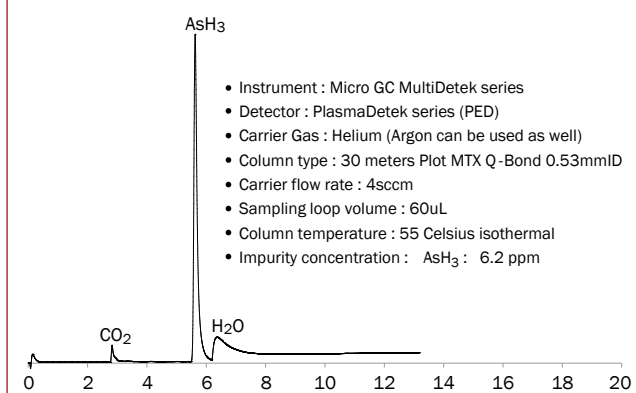


CHROMATOGRAM #20

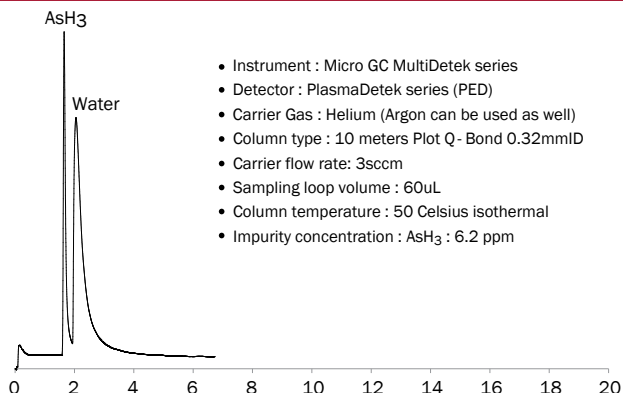


CHROMATOGRAM #22

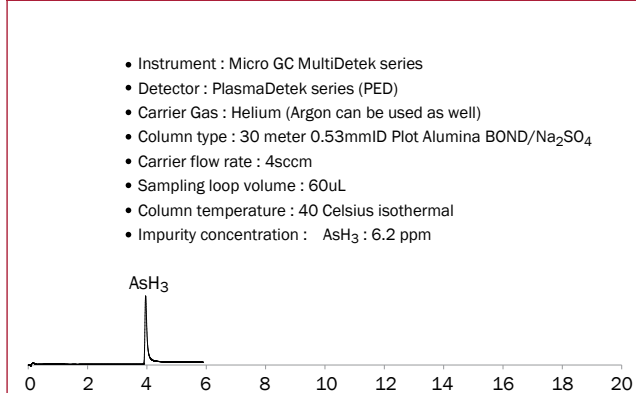


CHROMATOGRAM #23

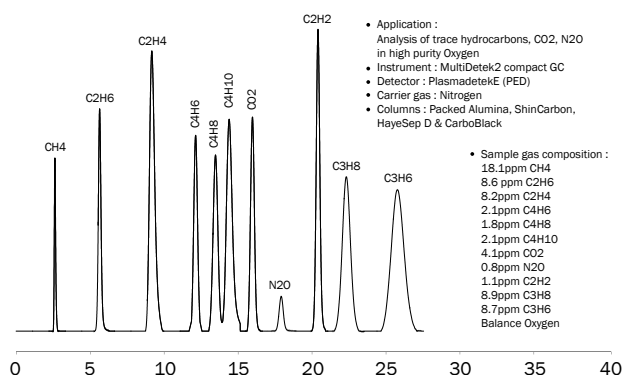


CHROMATOGRAM #24

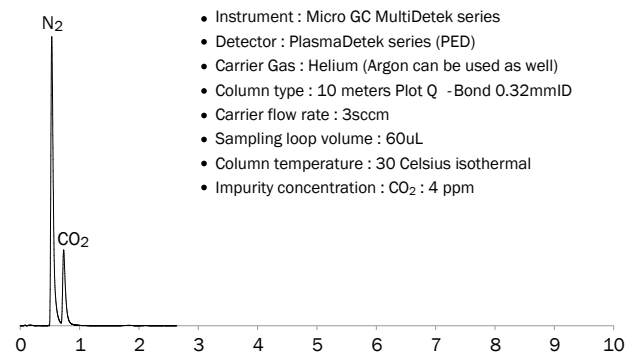


CHROMATOGRAM #25

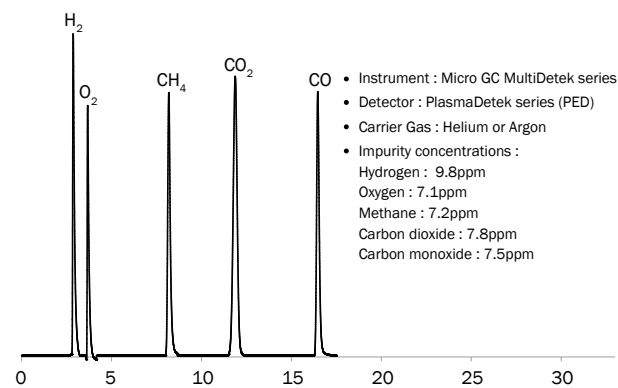


CHROMATOGRAM #26

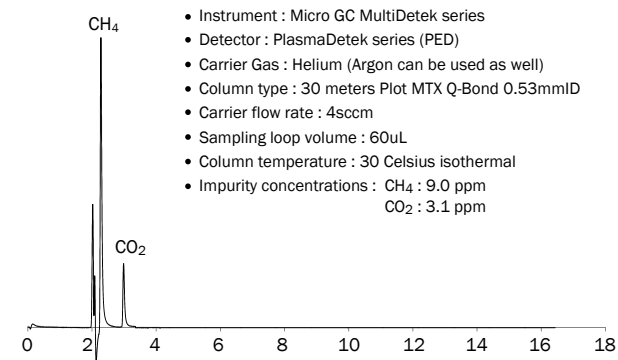


CHROMATOGRAM #27

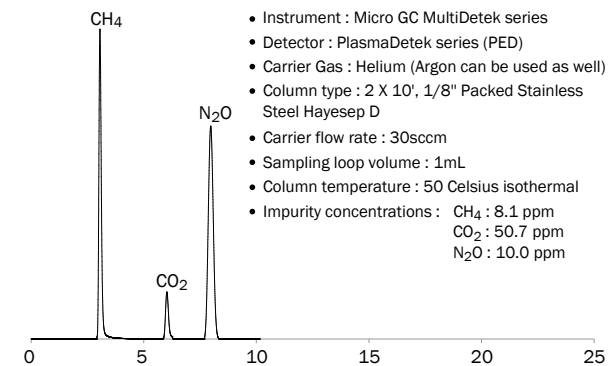


CHROMATOGRAM #30

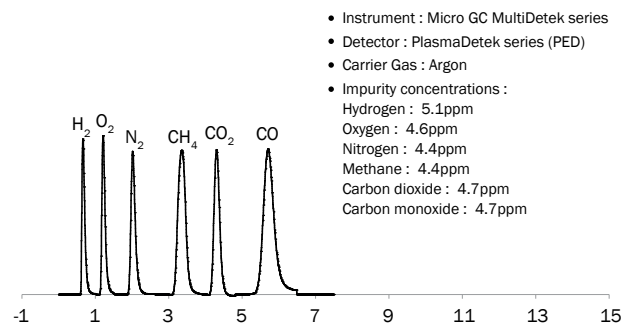

CHROMATOGRAM #31

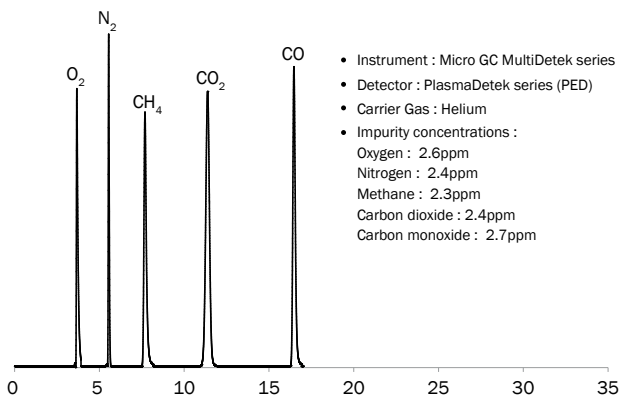


CHROMATOGRAM #32

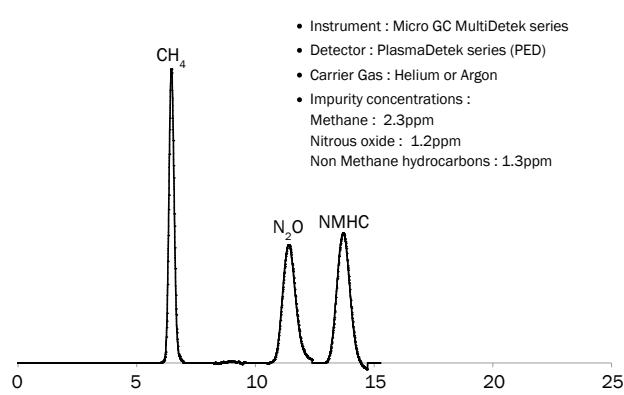


CHROMATOGRAM #33

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Argon
- Impurity concentrations :
Nitrogen : 0.9ppm
Carbon monoxide : 0.7ppm




CHROMATOGRAM #34

- Application : Analysis of low ppb H₂-NMHC-CH₄-N₂-CO₂-CO in electronic grade gas Oxygen
- Instrument : MultiDetek2 compact GC
- Detector : Plasmadetek-E (PED)
- Carrier gas : Helium
- Columns: Packed
- Sample gas composition :
H₂ : 3.1ppb
NMHC : 3.2ppb
CH₄ : 0.9ppb
N₂ : 2.1ppb
CO₂ : 2.3ppb
CO : 1.0ppb

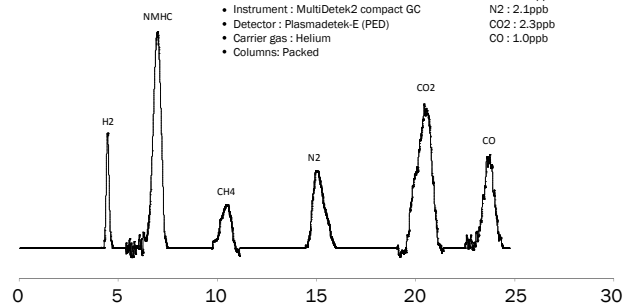


CHROMATOGRAM #35

- Application : Analysis of low ppb H₂-NMHC-CH₄-N₂-CO₂-CO in electronic grade gas Oxygen
- Instrument : MultiDetek2 compact GC
- Detector : Plasmadetek-E (PED)
- Carrier gas : Helium
- Columns: Packed
- Sample gas composition :
H₂= 7.5ppb
NMHC : 9.1ppb
CH₄= 6.1ppb
N₂= 7.2 ppb
CO₂=5.9ppb
CO= 4.1ppb

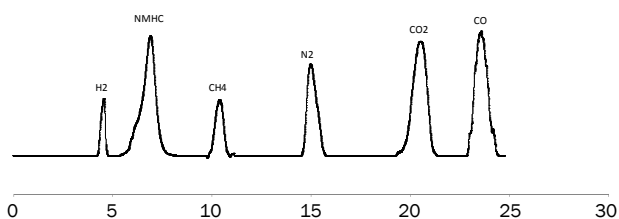


CHROMATOGRAM #36

- Application : Analysis of low ppb H₂-NMHC-CH₄-N₂-CO₂-CO in electronic grade gas Oxygen
- Instrument : MultiDetek2 compact GC
- Detector : Plasmadetek-E (PED)
- Carrier gas : Helium
- Columns: Packed
- Sample gas composition :
H₂ = 38.2ppb
NMHC : 25.2ppb
CH₄ = 36.8 ppb
N₂ = 36.9 ppb
CO₂= 26.4 ppb
CO= 36.4 ppb

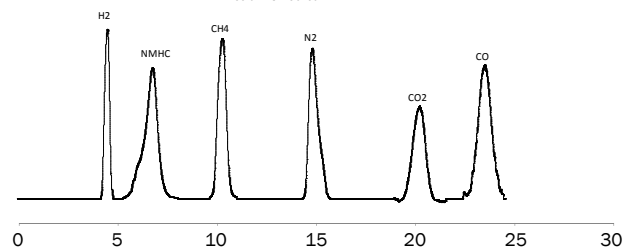


CHROMATOGRAM #37

- Application : Analysis of low ppb H₂-NMHC-CH₄-N₂-CO₂-CO in electronic grade gas Oxygen
- Instrument : MultiDetek2 compact GC
- Detector : Plasmadetek-E (PED)
- Carrier gas : Helium
- Columns: Packed
- Sample gas composition :
H₂ : 111.9ppb
NMHC : 129.2ppb
CH₄ : 87.6ppb
N₂ : 124.3ppb
CO₂ : 84.4ppb
CO : 95.6ppb

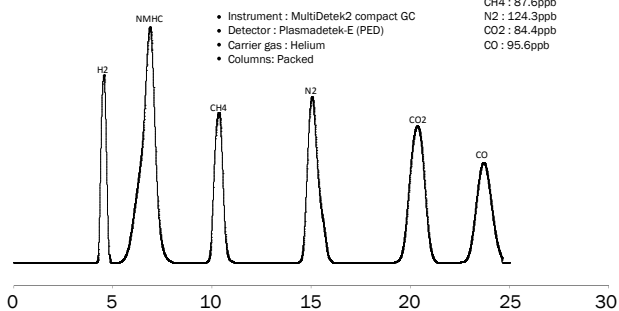


CHROMATOGRAM #38

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED) & TCD
- Carrier Gas : Helium & Argon
- Impurity concentrations :
Oxygen : 10.6ppm
Nitrogen : 10.4ppm
Methane : 10.4ppm
Carbon monoxide : 10.7ppm
Helium : 45ppm
Hydrogen : 0.5ppm

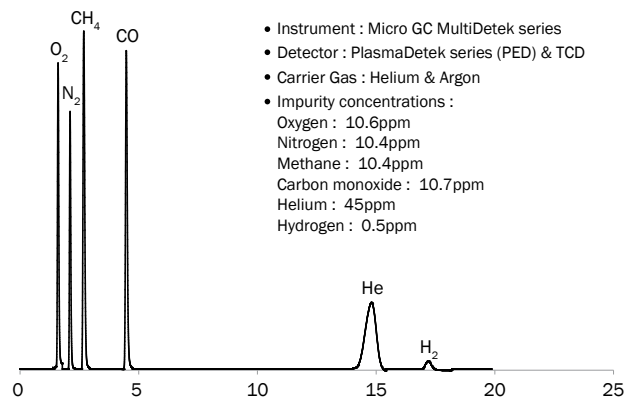


CHROMATOGRAM #39

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium
- Column type : 30 meters Plot Molecular Sieve 0.53mmID
- Carrier flow rate : 3sccm
- Sampling loop volume : 160uL
- Column temperature : 70 Celsius isothermal
- Impurity concentrations :
Hydrogen : 0.1ppm
Oxygen : 1.6ppm
Nitrogen : 1.4ppm
Methane : 1.4ppm
Carbon monoxide : 1.7ppm

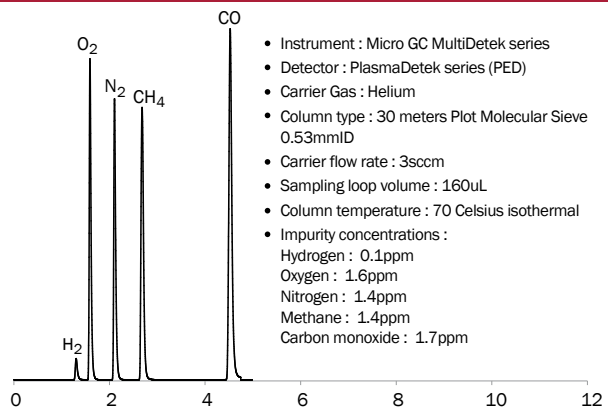


CHROMATOGRAM #40

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Argon
- Impurity concentrations :
Nitrogen : 1.1ppm
Methane : 1.2ppm
Carbon monoxide : 1.7ppm

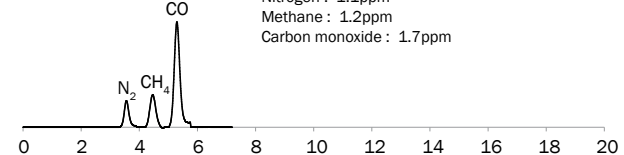


CHROMATOGRAM #41


- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium or Argon
- Impurity concentrations :
 - Methane : 5.38ppm
 - Carbon dioxide : 4.12ppm
 - Hydrogen : 4.73ppm
 - Nitrogen : 5.86ppm
 - Non Methane hydrocarbons : 5.38ppm
 - Carbon monoxide : 4.92ppm

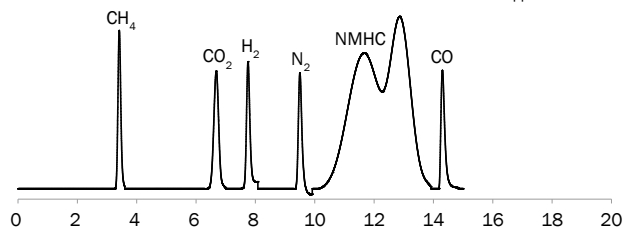**CHROMATOGRAM #42**


- Application : Sulfur hexafluoride purity (SF6)
- Instrument : MultiDetek2 GC
- Detector : Plasmadetek2
- Carrier gas : Argon or Helium
- Sample gas :
 - O2 : 1495ppm
 - N2 : 1448ppm
 - CF4 : 125ppm
 - CO : 199ppm in SF6

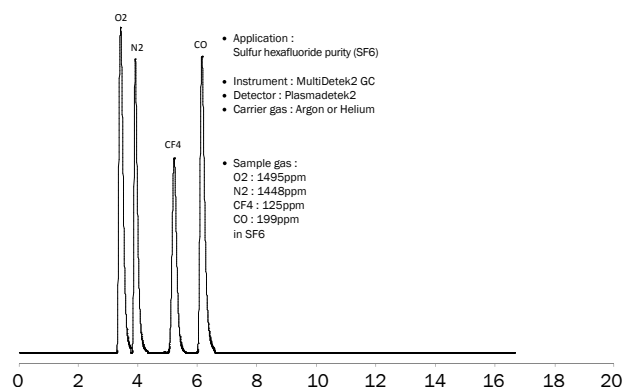**CHROMATOGRAM #43**


- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Argon (Helium can be used as well)
- Column type : 1 meter micro packed 1/16"OD Rt - XLSulfurs
- Carrier flow rate : 8sccm
- Sampling loop volume : 200uL
- Column temperature : 60 Celsius isothermal
- Impurity concentrations : H2S : 9.8 ppm, COS : 9.4 ppm

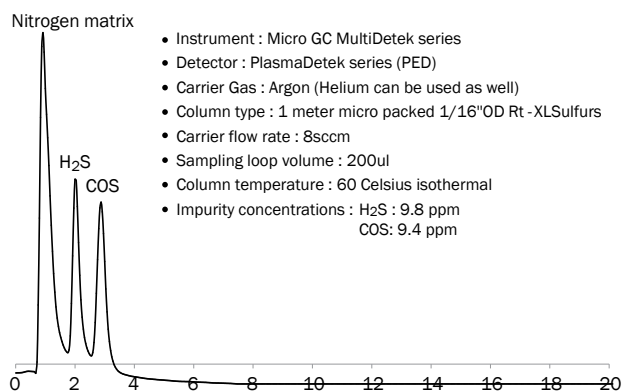**CHROMATOGRAM #44**


- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium (Argon can be used as well)
- Column type : 30 meters Plot MTX - Q-Bond 0.53mmID
- Carrier flow rate : 4sccm
- Sampling loop volume : 60uL
- Column temperature : 100 Celsius isothermal
- Impurity concentrations : H2S : 6.4 ppm, COS : 5.1 ppm

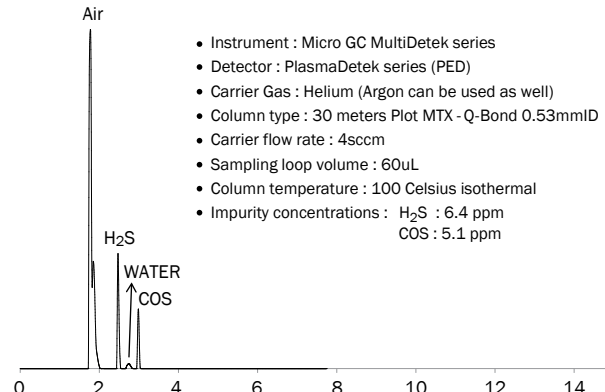**CHROMATOGRAM #45**


- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium (Argon can be used as well)
- Column type : 10 meters Plot Q - Bond 0.32mmID
- Carrier flow rate : 3sccm
- Sampling loop volume : 60uL
- Column temperature : 30 Celsius isothermal
- Impurity concentrations : H2S : 6.4 ppm, COS : 5.1 ppm

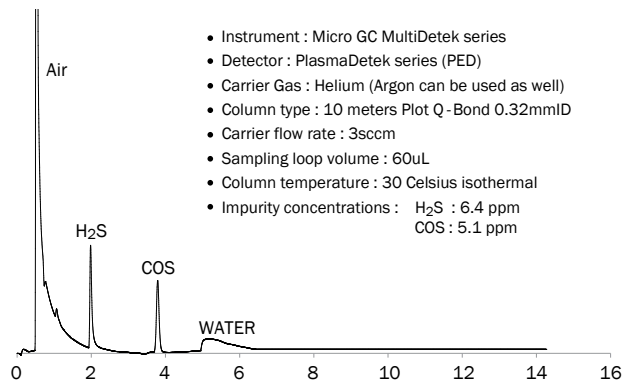**CHROMATOGRAM #47**


- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium (Argon can be used as well)
- Column type : 12 feet 1/8" Packed Stainless Steel HSR-Etek (LDetek's column)
- Carrier flow rate : 20sccm
- Sampling loop volume : 250uL
- Column temperature : 45 Celsius isothermal
- Impurity concentrations : Kr : 9.8 ppm, N2 : 10.9 ppm

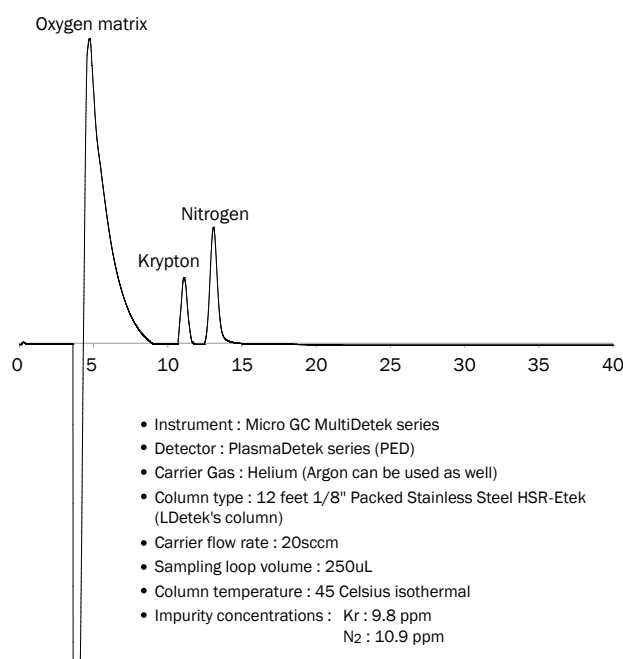**CHROMATOGRAM #46**


- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium (Argon can be used as well)
- Column type : 30 meters GasPro 0.32mmID
- Carrier flow rate : 3sccm
- Sampling loop volume : 140uL
- Impurity concentrations :
 - H2S : 1.1ppm
 - COS : 0.8ppm

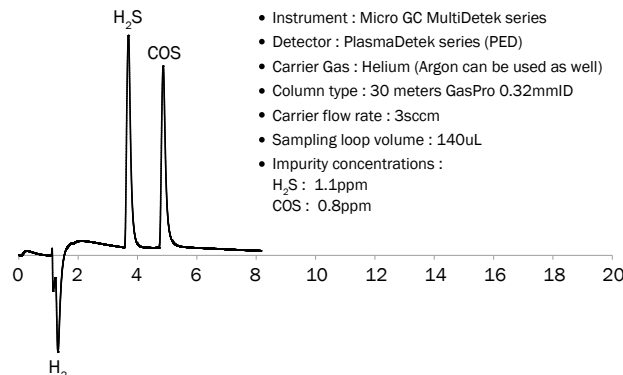


CHROMATOGRAM #48

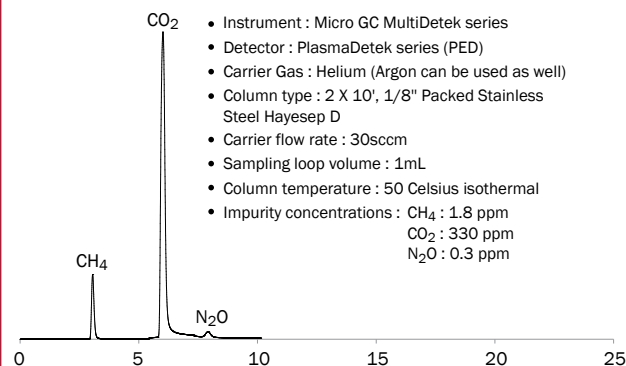


CHROMATOGRAM #49

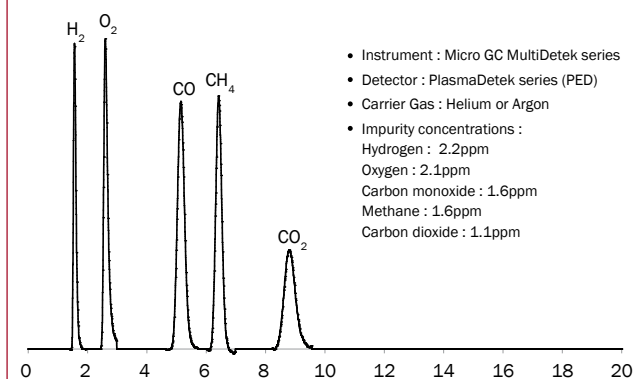


CHROMATOGRAM #52

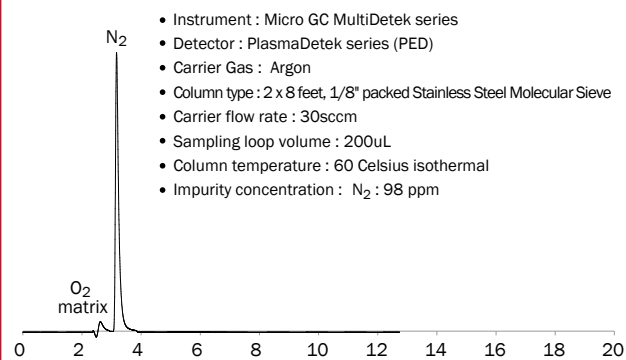


CHROMATOGRAM #53

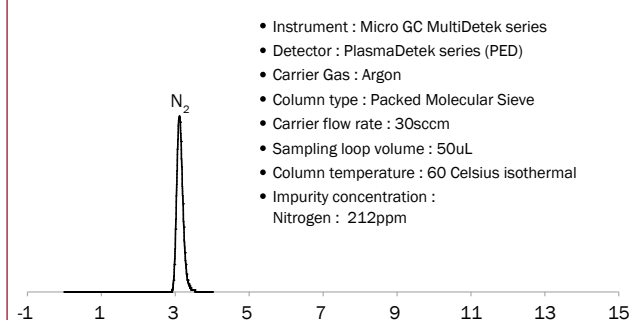


CHROMATOGRAM #54

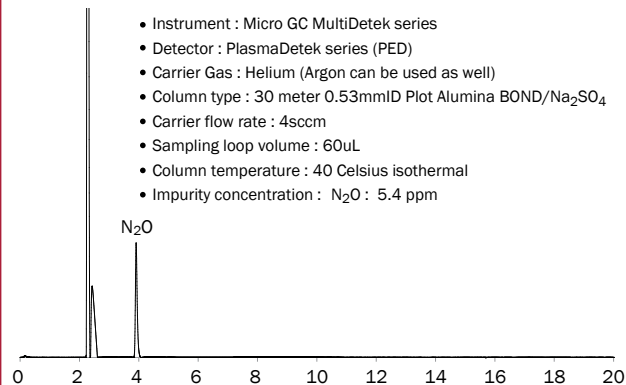


CHROMATOGRAM #56








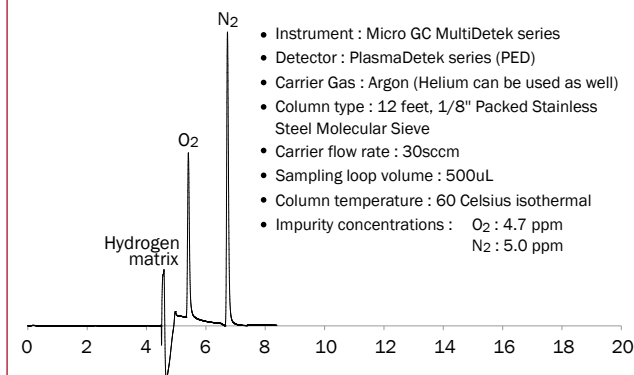


CHROMATOGRAM #57

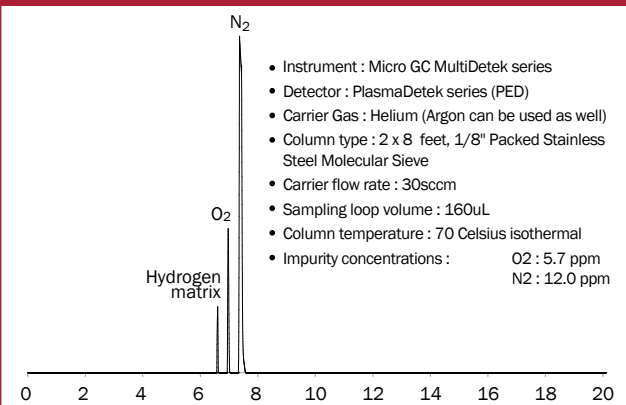


CHROMATOGRAM #58

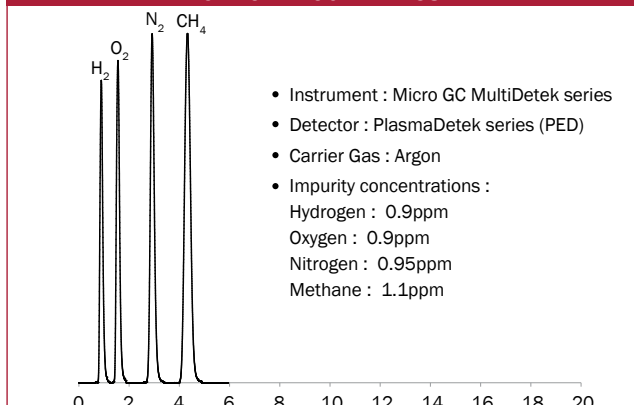


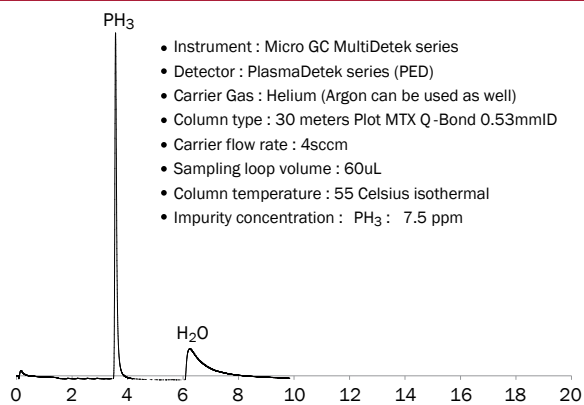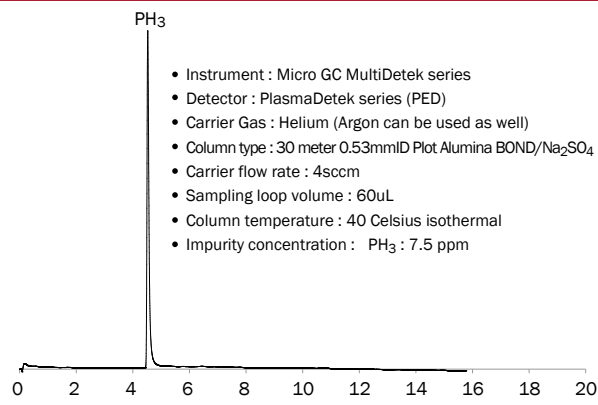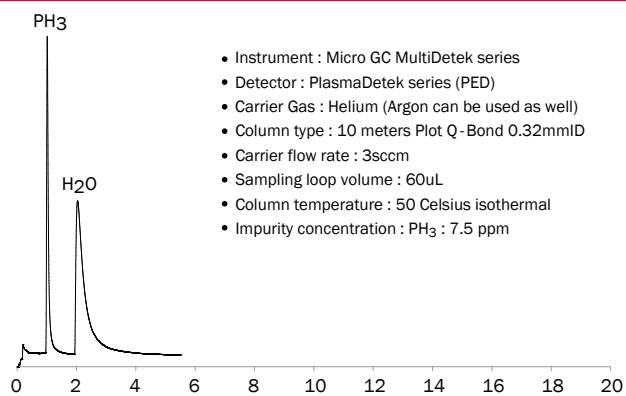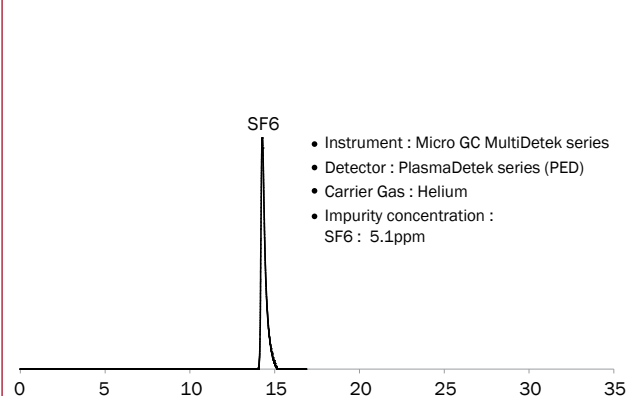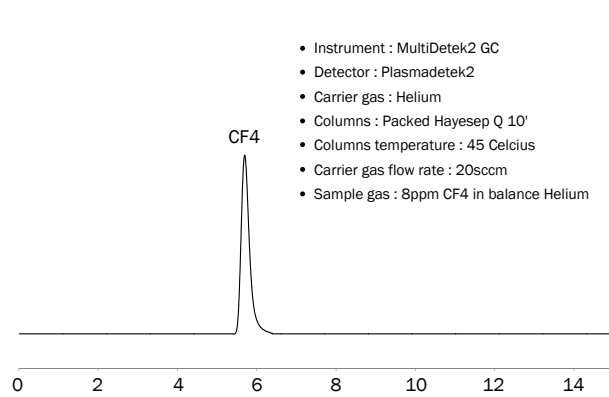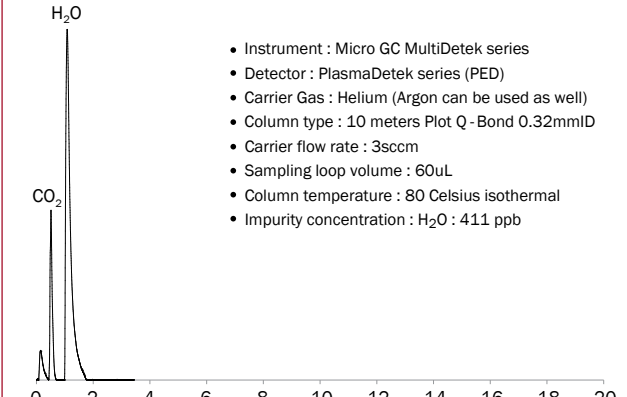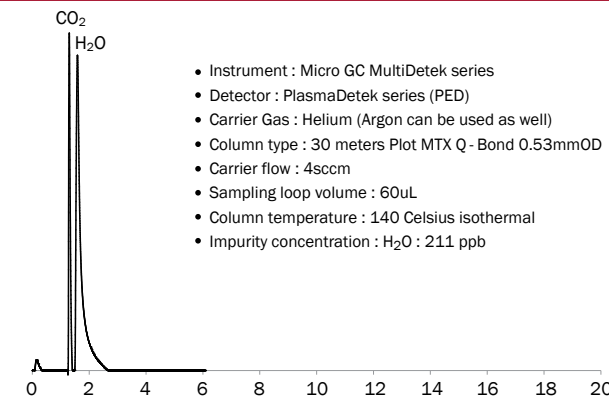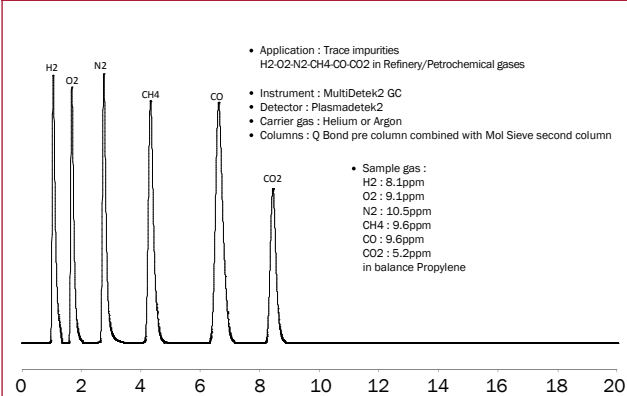CHROMATOGRAM #59**CHROMATOGRAM #60****CHROMATOGRAM #61****CHROMATOGRAM #62****CHROMATOGRAM #63****CHROMATOGRAM #64****CHROMATOGRAM #65****CHROMATOGRAM #66**


CHROMATOGRAM #67

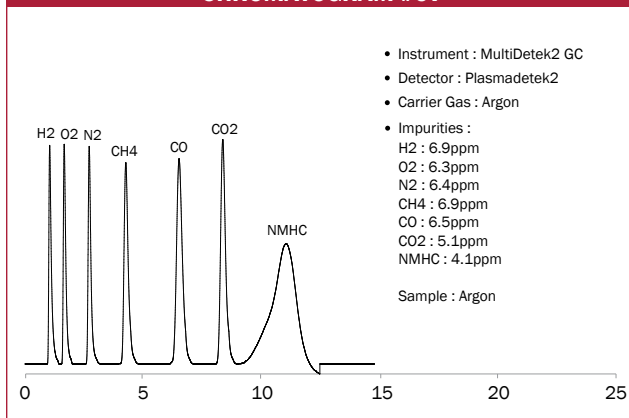


CHROMATOGRAM #68

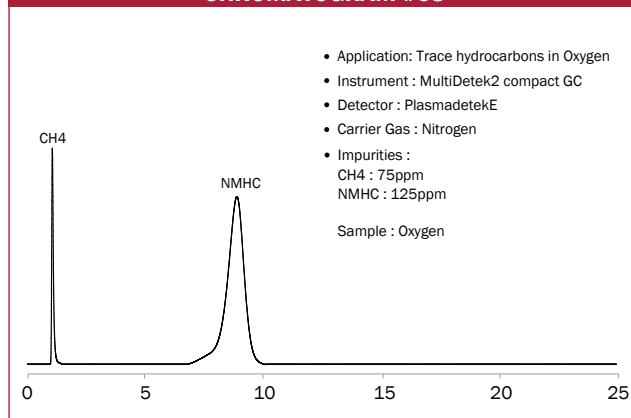


CHROMATOGRAM #69

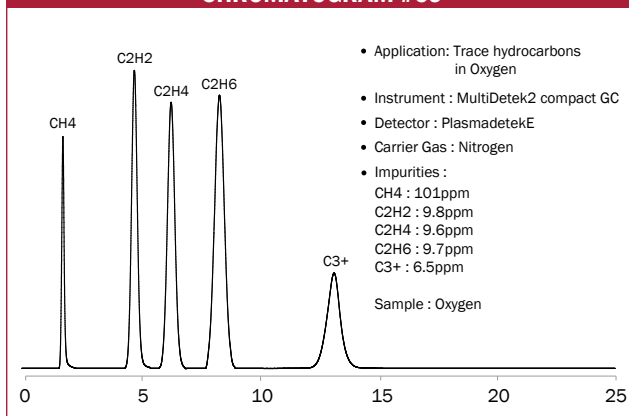


CHROMATOGRAM #70

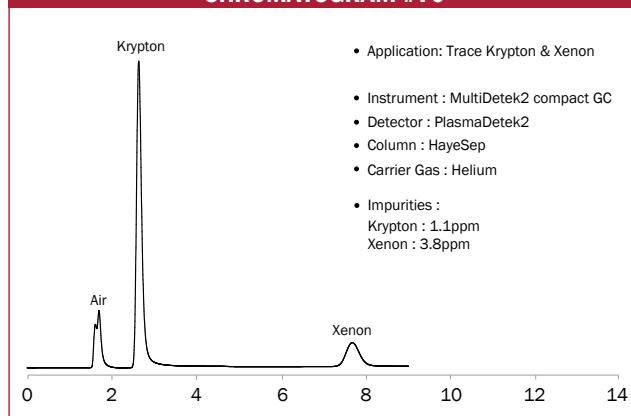


CHROMATOGRAM #71

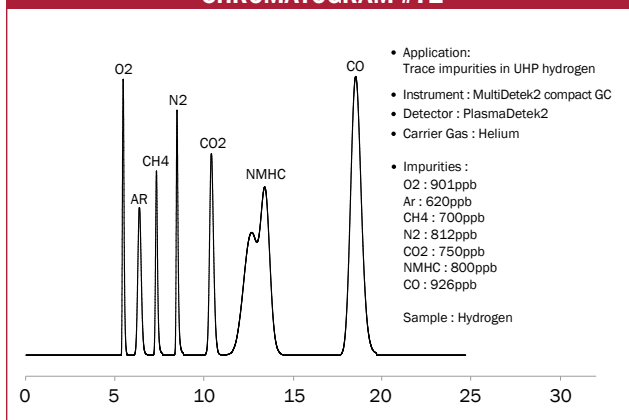


CHROMATOGRAM #72

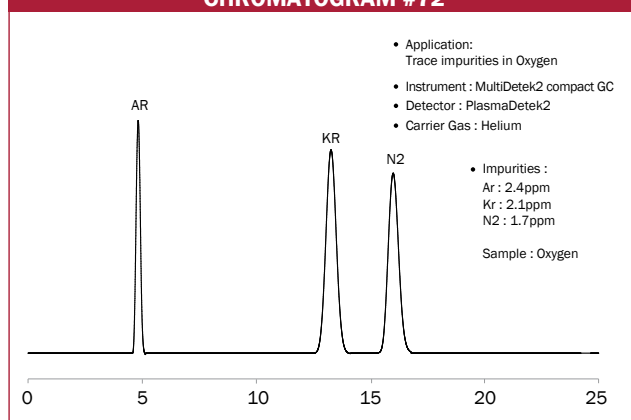


CHROMATOGRAM #73

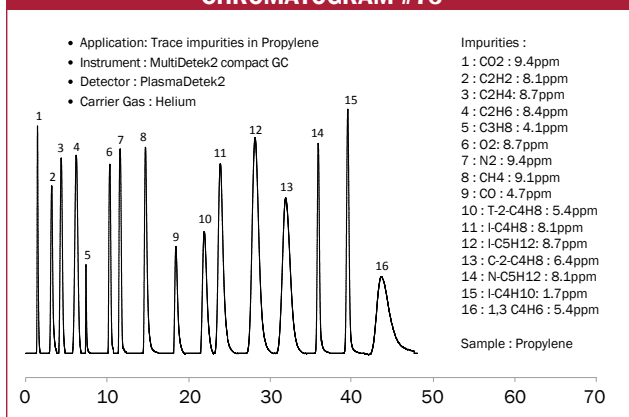


CHROMATOGRAM #74

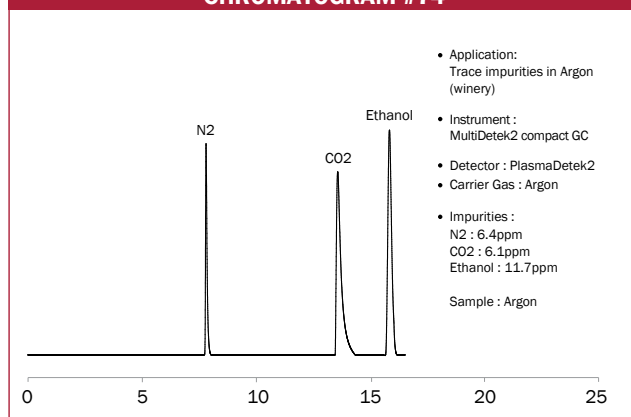


CHROMATOGRAM #75

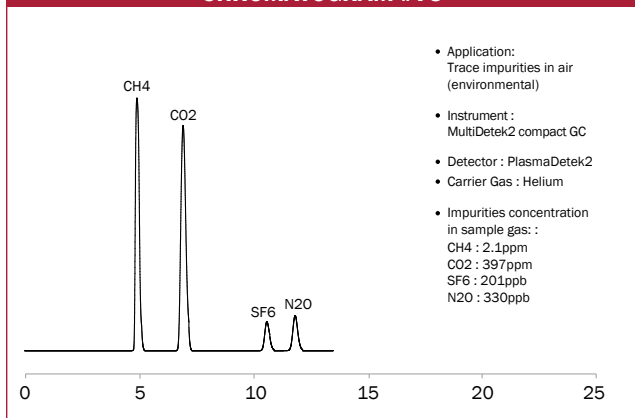


CHROMATOGRAM #76

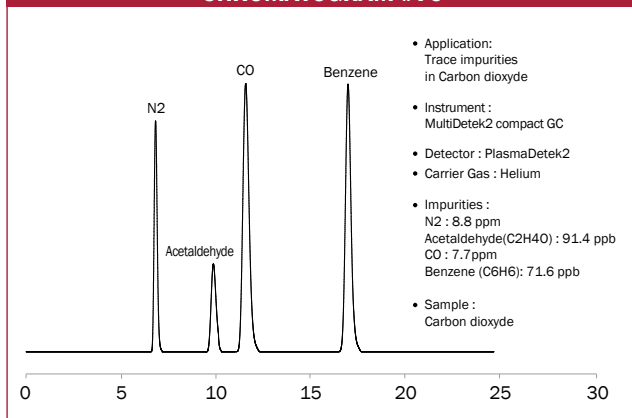


CHROMATOGRAM #77

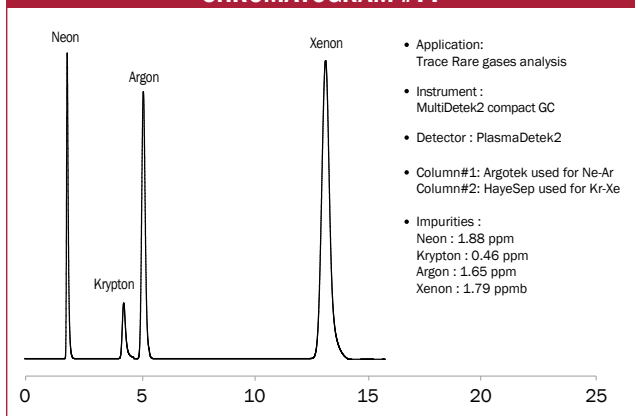


CHROMATOGRAM #78

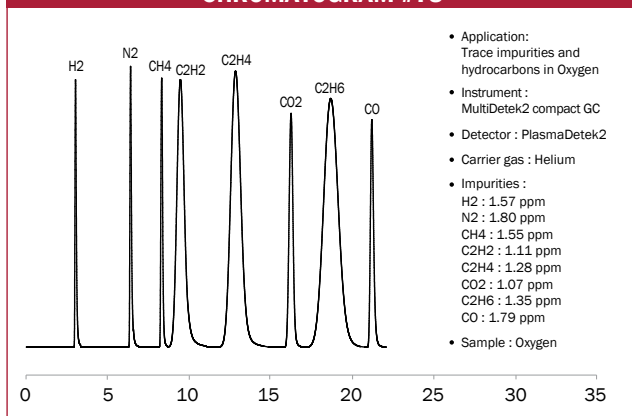


CHROMATOGRAM #79

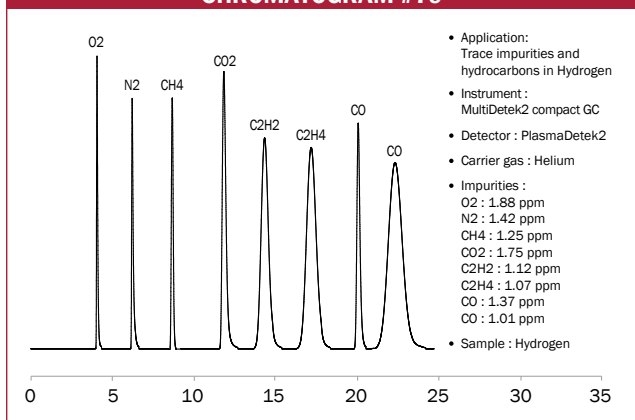


CHROMATOGRAM #80

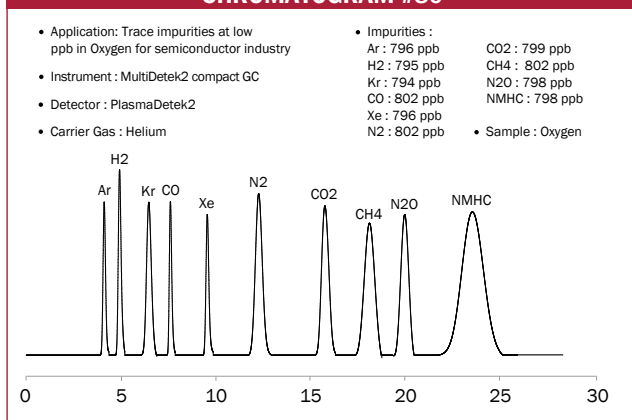


CHROMATOGRAM #81

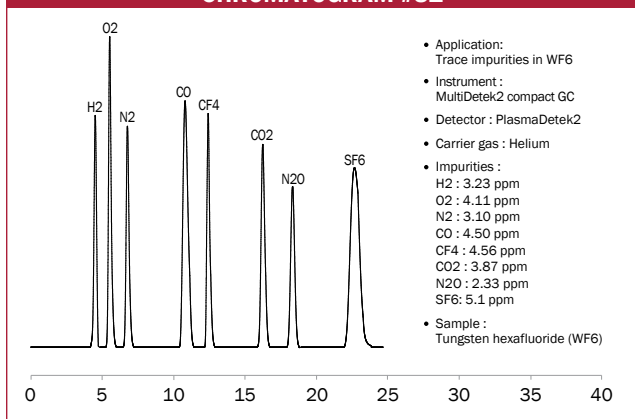


CHROMATOGRAM #82

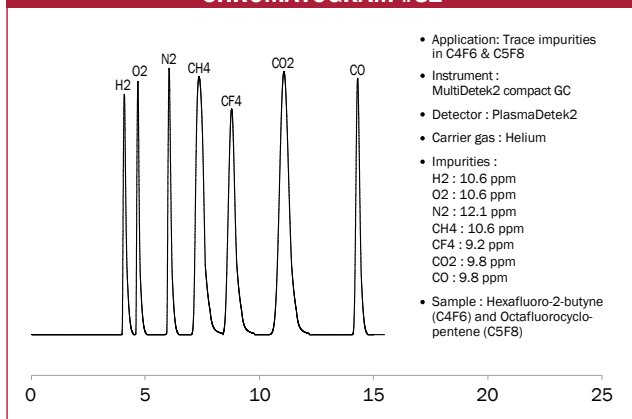


CHROMATOGRAM #83

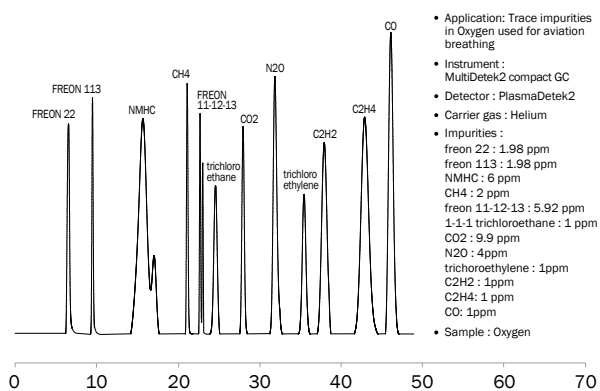


CHROMATOGRAM #84

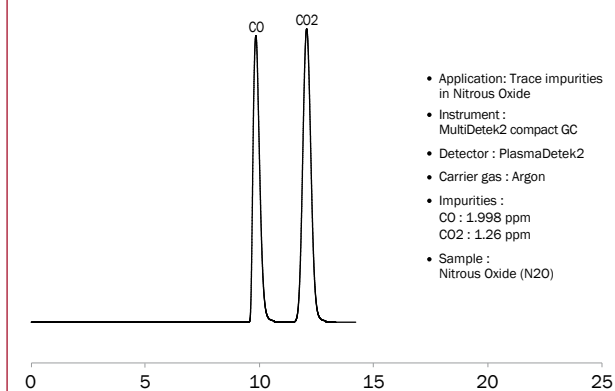


CHROMATOGRAM #85

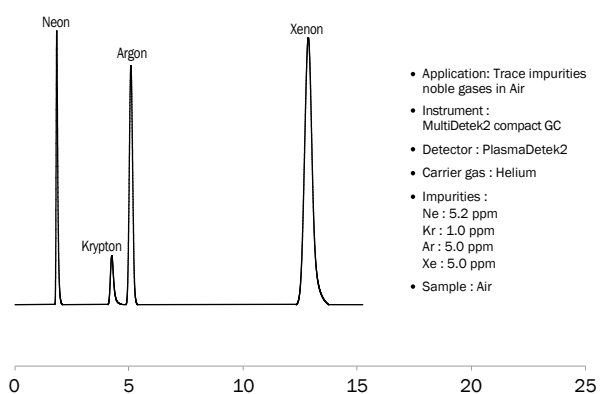


CHROMATOGRAM #86

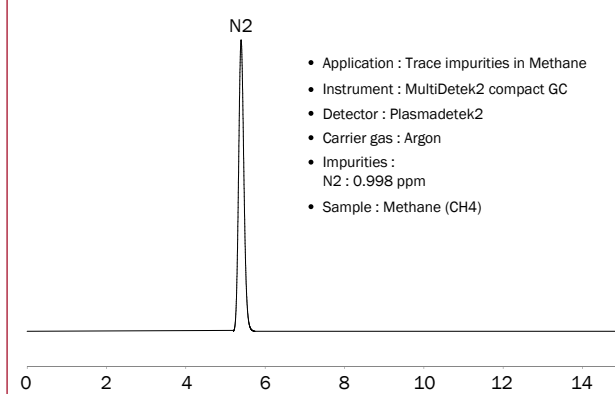


CHROMATOGRAM #87

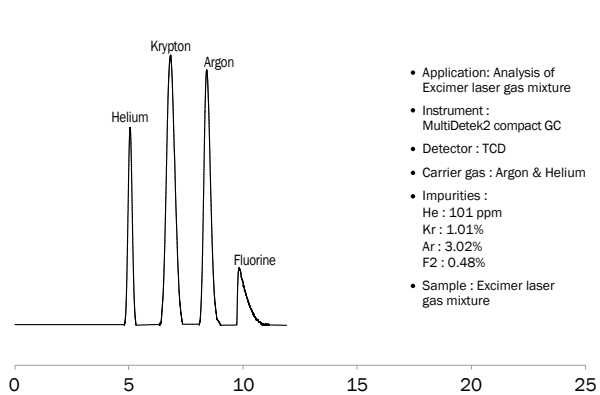


CHROMATOGRAM #88








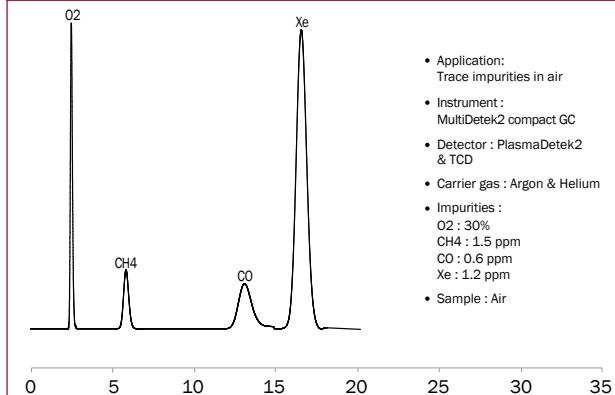


CHROMATOGRAM #89

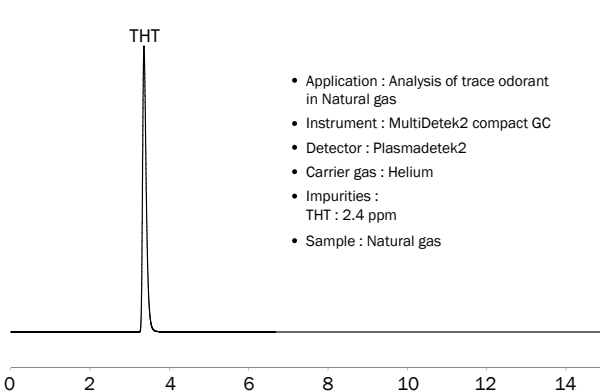


CHROMATOGRAM #90

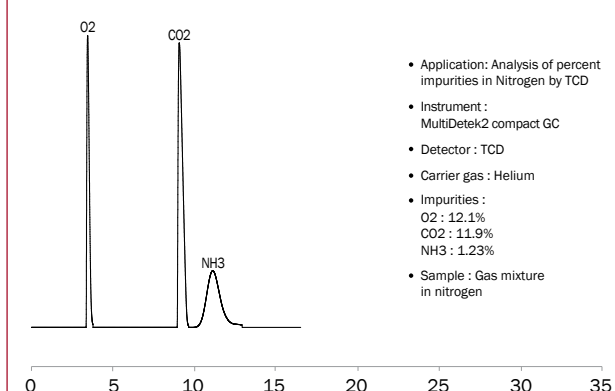


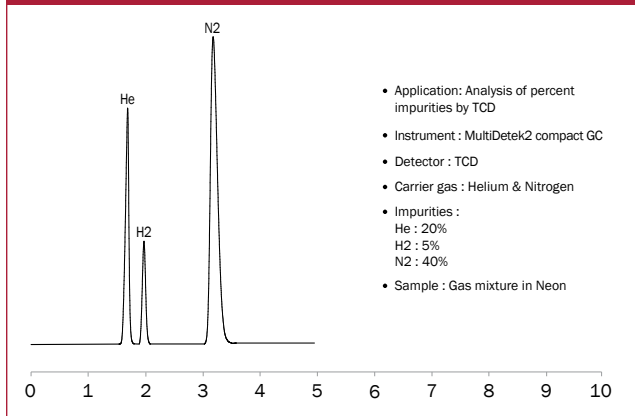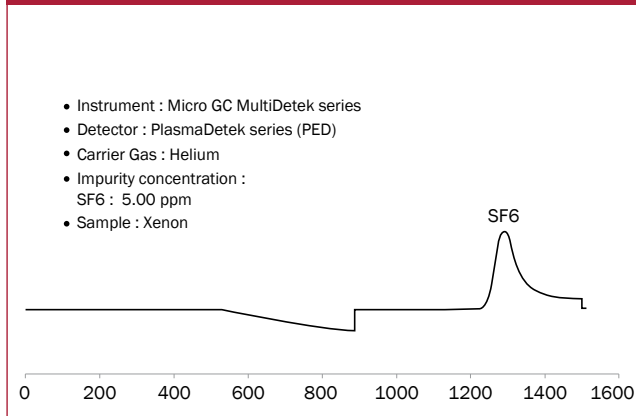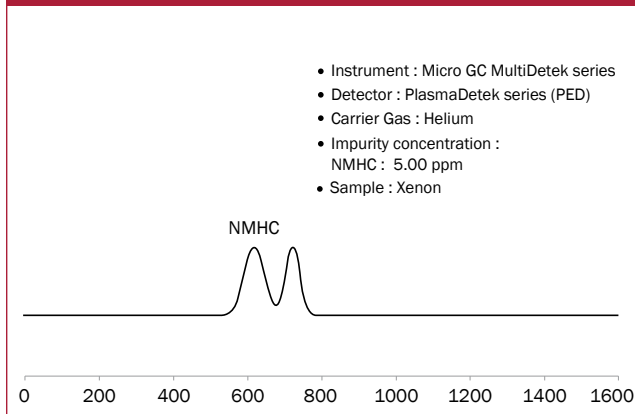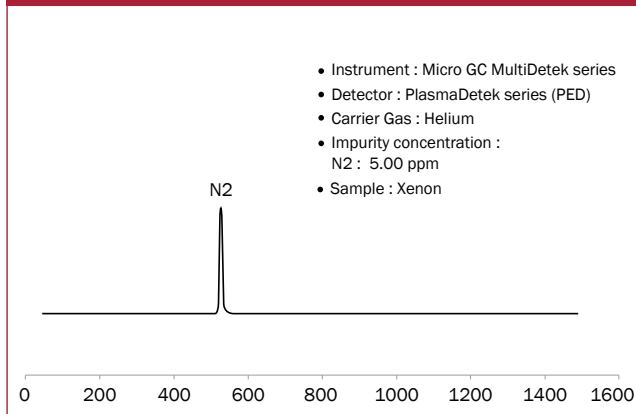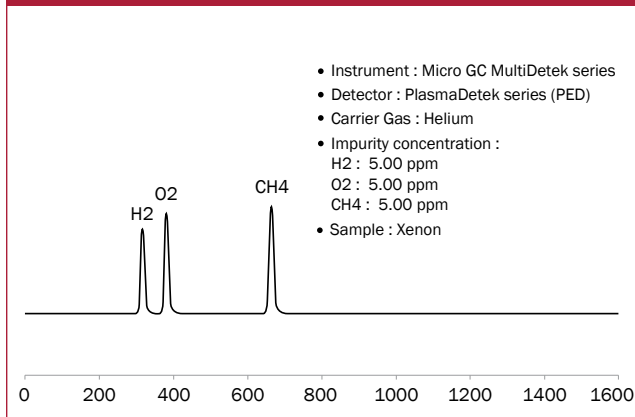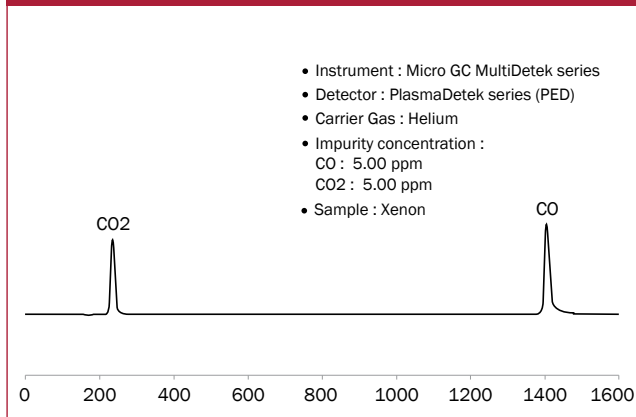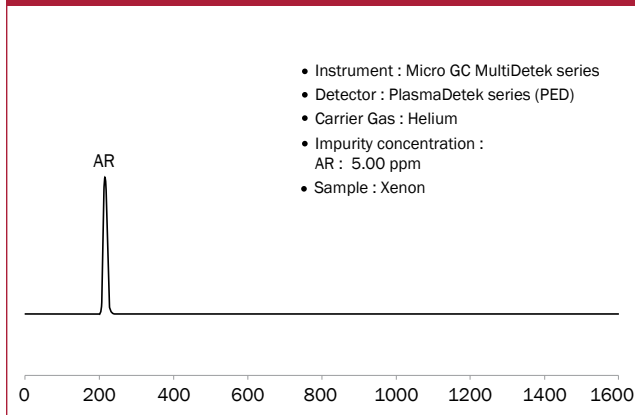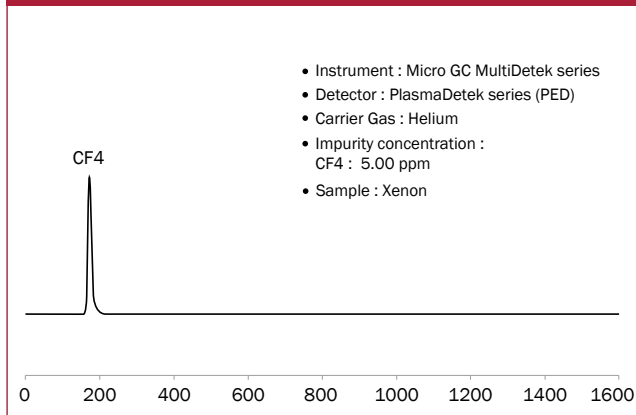CHROMATOGRAM #91**CHROMATOGRAM #92****CHROMATOGRAM #93****CHROMATOGRAM #94****CHROMATOGRAM #95****CHROMATOGRAM #96****CHROMATOGRAM #97****CHROMATOGRAM #98**


CHROMATOGRAM #99

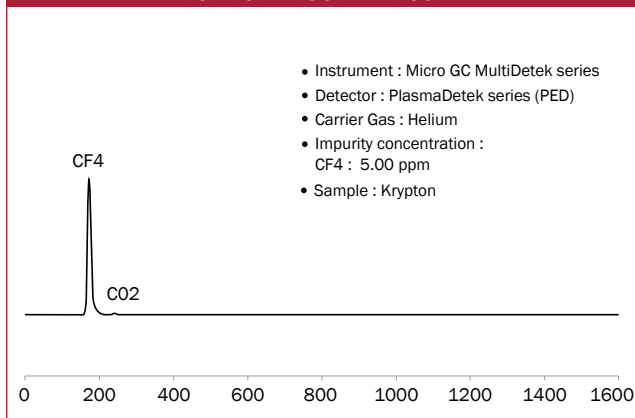


CHROMATOGRAM #100

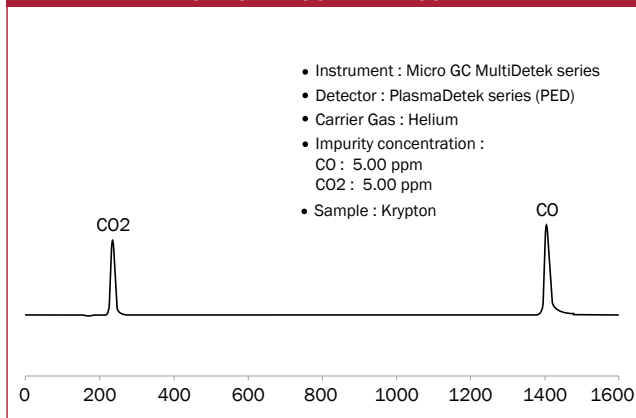


CHROMATOGRAM #101

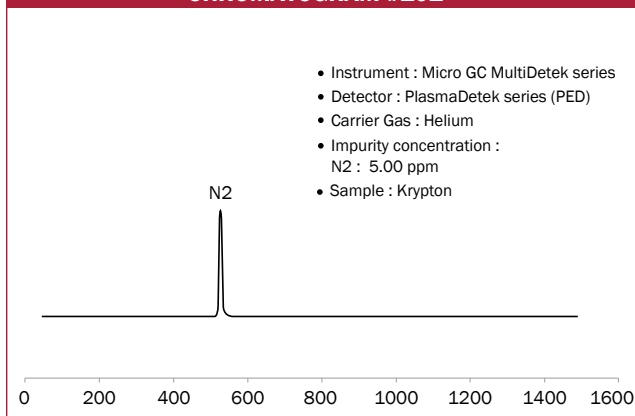


CHROMATOGRAM #102

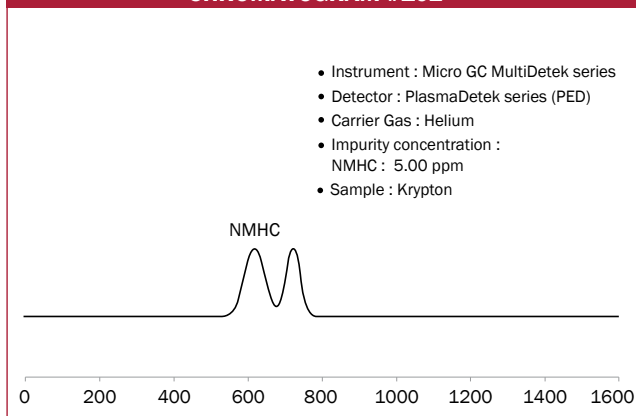


CHROMATOGRAM #103

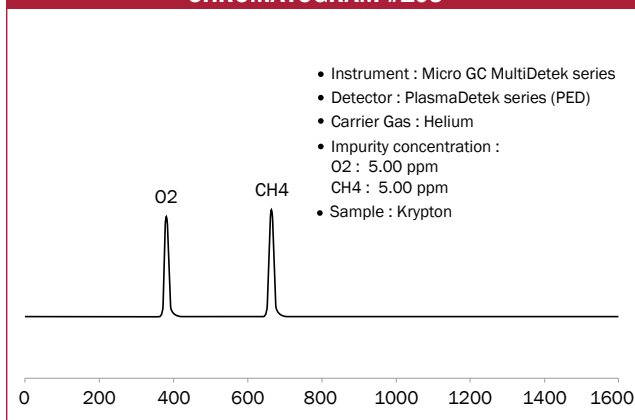


CHROMATOGRAM #104

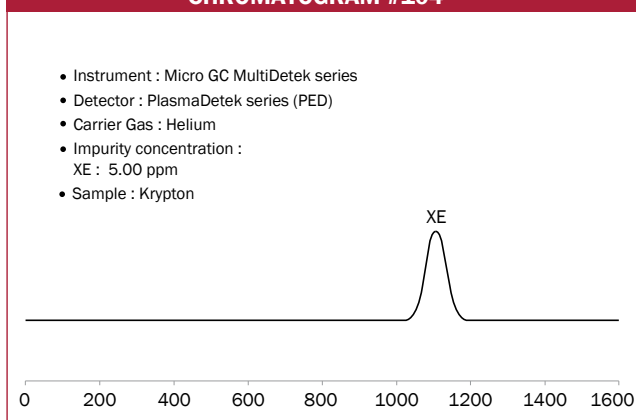


CHROMATOGRAM #105

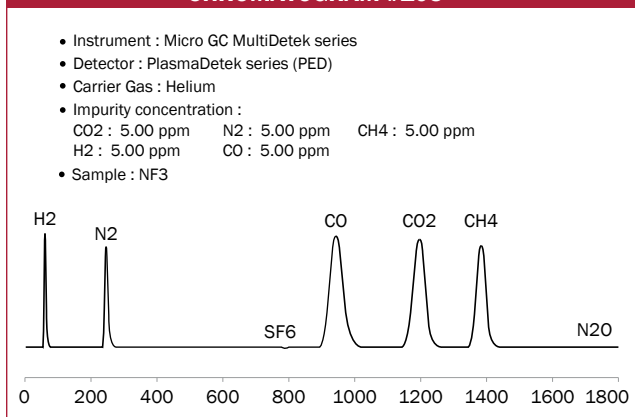


CHROMATOGRAM #106

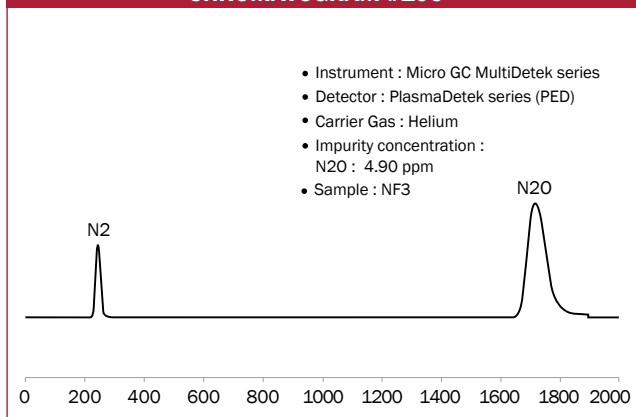


CHROMATOGRAM #107

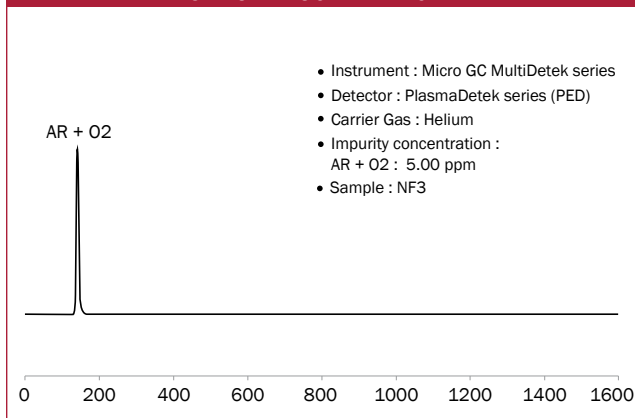


CHROMATOGRAM #108

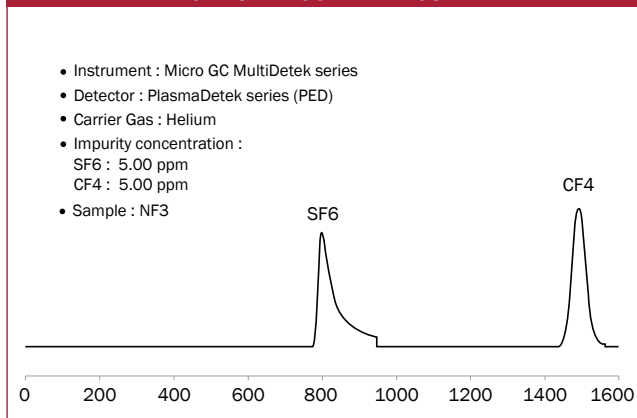


CHROMATOGRAM #109

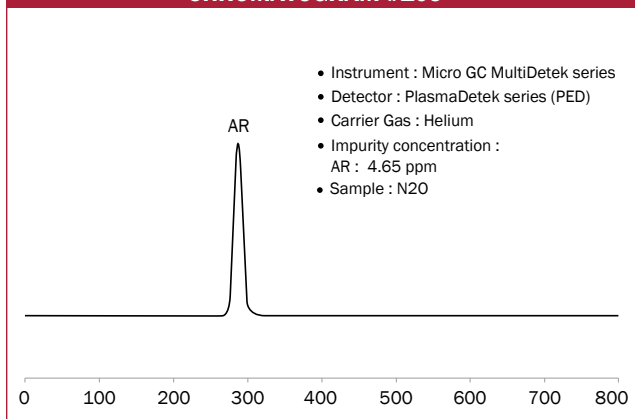


CHROMATOGRAM #110

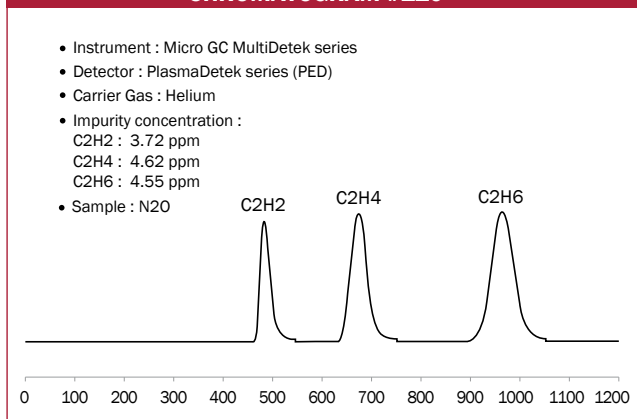


CHROMATOGRAM #111

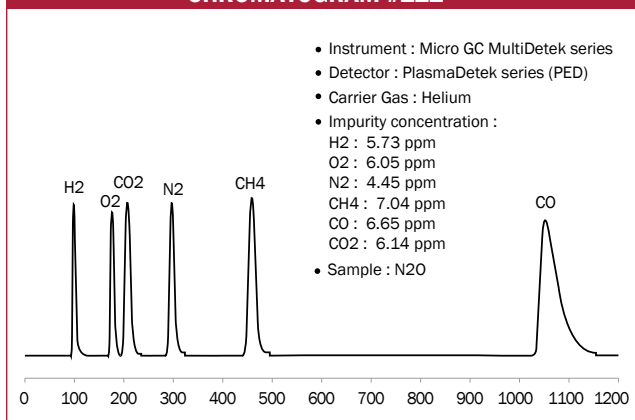


CHROMATOGRAM #112



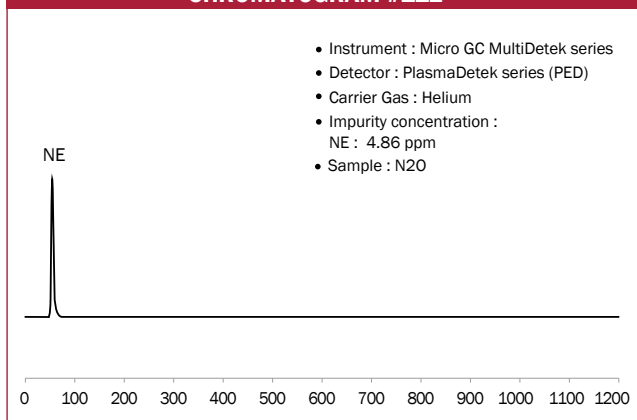


CHROMATOGRAM #113

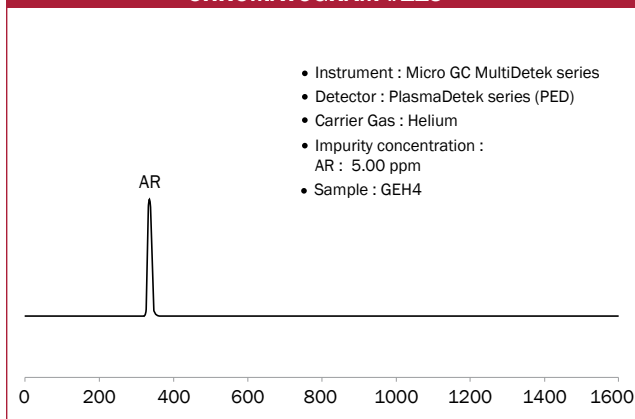

CHROMATOGRAM #114

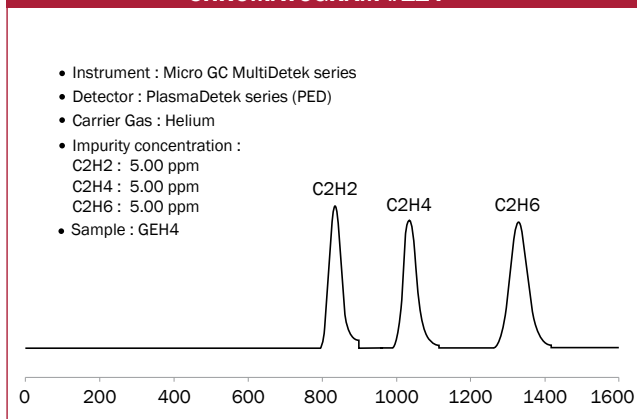

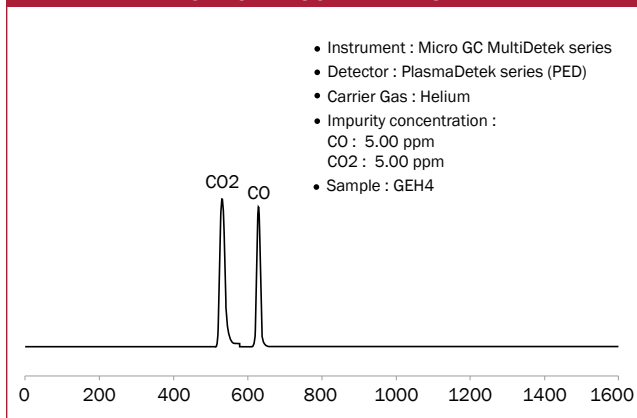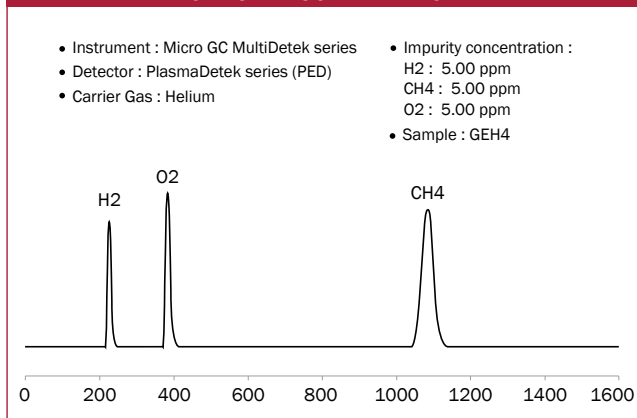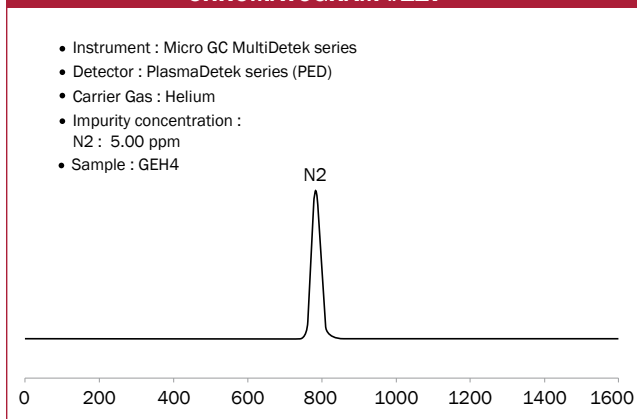
CHROMATOGRAM #115**CHROMATOGRAM #116****CHROMATOGRAM #117**

SAMPLES


Chromatograms

| | |
|---|--|
| Air | 5-10-44-45-48-75-85-88 |
| Argon | 30-54-58-67-74 |
| Carbon Dioxide | 76 |
| Crude Argon | 52-53 |
| Ethylene | 66 |
| Excimer laser gas mixture | 87 |
| Germane (GeH ₄) | 113-114-115-116-117 |
| Helium | 19-39 |
| Hexafluoro-2-butyne | 82 |
| Hydrogen | 15-31-40-46-56-57-71-79 |
| Hydrogen Chloride | 25 |
| Krypton | 99-100-101-102-103-104 |
| Methane | 86 |
| Natural gas | 50-51-89 |
| Neon | 38-91 |
| Nitrogen | 9-13-16-32-43-49-90 |
| Nitrogen trifluoride (NF ₃) | 105-106-107-108 |
| Nitrous oxide (N ₂ O) | 84-109-110-111-112 |
| Octafluorocyclopentene | 82 |
| Oxygen | 11-14-17-23-33-34-35-36-37-41-47-68-69-72-78-80-83 |
| Propylene | 66-73 |
| Sulfur hexafluoride | 42-63 |
| Syngas | 44-45 |
| Tungsten hexafluoride | 81 |
| Xenon | 62-92-93-94-95-96-97-98 |


CHROMATOGRAM #5

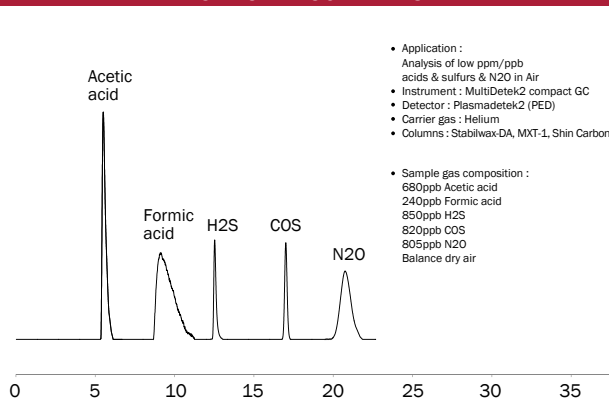


CHROMATOGRAM #10

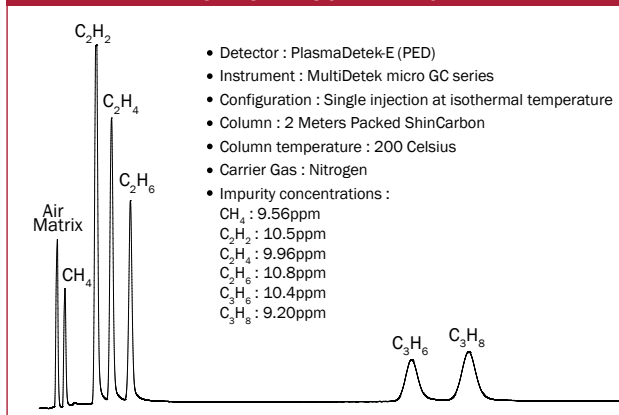


CHROMATOGRAM #9

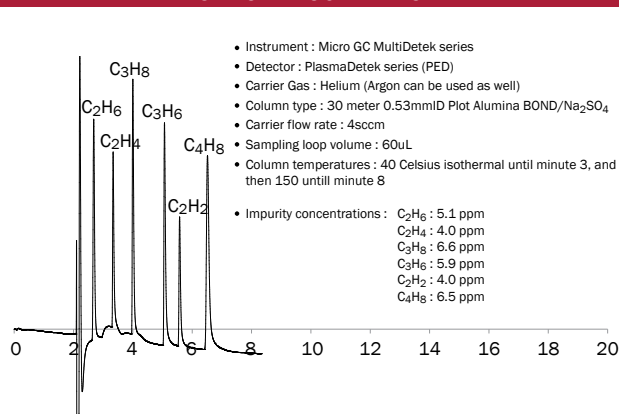


CHROMATOGRAM #11

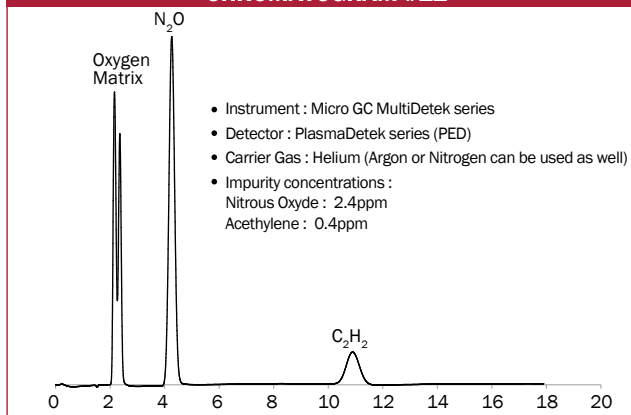


CHROMATOGRAM #13

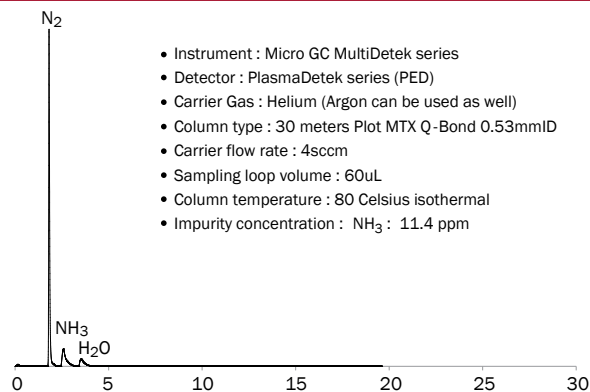


CHROMATOGRAM #14

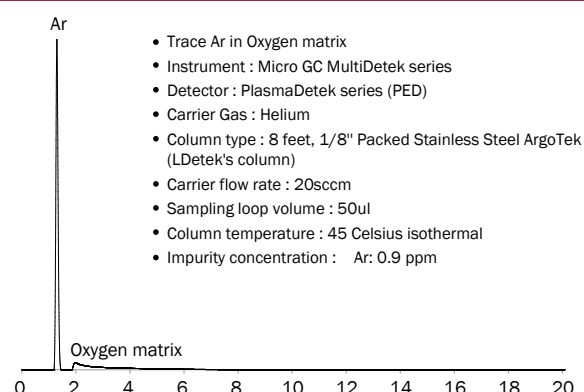


CHROMATOGRAM #15

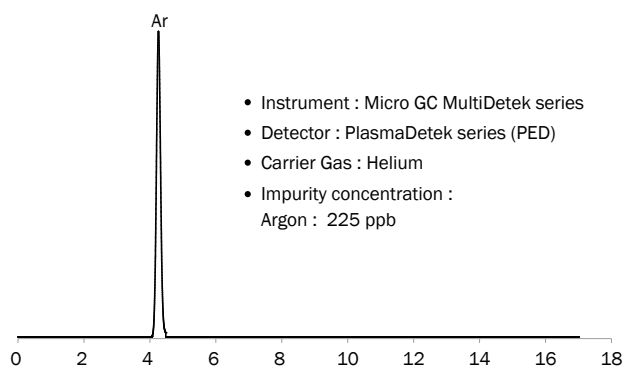


CHROMATOGRAM #16

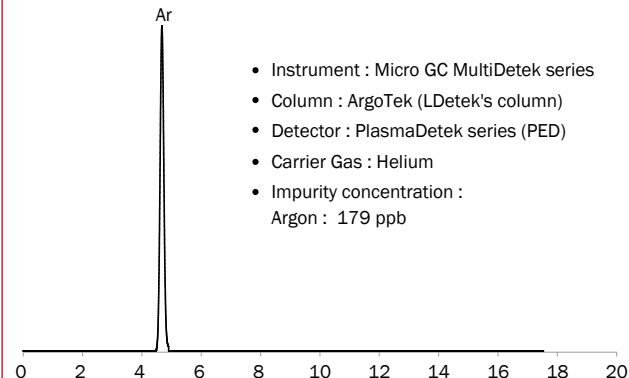


CHROMATOGRAM #17

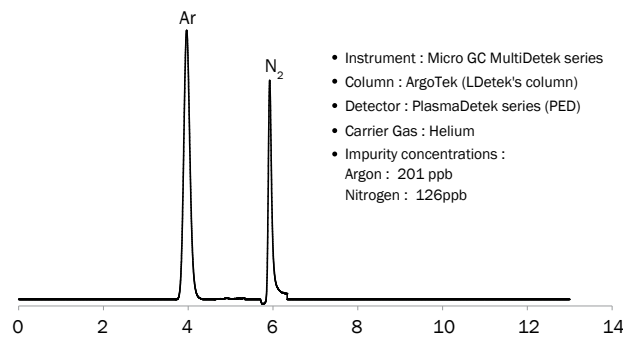


CHROMATOGRAM #19

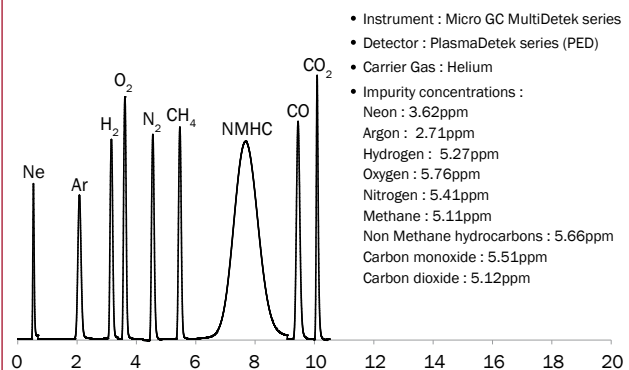


CHROMATOGRAM #23

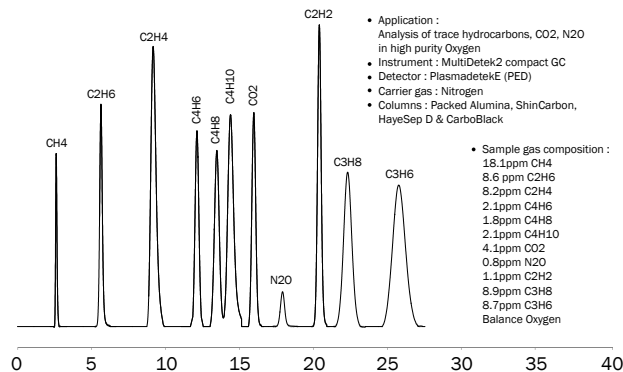


CHROMATOGRAM #25

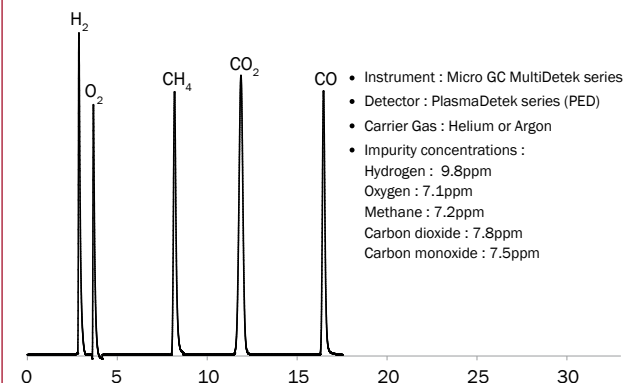


CHROMATOGRAM #30

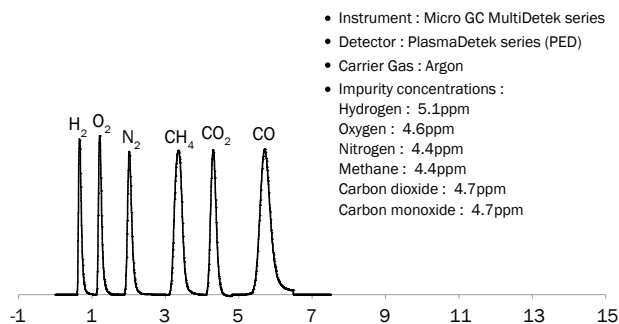


CHROMATOGRAM #31

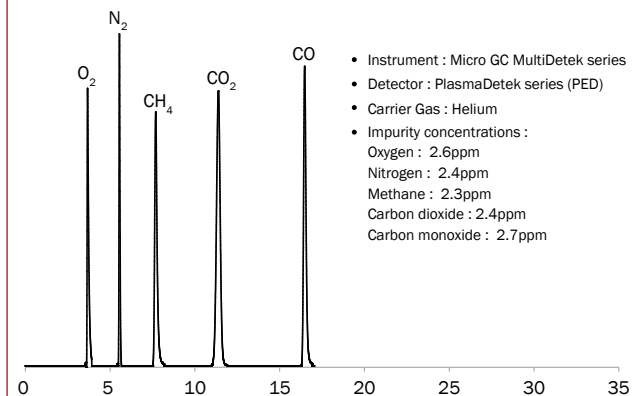


CHROMATOGRAM #32

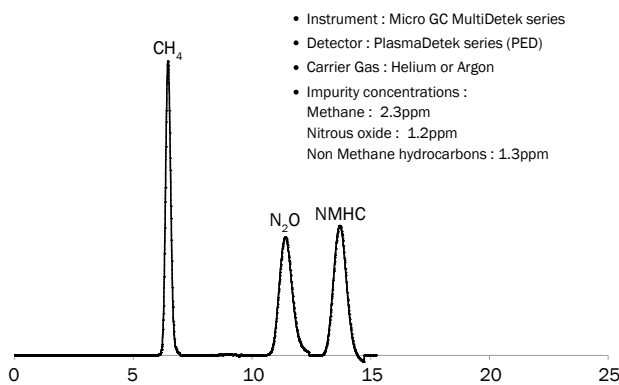


CHROMATOGRAM #33

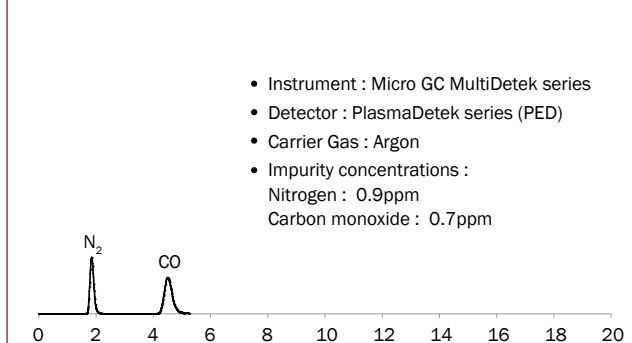


CHROMATOGRAM #34

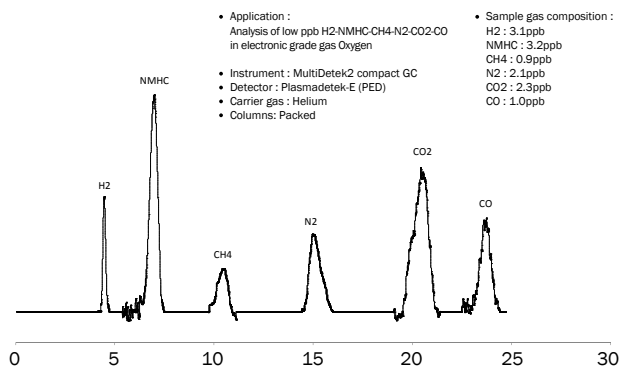


CHROMATOGRAM #35

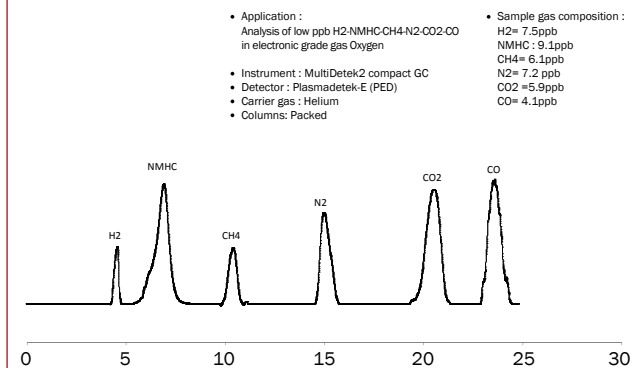


CHROMATOGRAM #36

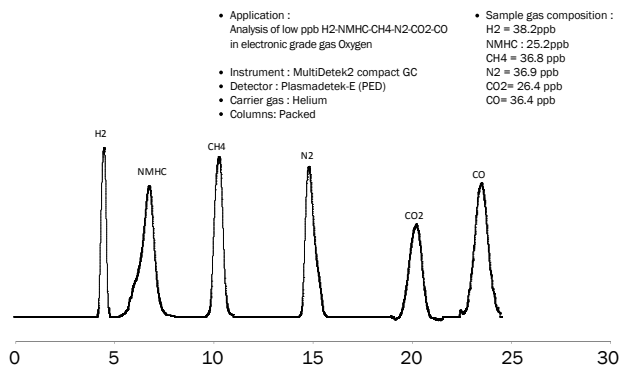


CHROMATOGRAM #37

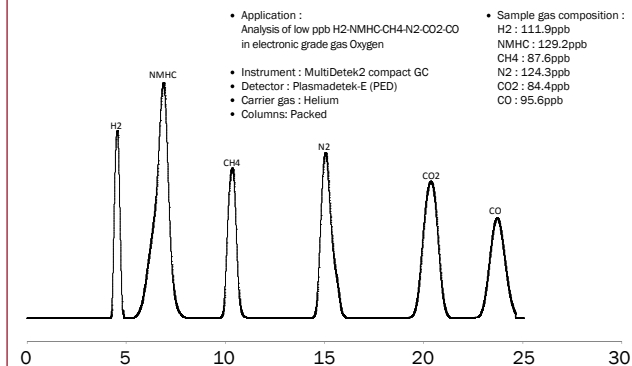


CHROMATOGRAM #38

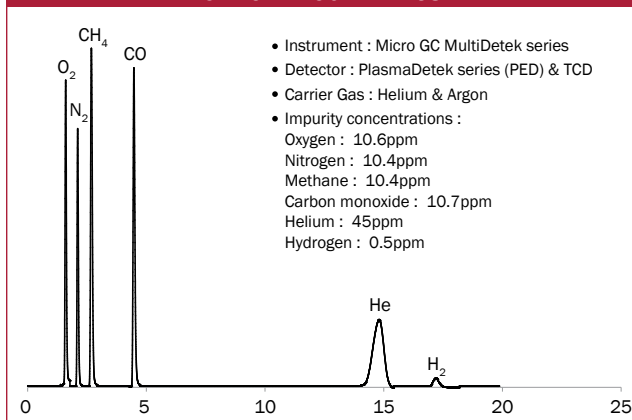


CHROMATOGRAM #39

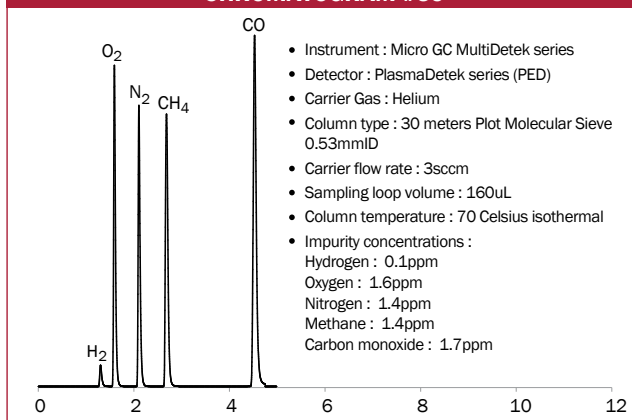


CHROMATOGRAM #40

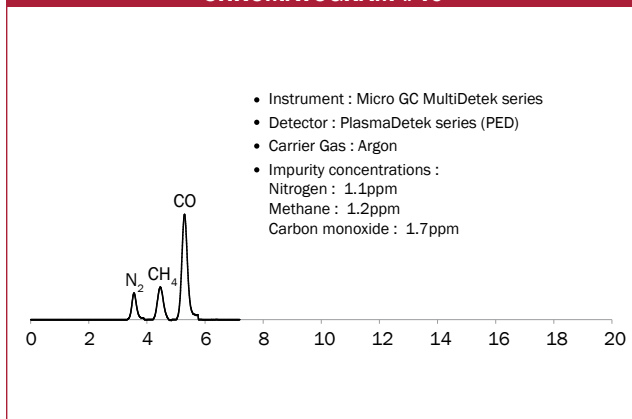


CHROMATOGRAM #41

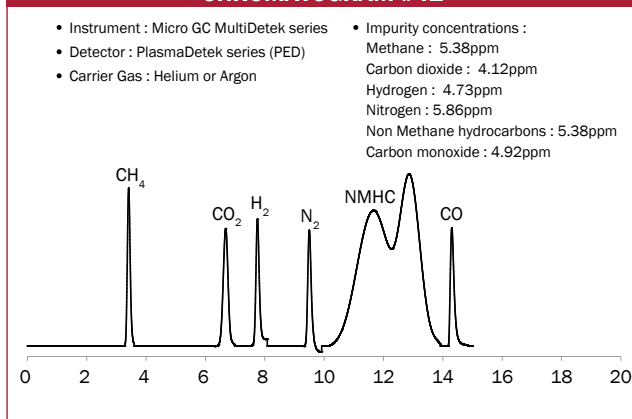


CHROMATOGRAM #42

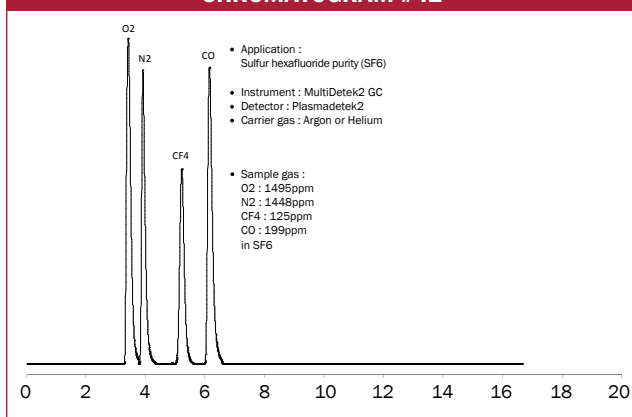


CHROMATOGRAM #43

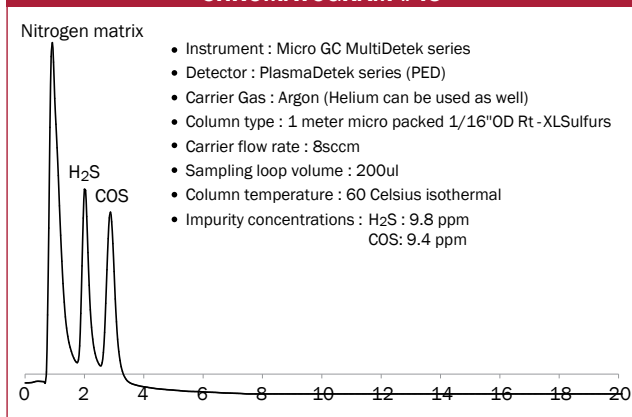


CHROMATOGRAM #44

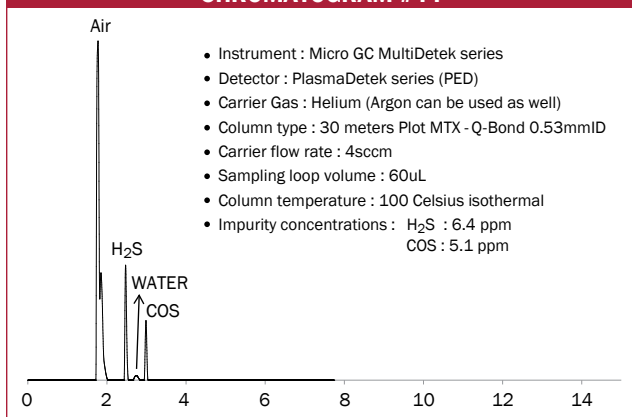


CHROMATOGRAM #45

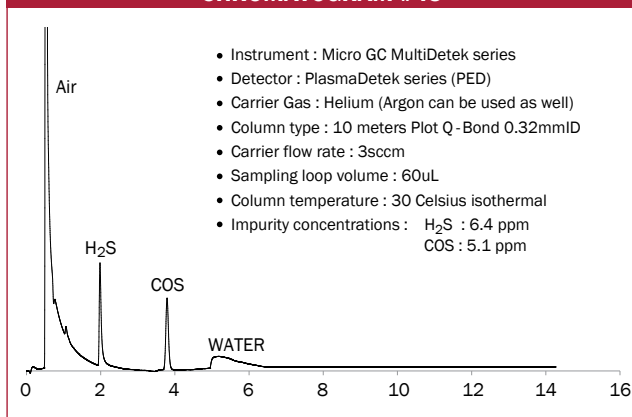


CHROMATOGRAM #46

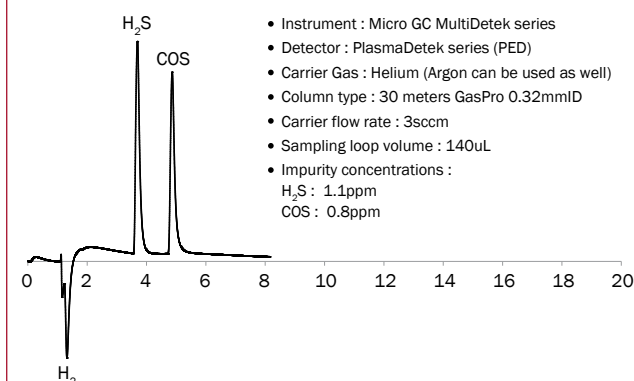


CHROMATOGRAM #48

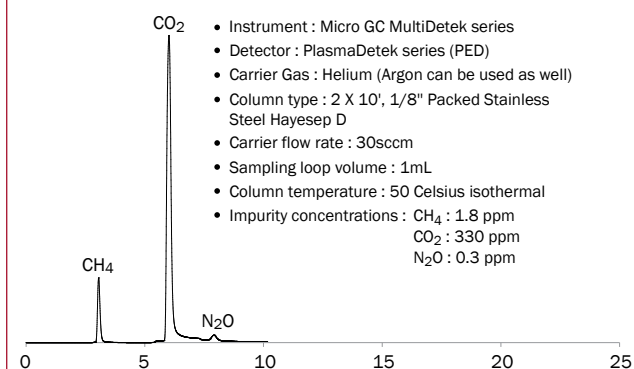


CHROMATOGRAM #49

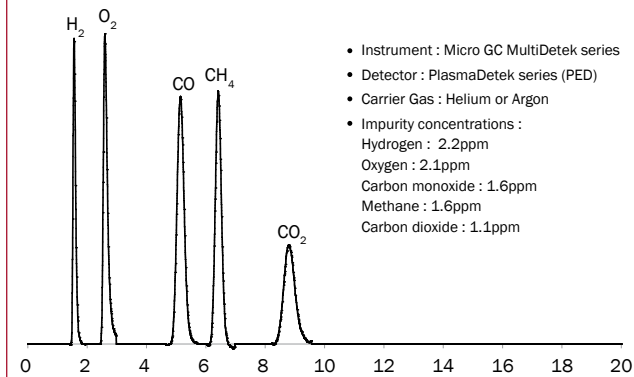


CHROMATOGRAM #51

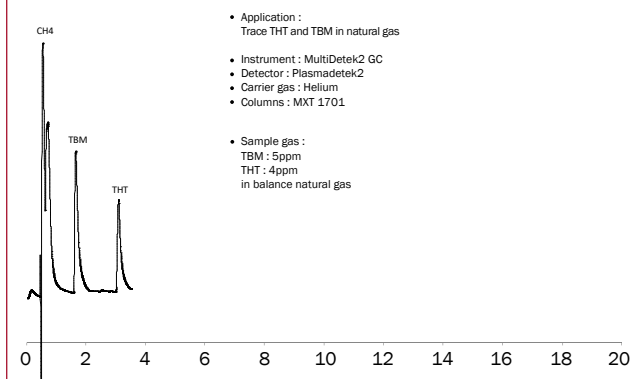


CHROMATOGRAM #47

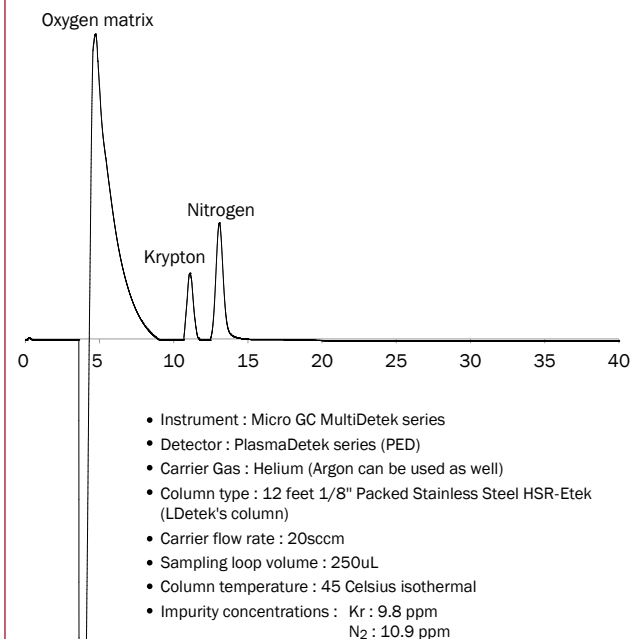


CHROMATOGRAM #50

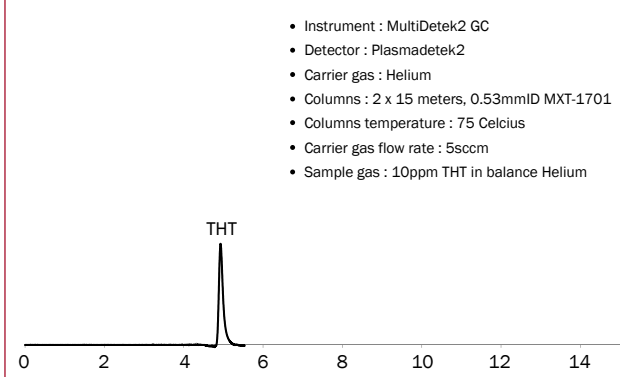


CHROMATOGRAM #52

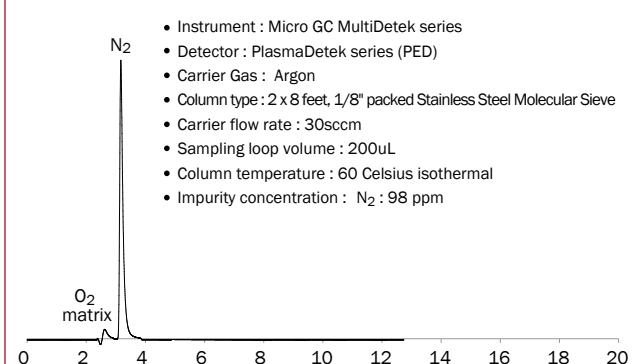


CHROMATOGRAM #53

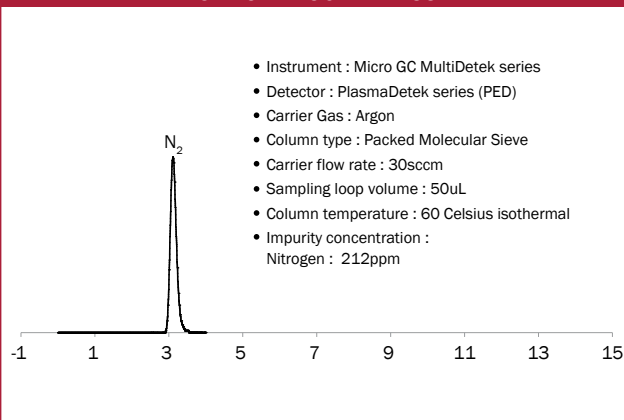


CHROMATOGRAM #54

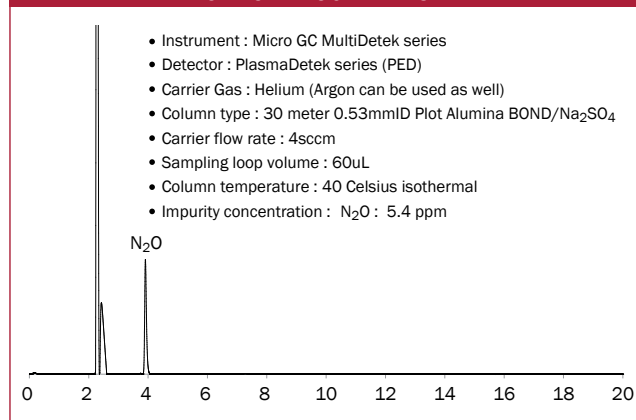


CHROMATOGRAM #56

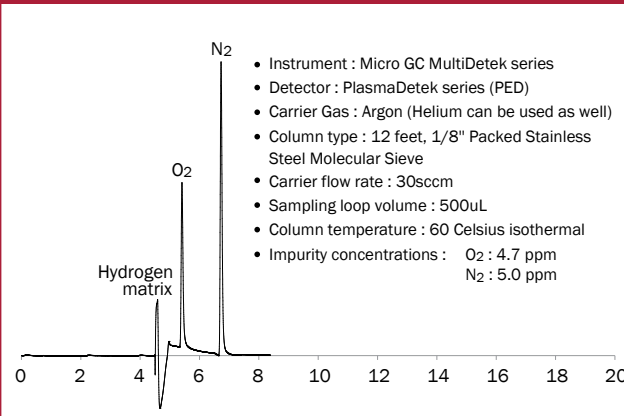


CHROMATOGRAM #57

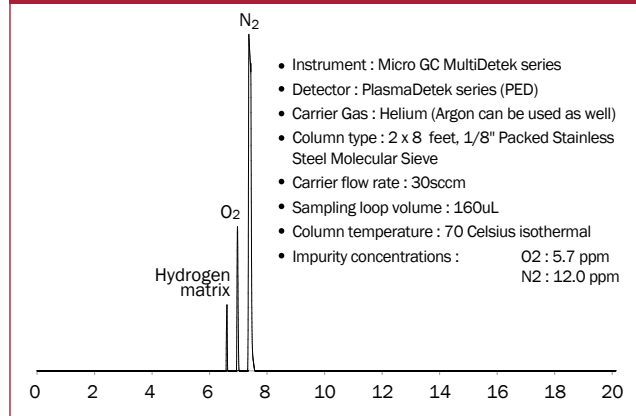


CHROMATOGRAM #58

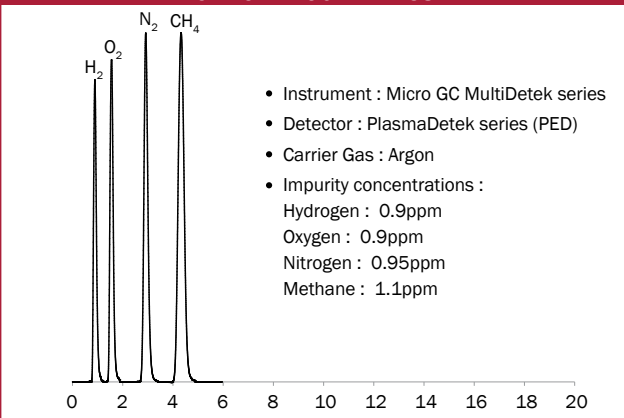


CHROMATOGRAM #62

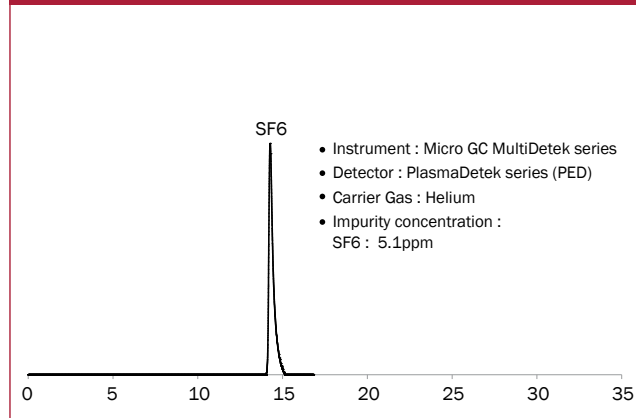


CHROMATOGRAM #63

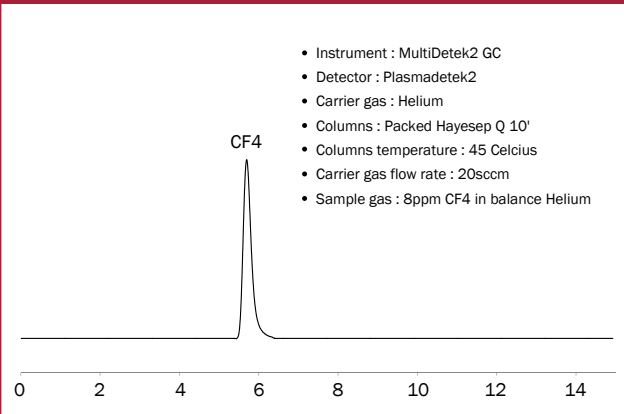


CHROMATOGRAM #66

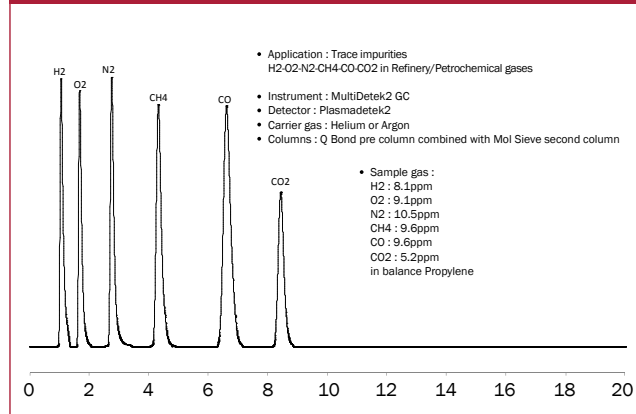


CHROMATOGRAM #67

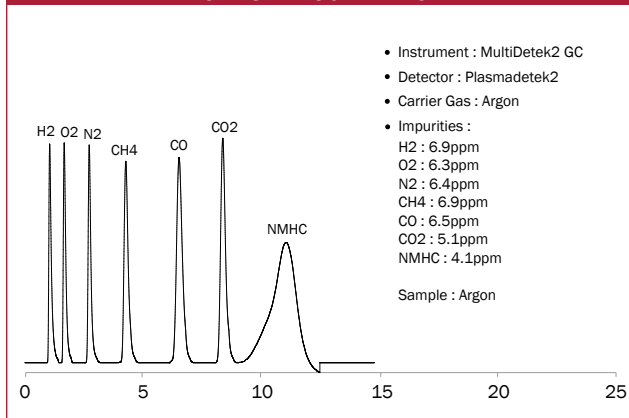


CHROMATOGRAM #68

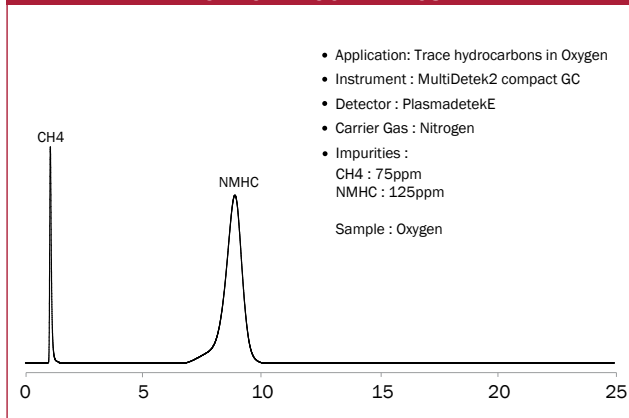


CHROMATOGRAM #69

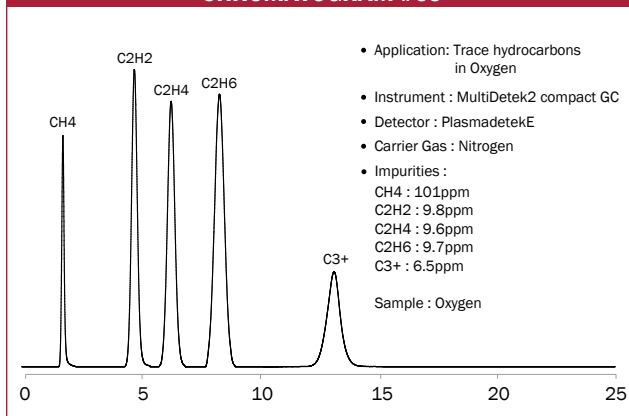


CHROMATOGRAM #71

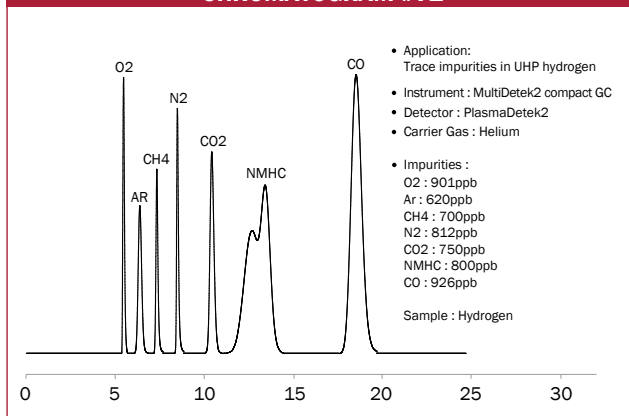


CHROMATOGRAM #72

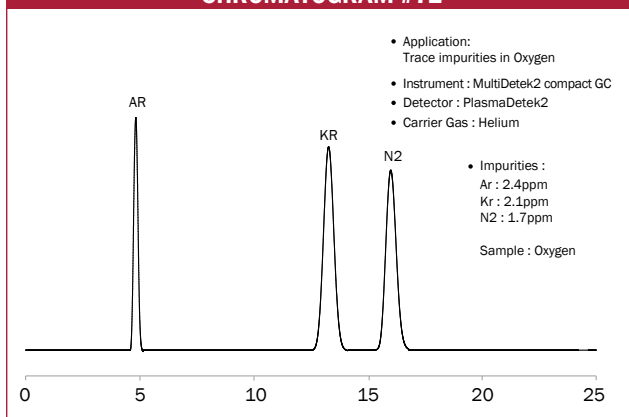


CHROMATOGRAM #73

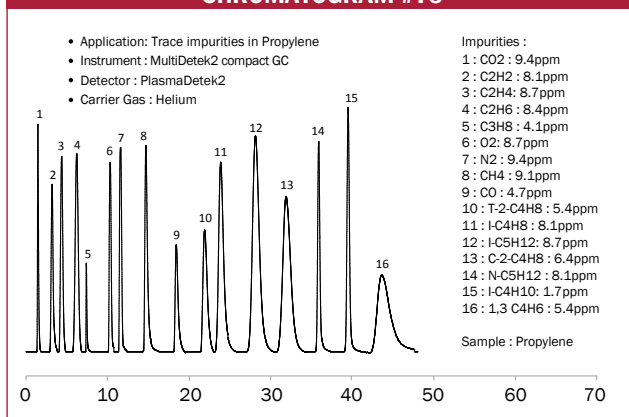


CHROMATOGRAM #74

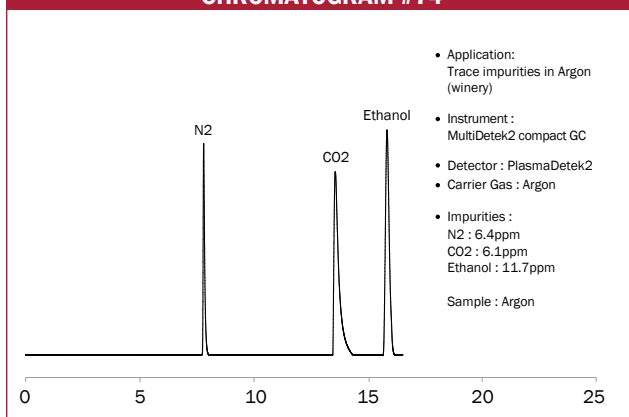


CHROMATOGRAM #75

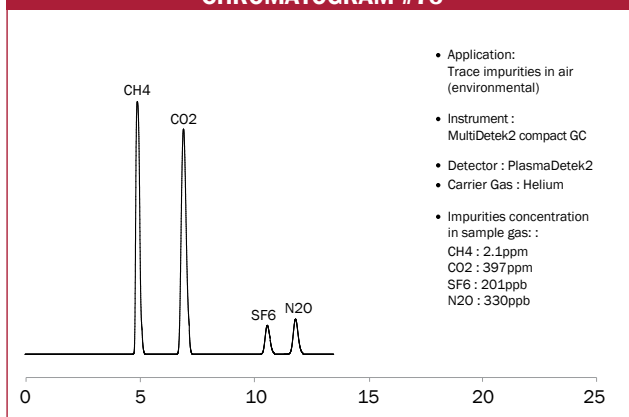


CHROMATOGRAM #76

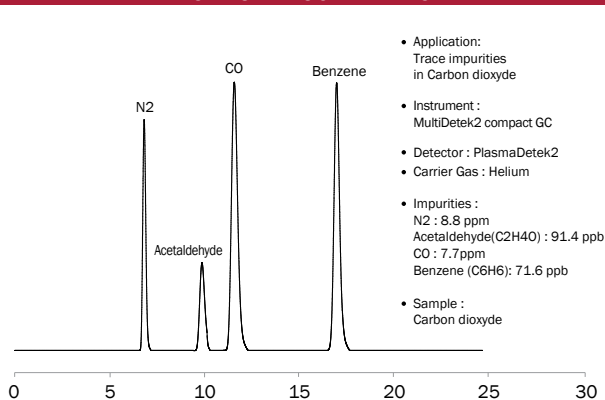


CHROMATOGRAM #78

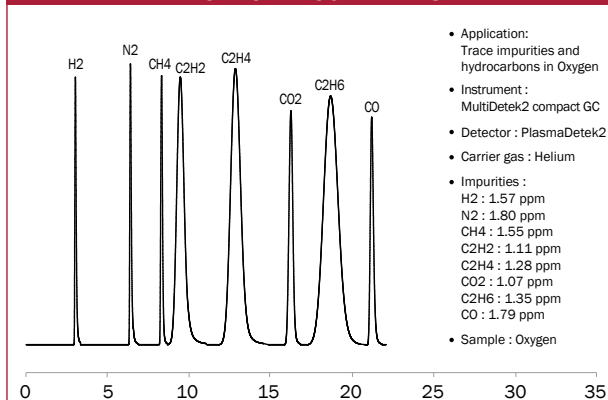


CHROMATOGRAM #79

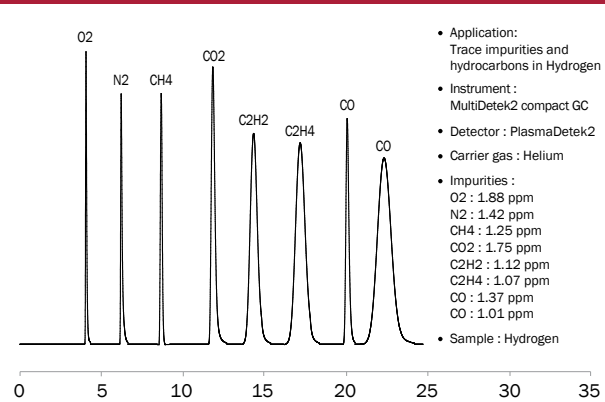


CHROMATOGRAM #80

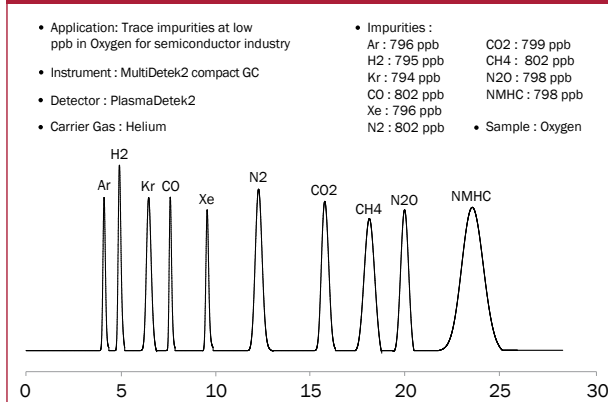


CHROMATOGRAM #81

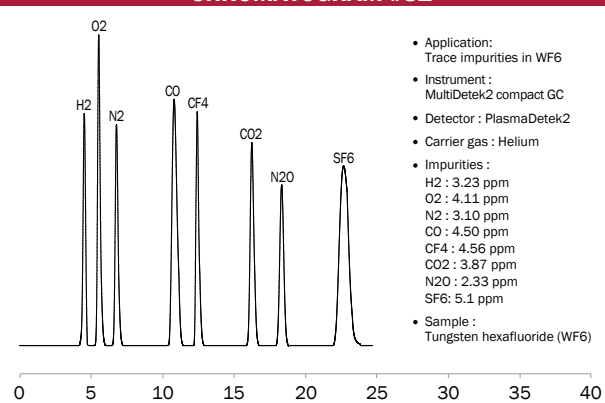


CHROMATOGRAM #82

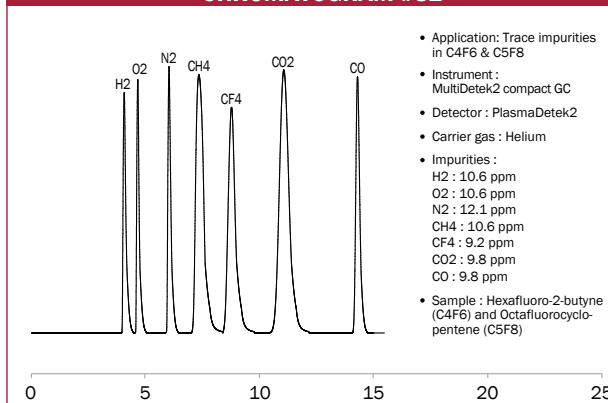


CHROMATOGRAM #83

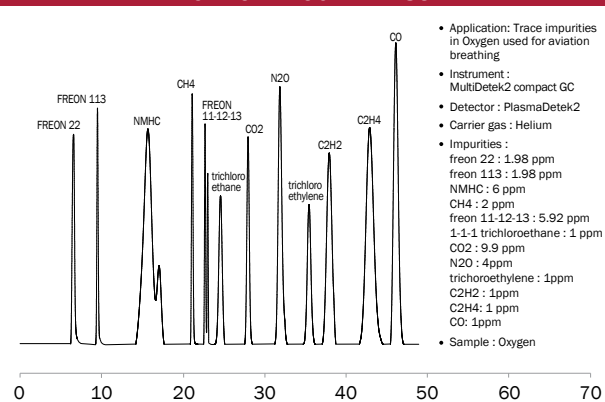


CHROMATOGRAM #84

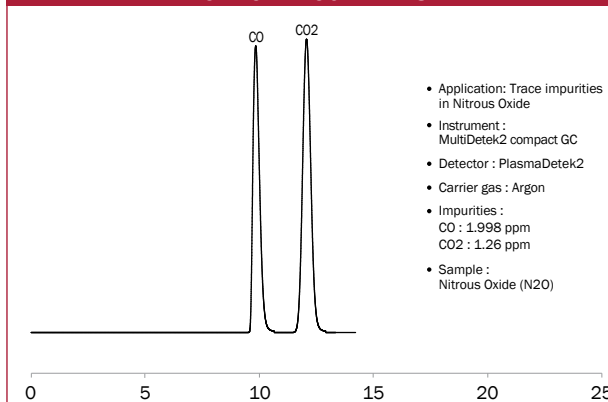


CHROMATOGRAM #85

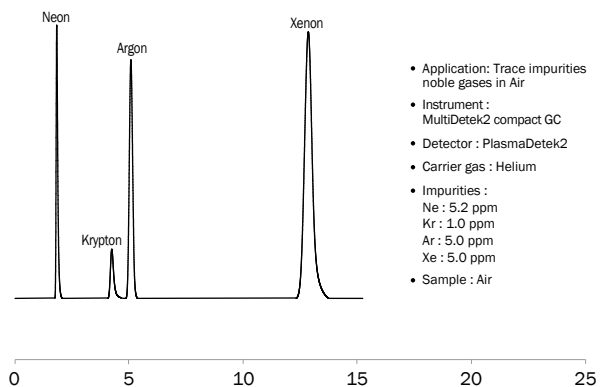


CHROMATOGRAM #86

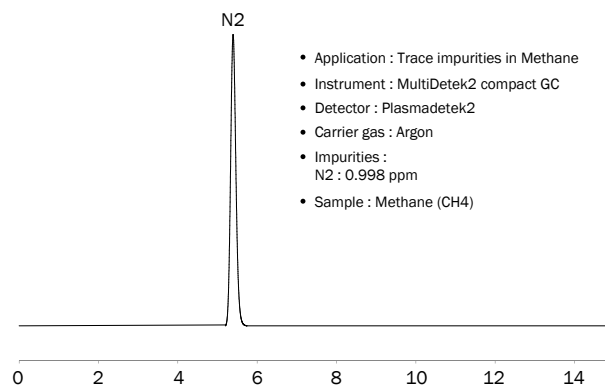


CHROMATOGRAM #87

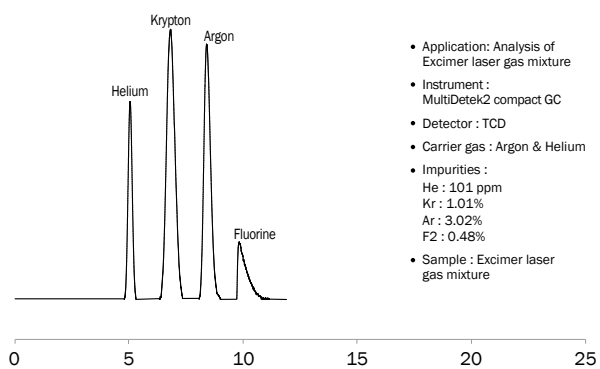


CHROMATOGRAM #88

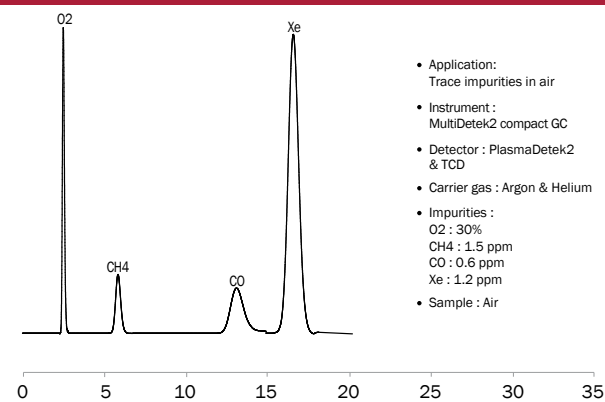


CHROMATOGRAM #89

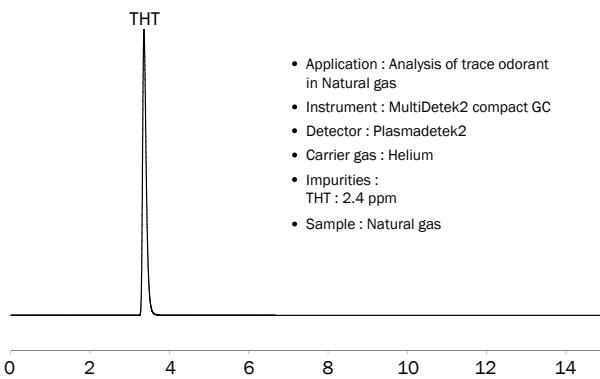


CHROMATOGRAM #90

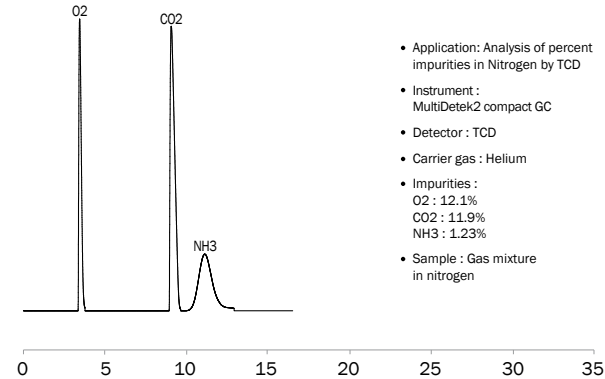

CHROMATOGRAM #91

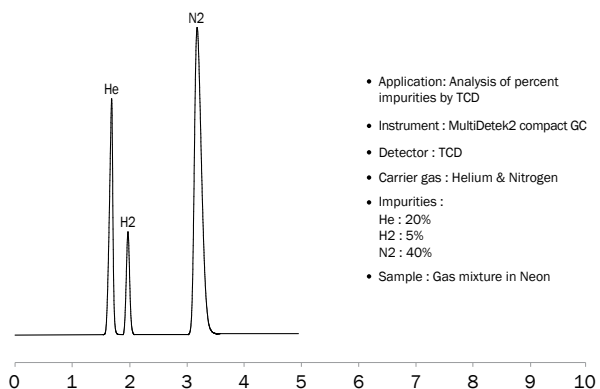


CHROMATOGRAM #92

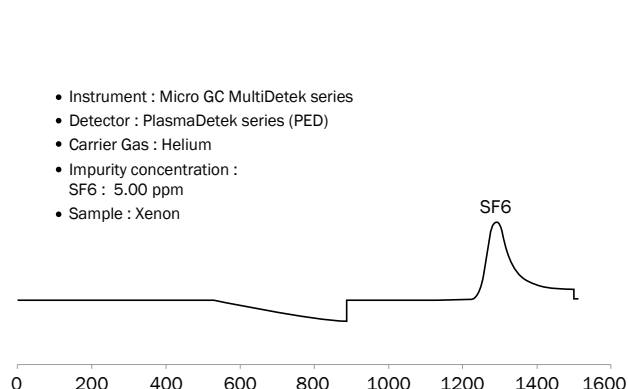


CHROMATOGRAM #93

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium
- Impurity concentration :
NMHC : 5.00 ppm
- Sample : Xenon

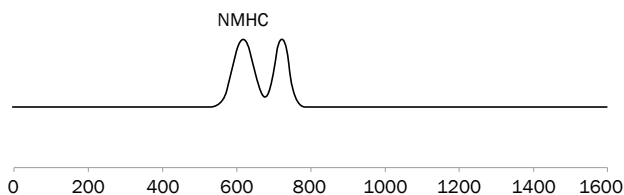


CHROMATOGRAM #94

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium
- Impurity concentration :
N2 : 5.00 ppm
- Sample : Xenon

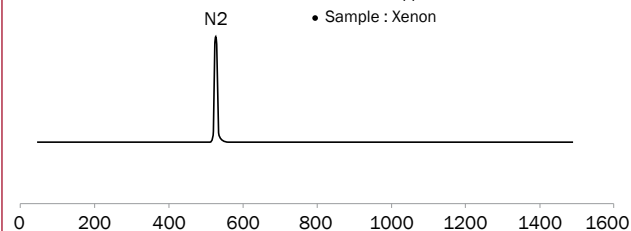


CHROMATOGRAM #95

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium
- Impurity concentration :
H2 : 5.00 ppm
O2 : 5.00 ppm
CH4 : 5.00 ppm
- Sample : Xenon

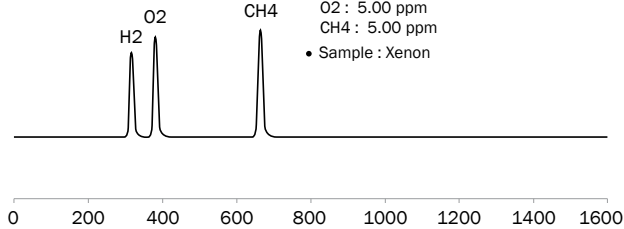


CHROMATOGRAM #96

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium
- Impurity concentration :
CO : 5.00 ppm
CO2 : 5.00 ppm
- Sample : Xenon

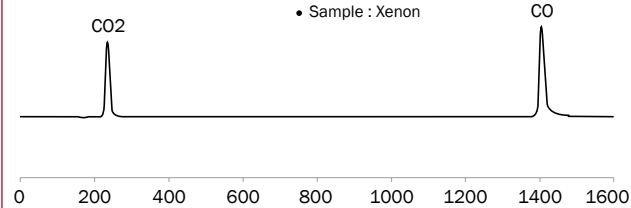


CHROMATOGRAM #97

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium
- Impurity concentration :
AR : 5.00 ppm
- Sample : Xenon

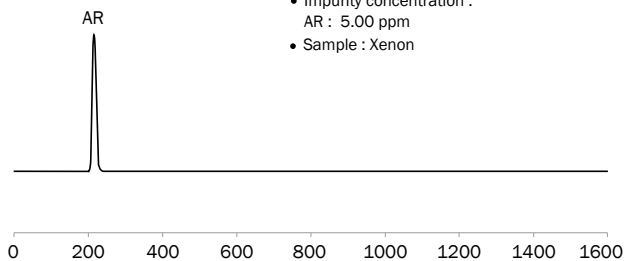


CHROMATOGRAM #98

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium
- Impurity concentration :
CF4 : 5.00 ppm
- Sample : Xenon

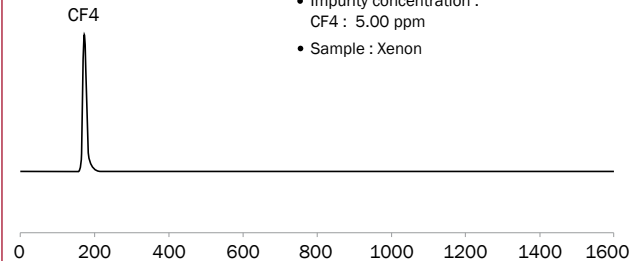


CHROMATOGRAM #99

- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium
- Impurity concentration :
CF4 : 5.00 ppm
- Sample : Krypton

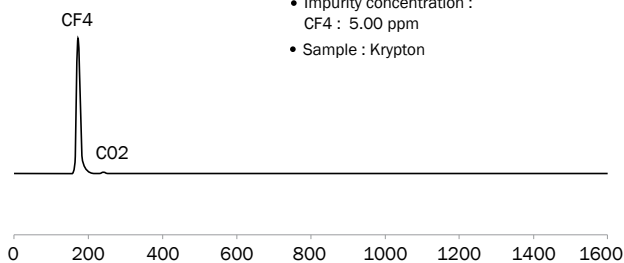


CHROMATOGRAM #100


- Instrument : Micro GC MultiDetek series
- Detector : PlasmaDetek series (PED)
- Carrier Gas : Helium
- Impurity concentration :
CO : 5.00 ppm
CO2 : 5.00 ppm
- Sample : Krypton

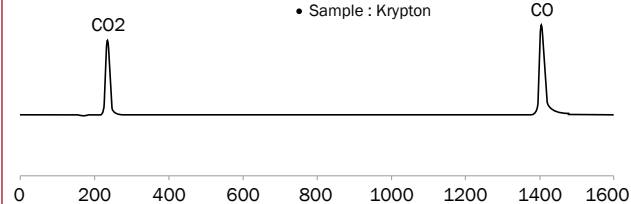


CHROMATOGRAM #101

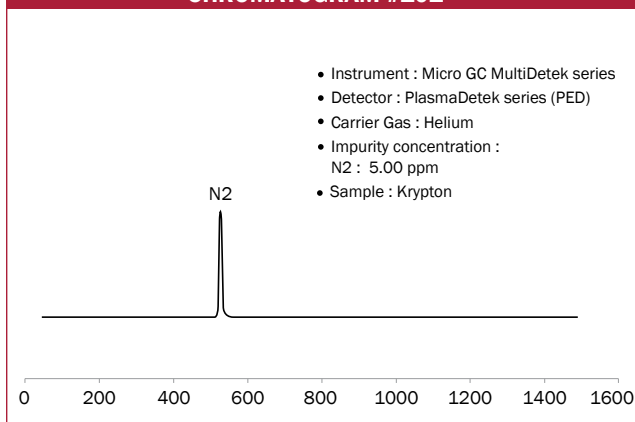


CHROMATOGRAM #102

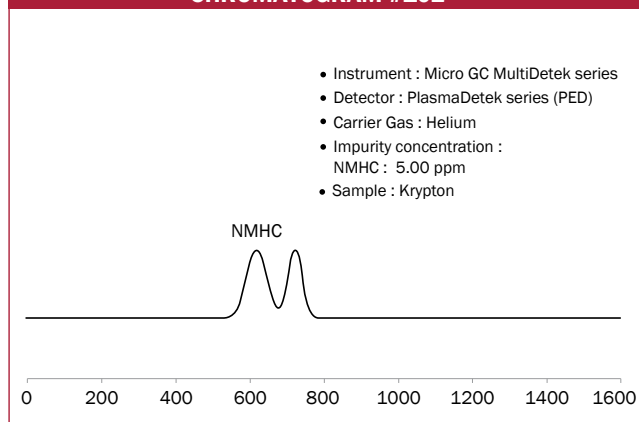


CHROMATOGRAM #103

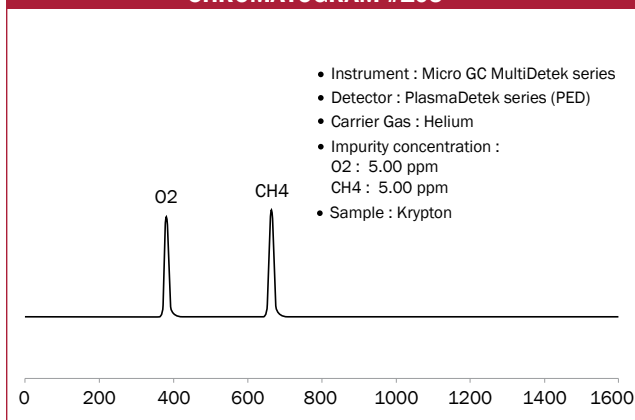


CHROMATOGRAM #104

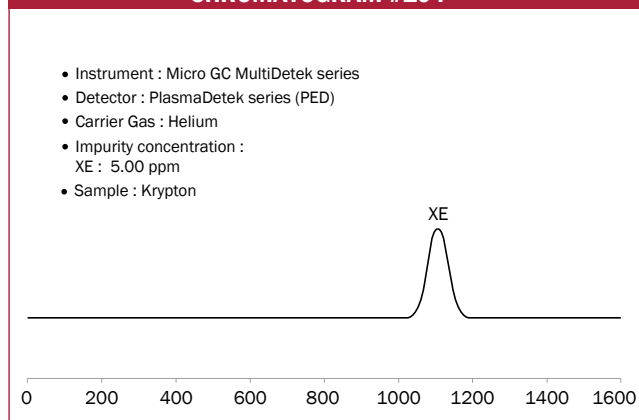


CHROMATOGRAM #105

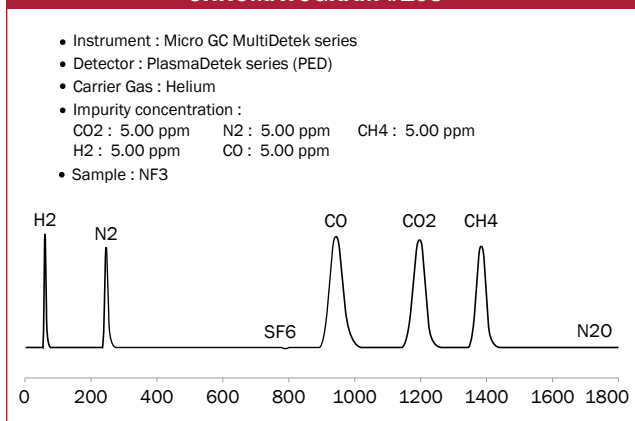


CHROMATOGRAM #106

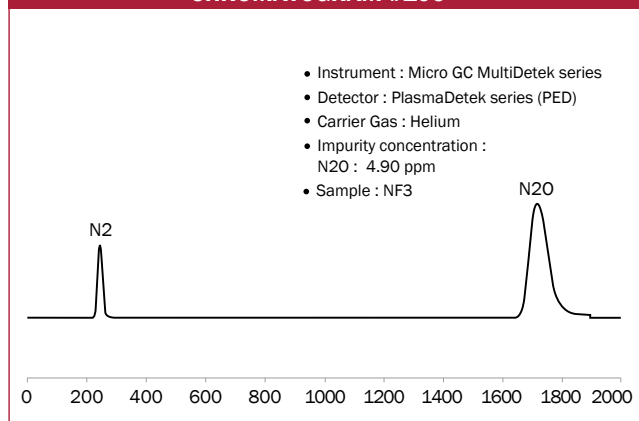


CHROMATOGRAM #107

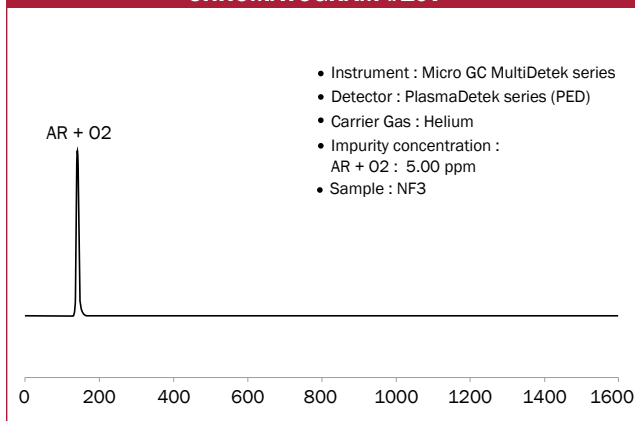


CHROMATOGRAM #108

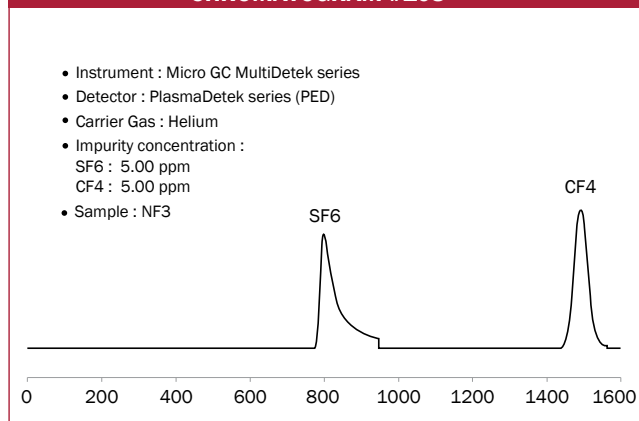


CHROMATOGRAM #109

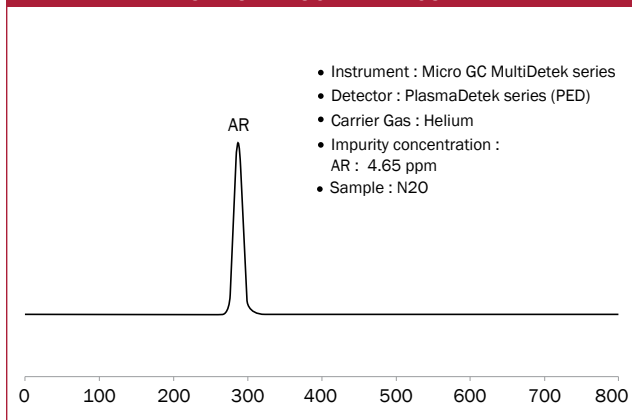


CHROMATOGRAM #110

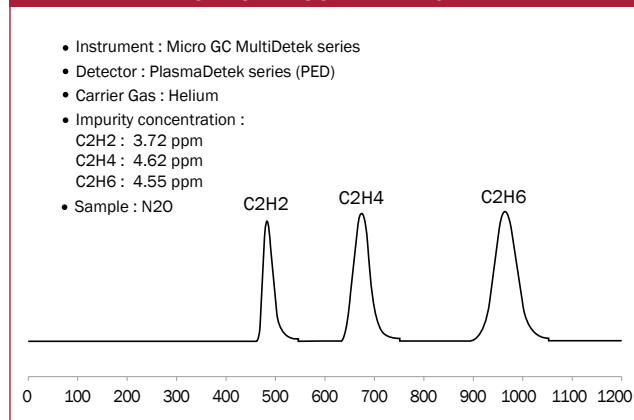


CHROMATOGRAM #111

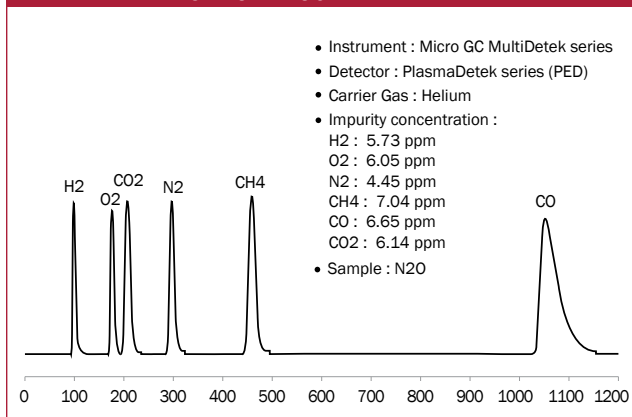


CHROMATOGRAM #112

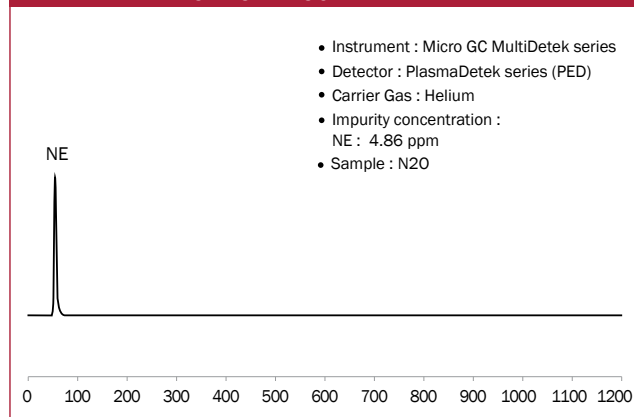


CHROMATOGRAM #113

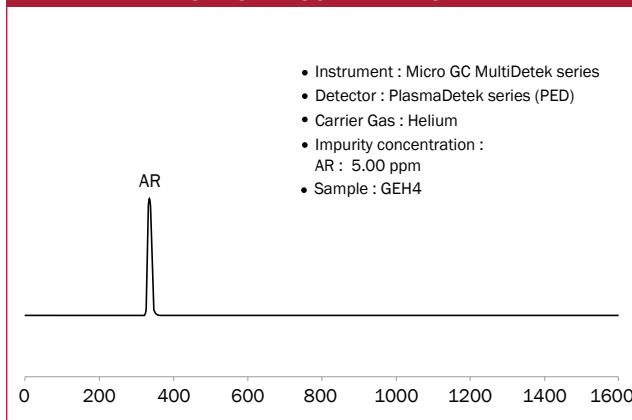


CHROMATOGRAM #114

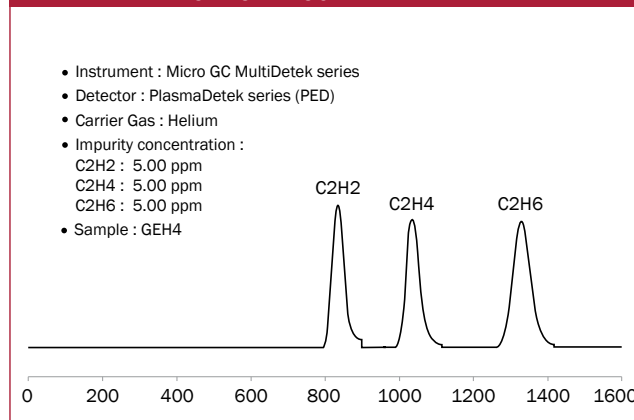


CHROMATOGRAM #115

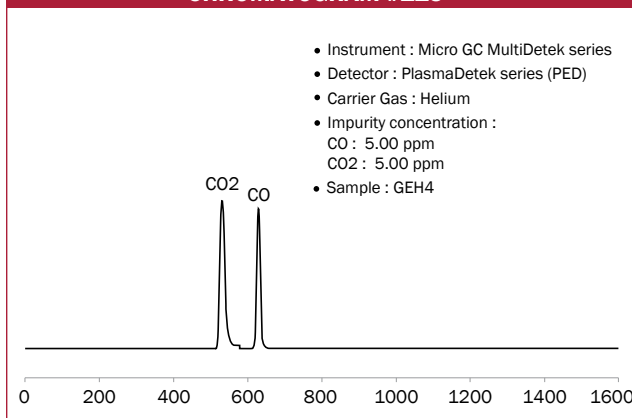

CHROMATOGRAM #116

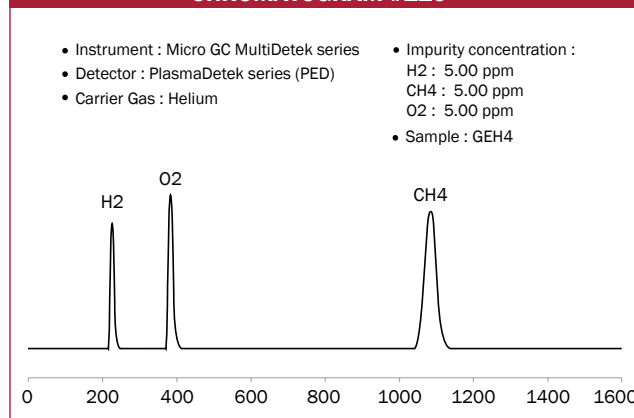

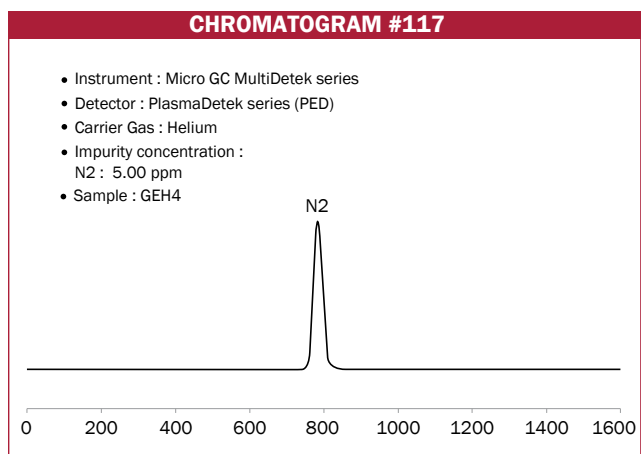

NOTES

[illegible]



Where **innovation** leads to **success**

990 Monfette Est, Thetford Mines, (Qc), Canada, G6G 7K6
Phone: 418 755-1319 • Fax: 418 755-1329
info@ldetek.com • www.ldetek.com